

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102822\
 Data File : FB028777.D
 Signal(s) : FID2B.CH
 Acq On : 28 Oct 2022 14:35
 Operator : AJ/MA
 Sample : N5236-02
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Oct 29 08:01:39 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100522.M
 Quant Title :
 QLast Update : Wed Oct 05 12:47:25 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.794	332116	25.671 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.712	23819	1.456 ng/ml
2) t 2,2,4-Trimethylpentane	7.376	151602	8.389 ng/ml
3) t n-Heptane	7.753	2561	0.151 ng/ml
6) t Toluene	10.616	8971	0.428 ng/ml
7) t Ethylbenzene	13.001	20039	1.010 ng/ml
8) t m-Xylene	13.186	21183	1.075 ng/ml
9) t O-Xylene	13.923	8709	0.448 ng/ml
10) t 1,2,4-Trimethylbenzene	16.125	13785	0.712 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102822\
Data File : FB028777.D
Signal(s) : FID2B.CH
Acq On : 28 Oct 2022 14:35
Operator : AJ/MA
Sample : N5236-02
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Oct 29 08:01:39 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100522.M
Quant Title :
QLast Update : Wed Oct 05 12:47:25 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

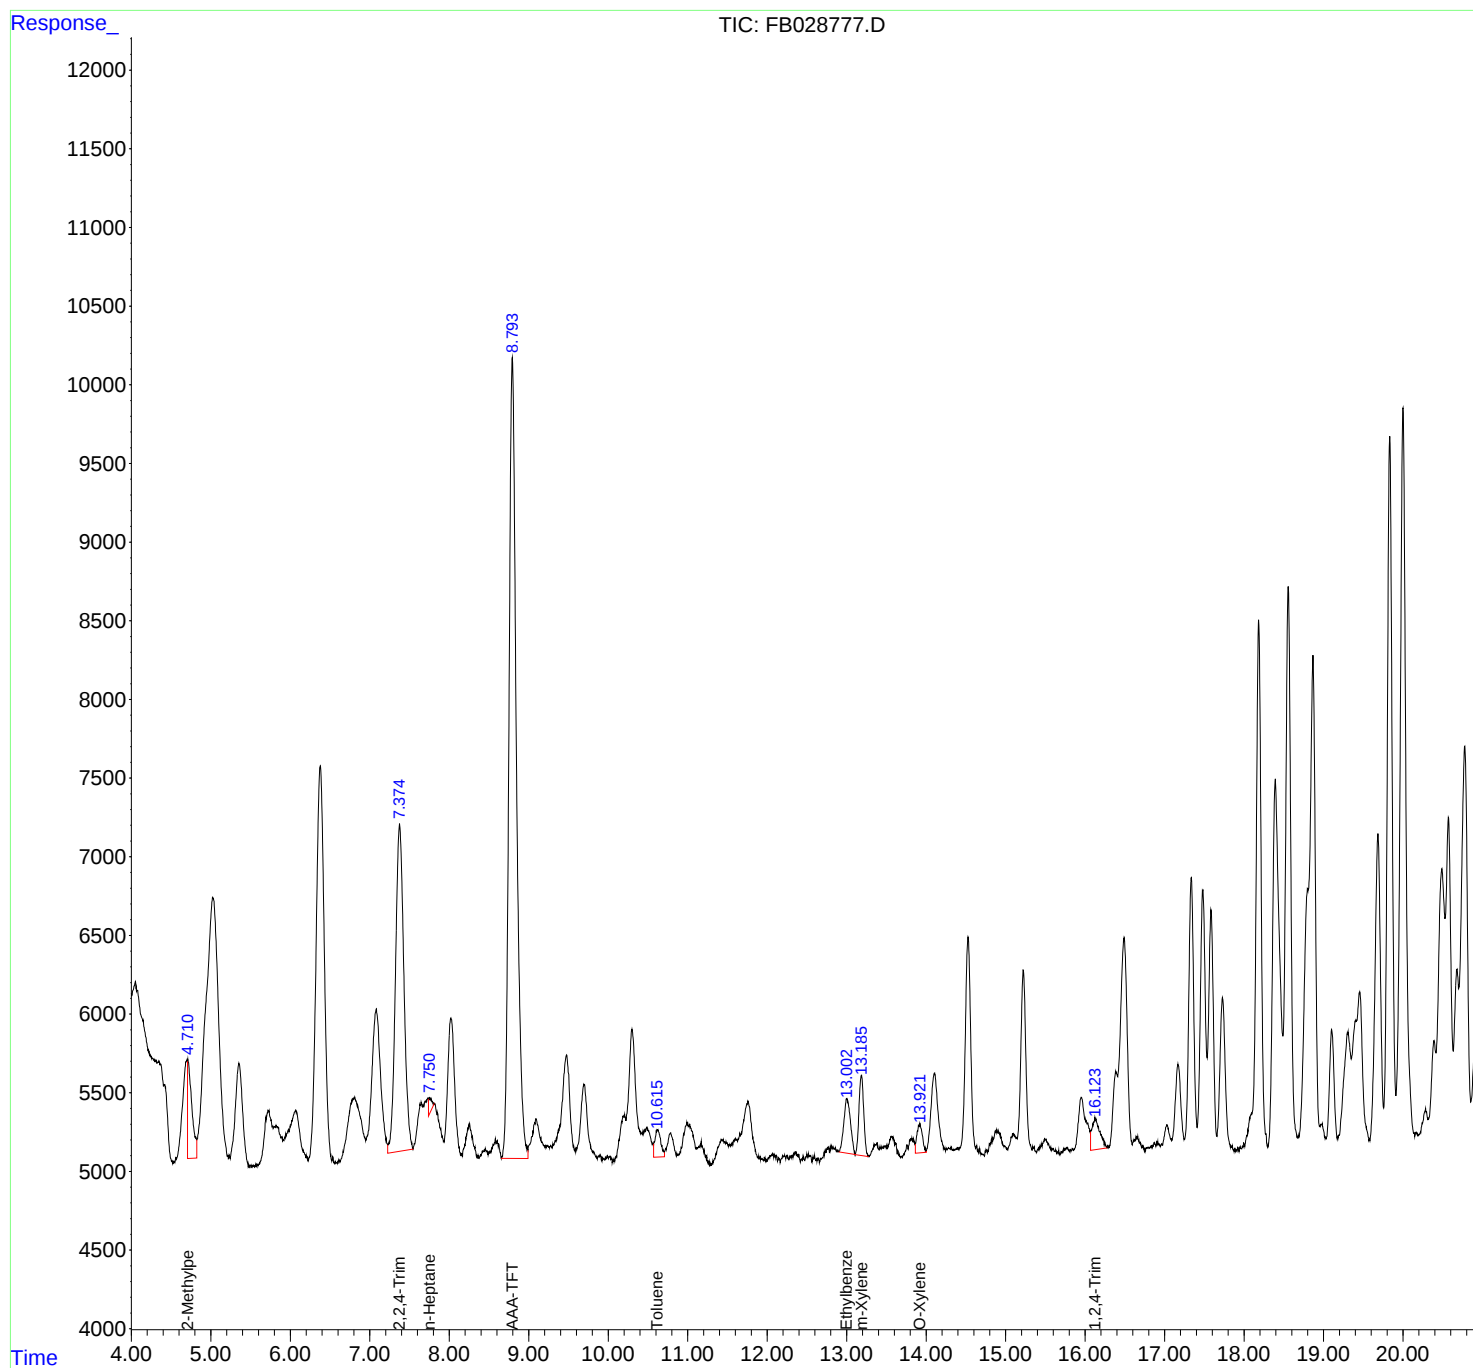


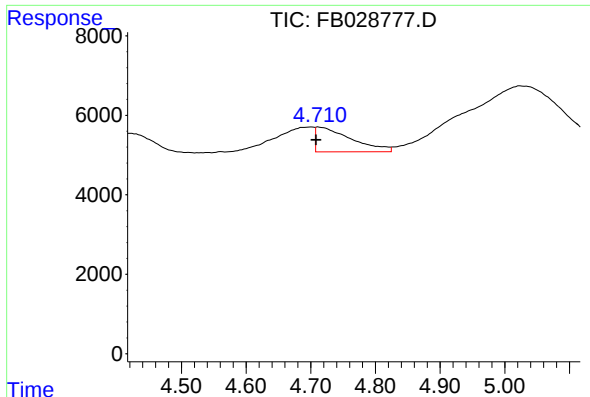

#1 2-Methylpentane


R.T.: 4.712 min
Delta R.T.: 0.004 min
Response: 23819
Conc: 1.46 ng/ml

Instrument :
FID_B
ClientSampleId :

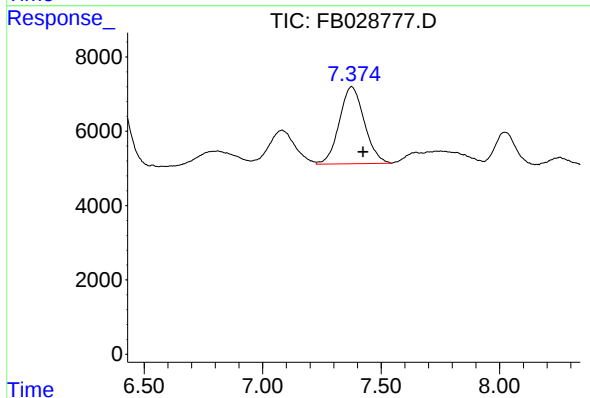


#2 2,2,4-Trimethylpentane

R.T.: 7.376 min
Delta R.T.: -0.048 min
Response: 151602
Conc: 8.39 ng/ml

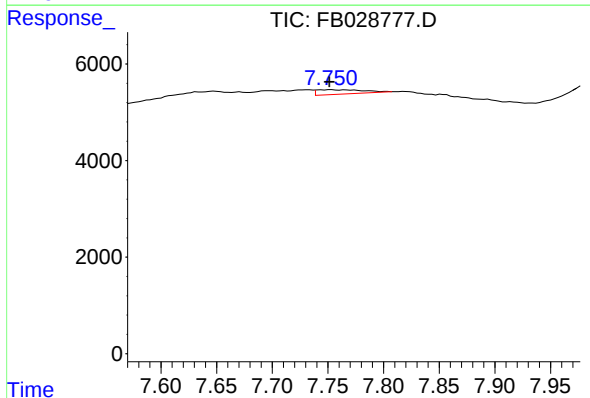


#3 n-Heptane

R.T.: 7.753 min
Delta R.T.: 0.002 min
Response: 2561
Conc: 0.15 ng/ml

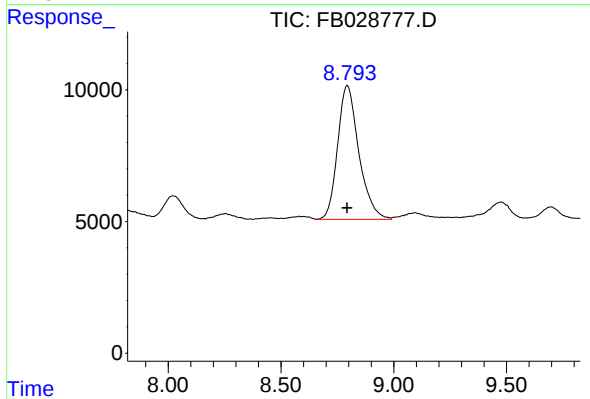

#5 AAA-TFT


R.T.: 8.794 min
Delta R.T.: 0.001 min
Response: 332116
Conc: 25.67 ng/ml

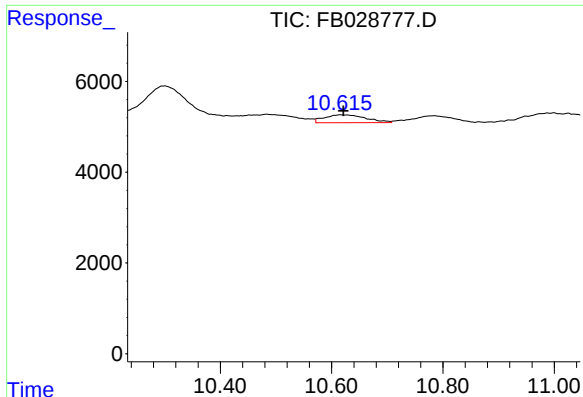

#6 Toluene


R.T.: 10.616 min
Delta R.T.: -0.005 min
Response: 8971
Conc: 0.43 ng/ml

Instrument :
FID_B
ClientSampleId :

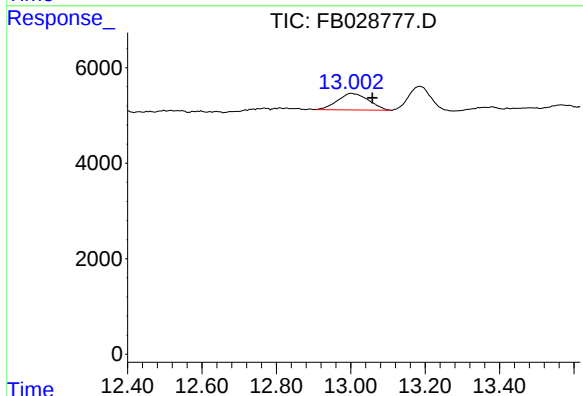


#7 Ethylbenzene

R.T.: 13.001 min
Delta R.T.: -0.057 min
Response: 20039
Conc: 1.01 ng/ml

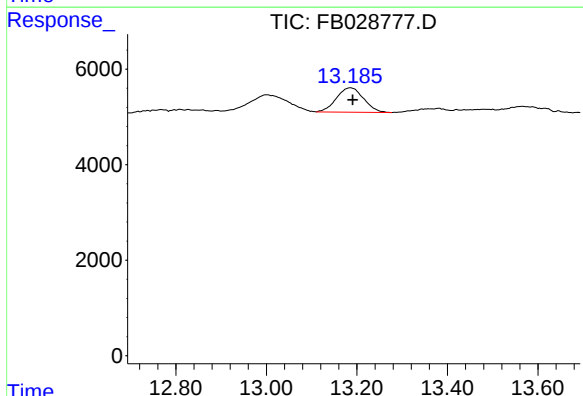


#8 m-Xylene

R.T.: 13.186 min
Delta R.T.: -0.004 min
Response: 21183
Conc: 1.08 ng/ml

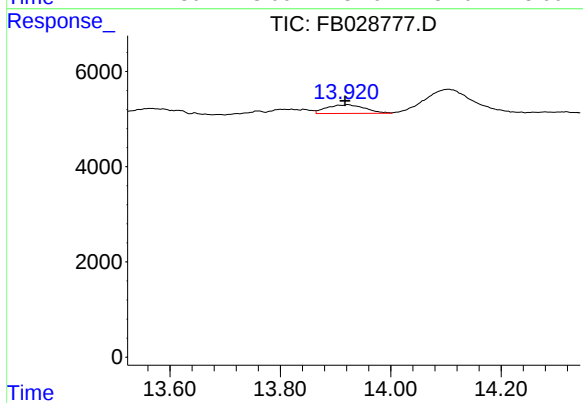

#9 O-Xylene

R.T.: 13.923 min
Delta R.T.: 0.006 min
Response: 8709
Conc: 0.45 ng/ml

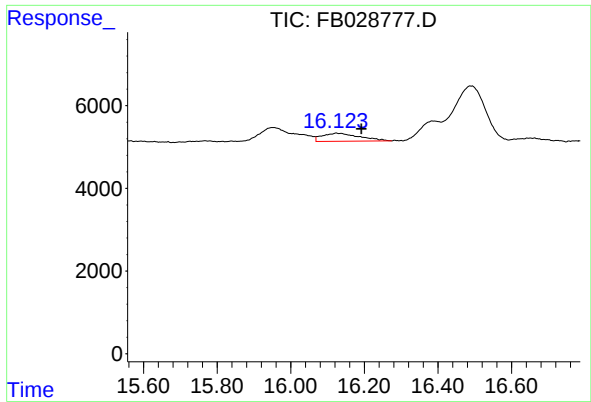

#10 1,2,4-Trimethylbenzene

R.T.: 16.125 min
Delta R.T.: -0.068 min
Response: 13785
Conc: 0.71 ng/ml

Instrument :
FID_B
ClientSampleId :