

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB102822\  
 Data File : FB028788.D  
 Signal(s) : FID2B.CH  
 Acq On : 28 Oct 2022 22:37  
 Operator : AJ/MA  
 Sample : BSF1028S2  
 Misc : 5.00G/5.00 ML DI WATER  
 ALS Vial : 17 Sample Multiplier: 1

Instrument :  
 FID\_B  
 ClientSampleId :

Integration File: Calibration.e  
 Quant Time: Oct 29 08:16:36 2022  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB100522.M  
 Quant Title :  
 QLast Update : Wed Oct 05 12:47:25 2022  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 5 g/ml  
 Signal Phase : RTX-502.2  
 Signal Info : 60mx0.53mmx3.00um

| Compound                     | R.T.   | Response | Conc Units   |
|------------------------------|--------|----------|--------------|
| -----                        |        |          |              |
| System Monitoring Compounds  |        |          |              |
| 5) s AAA-TFT                 | 8.789  | 271223   | 20.965 ng/ml |
| Target Compounds             |        |          |              |
| 1) t 2-Methylpentane         | 4.708  | 495197   | 30.271 ng/ml |
| 2) t 2,2,4-Trimethylpentane  | 7.420  | 539839   | 29.871 ng/ml |
| 3) t n-Heptane               | 7.749  | 180302   | 10.645 ng/ml |
| 4) t Benzene                 | 7.884  | 211600   | 9.634 ng/ml  |
| 6) t Toluene                 | 10.617 | 606817   | 28.951 ng/ml |
| 7) t Ethylbenzene            | 13.053 | 189048   | 9.526 ng/ml  |
| 8) t m-Xylene                | 13.186 | 377440   | 19.159 ng/ml |
| 9) t O-Xylene                | 13.912 | 365893   | 18.807 ng/ml |
| 10) t 1,2,4-Trimethylbenzene | 16.187 | 368359   | 19.028 ng/ml |
| -----                        |        |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB102822\  
Data File : FB028788.D  
Signal(s) : FID2B.CH  
Acq On : 28 Oct 2022 22:37  
Operator : AJ/MA  
Sample : BSF1028S2  
Misc : 5.00G/5.00 ML DI WATER  
ALS Vial : 17 Sample Multiplier: 1

Instrument :  
FID\_B  
ClientSampleId :

Integration File: Calibration.e  
Quant Time: Oct 29 08:16:36 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB100522.M  
Quant Title :  
QLast Update : Wed Oct 05 12:47:25 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

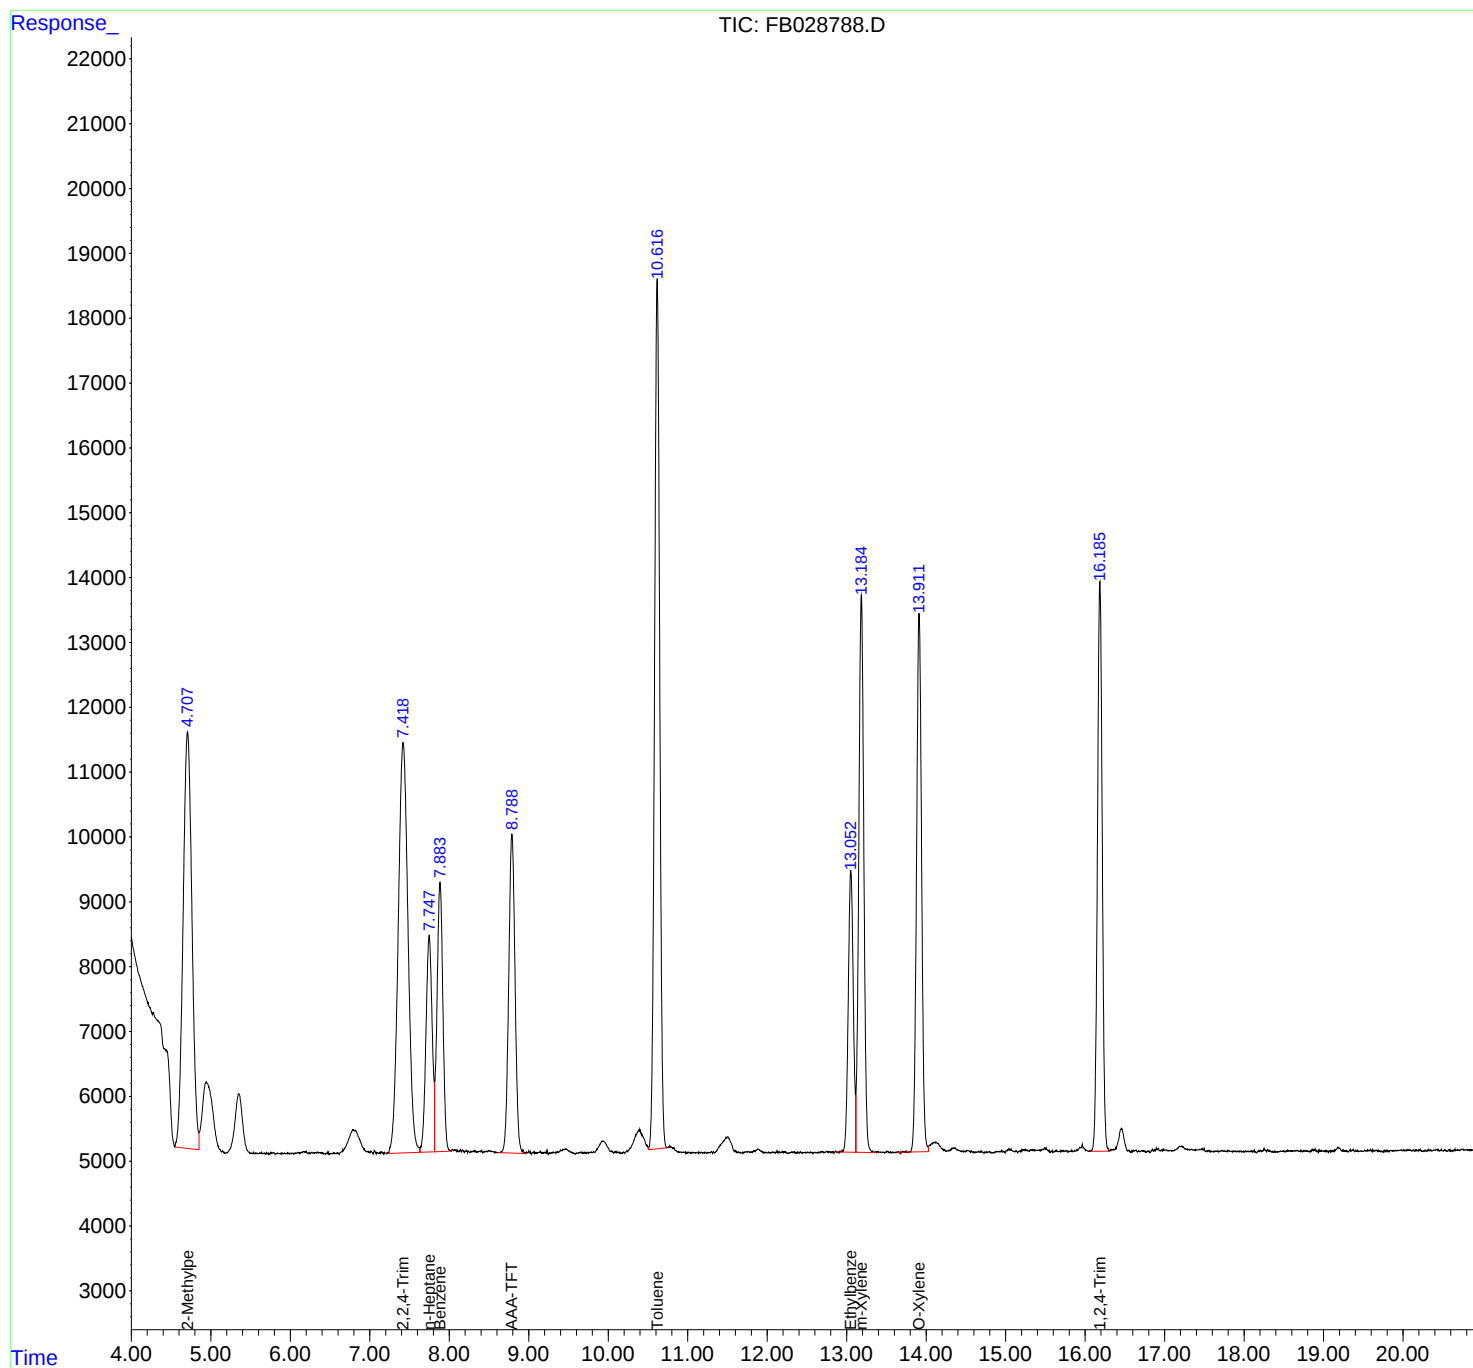


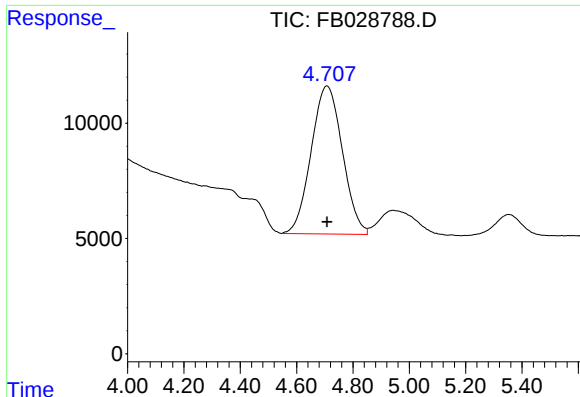

#1 2-Methylpentane


R.T.: 4.708 min  
Delta R.T.: 0.000 min  
Response: 495197  
Conc: 30.27 ng/ml

Instrument :  
FID\_B  
ClientSampleId :

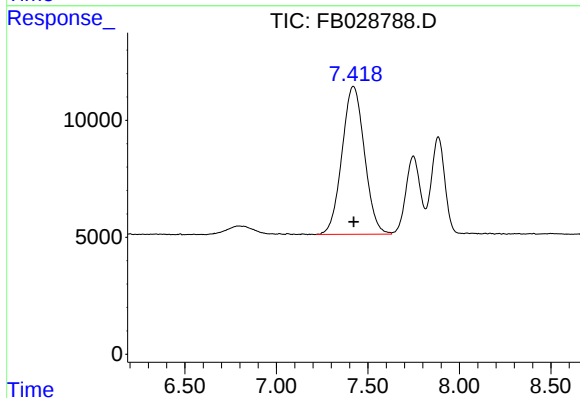


#2 2,2,4-Trimethylpentane

R.T.: 7.420 min  
Delta R.T.: -0.004 min  
Response: 539839  
Conc: 29.87 ng/ml

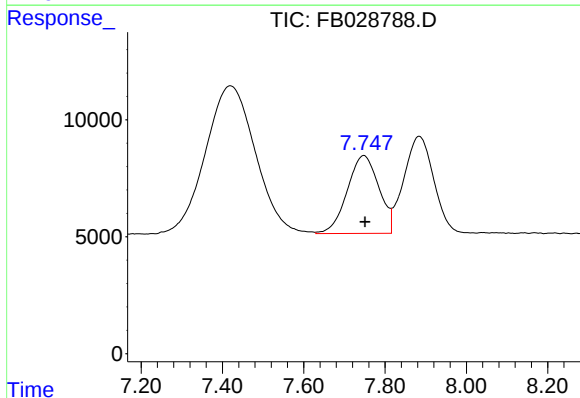


#3 n-Heptane

R.T.: 7.749 min  
Delta R.T.: -0.003 min  
Response: 180302  
Conc: 10.64 ng/ml

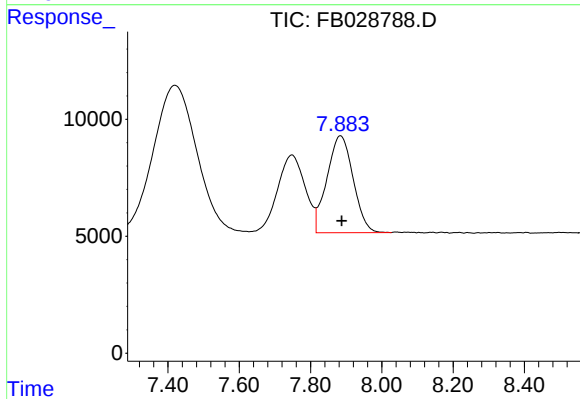

#4 Benzene


R.T.: 7.884 min  
Delta R.T.: -0.003 min  
Response: 211600  
Conc: 9.63 ng/ml

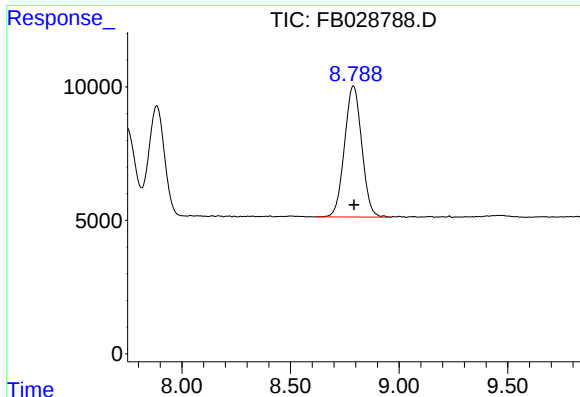

#5 AAA-TFT


R.T.: 8.789 min  
Delta R.T.: -0.003 min  
Response: 271223  
Conc: 20.96 ng/ml

Instrument :  
FID\_B  
ClientSampleId :

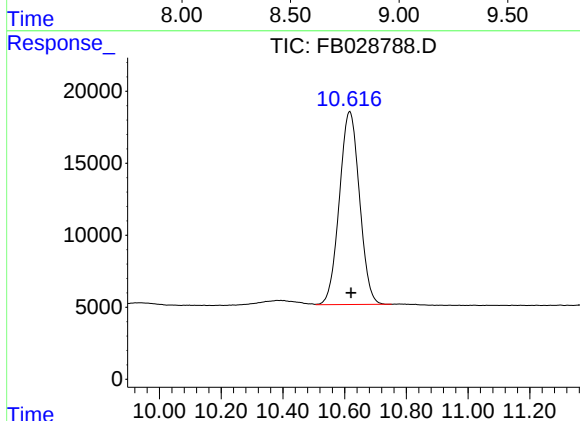


#6 Toluene

R.T.: 10.617 min  
Delta R.T.: -0.004 min  
Response: 606817  
Conc: 28.95 ng/ml

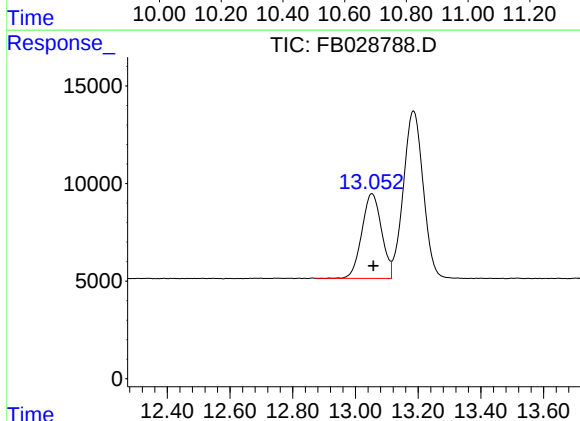


#7 Ethylbenzene

R.T.: 13.053 min  
Delta R.T.: -0.005 min  
Response: 189048  
Conc: 9.53 ng/ml

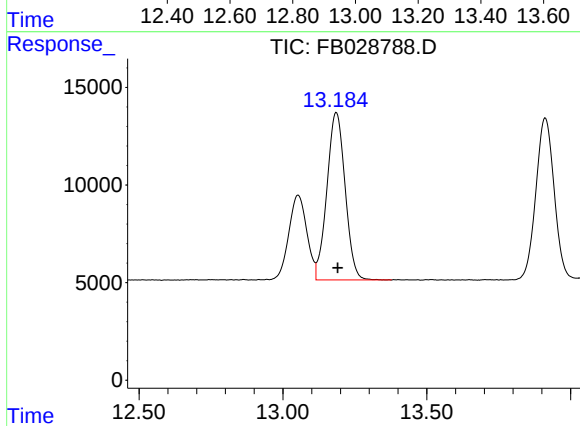

#8 m-Xylene


R.T.: 13.186 min  
Delta R.T.: -0.005 min  
Response: 377440  
Conc: 19.16 ng/ml

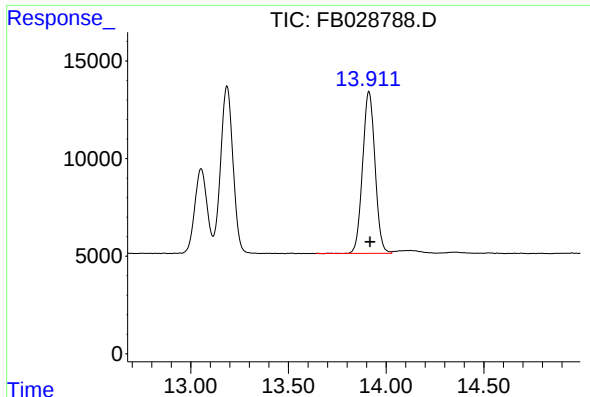

#9 O-Xylene

R.T.: 13.912 min  
Delta R.T.: -0.005 min  
Response: 365893  
Conc: 18.81 ng/ml

Instrument :  
FID\_B  
ClientSampleId :

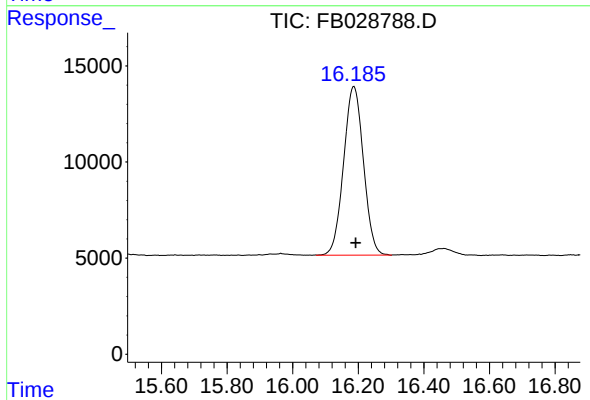

#10 1,2,4-Trimethylbenzene

R.T.: 16.187 min  
Delta R.T.: -0.006 min  
Response: 368359  
Conc: 19.03 ng/ml