

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102822\
 Data File : FB028784.D
 Signal(s) : FID2B.CH
 Acq On : 28 Oct 2022 19:32
 Operator : AJ/MA
 Sample : N5235-02MS 50X
 Misc : 2.48G/5.00 ML DI WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 LSP-SS-01-00-20MS

Integration File: Calibration.e
 Quant Time: Oct 29 08:16:18 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100522.M
 Quant Title :
 QLast Update : Wed Oct 05 12:47:25 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.788	258327	19.968 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.701	448303	27.404 ng/ml
2) t 2,2,4-Trimethylpentane	7.419	494464	27.361 ng/ml
3) t n-Heptane	7.747	171731	10.139 ng/ml
4) t Benzene	7.883	202273	9.209 ng/ml
6) t Toluene	10.616	587762	28.042 ng/ml
7) t Ethylbenzene	13.054	181625	9.152 ng/ml
8) t m-Xylene	13.186	358491	18.197 ng/ml
9) t O-Xylene	13.913	346272	17.799 ng/ml
10) t 1,2,4-Trimethylbenzene	16.188	325526	16.815 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102822\
Data File : FB028784.D
Signal(s) : FID2B.CH
Acq On : 28 Oct 2022 19:32
Operator : AJ/MA
Sample : N5235-02MS 50X
Misc : 2.48G/5.00 ML DI WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
LSP-SS-01-00-20MS

Integration File: Calibration.e
Quant Time: Oct 29 08:16:18 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100522.M
Quant Title :
QLast Update : Wed Oct 05 12:47:25 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

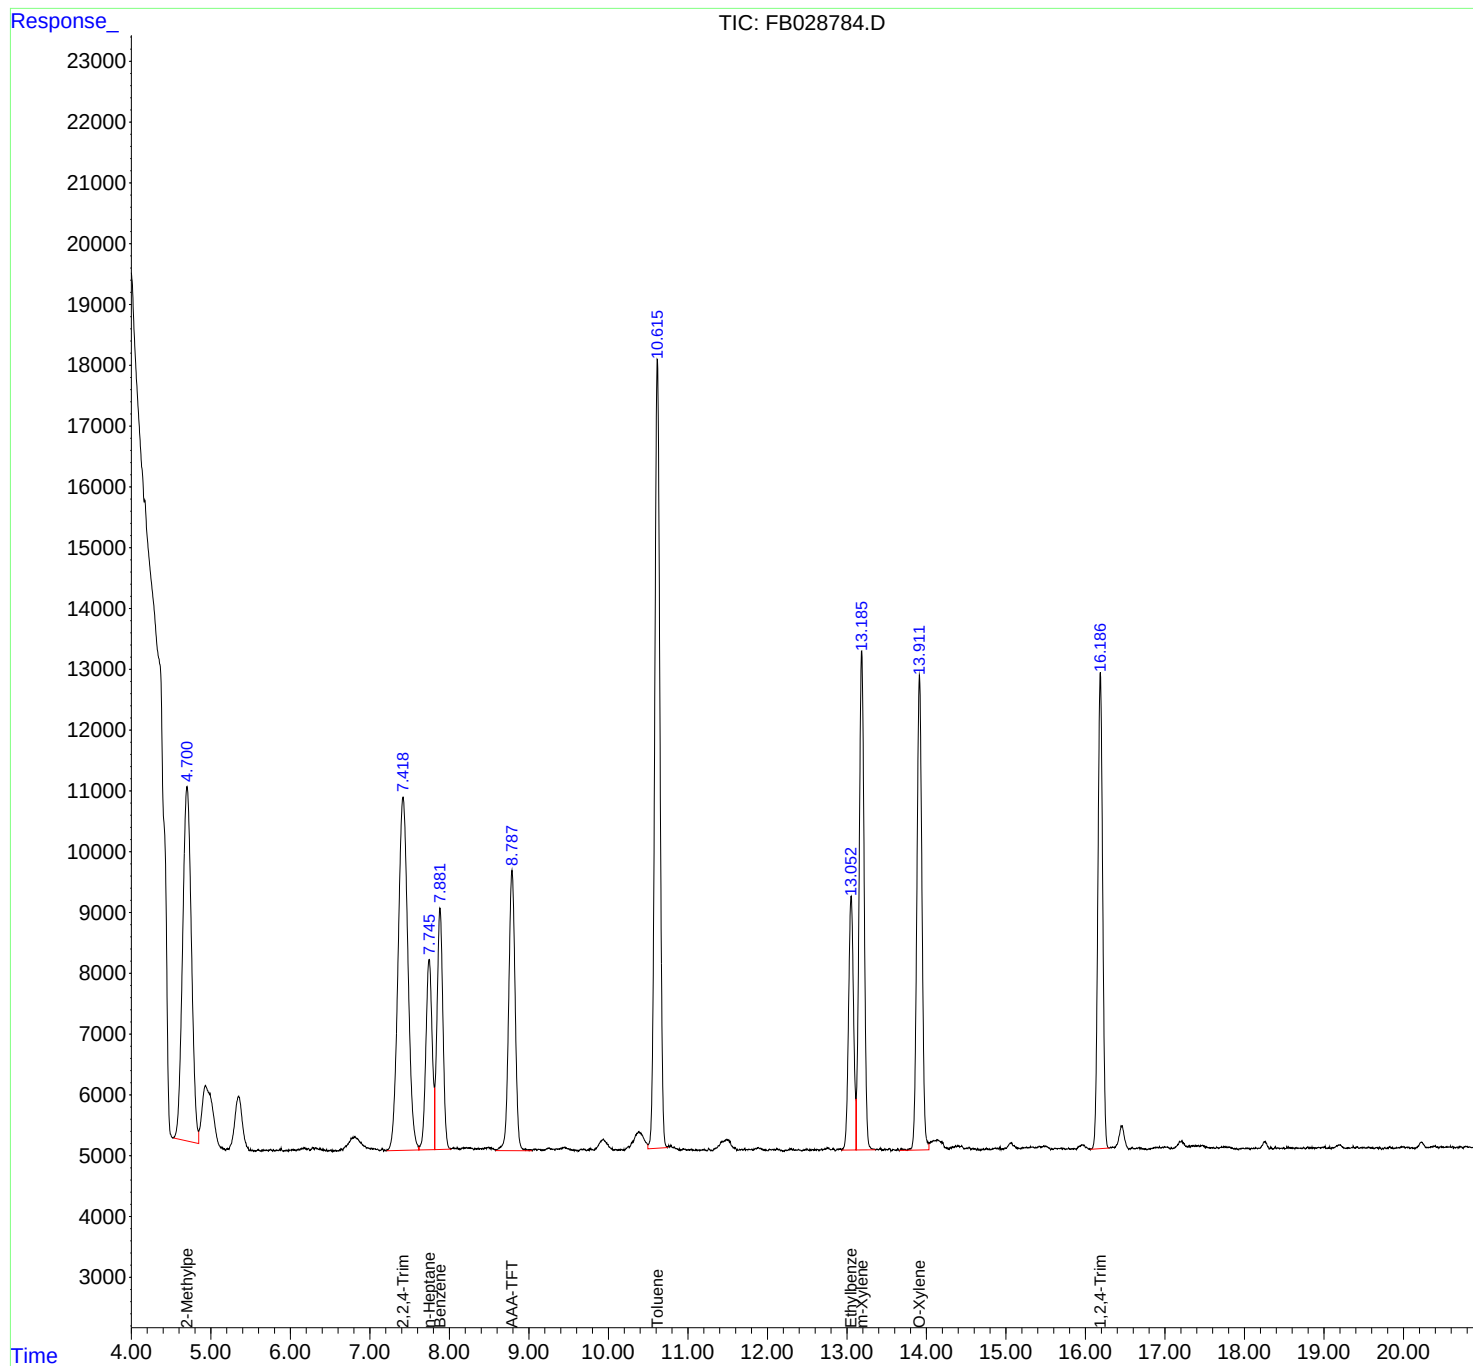


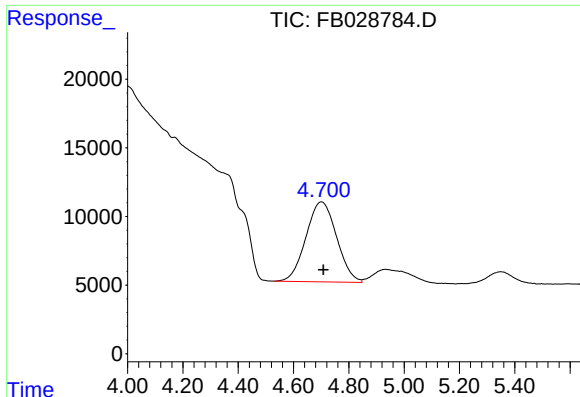

#1 2-Methylpentane


R.T.: 4.701 min
Delta R.T.: -0.007 min
Response: 448303
Conc: 27.40 ng/ml

Instrument :
FID_B
ClientSampleId :
LSP-SS-01-00-20MS

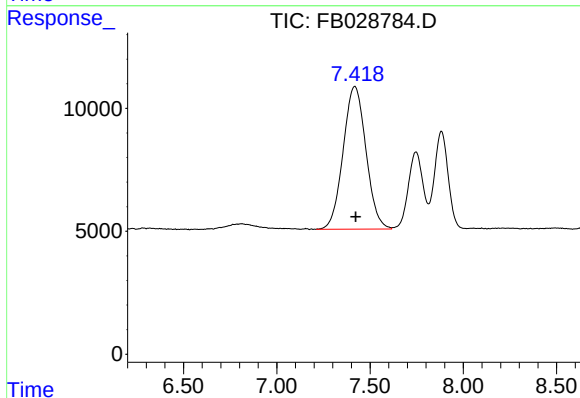


#2 2,2,4-Trimethylpentane

R.T.: 7.419 min
Delta R.T.: -0.004 min
Response: 494464
Conc: 27.36 ng/ml

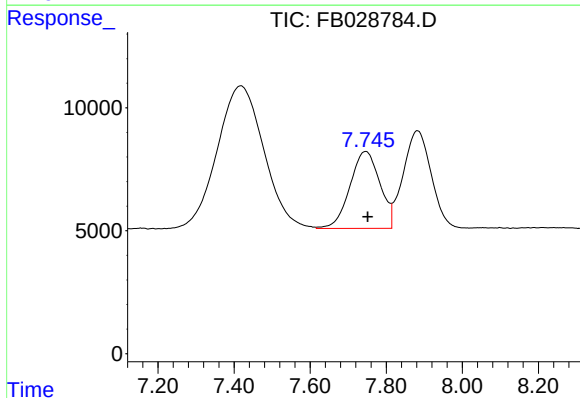


#3 n-Heptane

R.T.: 7.747 min
Delta R.T.: -0.005 min
Response: 171731
Conc: 10.14 ng/ml

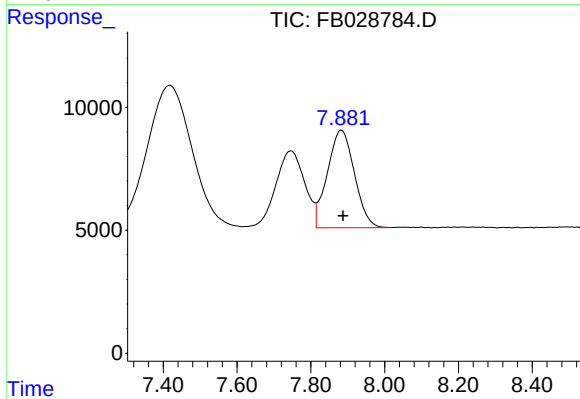

#4 Benzene


R.T.: 7.883 min
Delta R.T.: -0.005 min
Response: 202273
Conc: 9.21 ng/ml

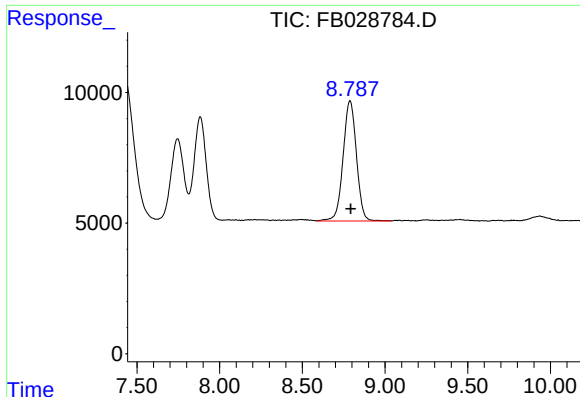

#5 AAA-TFT


R.T.: 8.788 min
Delta R.T.: -0.004 min
Response: 258327
Conc: 19.97 ng/ml

Instrument :
FID_B
ClientSampleId :
LSP-SS-01-00-20MS

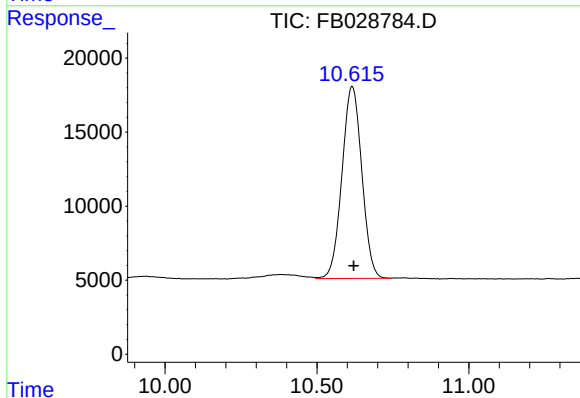


#6 Toluene

R.T.: 10.616 min
Delta R.T.: -0.005 min
Response: 587762
Conc: 28.04 ng/ml

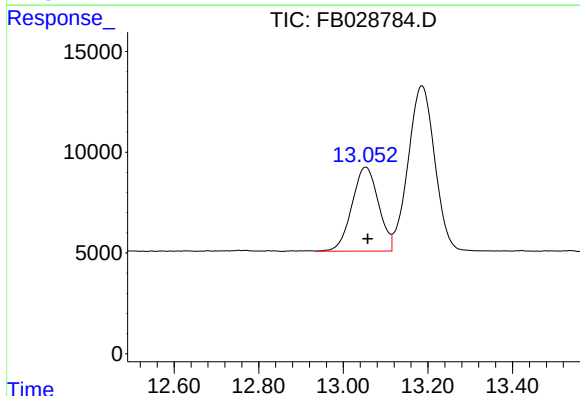


#7 Ethylbenzene

R.T.: 13.054 min
Delta R.T.: -0.004 min
Response: 181625
Conc: 9.15 ng/ml

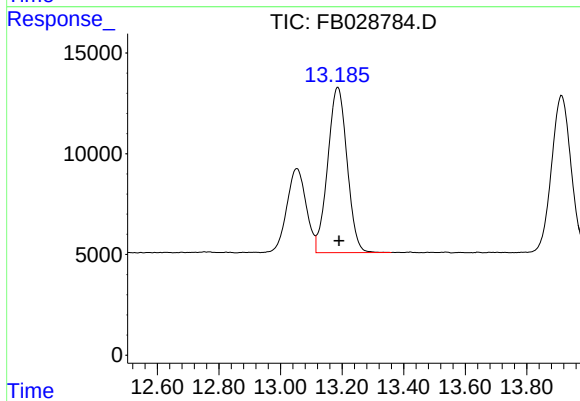

#8 m-Xylene


R.T.: 13.186 min
Delta R.T.: -0.004 min
Response: 358491
Conc: 18.20 ng/ml

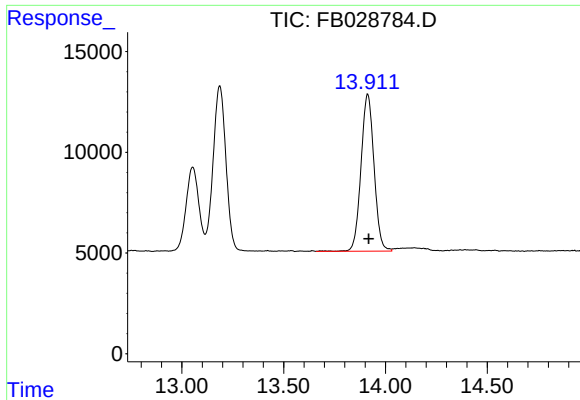

#9 O-Xylene

R.T.: 13.913 min
Delta R.T.: -0.004 min
Response: 346272
Conc: 17.80 ng/ml

Instrument :
FID_B
ClientSampleId :
LSP-SS-01-00-20MS

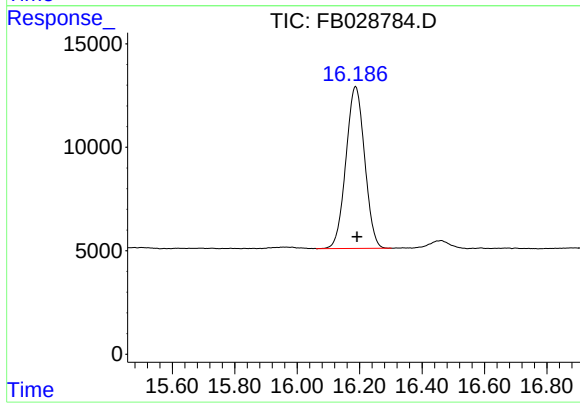

#10 1,2,4-Trimethylbenzene

R.T.: 16.188 min
Delta R.T.: -0.005 min
Response: 325526
Conc: 16.82 ng/ml