

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102822\
 Data File : FB028785.D
 Signal(s) : FID2B.CH
 Acq On : 28 Oct 2022 20:09
 Operator : AJ/MA
 Sample : N5235-03MSD 50X
 Misc : 2.32G/5.00 ML DI WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 LSP-SS-01-00-20MSD

Integration File: Calibration.e
 Quant Time: Oct 29 08:16:23 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100522.M
 Quant Title :
 QLast Update : Wed Oct 05 12:47:25 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.788	286767	22.166 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.701	476110	29.104 ng/ml
2) t 2,2,4-Trimethylpentane	7.417	529218	29.284 ng/ml
3) t n-Heptane	7.746	184352	10.884 ng/ml
4) t Benzene	7.882	217386	9.897 ng/ml
6) t Toluene	10.616	629832	30.049 ng/ml
7) t Ethylbenzene	13.053	196394	9.896 ng/ml
8) t m-Xylene	13.186	379949	19.286 ng/ml
9) t O-Xylene	13.913	365475	18.786 ng/ml
10) t 1,2,4-Trimethylbenzene	16.187	342182	17.675 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102822\
Data File : FB028785.D
Signal(s) : FID2B.CH
Acq On : 28 Oct 2022 20:09
Operator : AJ/MA
Sample : N5235-03MSD 50X
Misc : 2.32G/5.00 ML DI WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
LSP-SS-01-00-20MSD

Integration File: Calibration.e
Quant Time: Oct 29 08:16:23 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100522.M
Quant Title :
QLast Update : Wed Oct 05 12:47:25 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

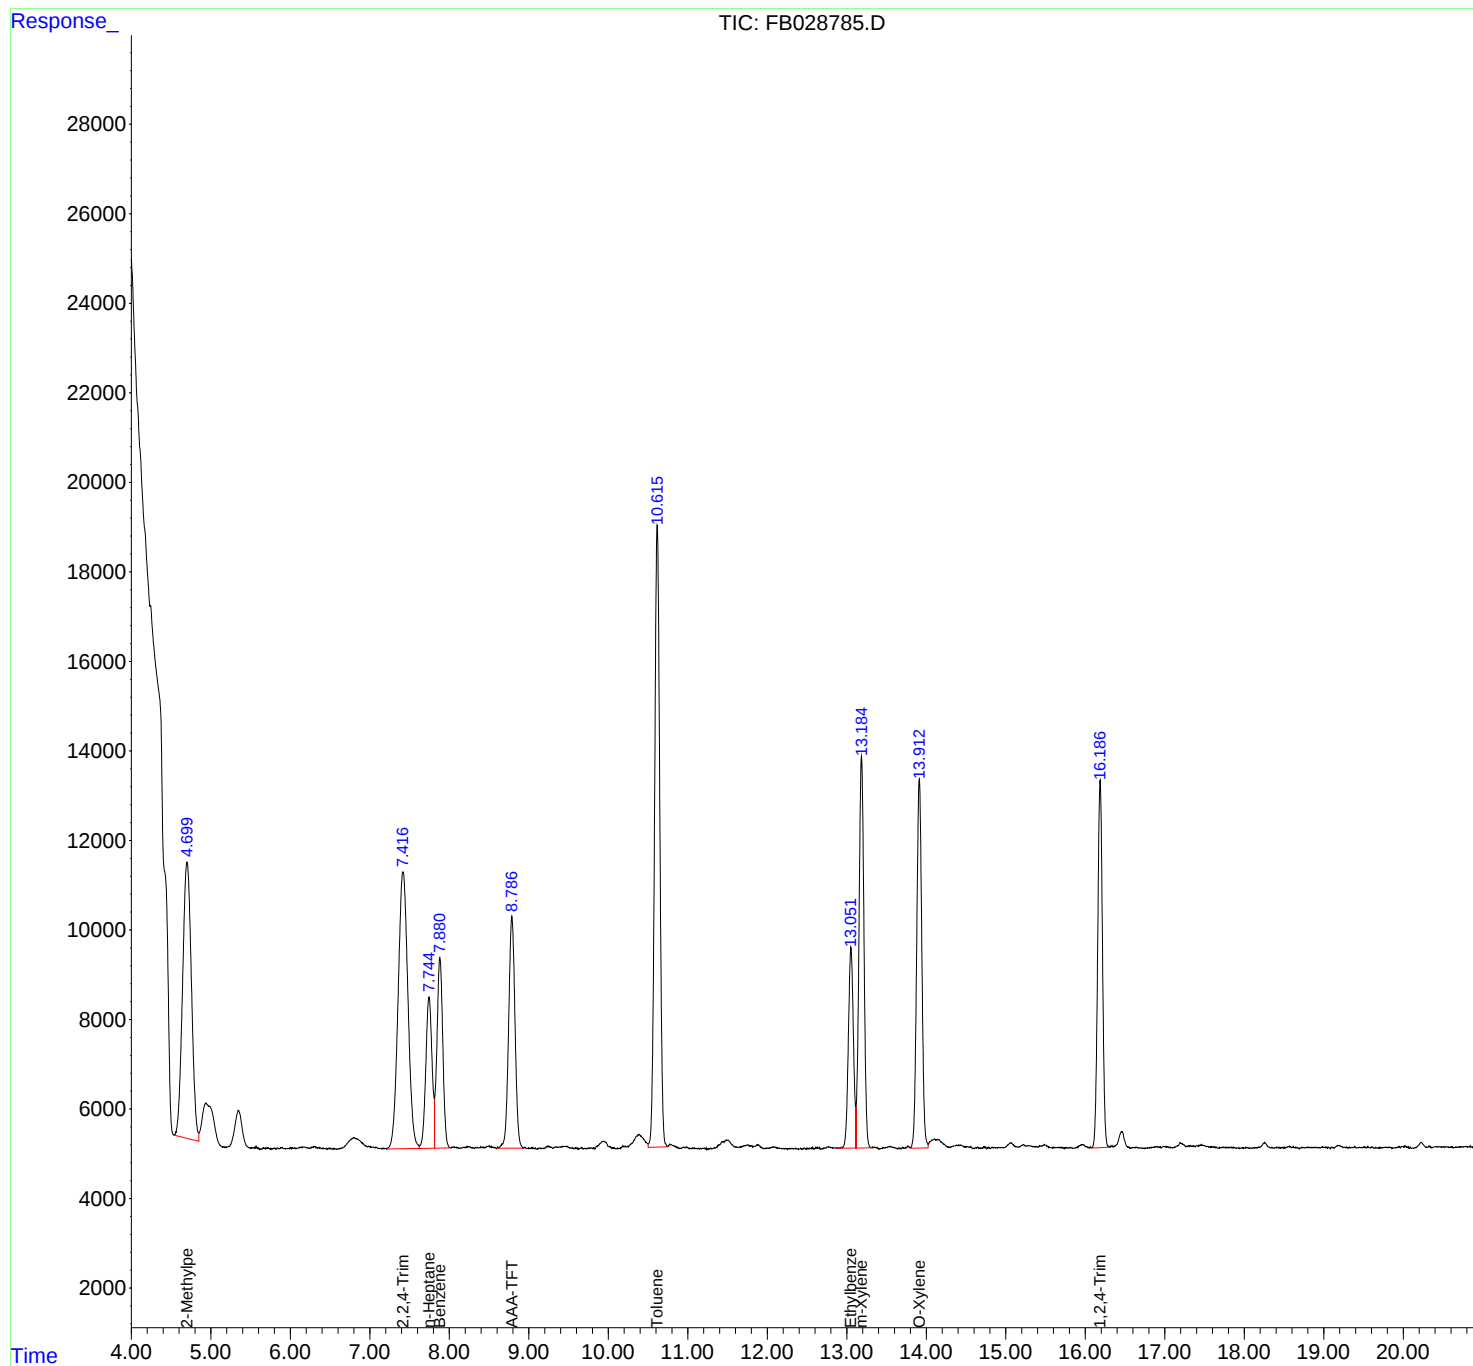


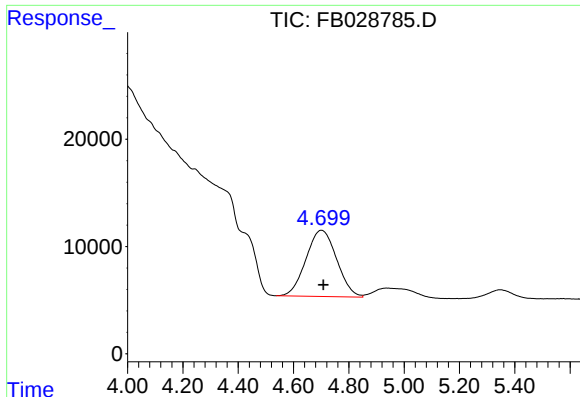

#1 2-Methylpentane


R.T.: 4.701 min
Delta R.T.: -0.007 min
Response: 476110
Conc: 29.10 ng/ml

Instrument :
FID_B
ClientSampleId :
LSP-SS-01-00-20MSD

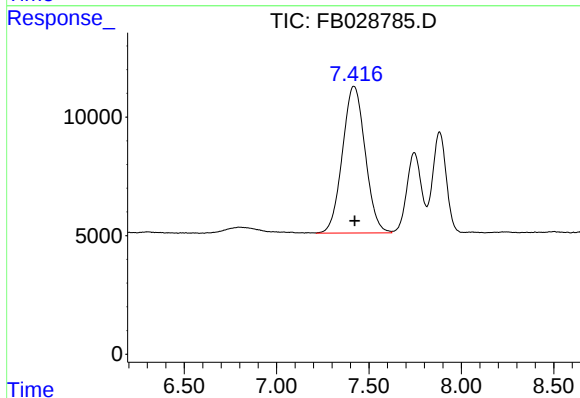


#2 2,2,4-Trimethylpentane

R.T.: 7.417 min
Delta R.T.: -0.006 min
Response: 529218
Conc: 29.28 ng/ml

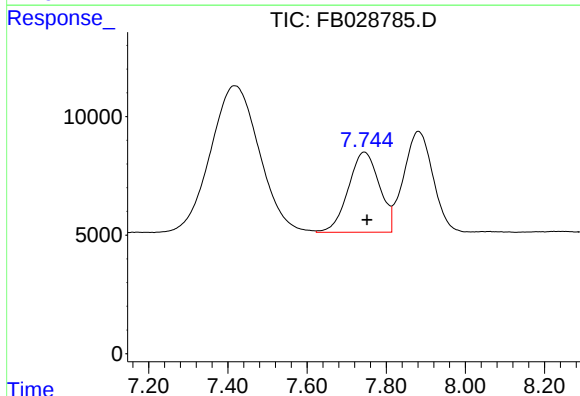


#3 n-Heptane

R.T.: 7.746 min
Delta R.T.: -0.006 min
Response: 184352
Conc: 10.88 ng/ml

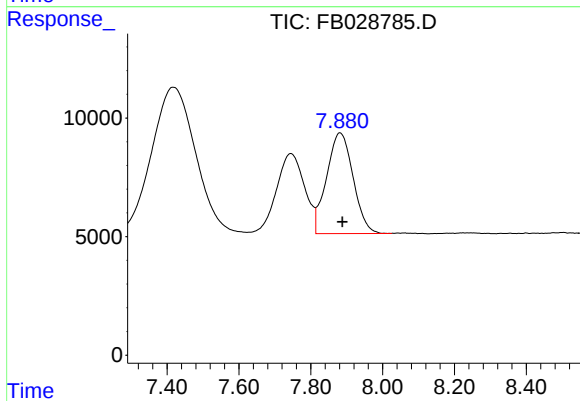

#4 Benzene


R.T.: 7.882 min
Delta R.T.: -0.006 min
Response: 217386
Conc: 9.90 ng/ml

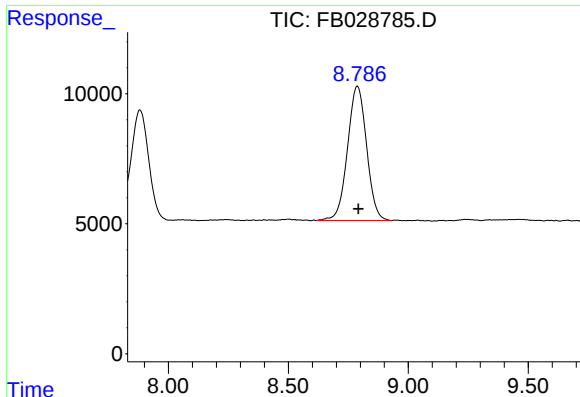

#5 AAA-TFT


R.T.: 8.788 min
Delta R.T.: -0.005 min
Response: 286767
Conc: 22.17 ng/ml

Instrument :
FID_B
ClientSampleId :
LSP-SS-01-00-20MSD

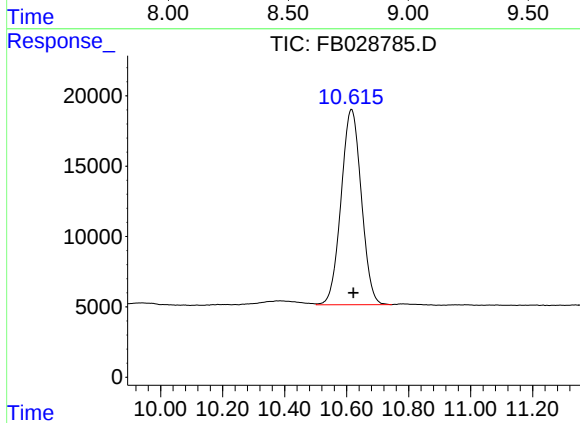


#6 Toluene

R.T.: 10.616 min
Delta R.T.: -0.005 min
Response: 629832
Conc: 30.05 ng/ml

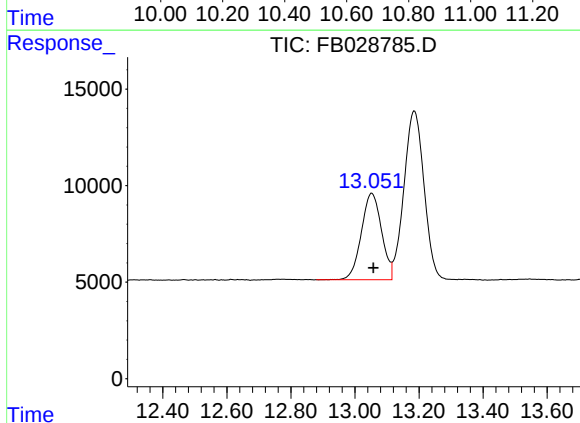


#7 Ethylbenzene

R.T.: 13.053 min
Delta R.T.: -0.005 min
Response: 196394
Conc: 9.90 ng/ml

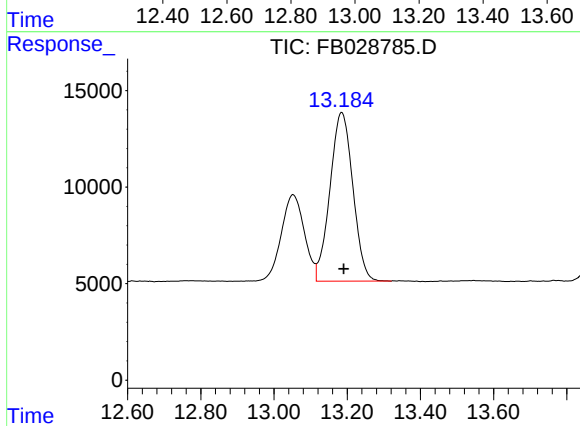

#8 m-Xylene


R.T.: 13.186 min
Delta R.T.: -0.005 min
Response: 379949
Conc: 19.29 ng/ml

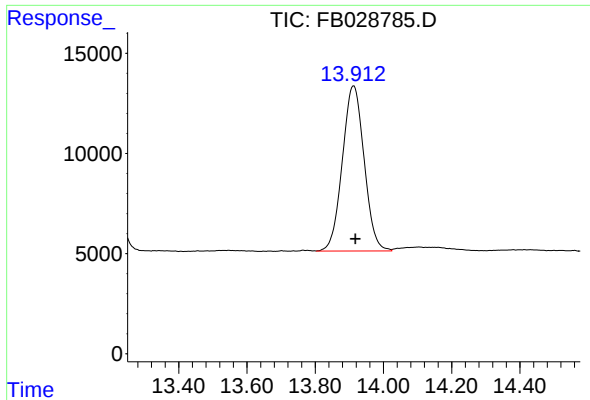

#9 O-Xylene

R.T.: 13.913 min
Delta R.T.: -0.005 min
Response: 365475
Conc: 18.79 ng/ml

Instrument :
FID_B
ClientSampleId :
LSP-SS-01-00-20MSD

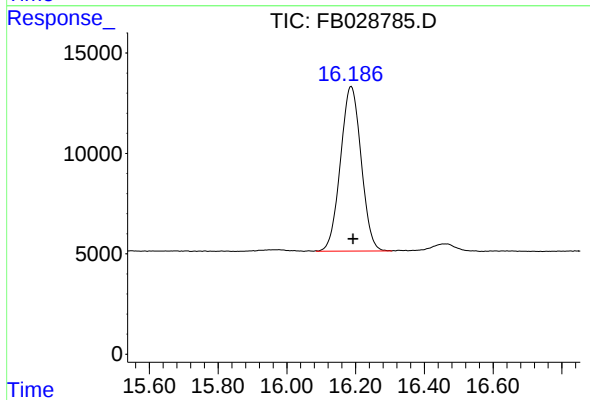

#10 1,2,4-Trimethylbenzene

R.T.: 16.187 min
Delta R.T.: -0.005 min
Response: 342182
Conc: 17.68 ng/ml