

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102822\
 Data File : FB028788.D
 Signal(s) : FID2B.CH
 Acq On : 28 Oct 2022 22:37
 Operator : AJ/MA
 Sample : BSF1028S2
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1028S2

Integration File: Calibration.e
 Quant Time: Oct 29 08:16:36 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100522.M
 Quant Title :
 QLast Update : Wed Oct 05 12:47:25 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.789	271223	20.965 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.708	495197	30.271 ng/ml
2) t 2,2,4-Trimethylpentane	7.420	539839	29.871 ng/ml
3) t n-Heptane	7.749	180302	10.645 ng/ml
4) t Benzene	7.884	211600	9.634 ng/ml
6) t Toluene	10.617	606817	28.951 ng/ml
7) t Ethylbenzene	13.053	189048	9.526 ng/ml
8) t m-Xylene	13.186	377440	19.159 ng/ml
9) t O-Xylene	13.912	365893	18.807 ng/ml
10) t 1,2,4-Trimethylbenzene	16.187	368359	19.028 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102822\
Data File : FB028788.D
Signal(s) : FID2B.CH
Acq On : 28 Oct 2022 22:37
Operator : AJ/MA
Sample : BSF1028S2
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1028S2

Integration File: Calibration.e
Quant Time: Oct 29 08:16:36 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100522.M
Quant Title :
QLast Update : Wed Oct 05 12:47:25 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

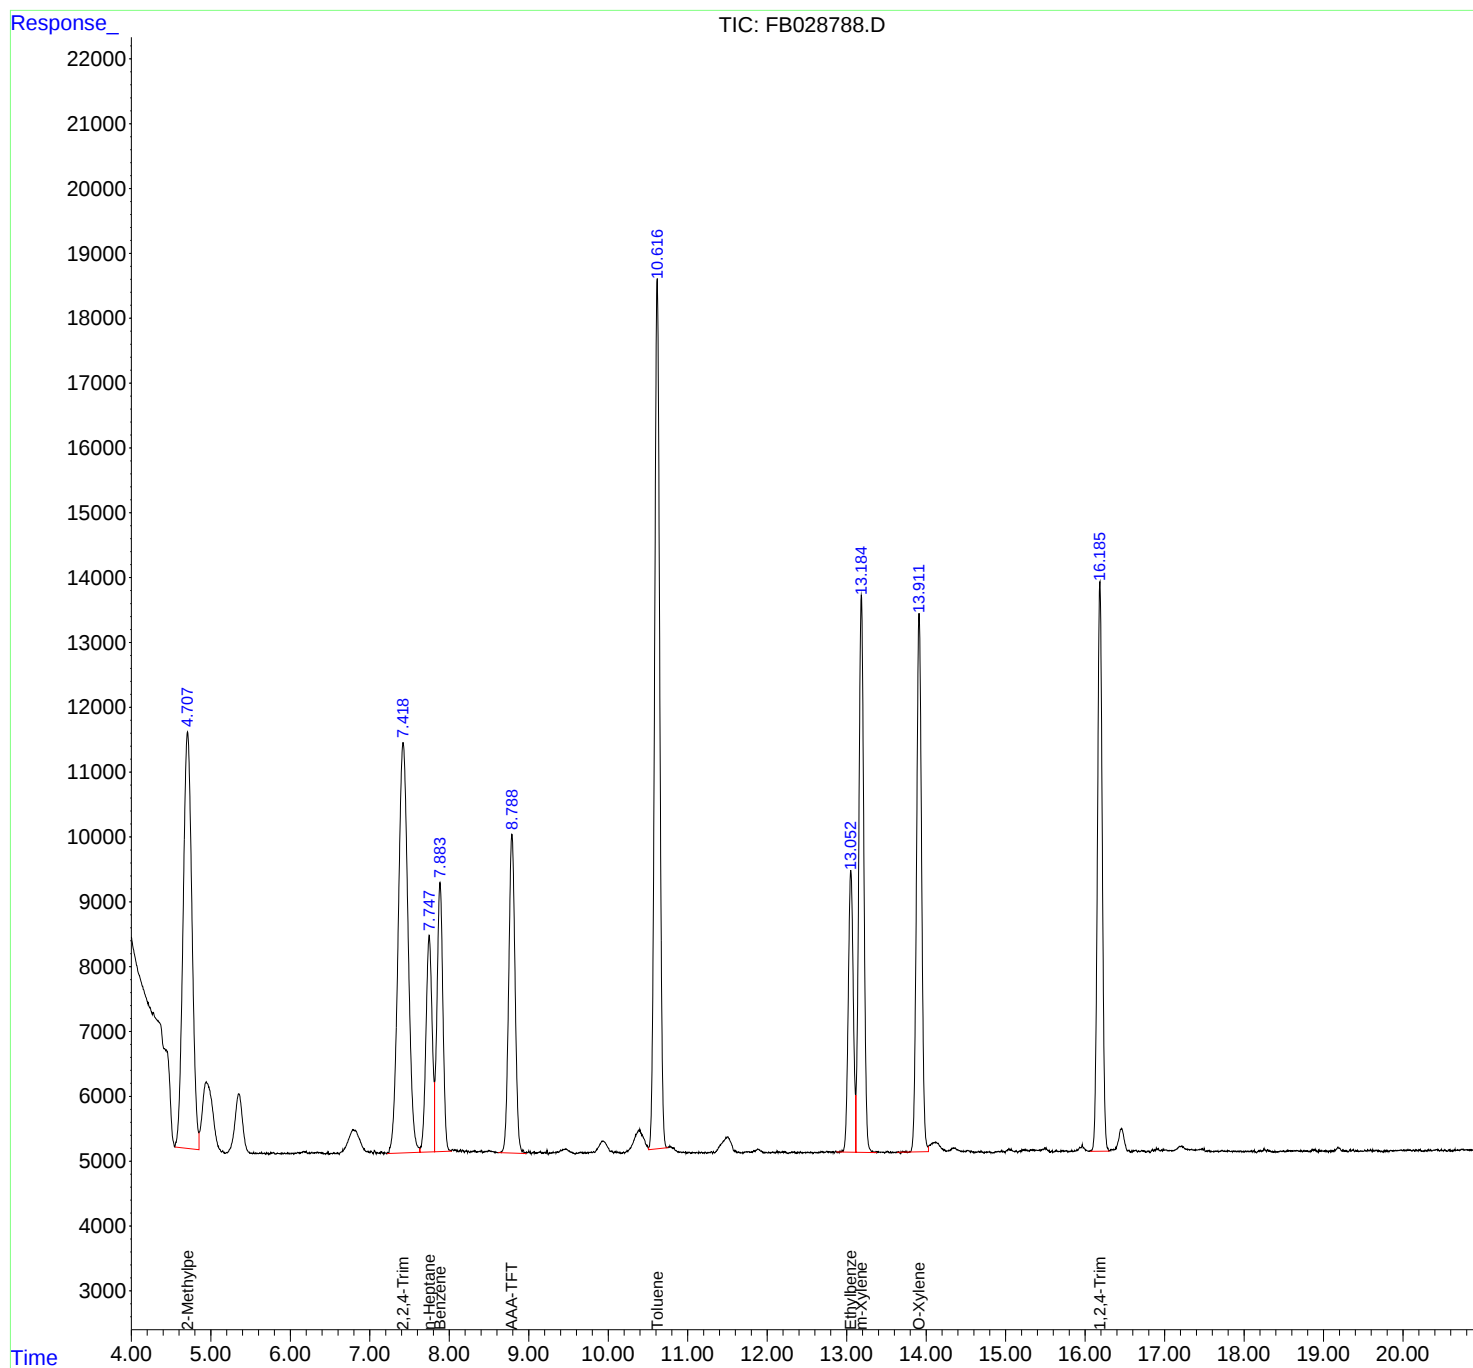


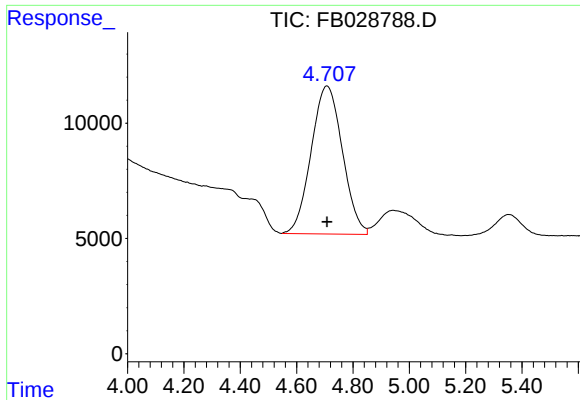

#1 2-Methylpentane


R.T.: 4.708 min
Delta R.T.: 0.000 min
Response: 495197
Conc: 30.27 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1028S2

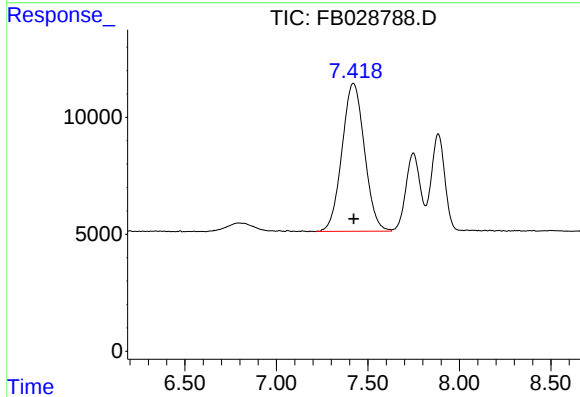


#2 2,2,4-Trimethylpentane

R.T.: 7.420 min
Delta R.T.: -0.004 min
Response: 539839
Conc: 29.87 ng/ml

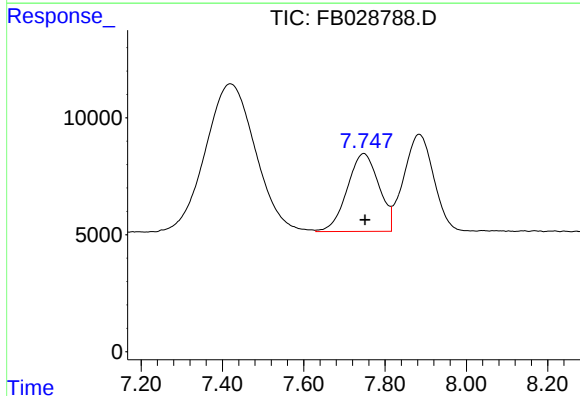


#3 n-Heptane

R.T.: 7.749 min
Delta R.T.: -0.003 min
Response: 180302
Conc: 10.64 ng/ml

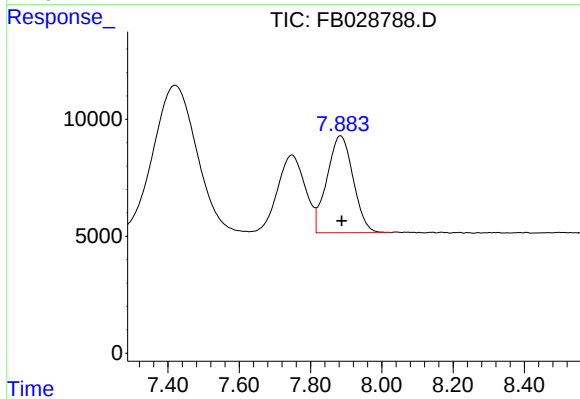

#4 Benzene


R.T.: 7.884 min
Delta R.T.: -0.003 min
Response: 211600
Conc: 9.63 ng/ml

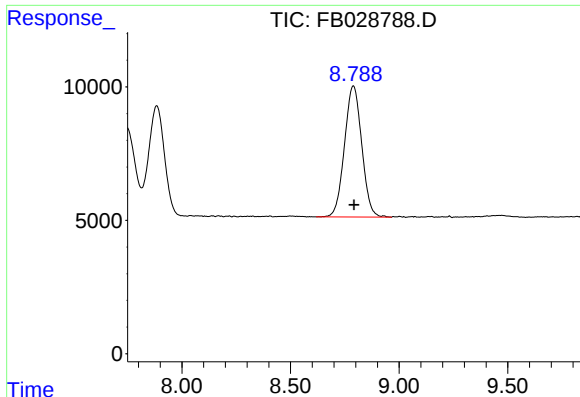

#5 AAA-TFT


R.T.: 8.789 min
Delta R.T.: -0.003 min
Response: 271223
Conc: 20.96 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1028S2

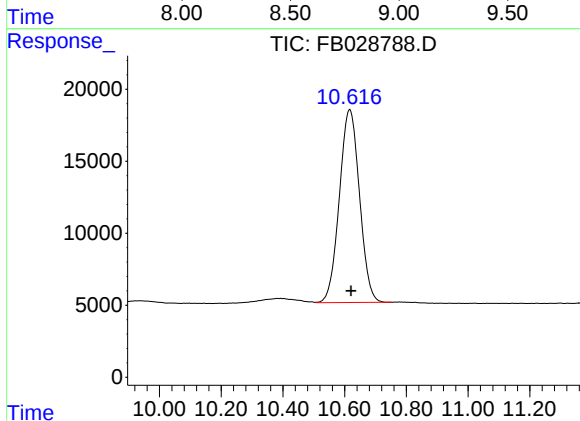


#6 Toluene

R.T.: 10.617 min
Delta R.T.: -0.004 min
Response: 606817
Conc: 28.95 ng/ml

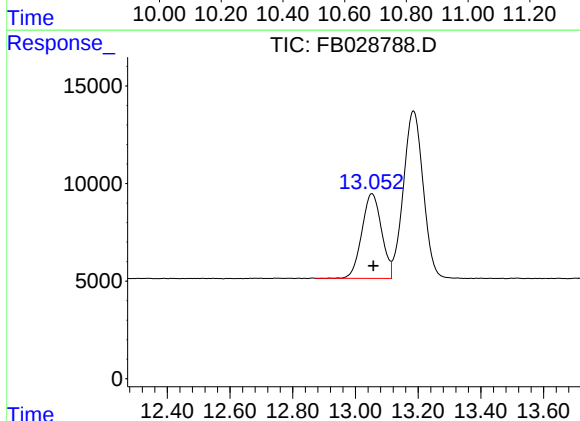


#7 Ethylbenzene

R.T.: 13.053 min
Delta R.T.: -0.005 min
Response: 189048
Conc: 9.53 ng/ml

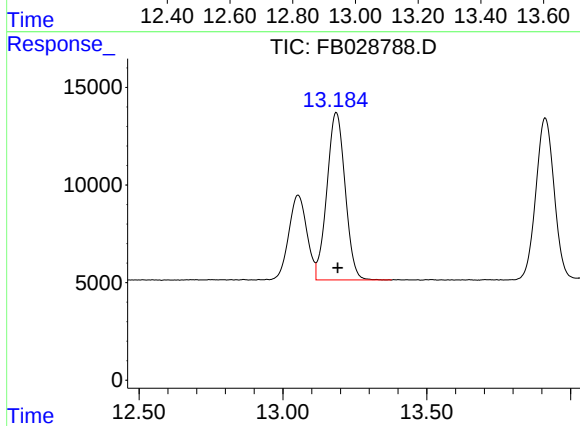

#8 m-Xylene


R.T.: 13.186 min
Delta R.T.: -0.005 min
Response: 377440
Conc: 19.16 ng/ml

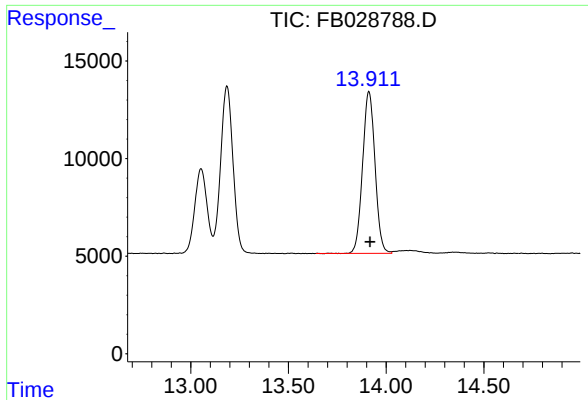

#9 O-Xylene

R.T.: 13.912 min
Delta R.T.: -0.005 min
Response: 365893
Conc: 18.81 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1028S2

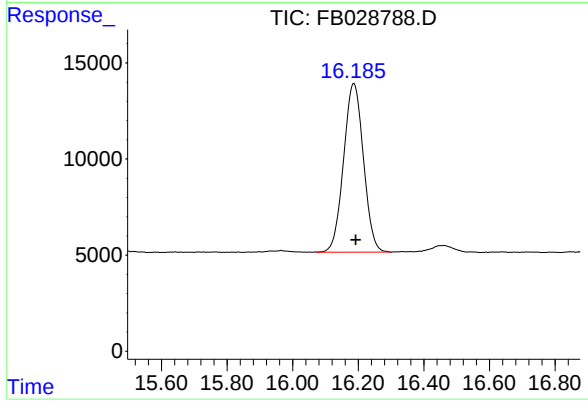

#10 1,2,4-Trimethylbenzene

R.T.: 16.187 min
Delta R.T.: -0.006 min
Response: 368359
Conc: 19.03 ng/ml