

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102824\
 Data File : FB031053.D
 Signal(s) : FID2B.CH
 Acq On : 28 Oct 2024 13:03
 Operator : YP/AJ
 Sample : FB102824GROICV
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 FB102824GROICV

Integration File: Calibration.e
 Quant Time: Oct 28 12:58:55 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102824.M
 Quant Title :
 QLast Update : Mon Oct 28 12:19:57 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.790	494146	17.902 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.716	1095536	27.894 ng/ml
2) t 2,2,4-Trimethylpentane	7.420	1345192	28.721 ng/ml
3) t n-Heptane	7.751	390234	8.611 ng/ml
4) t Benzene	7.890	507486	9.494 ng/ml
6) t Toluene	10.618	1398321	28.002 ng/ml
7) t Ethylbenzene	13.055	416703	9.309 ng/ml
8) t m-Xylene	13.188	904318	18.593 ng/ml
9) t O-Xylene	13.917	888512	19.492 ng/ml
10) t 1,2,4-Trimethylbenzene	16.193	675451	18.153 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102824\
Data File : FB031053.D
Signal(s) : FID2B.CH
Acq On : 28 Oct 2024 13:03
Operator : YP/AJ
Sample : FB102824GROICV
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
FB102824GROICV

Integration File: Calibration.e
Quant Time: Oct 28 12:58:55 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102824.M
Quant Title :
QLast Update : Mon Oct 28 12:19:57 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

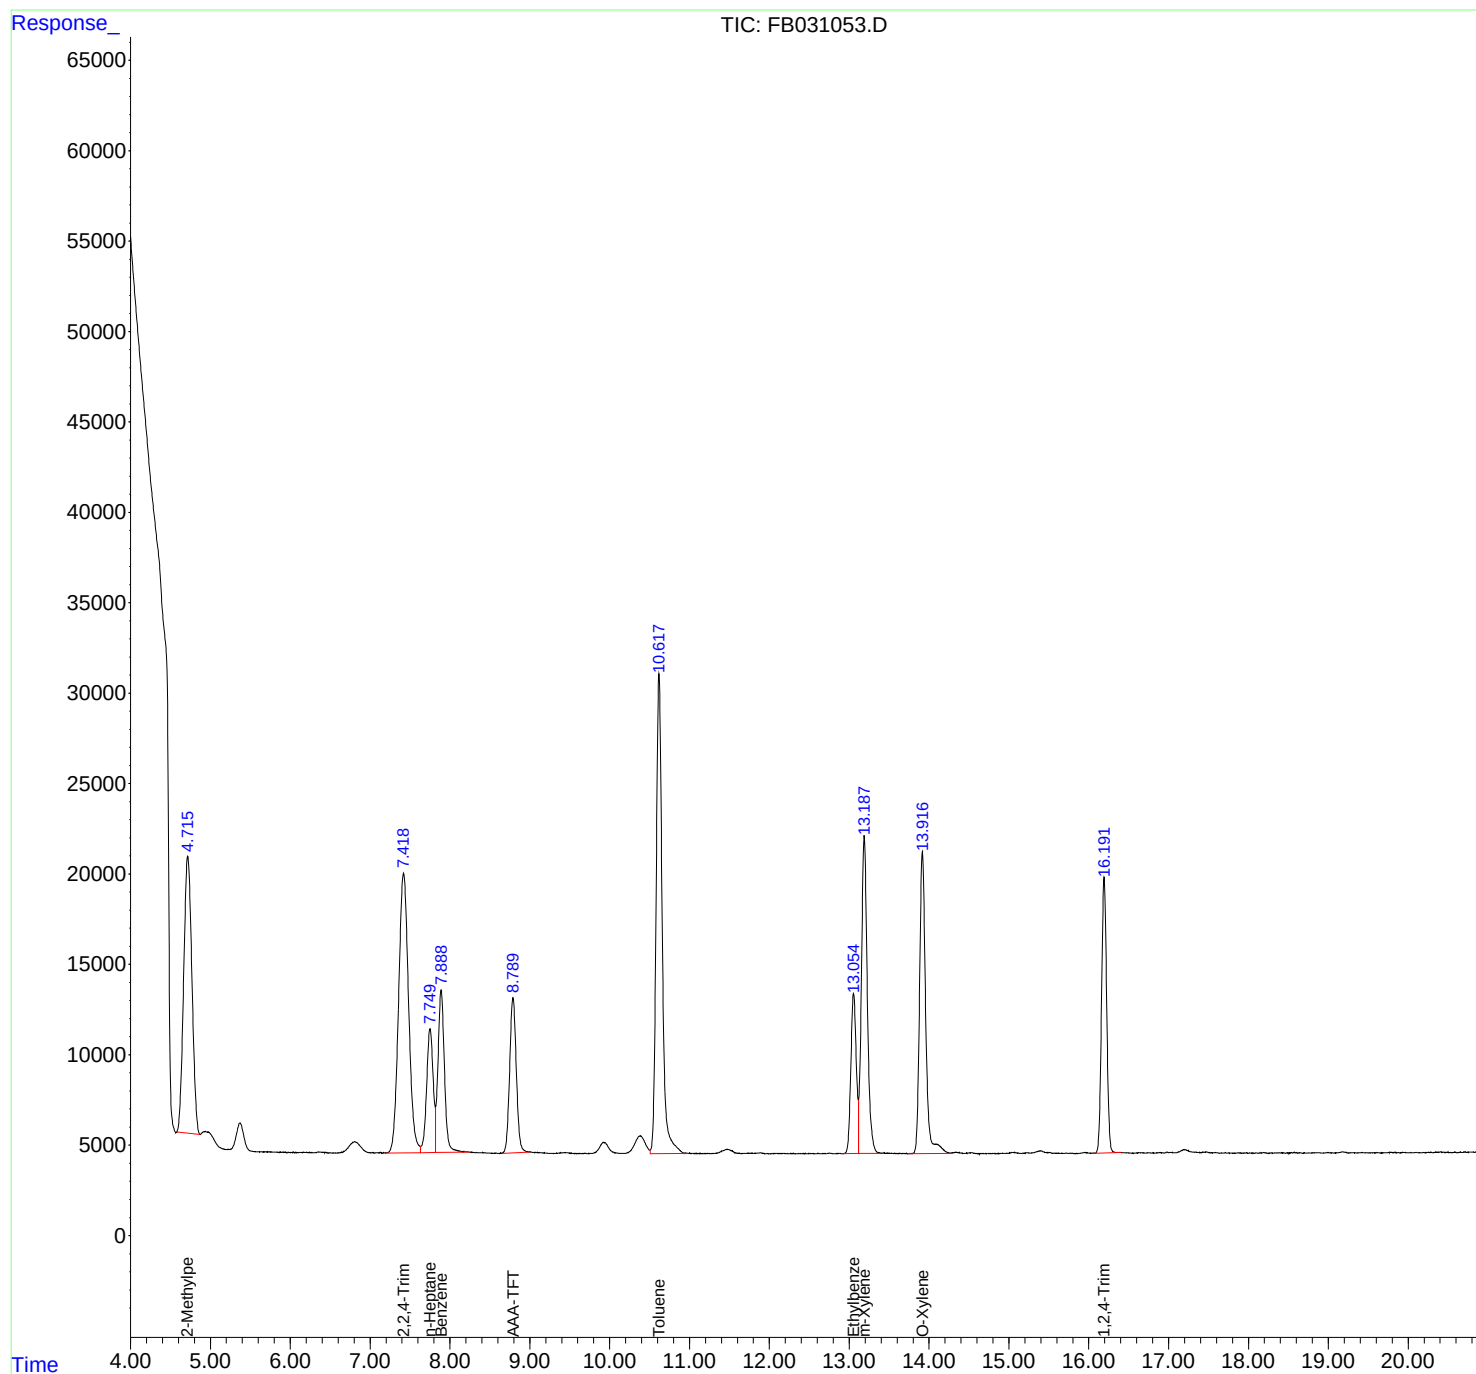


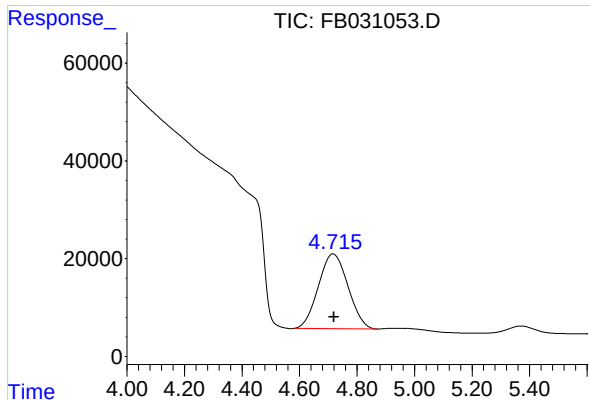

#1 2-Methylpentane


R.T.: 4.716 min
Delta R.T.: -0.004 min
Response: 1095536
Conc: 27.89 ng/ml

Instrument :
FID_B
ClientSampleId :
FB102824GROICV

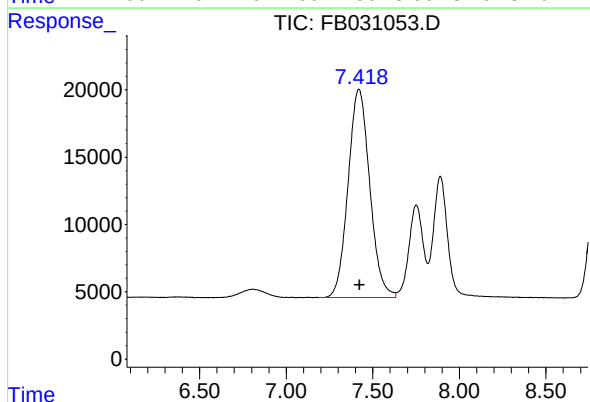


#2 2,2,4-Trimethylpentane

R.T.: 7.420 min
Delta R.T.: -0.005 min
Response: 1345192
Conc: 28.72 ng/ml

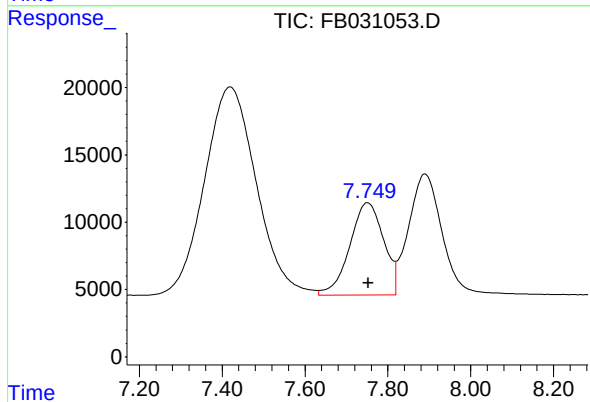


#3 n-Heptane

R.T.: 7.751 min
Delta R.T.: -0.002 min
Response: 390234
Conc: 8.61 ng/ml

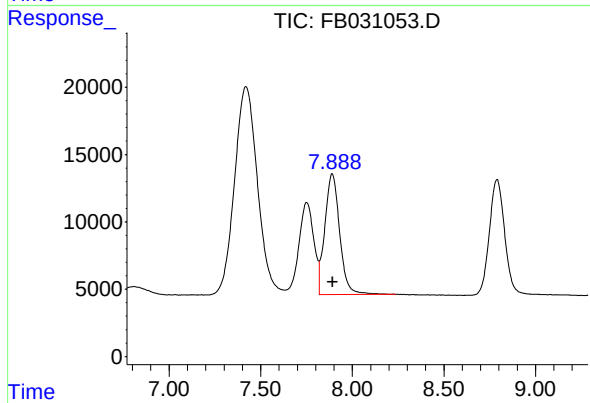

#4 Benzene


R.T.: 7.890 min
Delta R.T.: -0.002 min
Response: 507486
Conc: 9.49 ng/ml

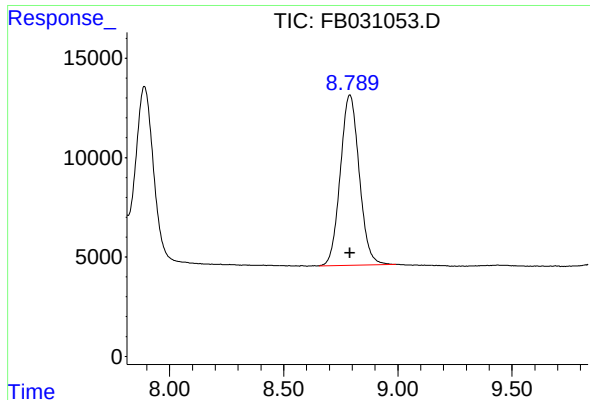

#5 AAA-TFT


R.T.: 8.790 min
Delta R.T.: 0.000 min
Response: 494146
Conc: 17.90 ng/ml

Instrument :
FID_B
ClientSampleId :
FB102824GROICV

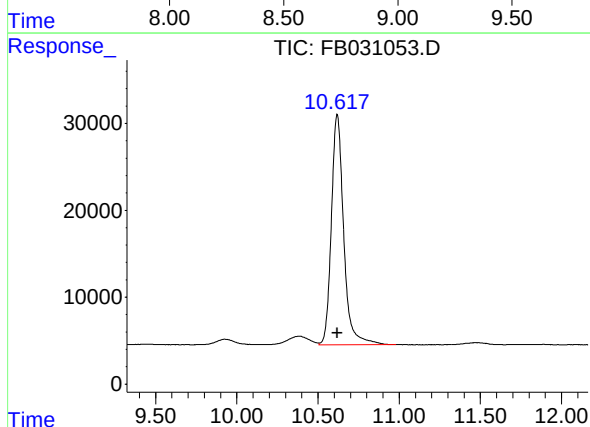


#6 Toluene

R.T.: 10.618 min
Delta R.T.: 0.000 min
Response: 1398321
Conc: 28.00 ng/ml

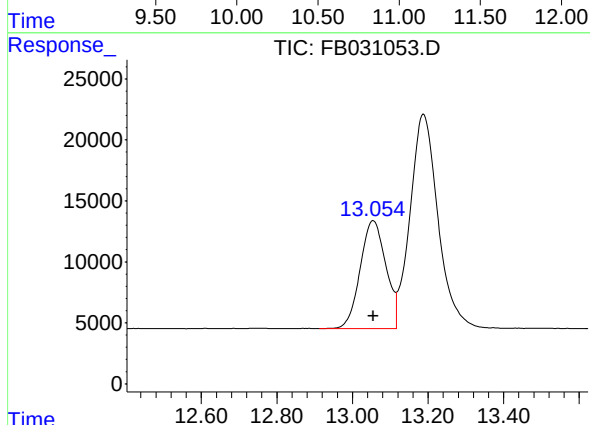


#7 Ethylbenzene

R.T.: 13.055 min
Delta R.T.: 0.000 min
Response: 416703
Conc: 9.31 ng/ml

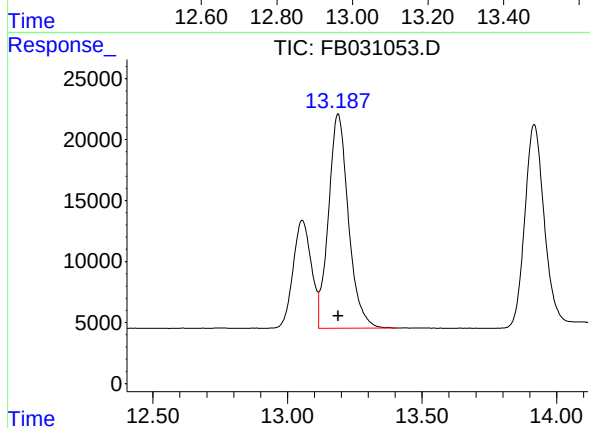

#8 m-Xylene


R.T.: 13.188 min
Delta R.T.: 0.000 min
Response: 904318
Conc: 18.59 ng/ml

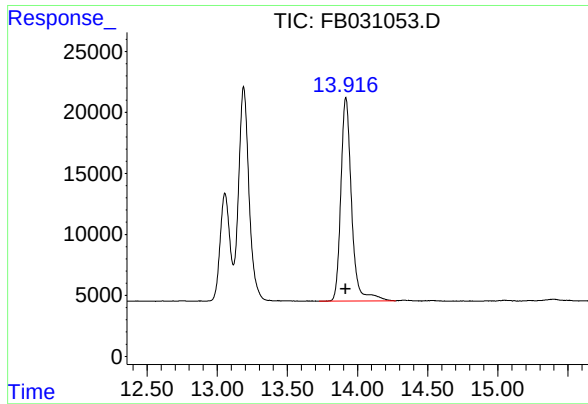

#9 O-Xylene

R.T.: 13.917 min
Delta R.T.: 0.000 min
Response: 888512
Conc: 19.49 ng/ml

Instrument :
FID_B
ClientSampleId :
FB102824GROICV

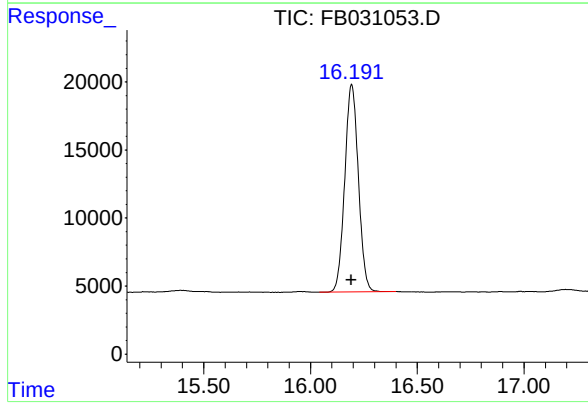

#10 1,2,4-Trimethylbenzene

R.T.: 16.193 min
Delta R.T.: 0.000 min
Response: 675451
Conc: 18.15 ng/ml