

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102918\
 Data File : FB018375.D
 Signal(s) : FID2B.CH
 Acq On : 29 Oct 2018 13:35
 Operator : MJ/SJ
 Sample : J5194-07MS
 Misc : 5.00g/5.00mL DI Water
 ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Oct 29 15:29:31 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101218.M
 Quant Title :
 QLast Update : Fri Oct 12 08:04:31 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.109	195801	22.734 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.962	437688	28.618 ng/ml
2) t 2,2,4-Trimethylpentane	7.726	407559	27.581 ng/ml
3) t n-Heptane	8.065	121898	8.602 ng/ml
4) t Benzene	8.205	200403	10.758 ng/ml
6) t Toluene	10.959	492334	32.304 ng/ml
7) t Ethylbenzene	13.409	163994	10.336 ng/ml
8) t m-Xylene	13.541	343011	20.615 ng/ml
9) t O-Xylene	14.273	421228	23.625 ng/ml
10) t 1,2,4-Trimethylbenzene	16.557	406699	19.992 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102918\
Data File : FB018375.D
Signal(s) : FID2B.CH
Acq On : 29 Oct 2018 13:35
Operator : MJ/SJ
Sample : J5194-07MS
Misc : 5.00g/5.00mL DI Water
ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 29 15:29:31 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101218.M
Quant Title :
QLast Update : Fri Oct 12 08:04:31 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

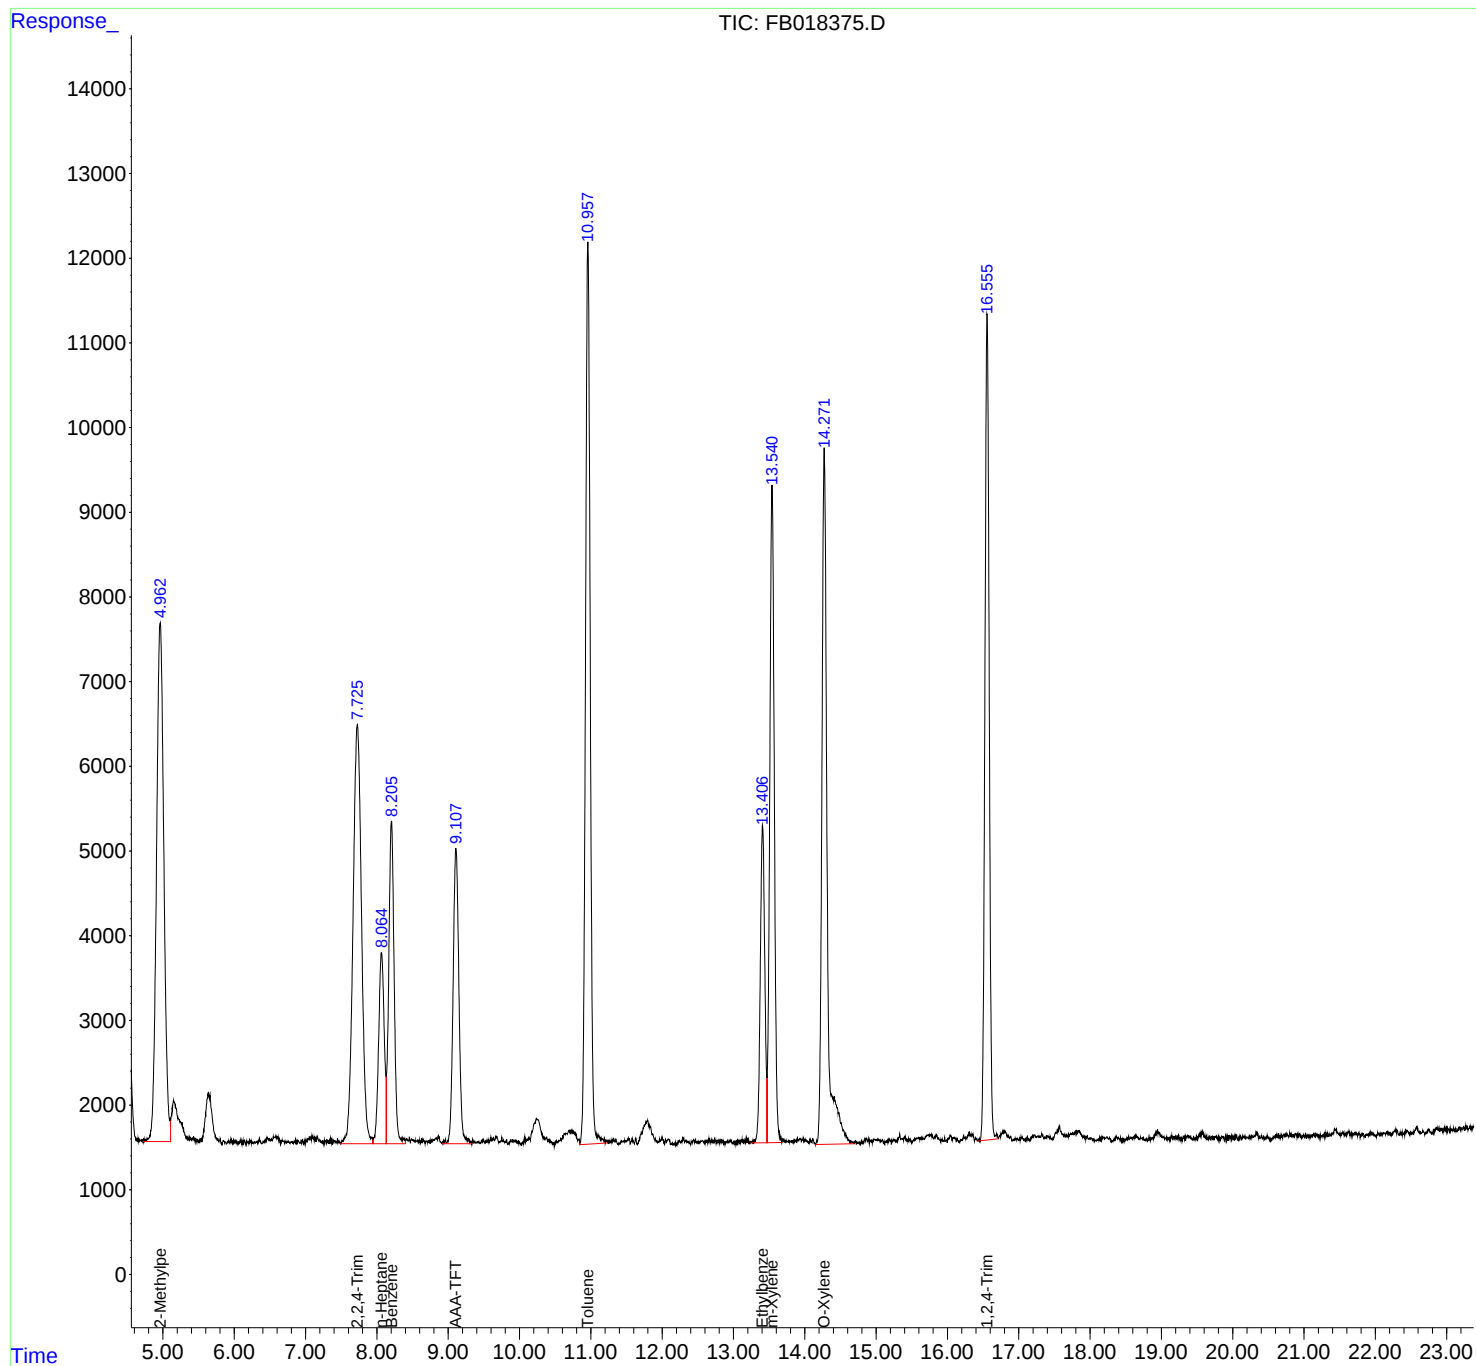

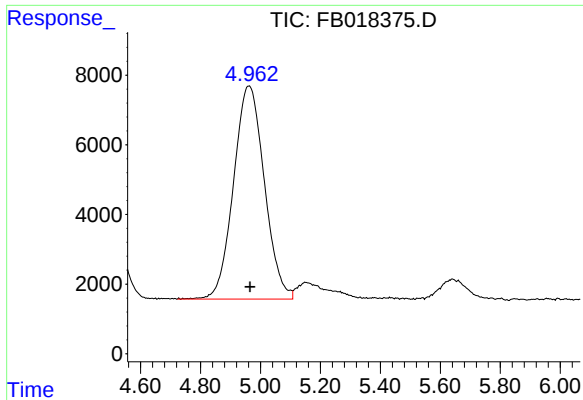


#1 2-Methylpentane

R.T.: 4.962 min
Delta R.T.: -0.003 min
Response: 437688
Conc: 28.62 ng/ml

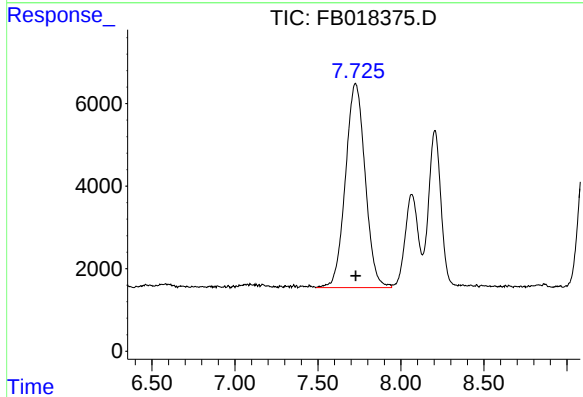


#2 2,2,4-Trimethylpentane

R.T.: 7.726 min
Delta R.T.: -0.002 min
Response: 407559
Conc: 27.58 ng/ml

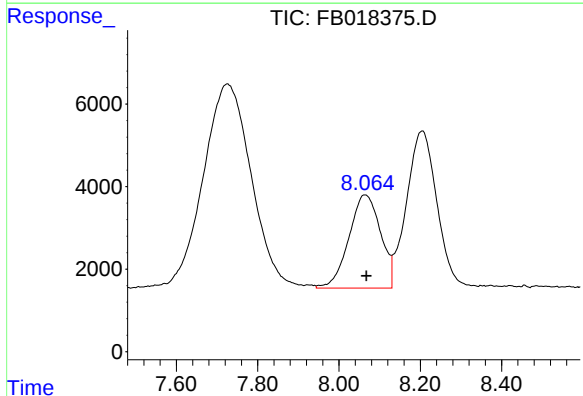


#3 n-Heptane

R.T.: 8.065 min
Delta R.T.: -0.003 min
Response: 121898
Conc: 8.60 ng/ml

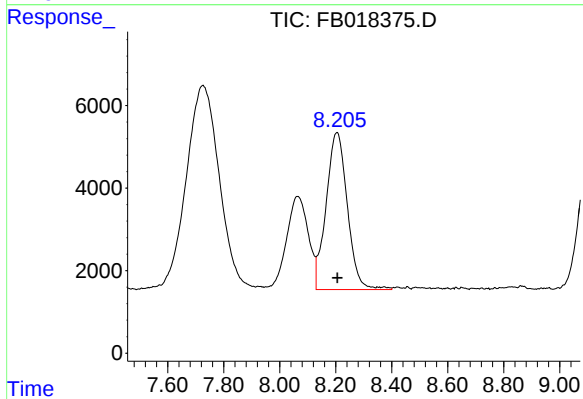


#4 Benzene

R.T.: 8.205 min
Delta R.T.: -0.002 min
Response: 200403
Conc: 10.76 ng/ml

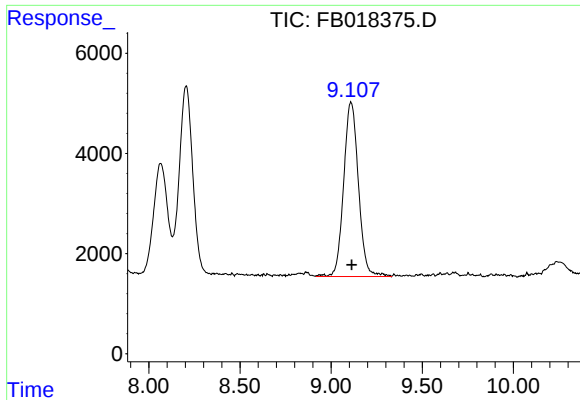


#5 AAA-TFT

R.T.: 9.109 min
Delta R.T.: -0.003 min
Response: 195801
Conc: 22.73 ng/ml

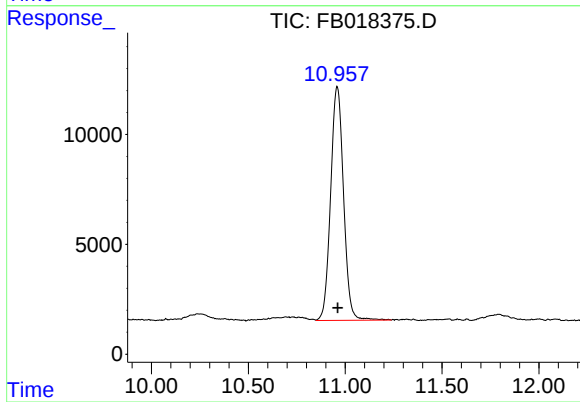


#6 Toluene

R.T.: 10.959 min
Delta R.T.: -0.003 min
Response: 492334
Conc: 32.30 ng/ml

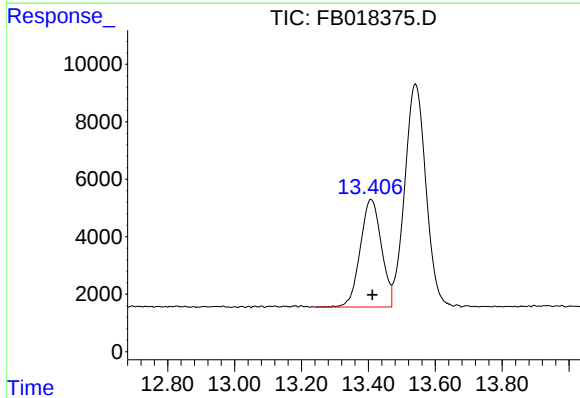


#7 Ethylbenzene

R.T.: 13.409 min
Delta R.T.: -0.004 min
Response: 163994
Conc: 10.34 ng/ml

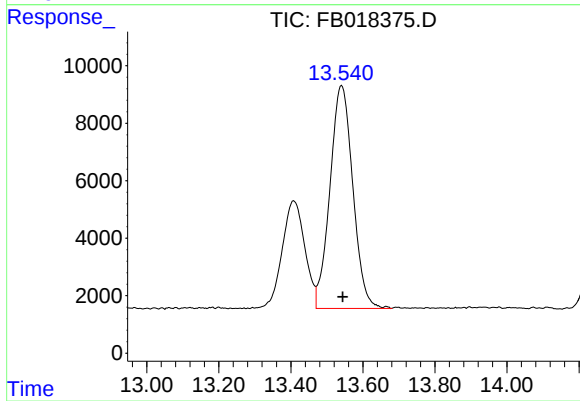


#8 m-Xylene

R.T.: 13.541 min
Delta R.T.: -0.003 min
Response: 343011
Conc: 20.61 ng/ml

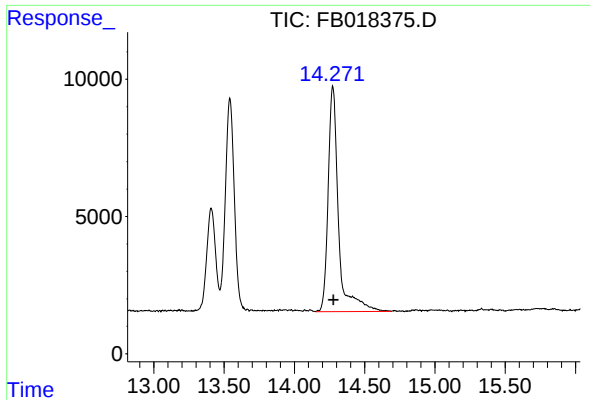

#9 O-Xylene

R.T.: 14.273 min
Delta R.T.: -0.003 min
Response: 421228
Conc: 23.63 ng/ml

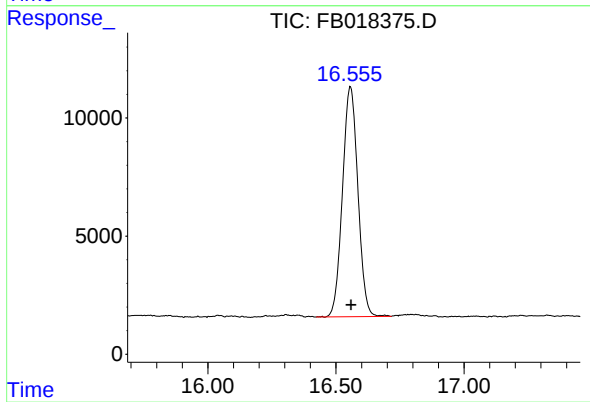

#10 1,2,4-Trimethylbenzene

R.T.: 16.557 min
Delta R.T.: -0.003 min
Response: 406699
Conc: 19.99 ng/ml