

Data Path : \\74.0.250.170\Terastorage\pestpcbsrv\HPCHEM1\FID_B\Data\FB102918\
 Data File : FB018376.D
 Signal(s) : FID2B.CH
 Acq On : 29 Oct 2018 14:05
 Operator : MJ/SJ
 Sample : J5194-07MSD
 Misc : 5.00g/5.00mL DI Water
 ALS Vial : 8 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Oct 29 15:29:34 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101218.M
 Quant Title :
 QLast Update : Fri Oct 12 08:04:31 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.111	188940	21.937 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.963	395032	25.829 ng/ml
2) t 2,2,4-Trimethylpentane	7.727	356123	24.100 ng/ml
3) t n-Heptane	8.066	107612	7.594 ng/ml
4) t Benzene	8.205	189993	10.199 ng/ml
6) t Toluene	10.959	468979	30.772 ng/ml
7) t Ethylbenzene	13.409	160510	10.117 ng/ml
8) t m-Xylene	13.541	337769	20.300 ng/ml
9) t O-Xylene	14.273	405674	22.753 ng/ml
10) t 1,2,4-Trimethylbenzene	16.556	386386	18.993 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : \\74.0.250.170\Terastorage\pestpcbsrv\HPCHEM1\FID_B\Data\FB102918\
Data File : FB018376.D
Signal(s) : FID2B.CH
Acq On : 29 Oct 2018 14:05
Operator : MJ/SJ
Sample : J5194-07MSD
Misc : 5.00g/5.00mL DI Water
ALS Vial : 8 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 29 15:29:34 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101218.M
Quant Title :
QLast Update : Fri Oct 12 08:04:31 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

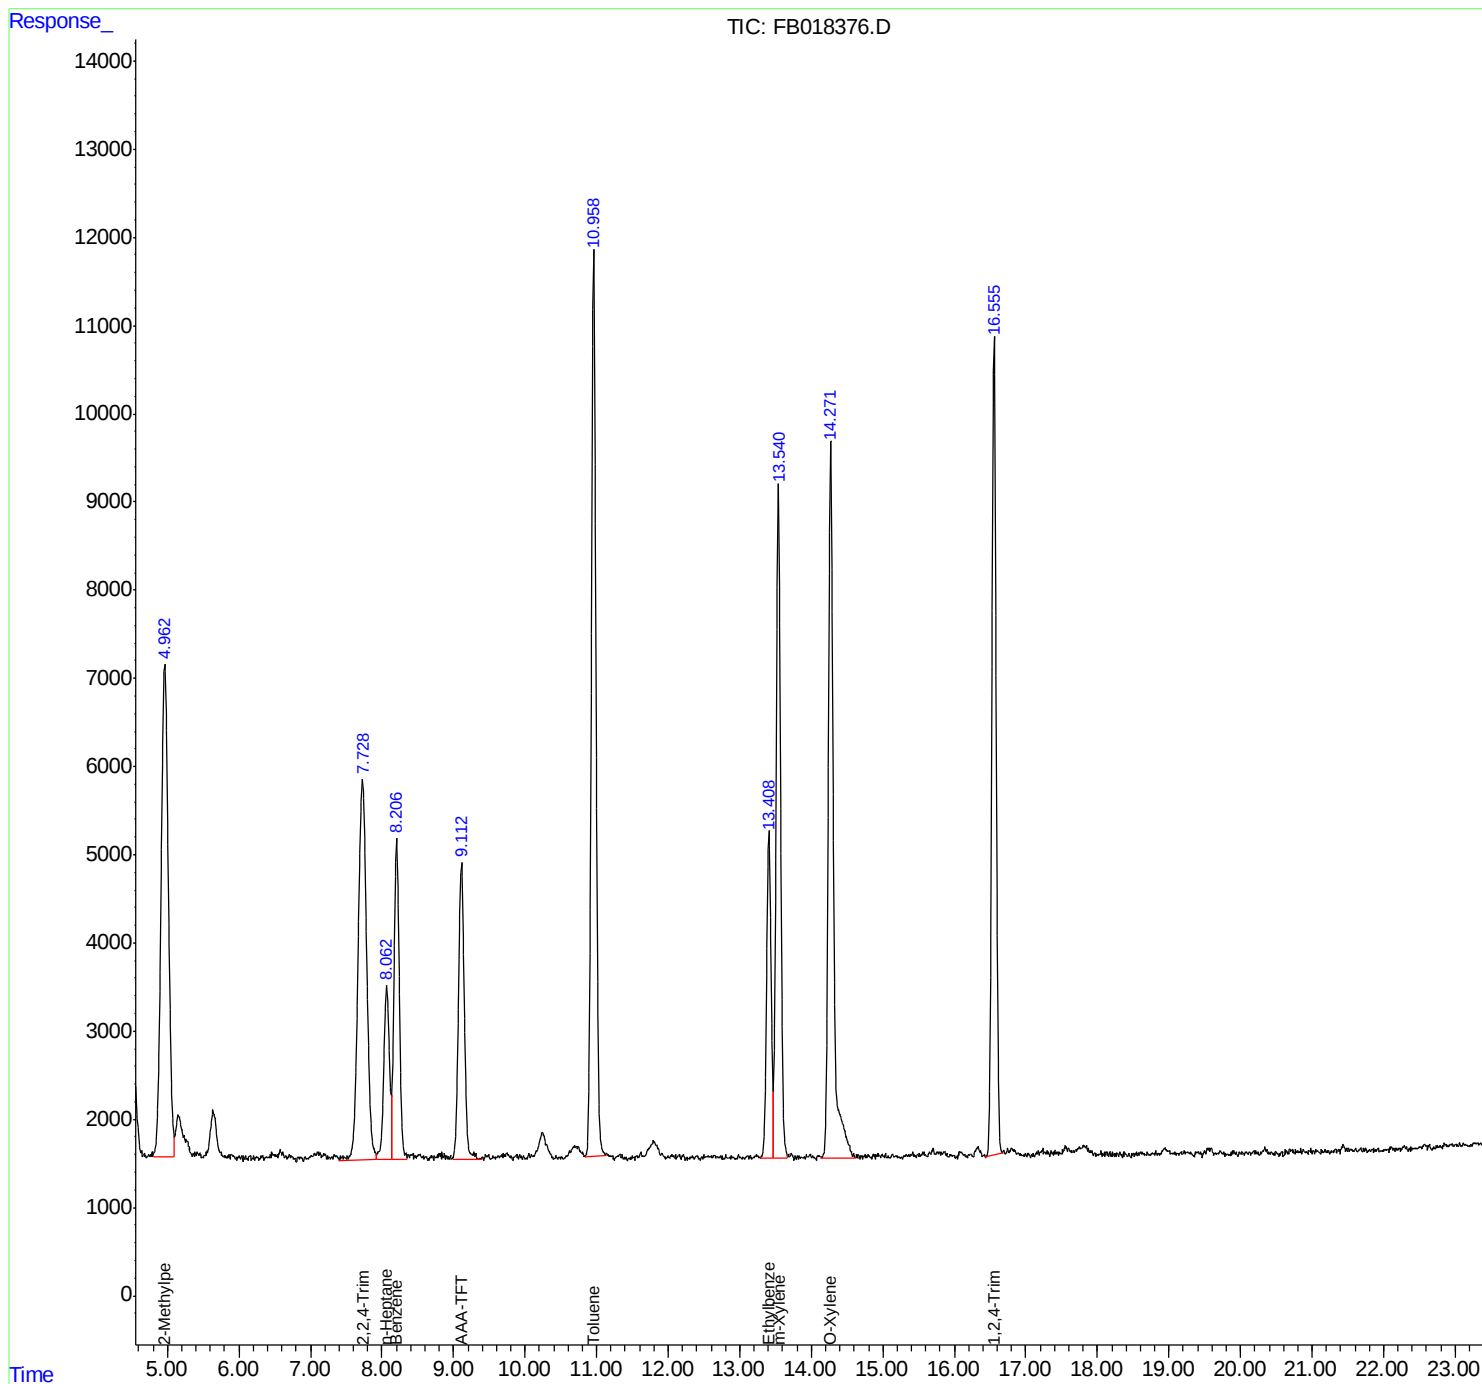

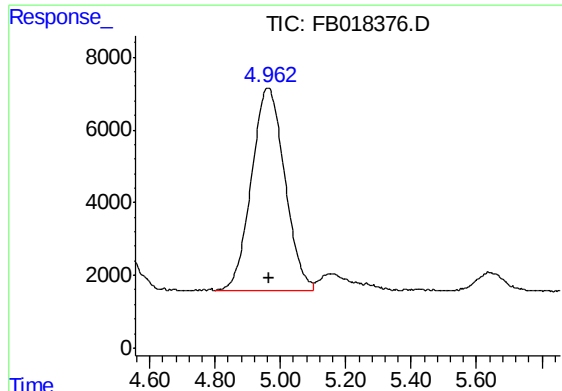


#1 2-Methylpentane

R.T.: 4.963 min
Delta R.T.: -0.002 min
Response: 395032
Conc: 25.83 ng/ml

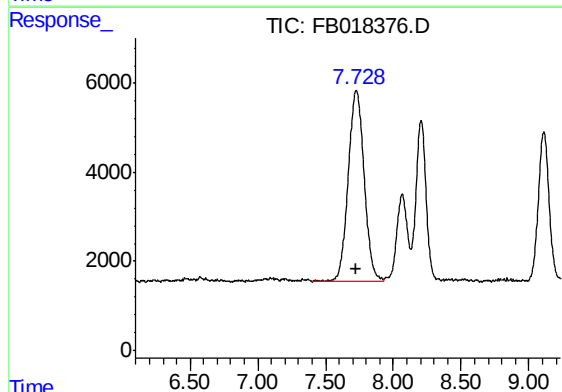


#2 2,2,4-Trimethylpentane

R.T.: 7.727 min
Delta R.T.: -0.002 min
Response: 356123
Conc: 24.10 ng/ml

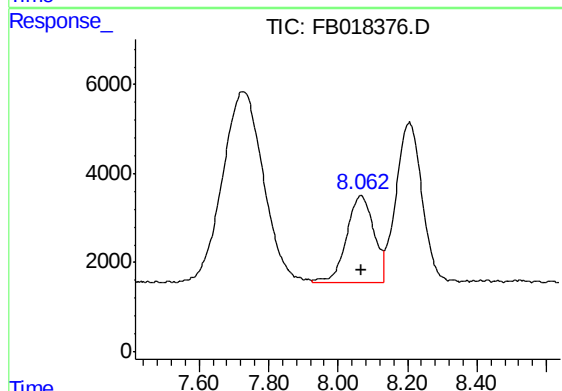


#3 n-Heptane

R.T.: 8.066 min
Delta R.T.: -0.001 min
Response: 107612
Conc: 7.59 ng/ml

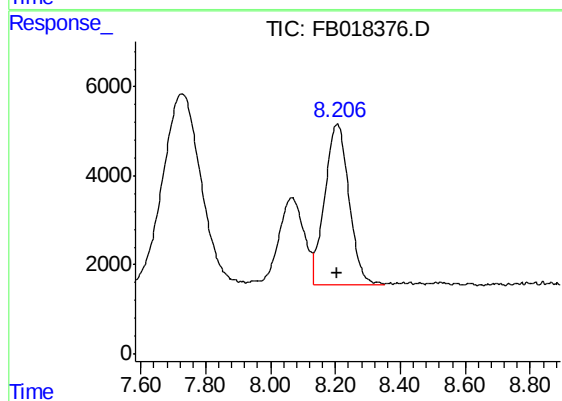


#4 Benzene

R.T.: 8.205 min
Delta R.T.: -0.001 min
Response: 189993
Conc: 10.20 ng/ml

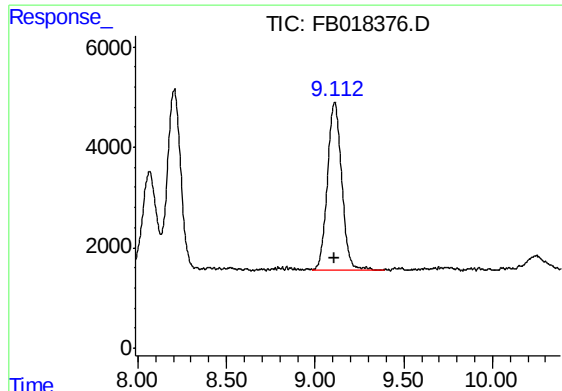


#5 AAA-TFT

R.T.: 9.111 min
Delta R.T.: -0.002 min
Response: 188940
Conc: 21.94 ng/ml

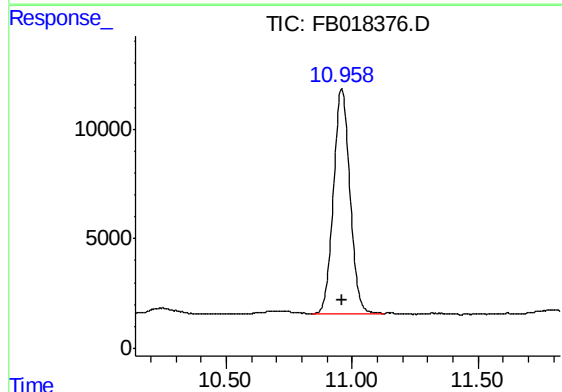


#6 Toluene

R.T.: 10.959 min
Delta R.T.: -0.003 min
Response: 468979
Conc: 30.77 ng/ml

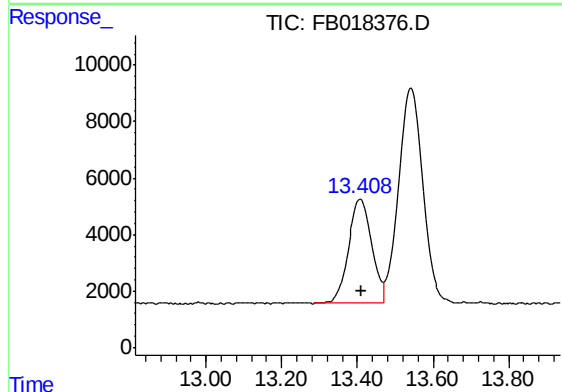


#7 Ethylbenzene

R.T.: 13.409 min
Delta R.T.: -0.003 min
Response: 160510
Conc: 10.12 ng/ml

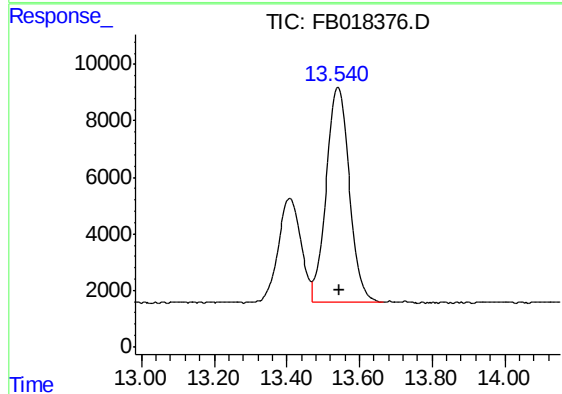


#8 m-Xylene

R.T.: 13.541 min
Delta R.T.: -0.003 min
Response: 337769
Conc: 20.30 ng/ml

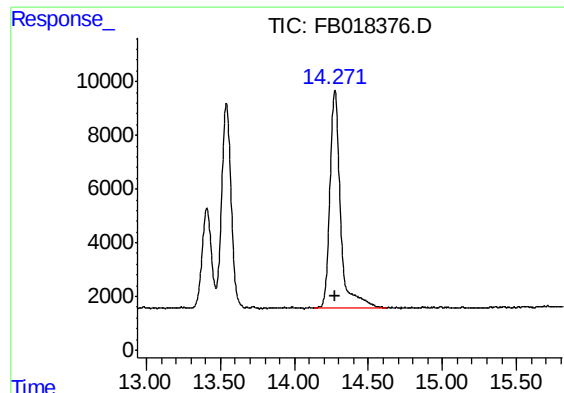

#9 O-Xylene

R.T.: 14.273 min
Delta R.T.: -0.003 min
Response: 405674
Conc: 22.75 ng/ml

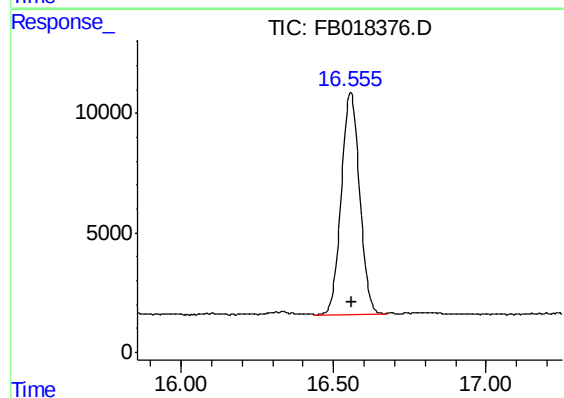

#10 1,2,4-Trimethylbenzene

R.T.: 16.556 min
Delta R.T.: -0.003 min
Response: 386386
Conc: 18.99 ng/ml