

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102919\
 Data File : FB022847.D
 Signal(s) : FID2B.CH
 Acq On : 29 Oct 2019 12:06
 Operator : DD/AJ
 Sample : K5149-08MS
 Misc : 5.05g/5.00ml DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Oct 29 15:42:47 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101619.M
 Quant Title :
 QLast Update : Wed Oct 16 15:04:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.797	506808	20.029 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.688	847765	24.946 ng/ml
2) t 2,2,4-Trimethylpentane	7.417	829590	22.799 ng/ml
3) t n-Heptane	7.756	274676	7.528 ng/ml
4) t Benzene	7.890	407617	9.232 ng/ml
6) t Toluene	10.628	1170886	27.166 ng/ml
7) t Ethylbenzene	13.068	353143	8.695 ng/ml
8) t m-Xylene	13.202	654029	16.998 ng/ml
9) t O-Xylene	13.929	629339	17.279 ng/ml
10) t 1,2,4-Trimethylbenzene	16.207	523834	18.383 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102919\
Data File : FB022847.D
Signal(s) : FID2B.CH
Acq On : 29 Oct 2019 12:06
Operator : DD/AJ
Sample : K5149-08MS
Misc : 5.05g/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 29 15:42:47 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101619.M
Quant Title :
QLast Update : Wed Oct 16 15:04:00 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

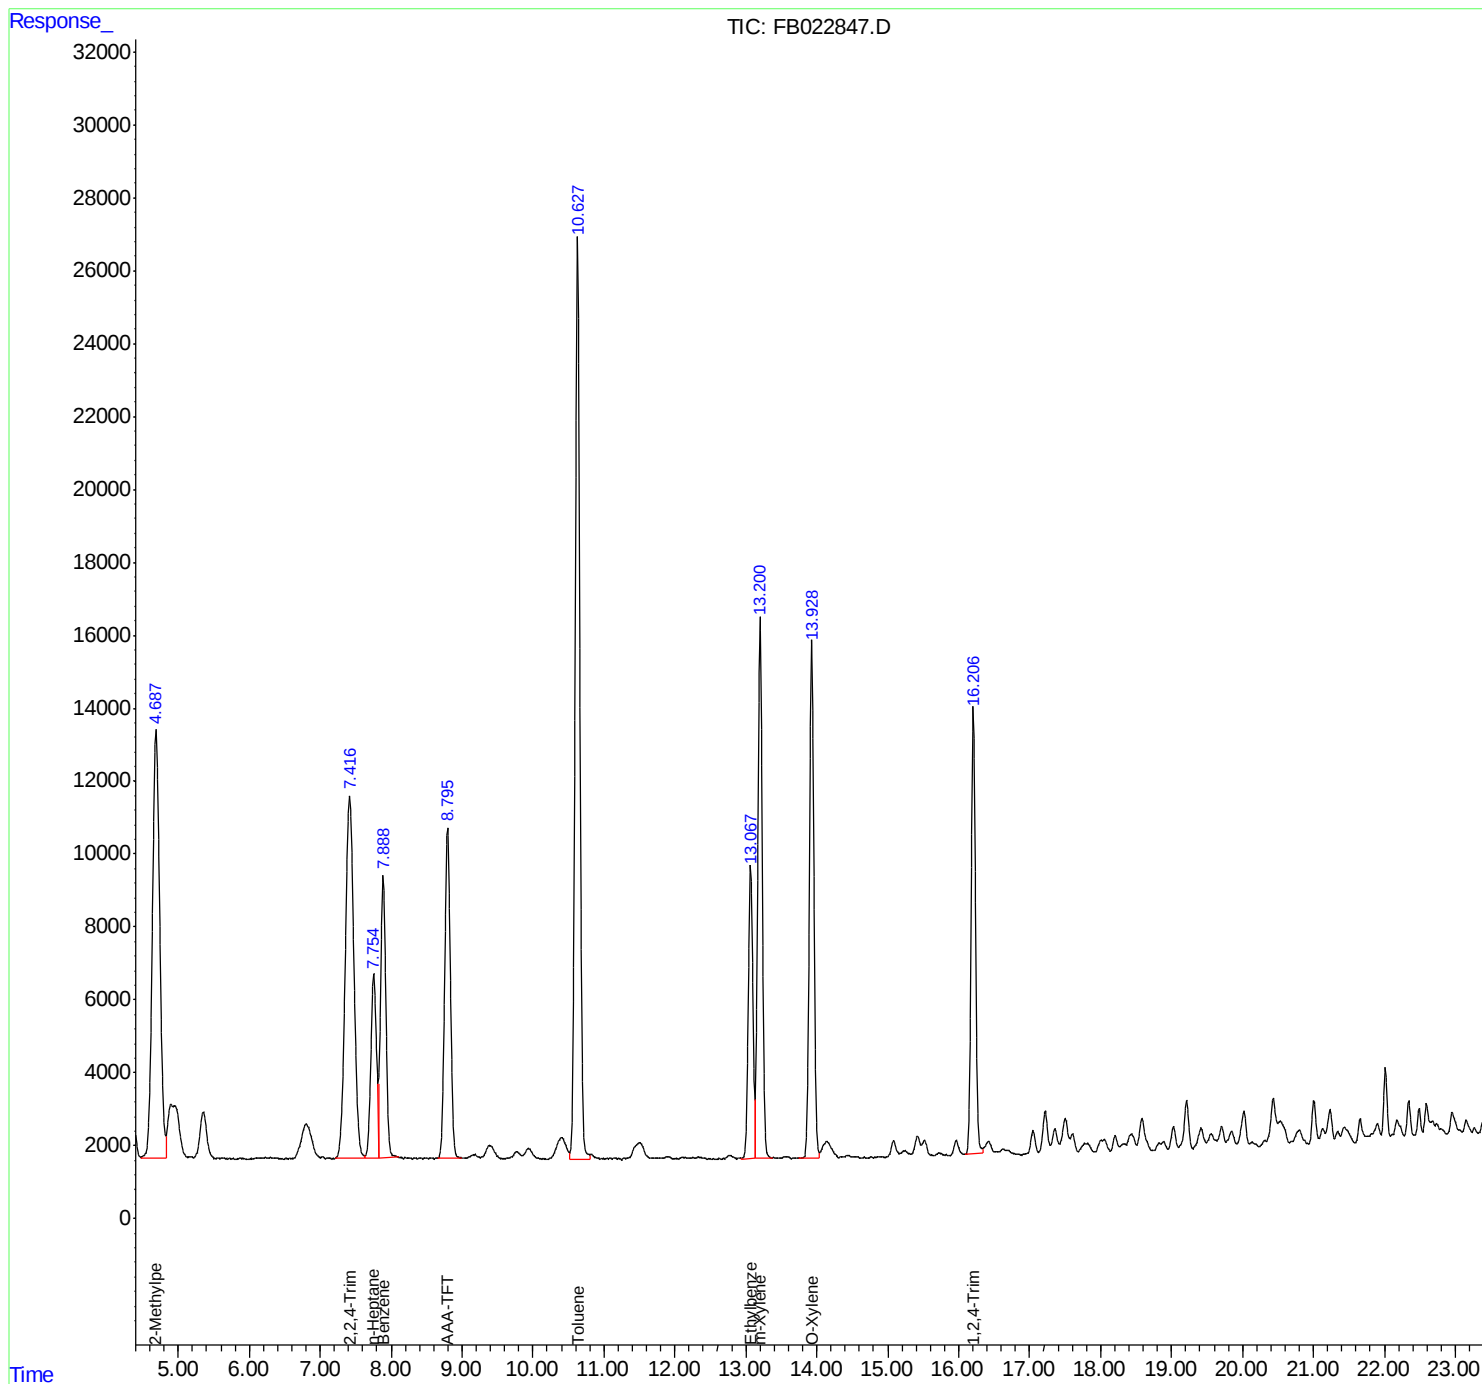

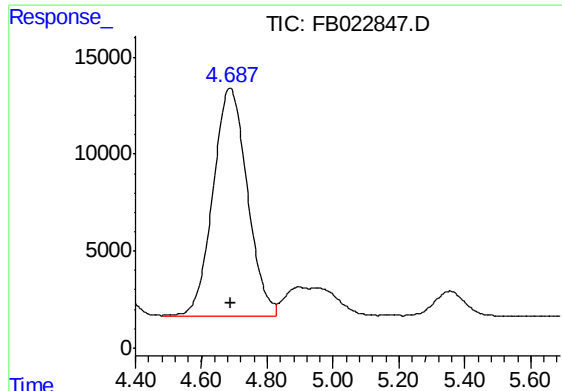


#1 2-Methylpentane

R.T.: 4.688 min
Delta R.T.: -0.002 min
Response: 847765
Conc: 24.95 ng/ml

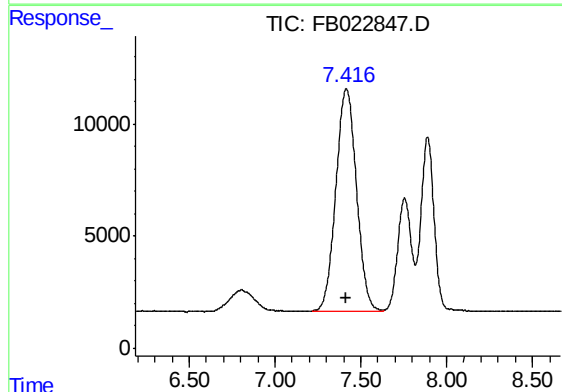


#2 2,2,4-Trimethylpentane

R.T.: 7.417 min
Delta R.T.: 0.000 min
Response: 829590
Conc: 22.80 ng/ml

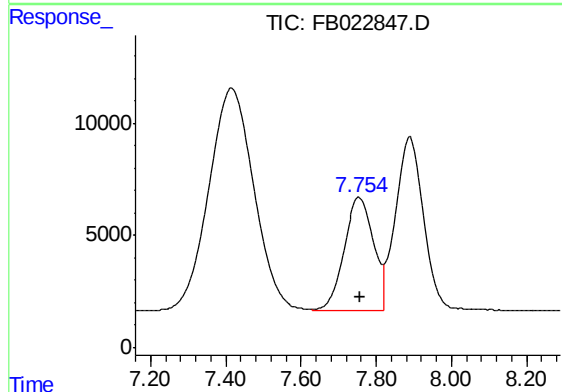


#3 n-Heptane

R.T.: 7.756 min
Delta R.T.: -0.001 min
Response: 274676
Conc: 7.53 ng/ml

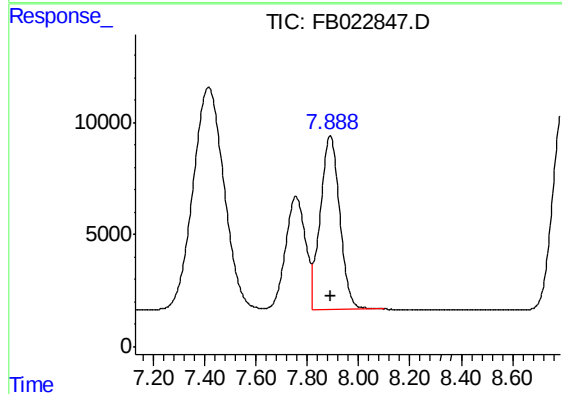


#4 Benzene

R.T.: 7.890 min
Delta R.T.: -0.002 min
Response: 407617
Conc: 9.23 ng/ml

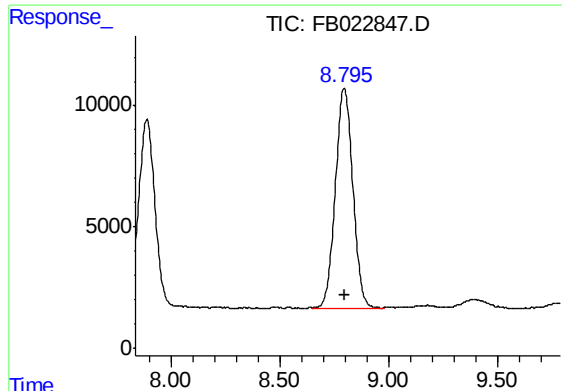


#5 AAA-TFT

R.T.: 8.797 min
Delta R.T.: -0.002 min
Response: 506808
Conc: 20.03 ng/ml

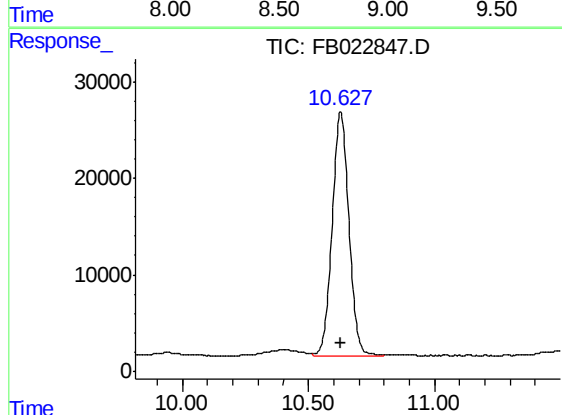


#6 Toluene

R.T.: 10.628 min
Delta R.T.: -0.001 min
Response: 1170886
Conc: 27.17 ng/ml

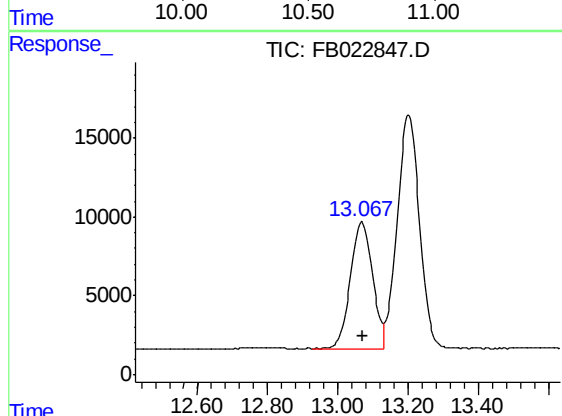


#7 Ethylbenzene

R.T.: 13.068 min
Delta R.T.: -0.001 min
Response: 353143
Conc: 8.69 ng/ml

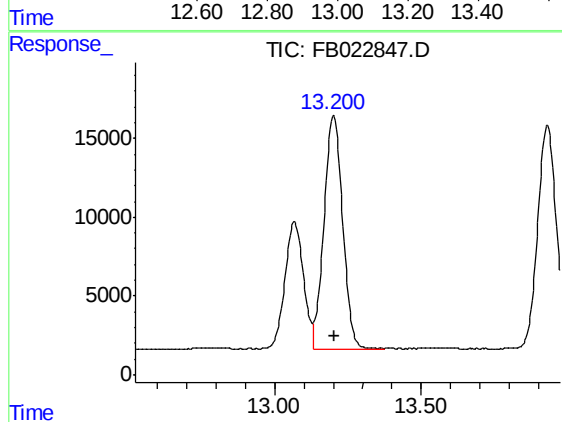


#8 m-Xylene

R.T.: 13.202 min
Delta R.T.: -0.001 min
Response: 654029
Conc: 17.00 ng/ml

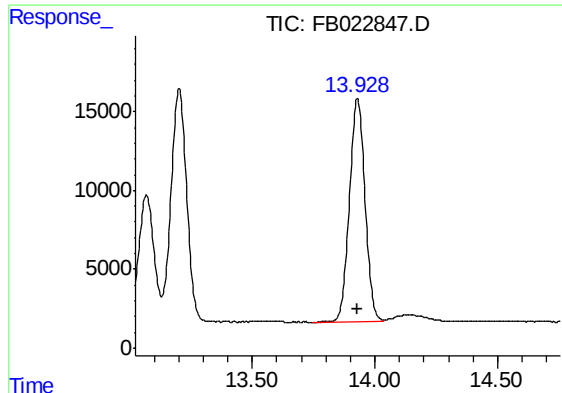

#9 O-Xylene

R.T.: 13.929 min
Delta R.T.: -0.001 min
Response: 629339
Conc: 17.28 ng/ml

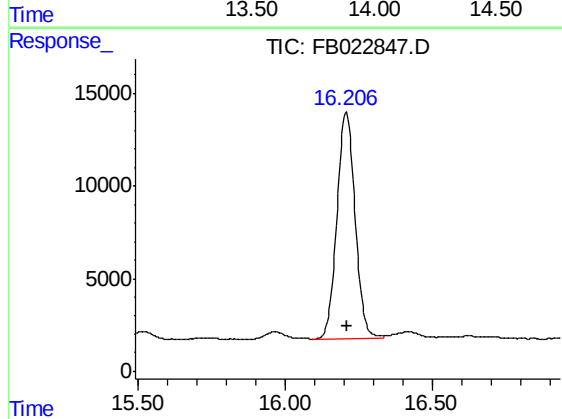

#10 1,2,4-Trimethylbenzene

R.T.: 16.207 min
Delta R.T.: -0.002 min
Response: 523834
Conc: 18.38 ng/ml