

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102921\
 Data File : FB026332.D
 Signal(s) : FID2B.CH
 Acq On : 29 Oct 2021 13:11
 Operator : AJ/MA
 Sample : BSF1029S1
 Misc : 5.02G\5.00 ML DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Oct 29 22:44:02 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102721.M
 Quant Title :
 QLast Update : Thu Oct 28 05:34:31 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.794	235433	19.873 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.708	515200	30.941 ng/ml
2) t 2,2,4-Trimethylpentane	7.443	601312	30.838 ng/ml
3) t n-Heptane	7.753	192843	10.452 ng/ml
4) t Benzene	7.888	223421	10.248 ng/ml
6) t Toluene	10.622	646736	31.182 ng/ml
7) t Ethylbenzene	13.059	200909	10.639 ng/ml
8) t m-Xylene	13.192	395811	20.810 ng/ml
9) t O-Xylene	13.919	380378	20.595 ng/ml
10) t 1,2,4-Trimethylbenzene	16.195	391906	20.672 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102921\
Data File : FB026332.D
Signal(s) : FID2B.CH
Acq On : 29 Oct 2021 13:11
Operator : AJ/MA
Sample : BSF1029S1
Misc : 5.02G\5.00 ML DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 29 22:44:02 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102721.M
Quant Title :
QLast Update : Thu Oct 28 05:34:31 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

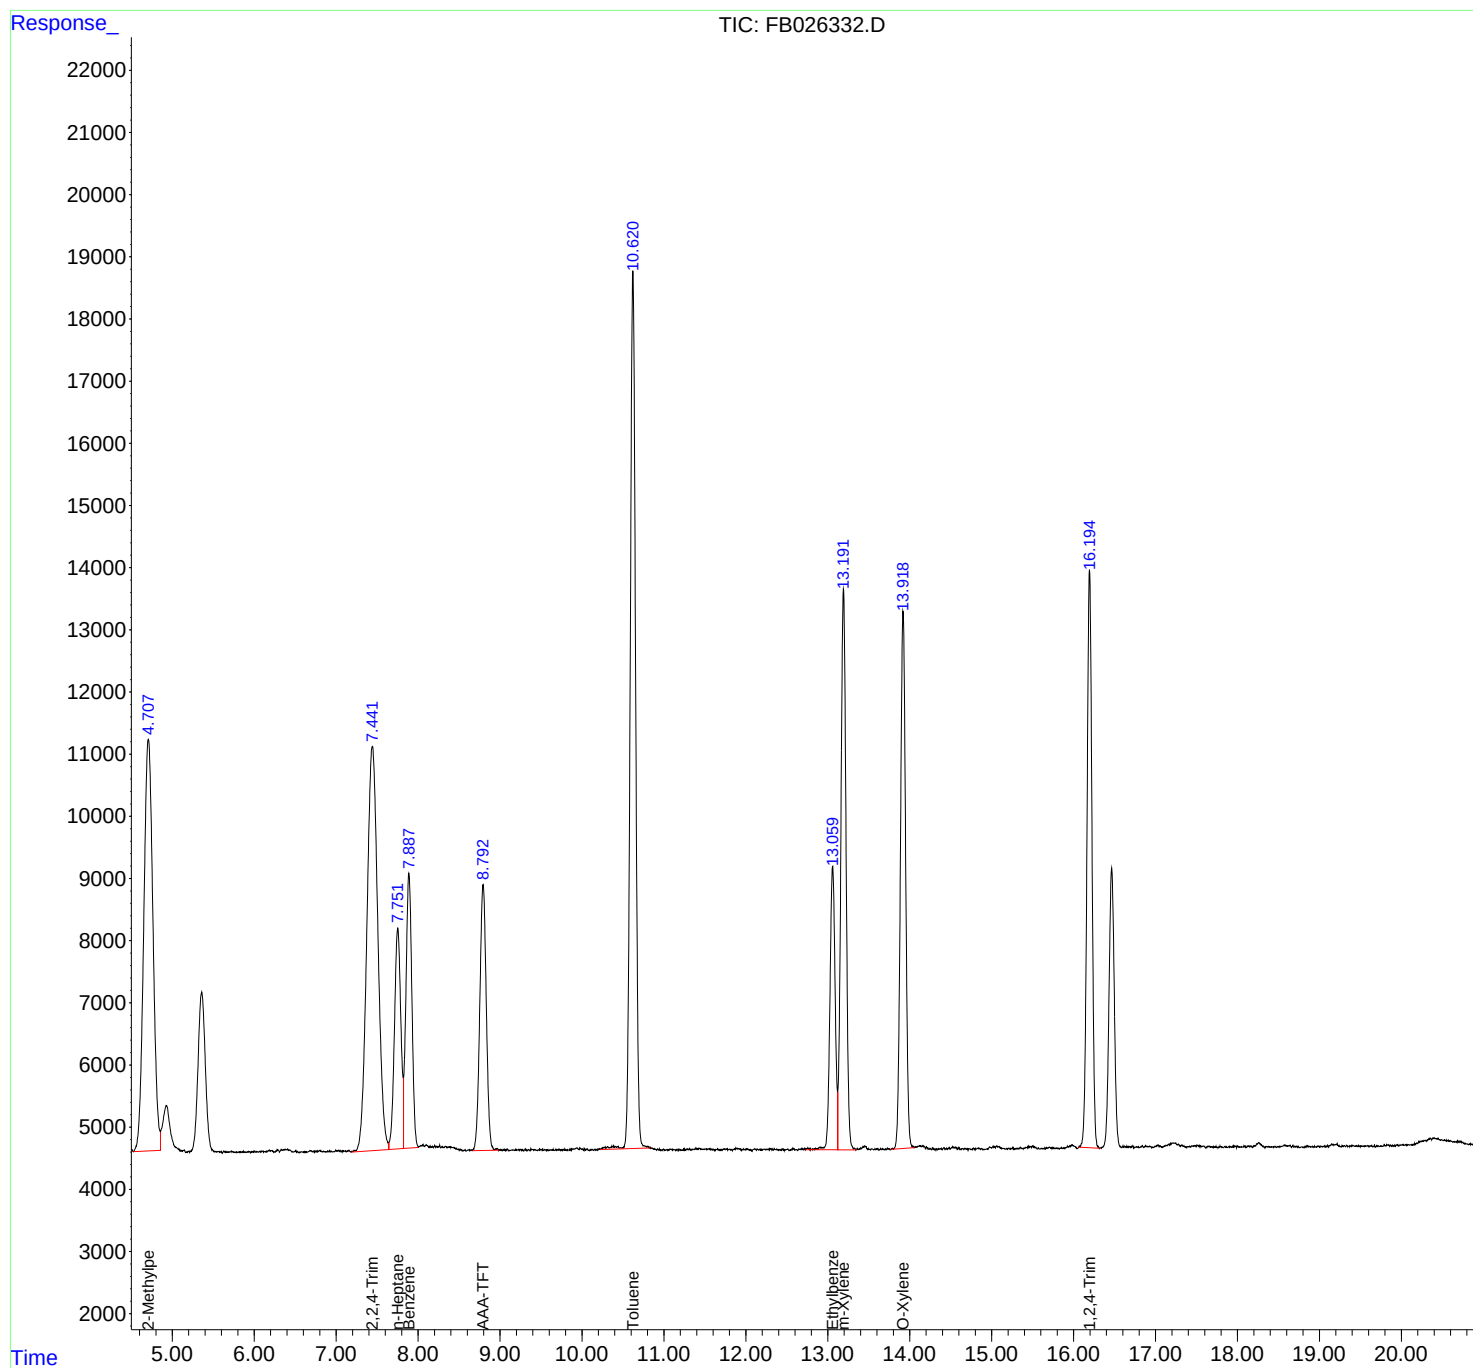

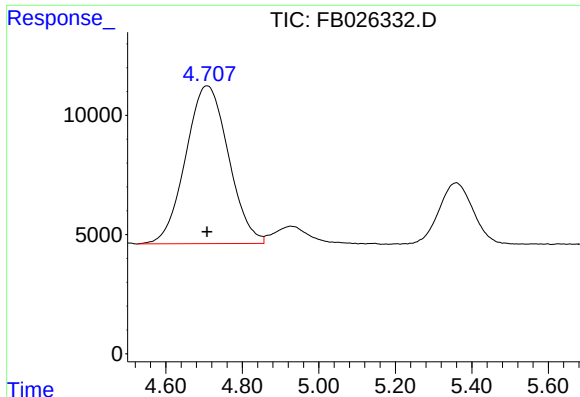


#1 2-Methylpentane

R.T.: 4.708 min
Delta R.T.: 0.000 min
Response: 515200
Conc: 30.94 ng/ml

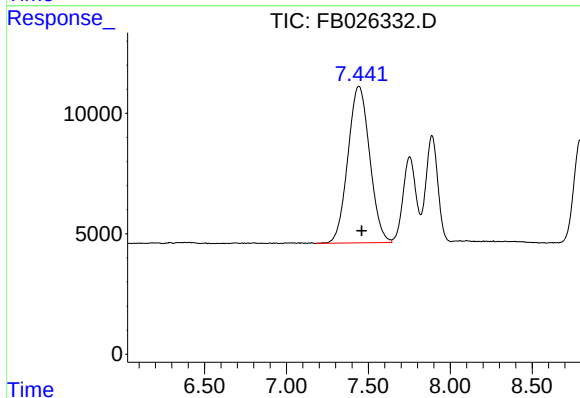


#2 2,2,4-Trimethylpentane

R.T.: 7.443 min
Delta R.T.: -0.017 min
Response: 601312
Conc: 30.84 ng/ml

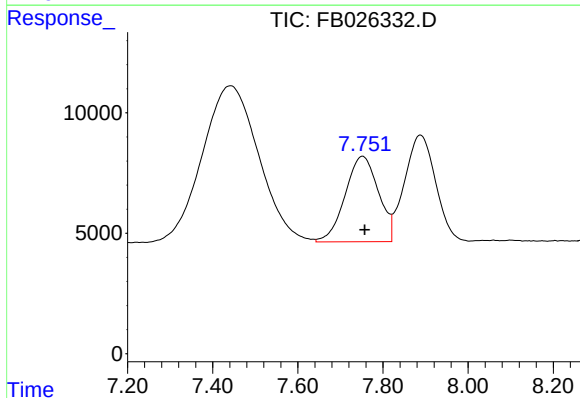


#3 n-Heptane

R.T.: 7.753 min
Delta R.T.: -0.004 min
Response: 192843
Conc: 10.45 ng/ml

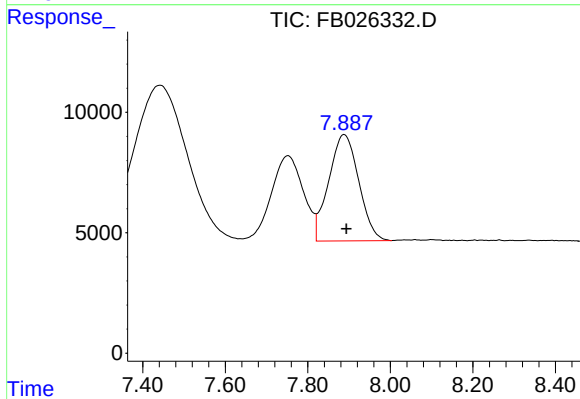


#4 Benzene

R.T.: 7.888 min
Delta R.T.: -0.005 min
Response: 223421
Conc: 10.25 ng/ml

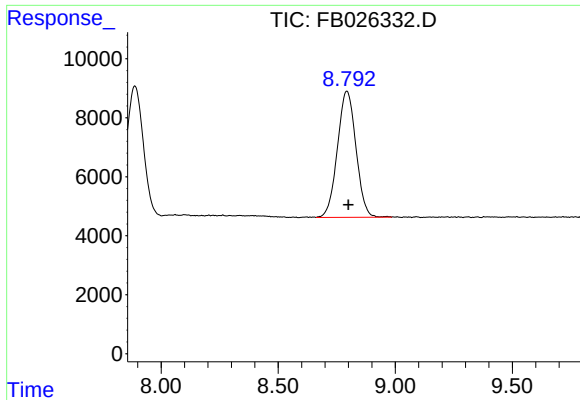


#5 AAA-TFT

R.T.: 8.794 min
Delta R.T.: -0.007 min
Response: 235433
Conc: 19.87 ng/ml

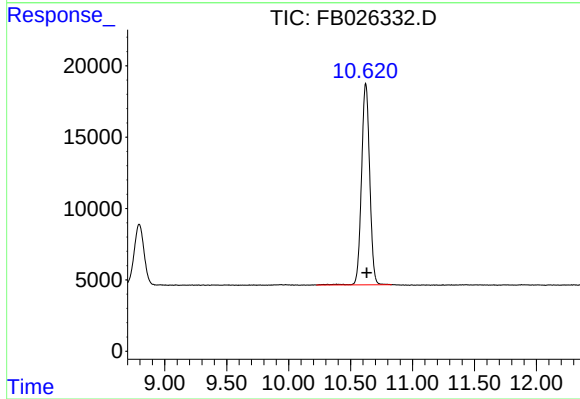


#6 Toluene

R.T.: 10.622 min
Delta R.T.: -0.009 min
Response: 646736
Conc: 31.18 ng/ml

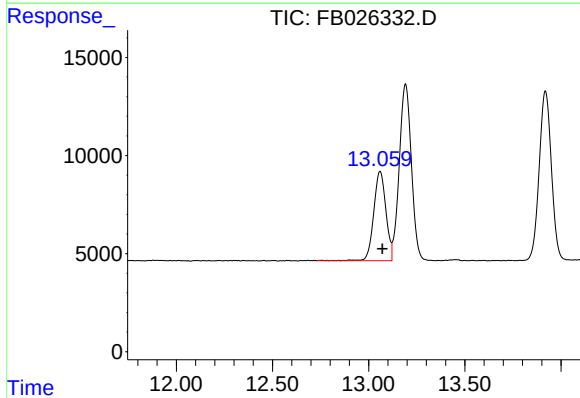


#7 Ethylbenzene

R.T.: 13.059 min
Delta R.T.: -0.012 min
Response: 200909
Conc: 10.64 ng/ml

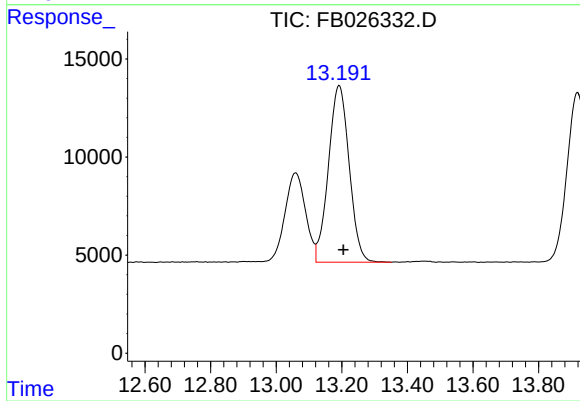


#8 m-Xylene

R.T.: 13.192 min
Delta R.T.: -0.013 min
Response: 395811
Conc: 20.81 ng/ml

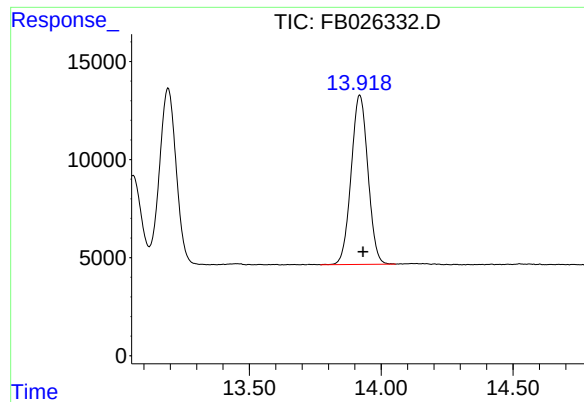

#9 O-Xylene

R.T.: 13.919 min
Delta R.T.: -0.012 min
Response: 380378
Conc: 20.59 ng/ml

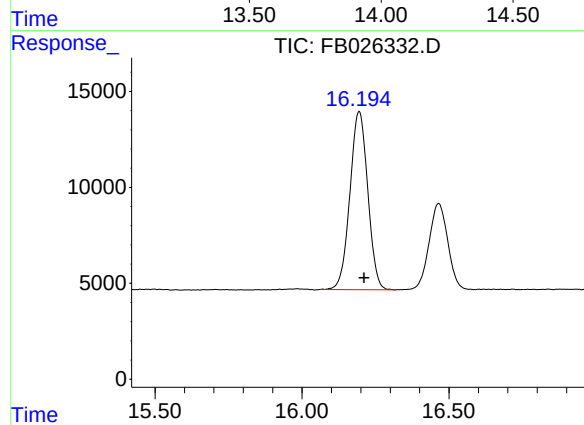

#10 1,2,4-Trimethylbenzene

R.T.: 16.195 min
Delta R.T.: -0.016 min
Response: 391906
Conc: 20.67 ng/ml