

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102921\
 Data File : FB026337.D
 Signal(s) : FID2B.CH
 Acq On : 29 Oct 2021 16:23
 Operator : AJ/MA
 Sample : M4068-03
 Misc : 4.99G\5.00 ML DI WATER
 ALS Vial : 8 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Oct 29 22:44:50 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102721.M
 Quant Title :
 QLast Update : Thu Oct 28 05:34:31 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.796	182180	15.378 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.704	20772	1.247 ng/ml
2) t 2,2,4-Trimethylpentane	7.412	30079	1.543 ng/mlm
3) t n-Heptane	7.767	10900	0.591 ng/mlm
4) t Benzene	7.890	10318	0.473 ng/mlm
6) t Toluene	10.621	29625	1.428 ng/ml
7) t Ethylbenzene	13.063	8803	0.466 ng/ml
8) t m-Xylene	13.191	18779	0.987 ng/ml
9) t O-Xylene	13.923	19031	1.030 ng/ml
10) t 1,2,4-Trimethylbenzene	16.195	23632	1.247 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102921\
Data File : FB026337.D
Signal(s) : FID2B.CH
Acq On : 29 Oct 2021 16:23
Operator : AJ/MA
Sample : M4068-03
Misc : 4.99G\5.00 ML DI WATER
ALS Vial : 8 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 29 22:44:50 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102721.M
Quant Title :
QLast Update : Thu Oct 28 05:34:31 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

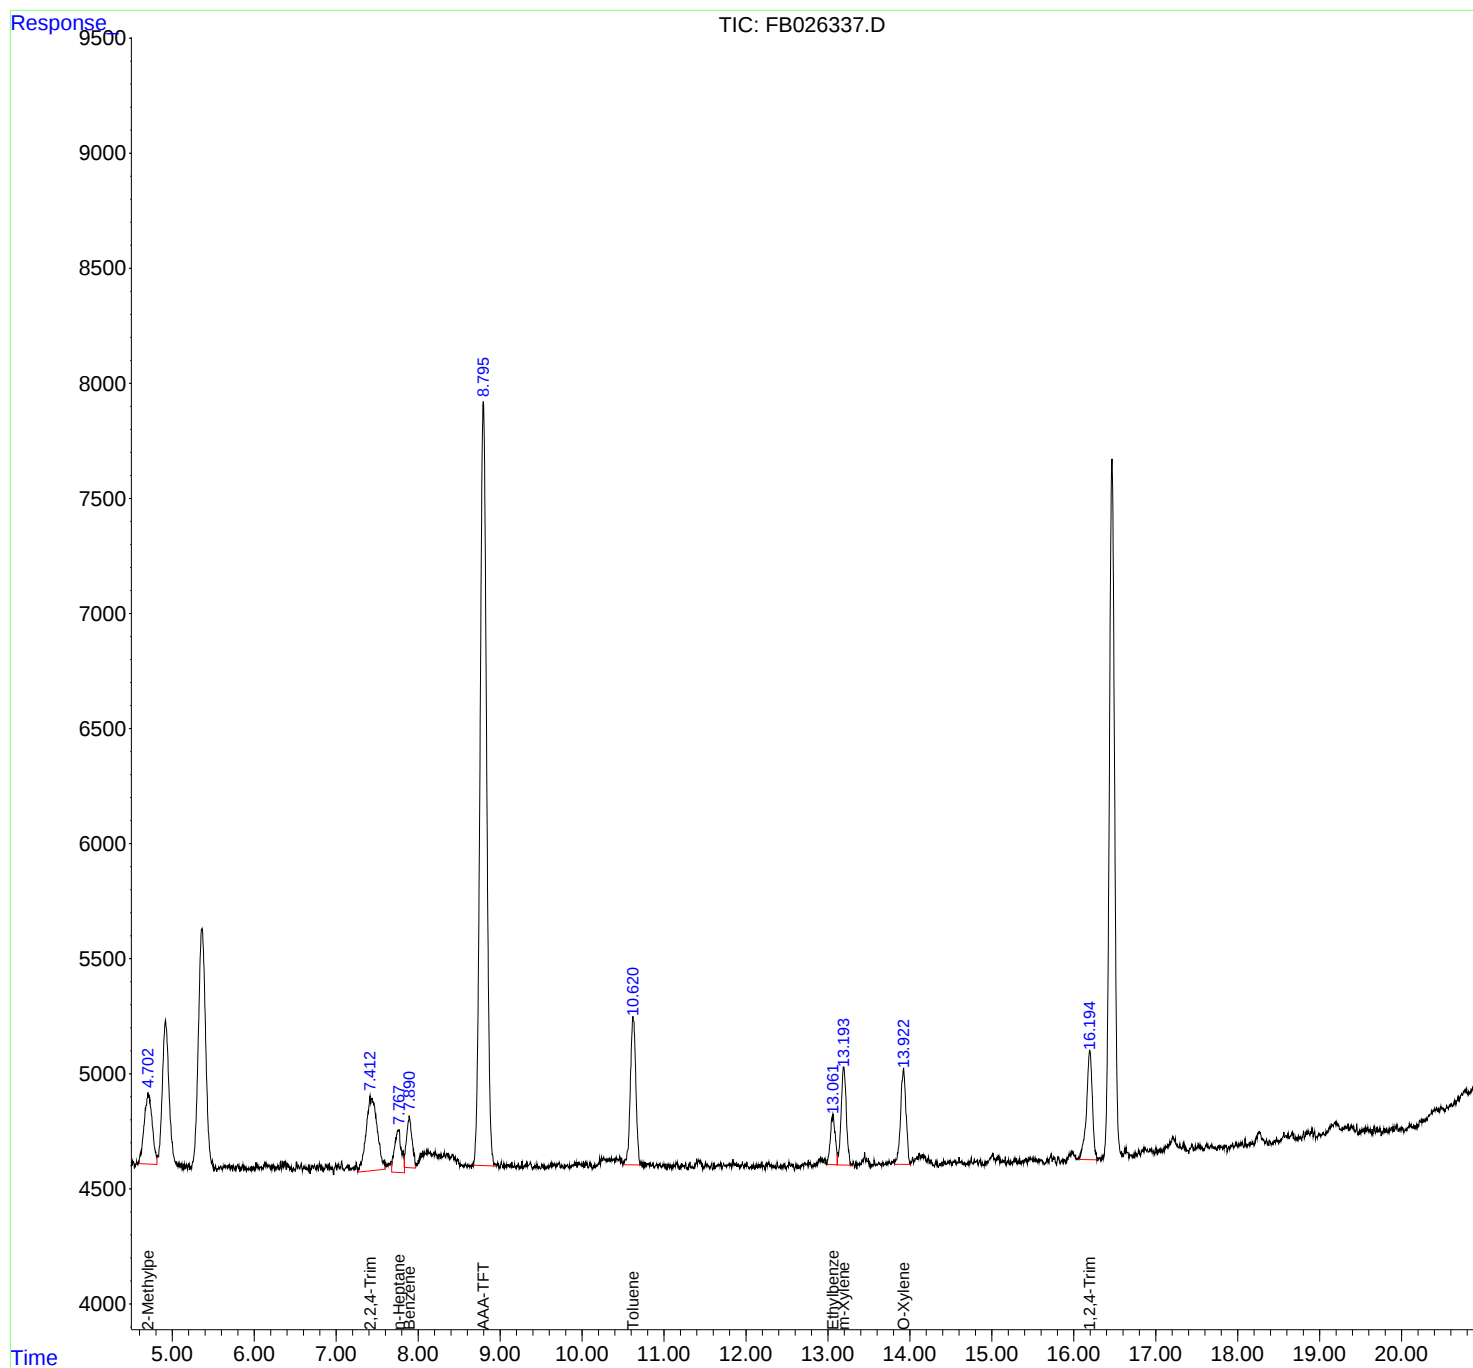

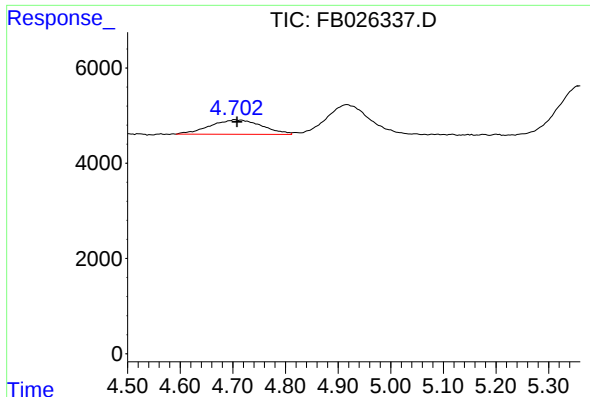


#1 2-Methylpentane

R.T.: 4.704 min
Delta R.T.: -0.004 min
Response: 20772
Conc: 1.25 ng/ml

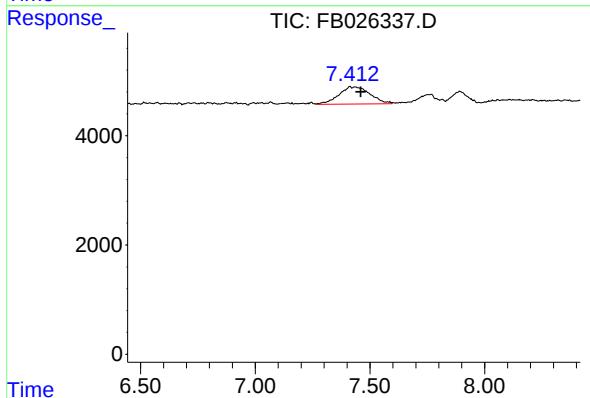


#2 2,2,4-Trimethylpentane

R.T.: 7.412 min
Delta R.T.: -0.047 min
Response: 30079
Conc: 1.54 ng/ml m

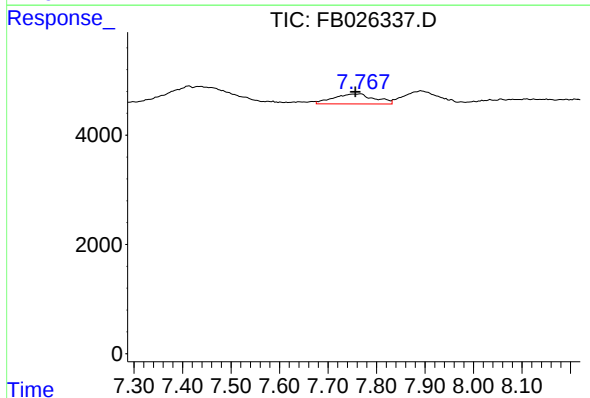


#3 n-Heptane

R.T.: 7.767 min
Delta R.T.: 0.010 min
Response: 10900
Conc: 0.59 ng/ml m

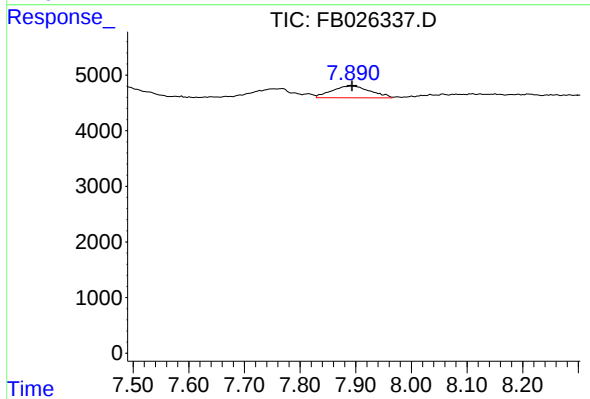


#4 Benzene

R.T.: 7.890 min
Delta R.T.: -0.003 min
Response: 10318
Conc: 0.47 ng/ml m

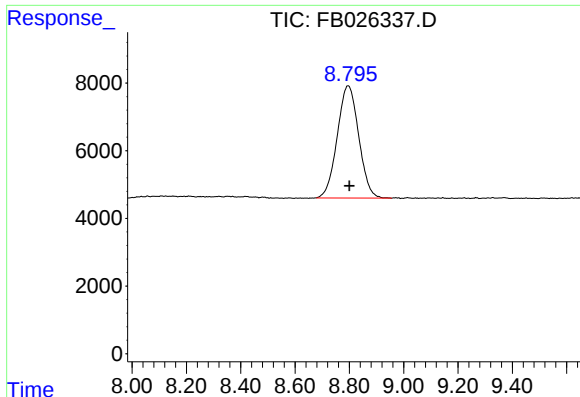


#5 AAA-TFT

R.T.: 8.796 min
Delta R.T.: -0.004 min
Response: 182180
Conc: 15.38 ng/ml

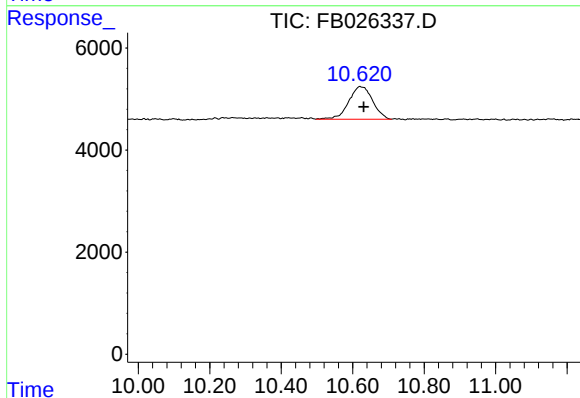


#6 Toluene

R.T.: 10.621 min
Delta R.T.: -0.010 min
Response: 29625
Conc: 1.43 ng/ml

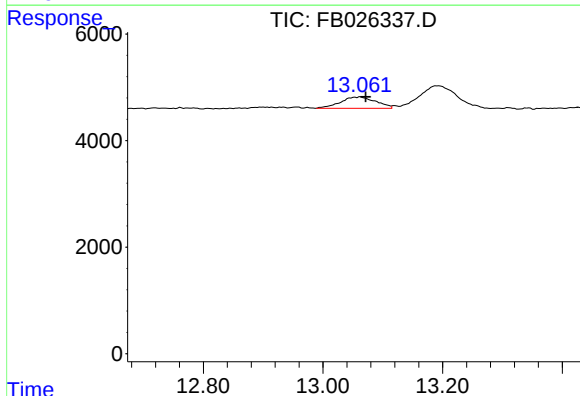


#7 Ethylbenzene

R.T.: 13.063 min
Delta R.T.: -0.009 min
Response: 8803
Conc: 0.47 ng/ml

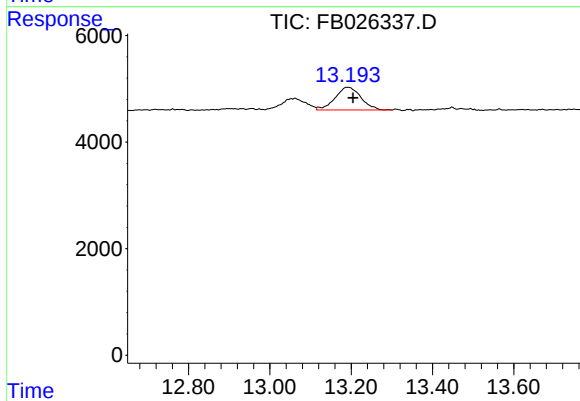


#8 m-Xylene

R.T.: 13.191 min
Delta R.T.: -0.014 min
Response: 18779
Conc: 0.99 ng/ml

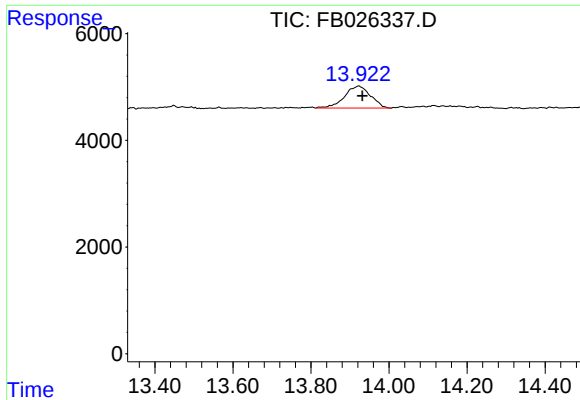

#9 O-Xylene

R.T.: 13.923 min
Delta R.T.: -0.008 min
Response: 19031
Conc: 1.03 ng/ml

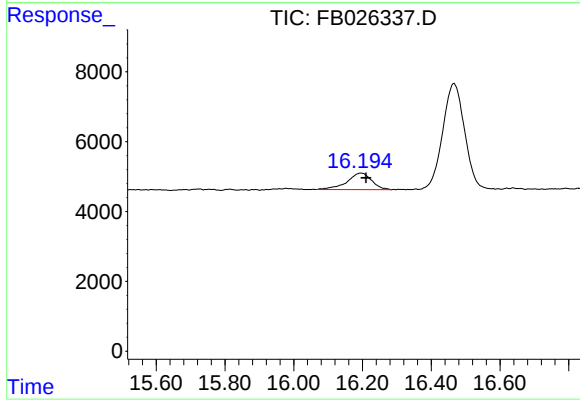

#10 1,2,4-Trimethylbenzene

R.T.: 16.195 min
Delta R.T.: -0.016 min
Response: 23632
Conc: 1.25 ng/ml