

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102924\
 Data File : FB031055.D
 Signal(s) : FID2B.CH
 Acq On : 29 Oct 2024 10:24
 Operator : YP/AJ
 Sample : VBF1029S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Oct 30 05:19:55 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102824.M
 Quant Title :
 QLast Update : Mon Oct 28 12:19:57 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.790	523894	18.980 ng/ml
Target Compounds			
6) t Toluene	10.616	9726	0.195 ng/ml
8) t m-Xylene	13.180	9588	0.197 ng/ml
9) t O-Xylene	13.922	9403	0.206 ng/ml
10) t 1,2,4-Trimethylbenzene	16.196	20540	0.552 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102924\
Data File : FB031055.D
Signal(s) : FID2B.CH
Acq On : 29 Oct 2024 10:24
Operator : YP/AJ
Sample : VBF1029S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Oct 30 05:19:55 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102824.M
Quant Title :
QLast Update : Mon Oct 28 12:19:57 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

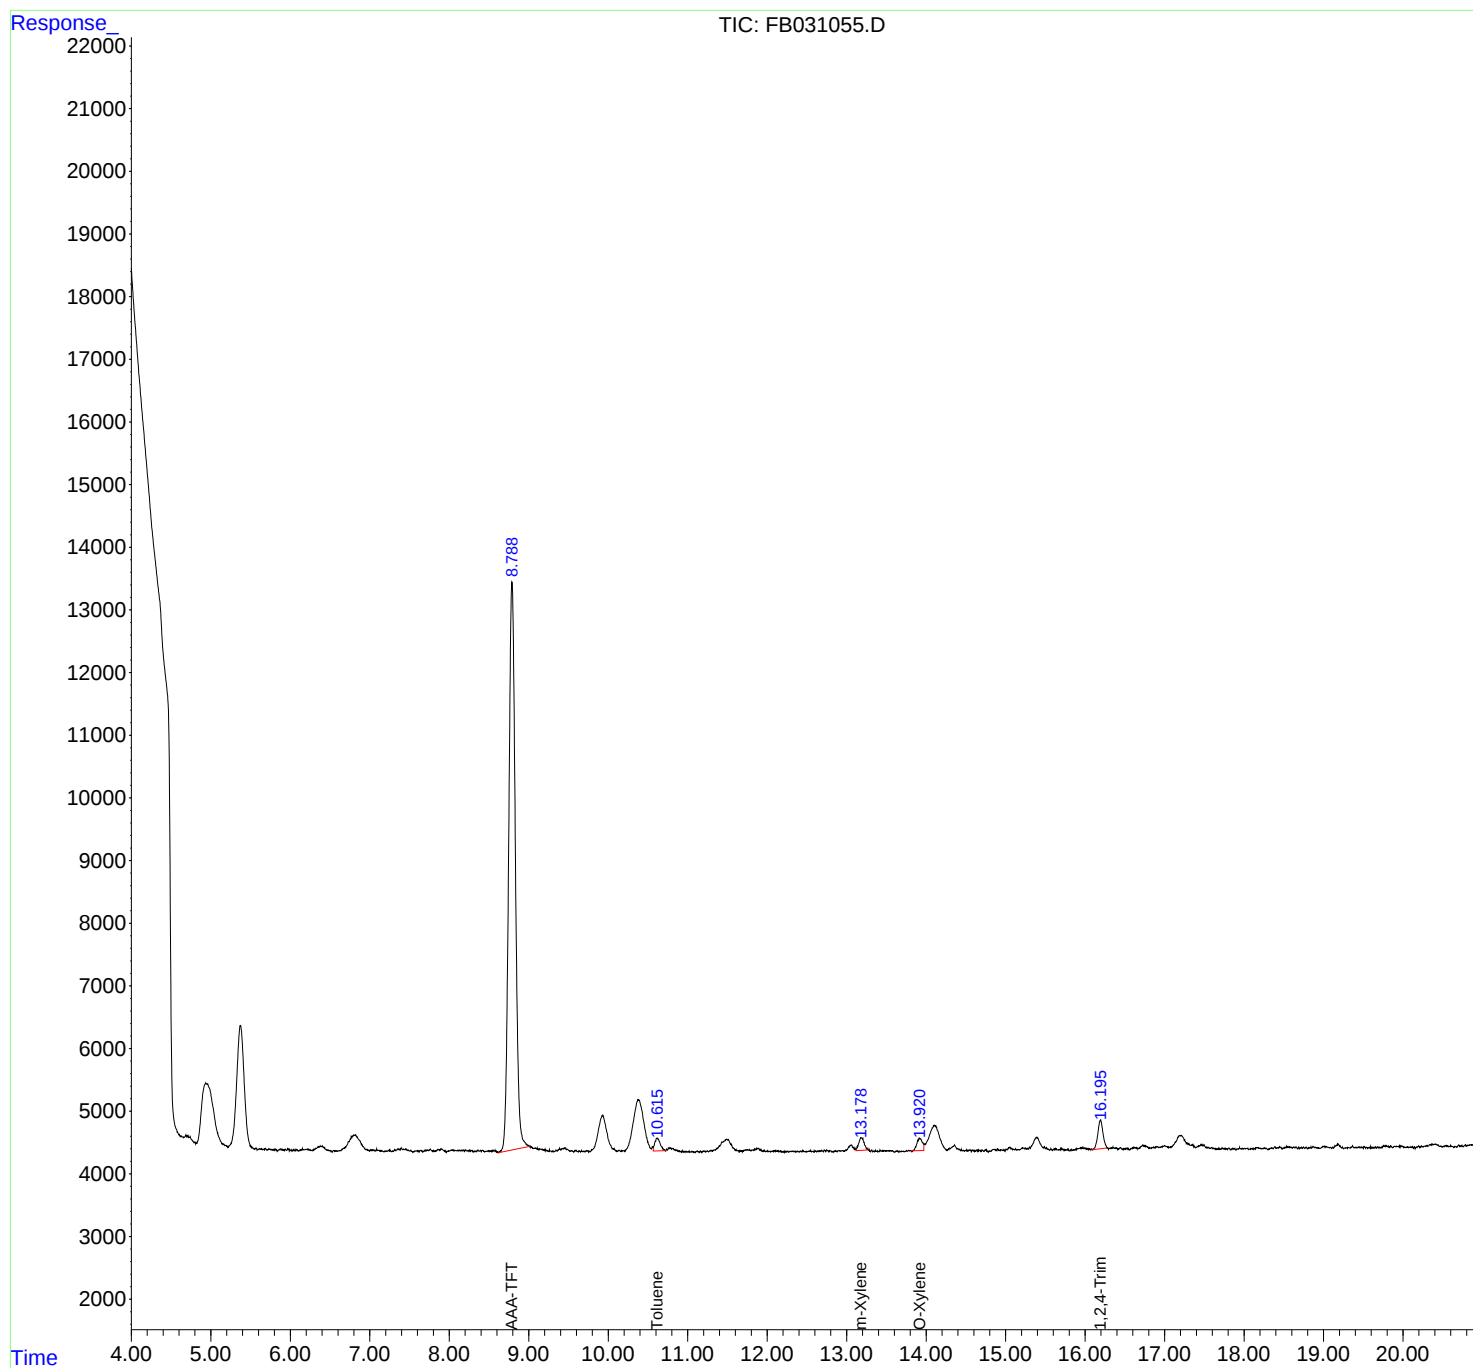


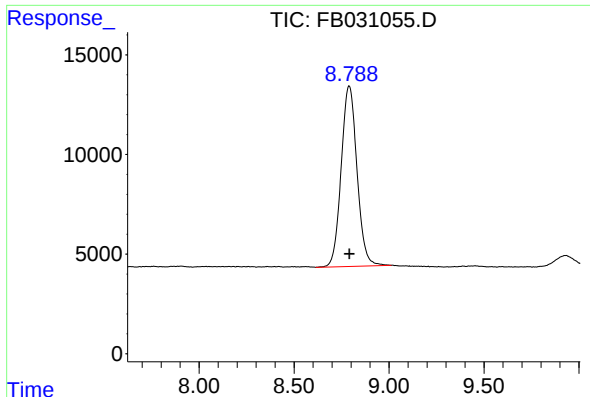

#5 AAA-TFT


R.T.: 8.790 min
Delta R.T.: 0.000 min
Response: 523894
Conc: 18.98 ng/ml

Instrument :
FID_B
ClientSampleId :

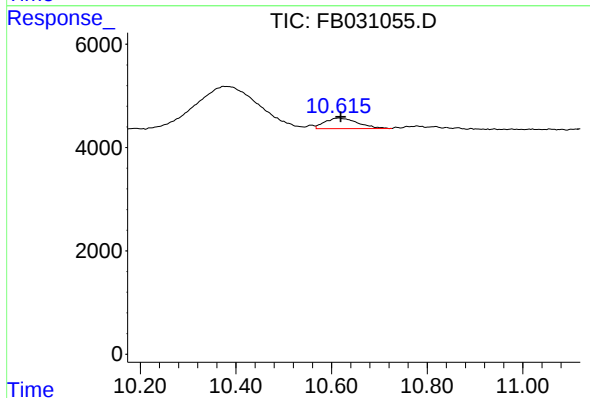


#6 Toluene

R.T.: 10.616 min
Delta R.T.: -0.003 min
Response: 9726
Conc: 0.19 ng/ml

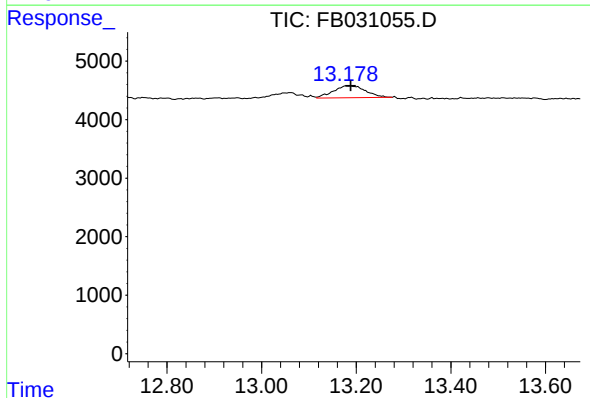


#8 m-Xylene

R.T.: 13.180 min
Delta R.T.: -0.008 min
Response: 9588
Conc: 0.20 ng/ml

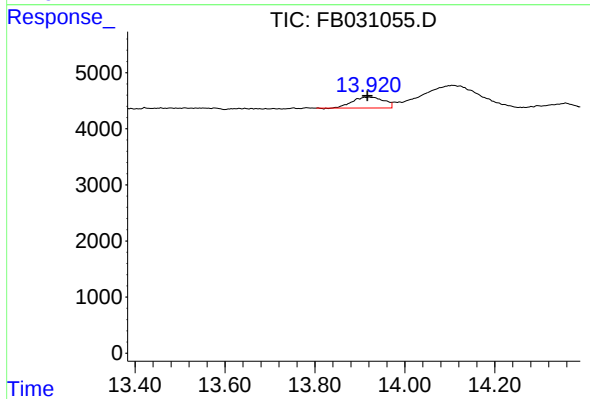

#9 O-Xylene

R.T.: 13.922 min
Delta R.T.: 0.005 min
Response: 9403
Conc: 0.21 ng/ml

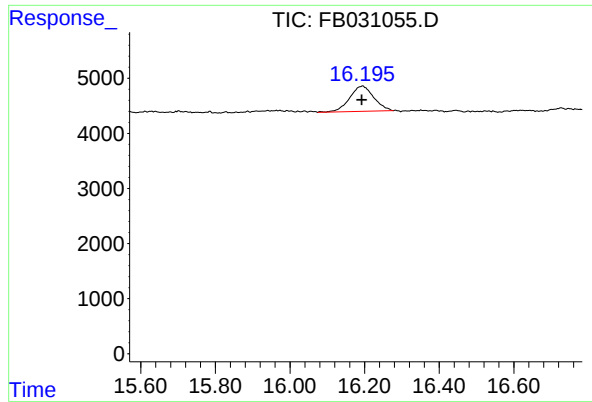

#10 1,2,4-Trimethylbenzene

R.T.: 16.196 min
Delta R.T.: 0.004 min
Response: 20540
Conc: 0.55 ng/ml

Instrument :
FID_B
ClientSampleId :