

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102924\
 Data File : FB031073.D
 Signal(s) : FID2B.CH
 Acq On : 29 Oct 2024 19:45
 Operator : YP/AJ
 Sample : BSF1029S3
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1029S3

Integration File: Calibration.e
 Quant Time: Oct 30 05:26:23 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102824.M
 Quant Title :
 QLast Update : Mon Oct 28 12:19:57 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.793	579486	20.994 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.719	1122348	28.577 ng/ml
2) t 2,2,4-Trimethylpentane	7.423	1366092	29.167 ng/ml
3) t n-Heptane	7.754	415959	9.178 ng/ml
4) t Benzene	7.893	501694	9.385 ng/ml
6) t Toluene	10.622	1384410	27.723 ng/ml
7) t Ethylbenzene	13.057	428552	9.574 ng/ml
8) t m-Xylene	13.192	874360	17.977 ng/ml
9) t O-Xylene	13.920	823248	18.060 ng/ml
10) t 1,2,4-Trimethylbenzene	16.195	613020	16.475 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102924\
Data File : FB031073.D
Signal(s) : FID2B.CH
Acq On : 29 Oct 2024 19:45
Operator : YP/AJ
Sample : BSF1029S3
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1029S3

Integration File: Calibration.e
Quant Time: Oct 30 05:26:23 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102824.M
Quant Title :
QLast Update : Mon Oct 28 12:19:57 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

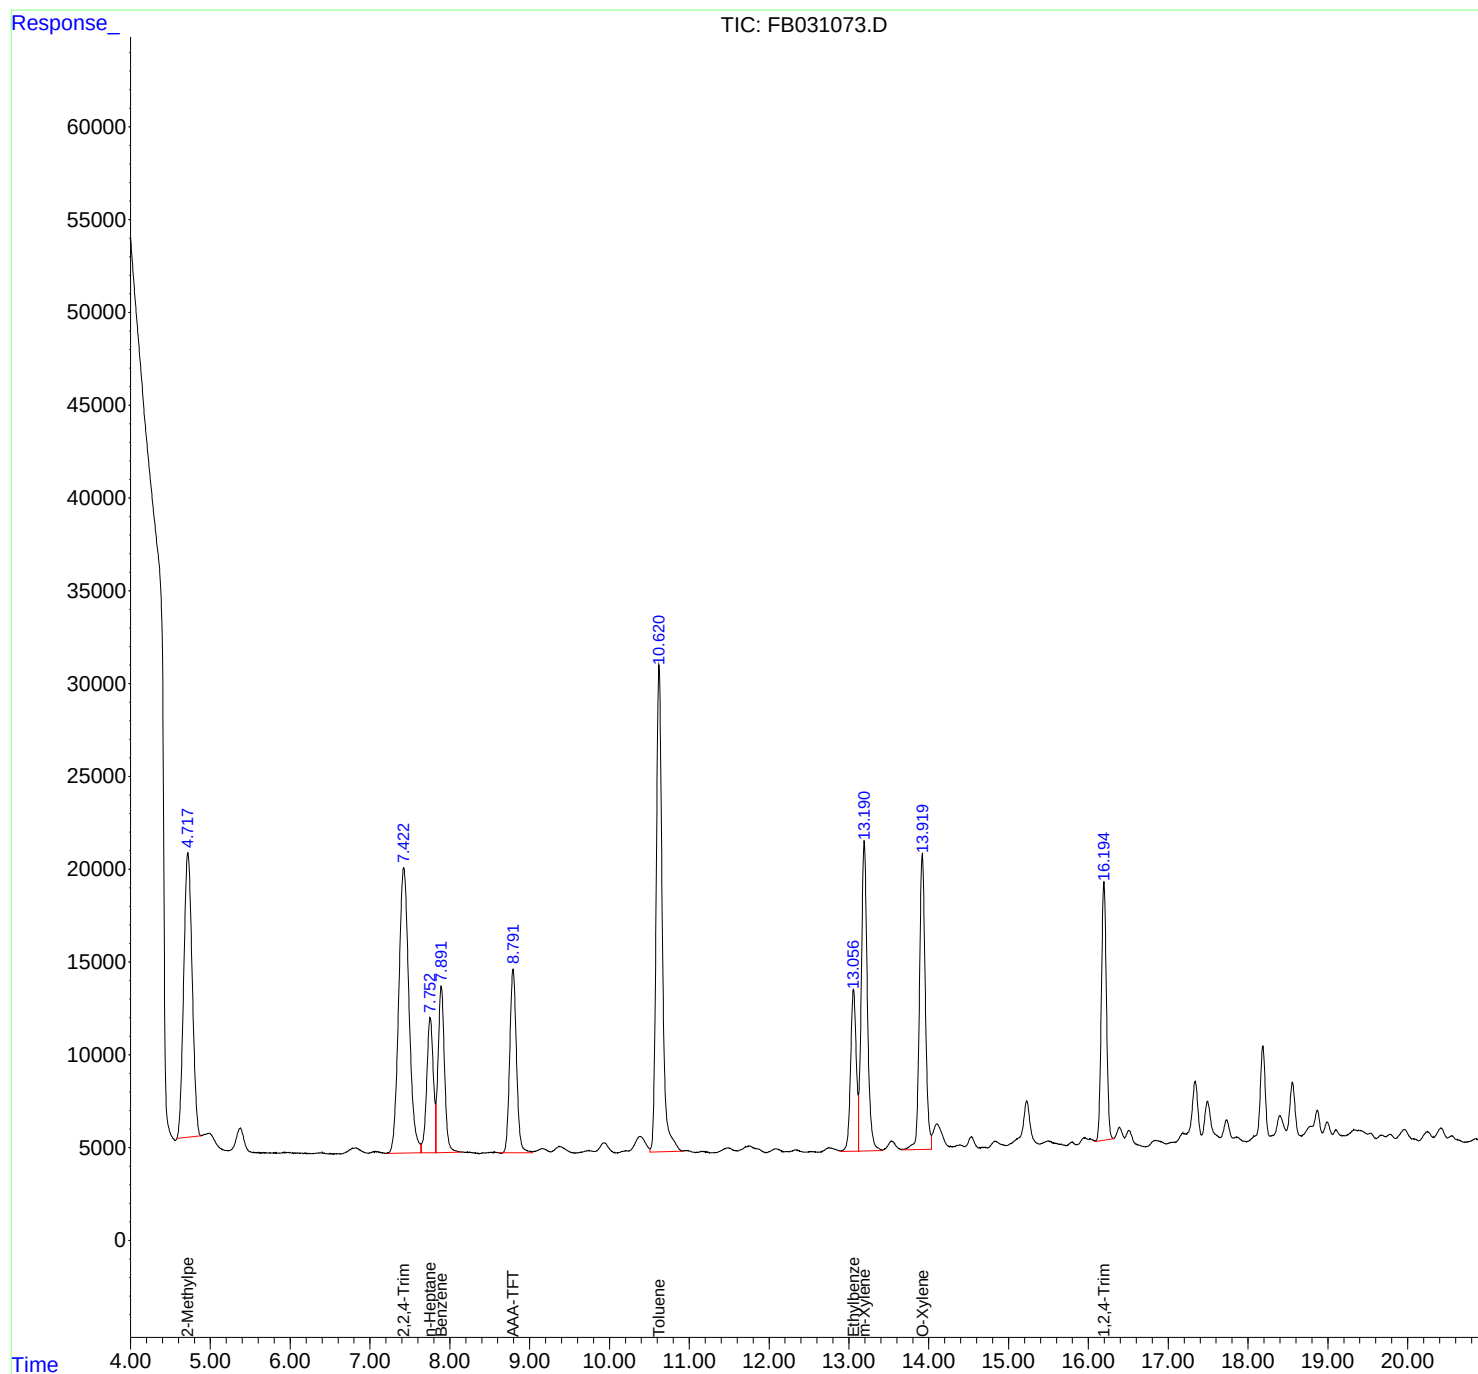


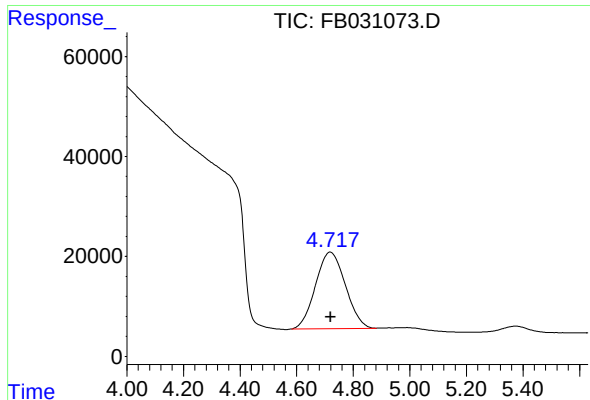

#1 2-Methylpentane


R.T.: 4.719 min
Delta R.T.: -0.001 min
Response: 1122348
Conc: 28.58 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1029S3

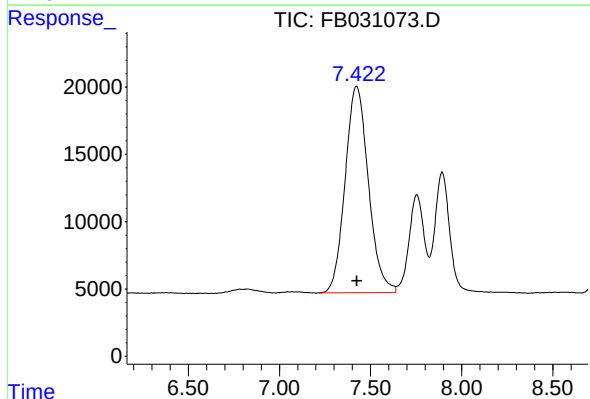


#2 2,2,4-Trimethylpentane

R.T.: 7.423 min
Delta R.T.: -0.002 min
Response: 1366092
Conc: 29.17 ng/ml

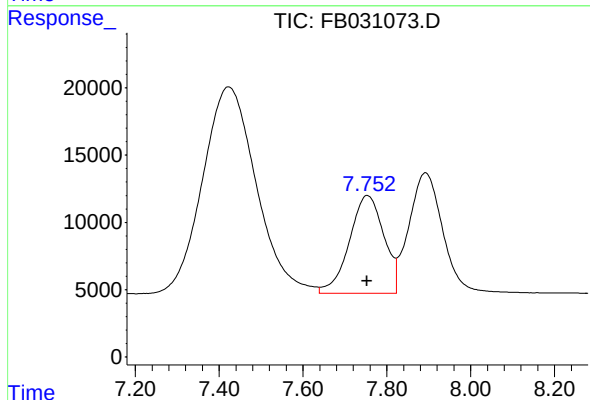


#3 n-Heptane

R.T.: 7.754 min
Delta R.T.: 0.000 min
Response: 415959
Conc: 9.18 ng/ml

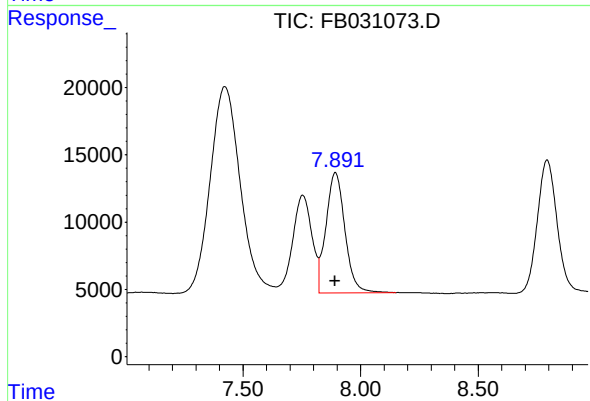

#4 Benzene


R.T.: 7.893 min
Delta R.T.: 0.001 min
Response: 501694
Conc: 9.39 ng/ml

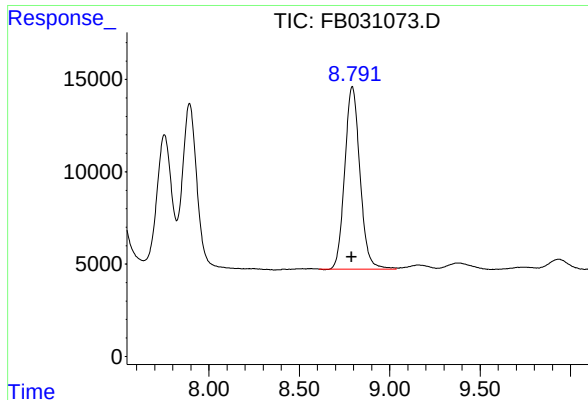

#5 AAA-TFT


R.T.: 8.793 min
Delta R.T.: 0.002 min
Response: 579486
Conc: 20.99 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1029S3

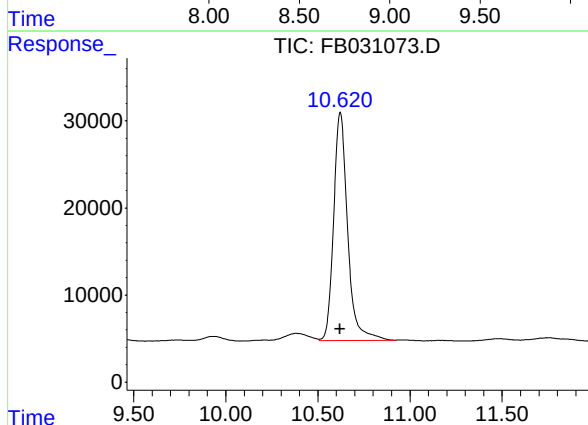


#6 Toluene

R.T.: 10.622 min
Delta R.T.: 0.002 min
Response: 1384410
Conc: 27.72 ng/ml

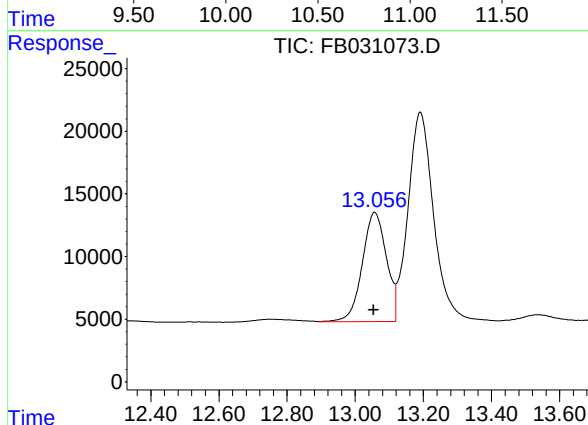


#7 Ethylbenzene

R.T.: 13.057 min
Delta R.T.: 0.003 min
Response: 428552
Conc: 9.57 ng/ml

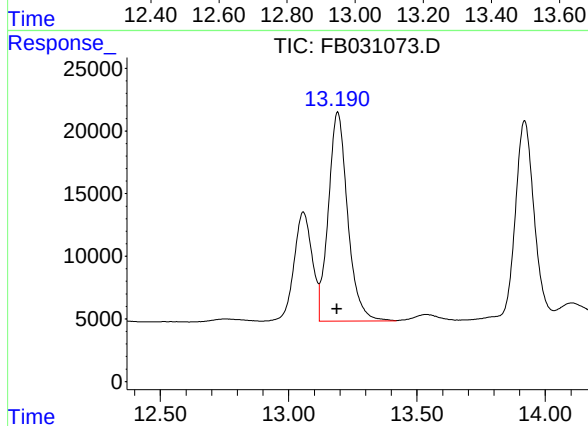

#8 m-Xylene


R.T.: 13.192 min
Delta R.T.: 0.003 min
Response: 874360
Conc: 17.98 ng/ml

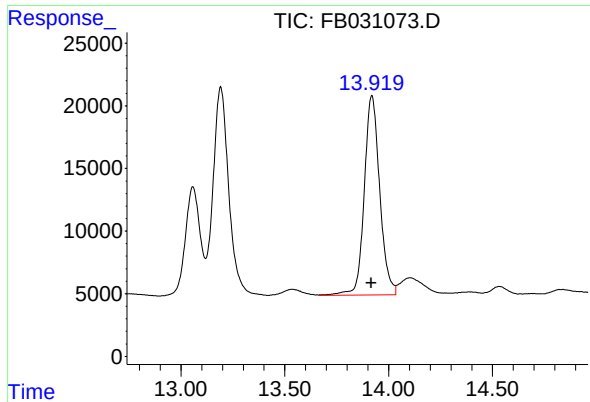

#9 O-Xylene

R.T.: 13.920 min
Delta R.T.: 0.003 min
Response: 823248
Conc: 18.06 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1029S3

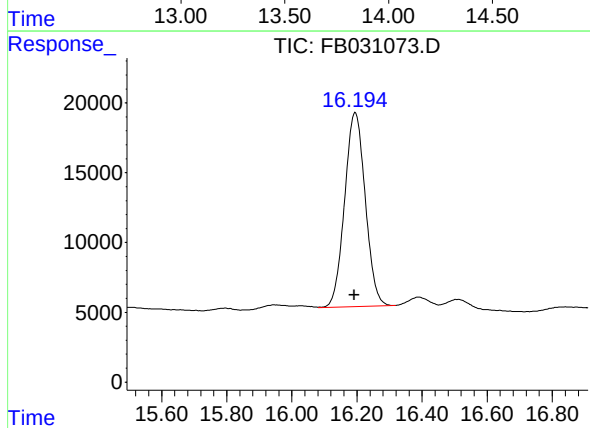

#10 1,2,4-Trimethylbenzene

R.T.: 16.195 min
Delta R.T.: 0.003 min
Response: 613020
Conc: 16.48 ng/ml