

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102924\
 Data File : FB031083.D
 Signal(s) : FID2B.CH
 Acq On : 30 Oct 2024 1:02
 Operator : YP/AJ
 Sample : BSF1029S4
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1029S4

Integration File: Calibration.e
 Quant Time: Oct 30 05:28:02 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102824.M
 Quant Title :
 QLast Update : Mon Oct 28 12:19:57 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.792	537562	19.475 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.720	1180322	30.053 ng/ml
2) t 2,2,4-Trimethylpentane	7.424	1417328	30.261 ng/ml
3) t n-Heptane	7.754	444809	9.815 ng/ml
4) t Benzene	7.892	542101	10.141 ng/ml
6) t Toluene	10.622	1483442	29.706 ng/ml
7) t Ethylbenzene	13.059	433084	9.675 ng/ml
8) t m-Xylene	13.192	927379	19.067 ng/ml
9) t O-Xylene	13.920	866709	19.014 ng/ml
10) t 1,2,4-Trimethylbenzene	16.195	647281	17.396 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102924\
Data File : FB031083.D
Signal(s) : FID2B.CH
Acq On : 30 Oct 2024 1:02
Operator : YP/AJ
Sample : BSF1029S4
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1029S4

Integration File: Calibration.e
Quant Time: Oct 30 05:28:02 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102824.M
Quant Title :
QLast Update : Mon Oct 28 12:19:57 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

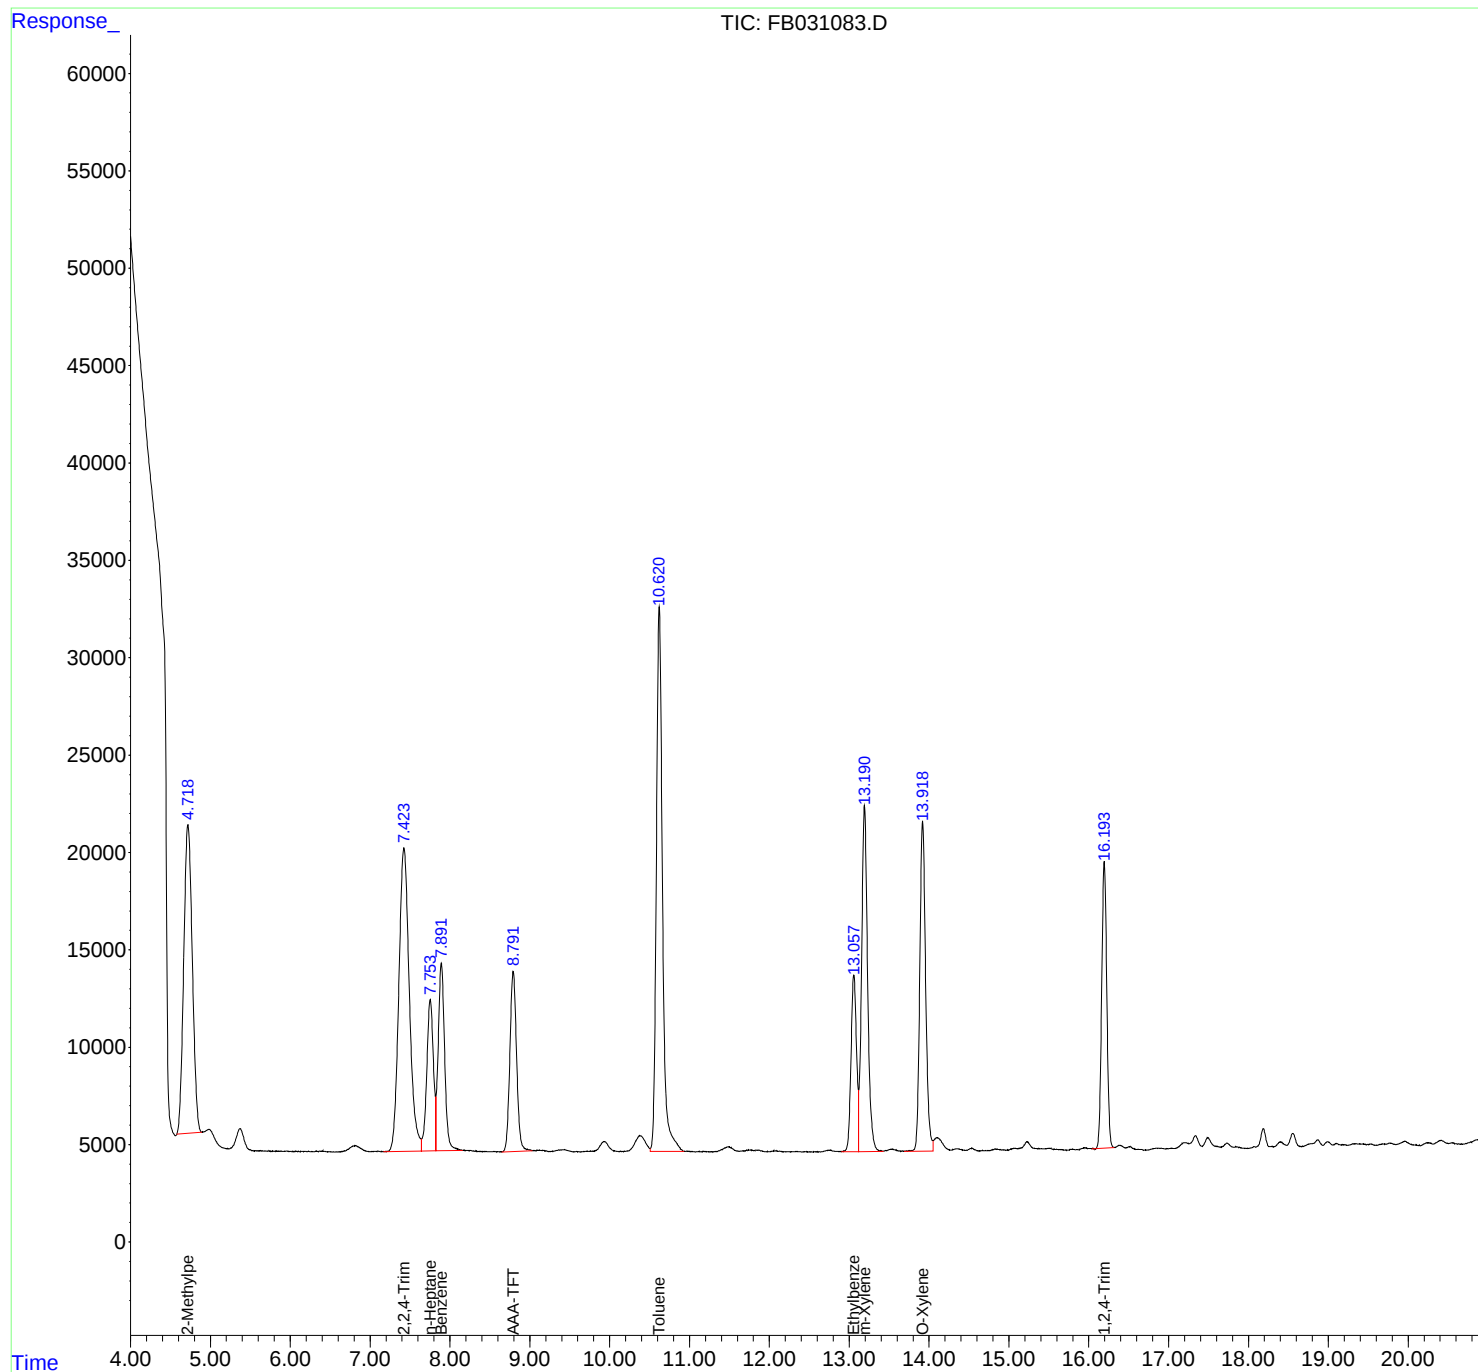


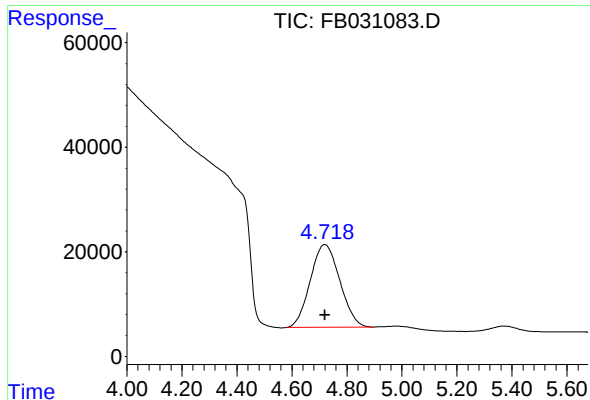

#1 2-Methylpentane


R.T.: 4.720 min
Delta R.T.: 0.000 min
Response: 1180322
Conc: 30.05 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1029S4

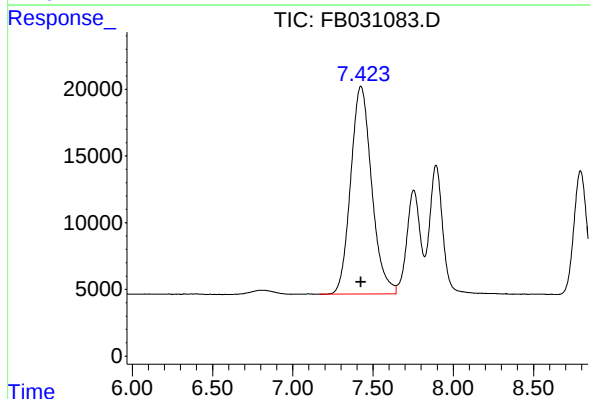


#2 2,2,4-Trimethylpentane

R.T.: 7.424 min
Delta R.T.: 0.000 min
Response: 1417328
Conc: 30.26 ng/ml

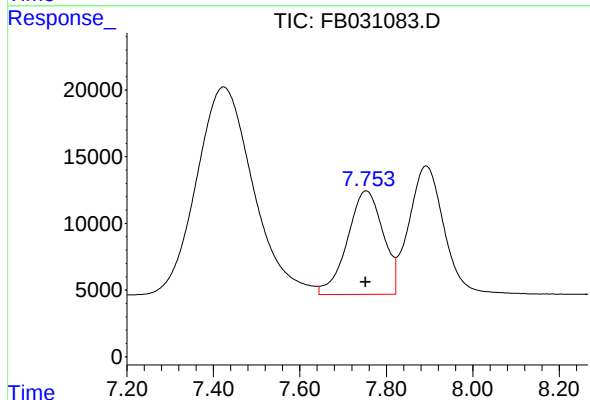


#3 n-Heptane

R.T.: 7.754 min
Delta R.T.: 0.001 min
Response: 444809
Conc: 9.81 ng/ml

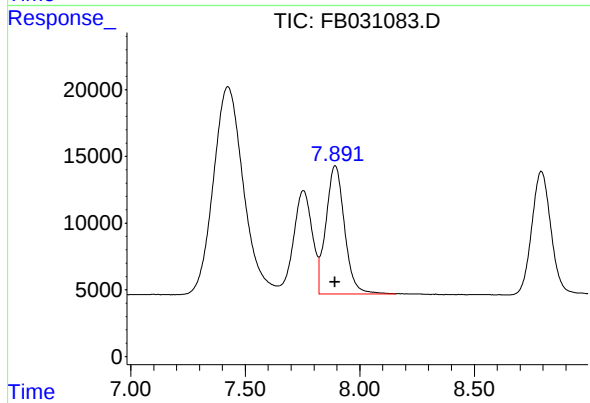

#4 Benzene


R.T.: 7.892 min
Delta R.T.: 0.000 min
Response: 542101
Conc: 10.14 ng/ml

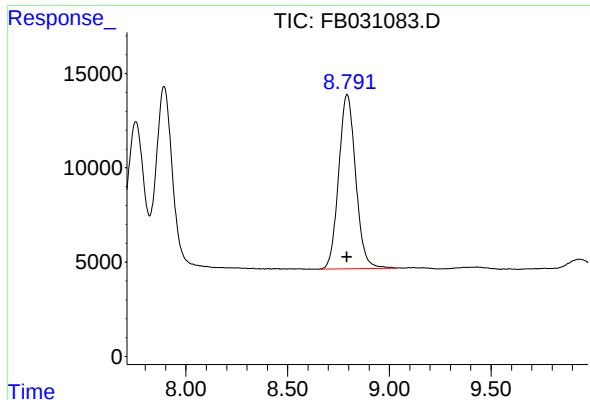

#5 AAA-TFT


R.T.: 8.792 min
Delta R.T.: 0.002 min
Response: 537562
Conc: 19.47 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1029S4

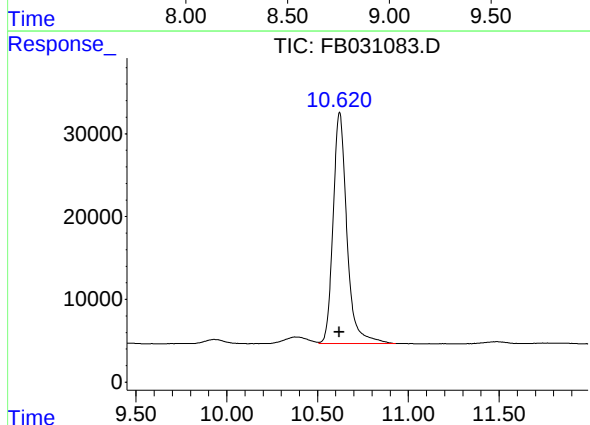


#6 Toluene

R.T.: 10.622 min
Delta R.T.: 0.002 min
Response: 1483442
Conc: 29.71 ng/ml

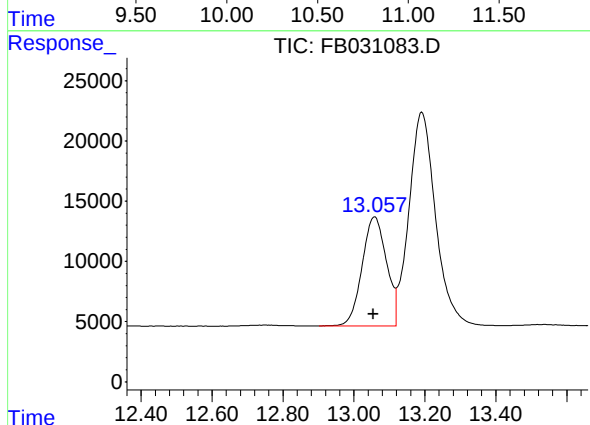


#7 Ethylbenzene

R.T.: 13.059 min
Delta R.T.: 0.004 min
Response: 433084
Conc: 9.68 ng/ml

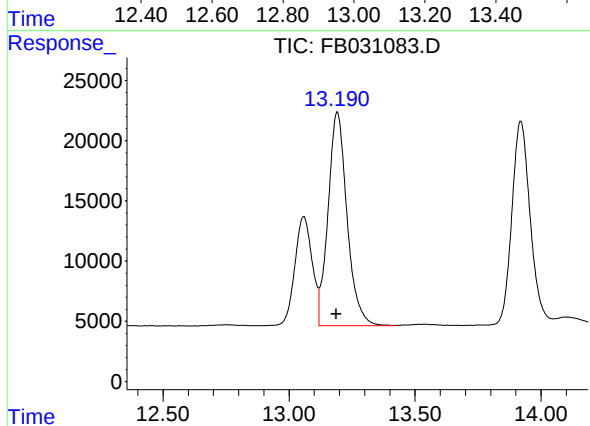

#8 m-Xylene


R.T.: 13.192 min
Delta R.T.: 0.004 min
Response: 927379
Conc: 19.07 ng/ml

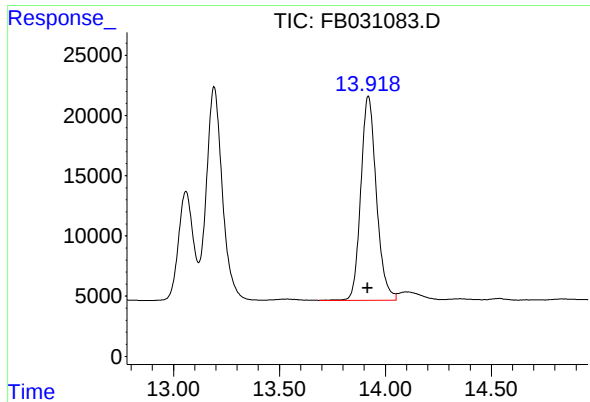

#9 O-Xylene

R.T.: 13.920 min
Delta R.T.: 0.003 min
Response: 866709
Conc: 19.01 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1029S4

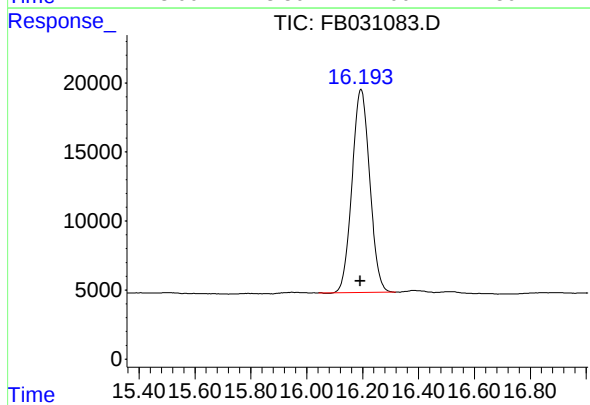

#10 1,2,4-Trimethylbenzene

R.T.: 16.195 min
Delta R.T.: 0.003 min
Response: 647281
Conc: 17.40 ng/ml