

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB103019\
Data File : FB022857.D
Signal(s) : FID2B.CH
Acq On : 30 Oct 2019 16:50
Operator : DD/AJ
Sample : K5146-16
Misc : 5.06g/5.00ml DI WATER
ALS Vial : 8 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 31 00:55:34 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101619.M
Quant Title :
QLast Update : Wed Oct 16 15:04:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.798	566701	22.396 ng/ml
Target Compounds			
6) t Toluene	10.631	751	0.017 ng/ml
8) t m-Xylene	13.192	2172	0.056 ng/ml
9) t O-Xylene	13.922	542	0.015 ng/ml
10) t 1,2,4-Trimethylbenzene	16.214	4906	0.172 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB103019\
Data File : FB022857.D
Signal(s) : FID2B.CH
Acq On : 30 Oct 2019 16:50
Operator : DD/AJ
Sample : K5146-16
Misc : 5.06g/5.00ml DI WATER
ALS Vial : 8 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 31 00:55:34 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101619.M
Quant Title :
QLast Update : Wed Oct 16 15:04:00 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

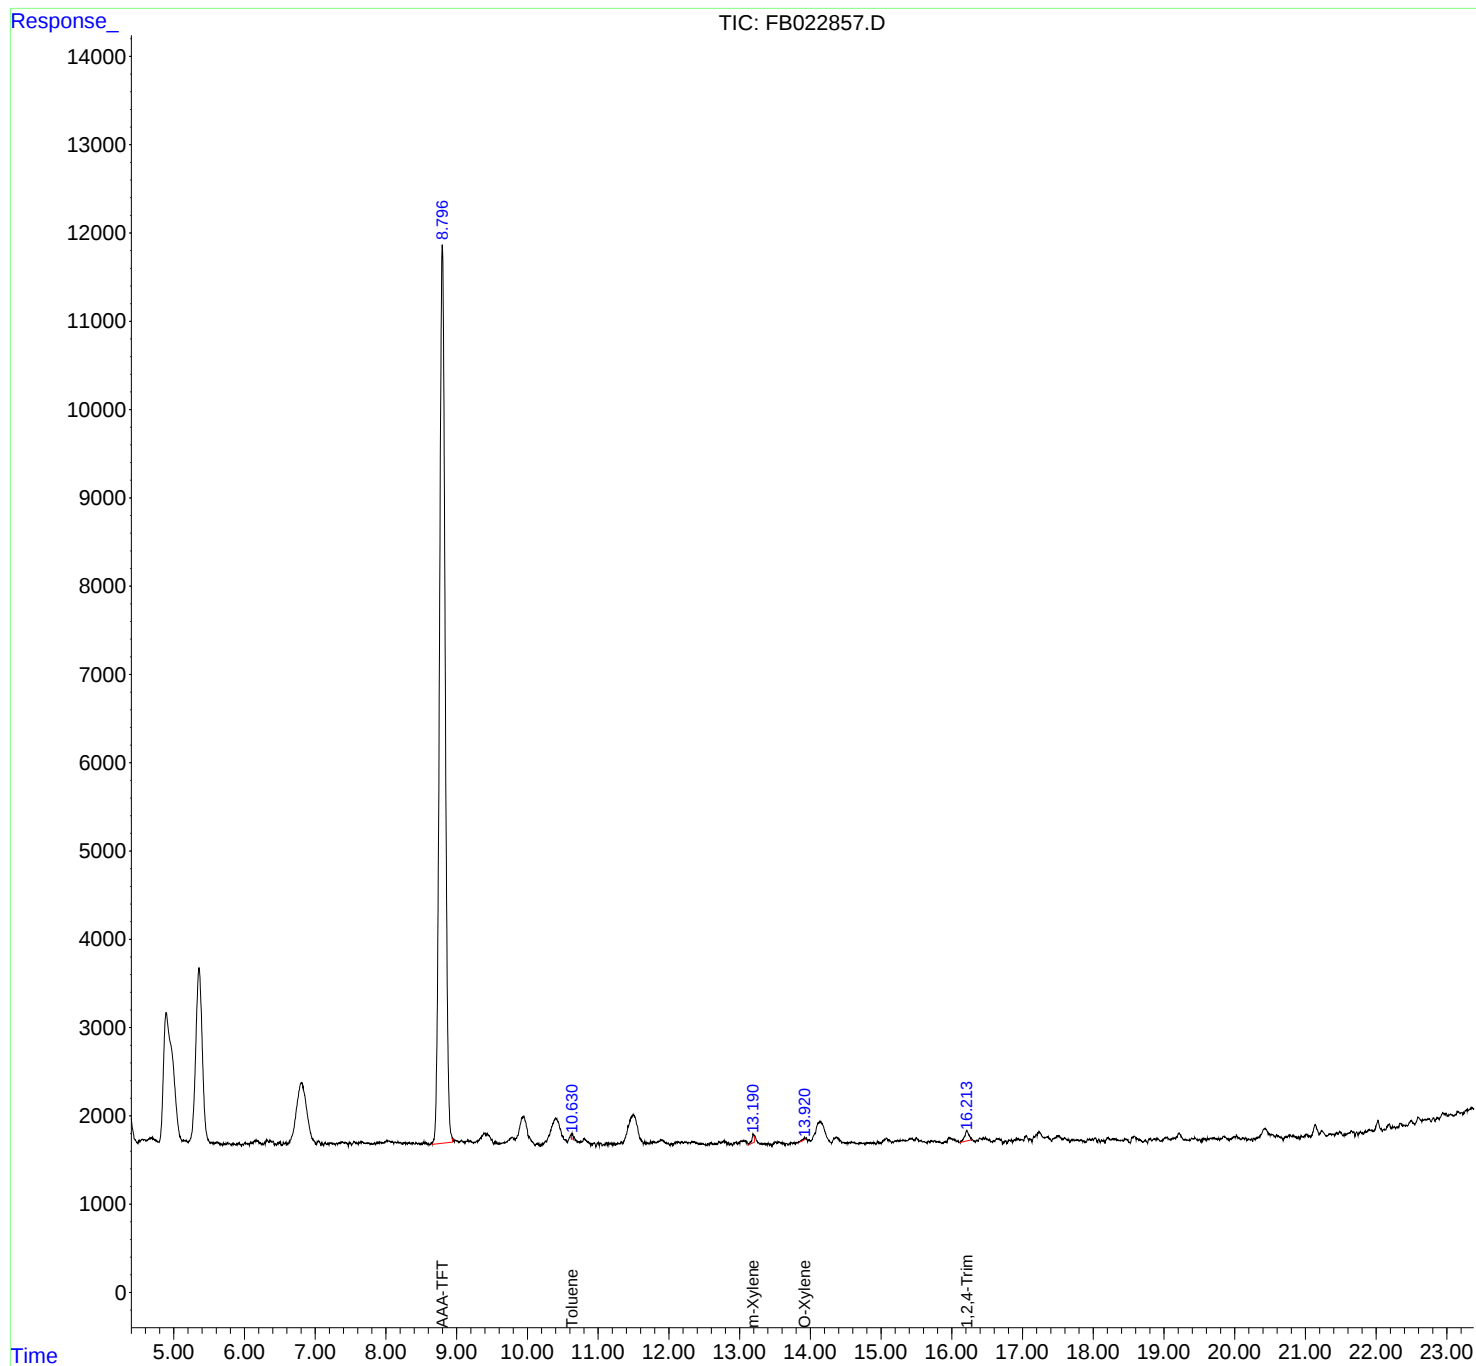

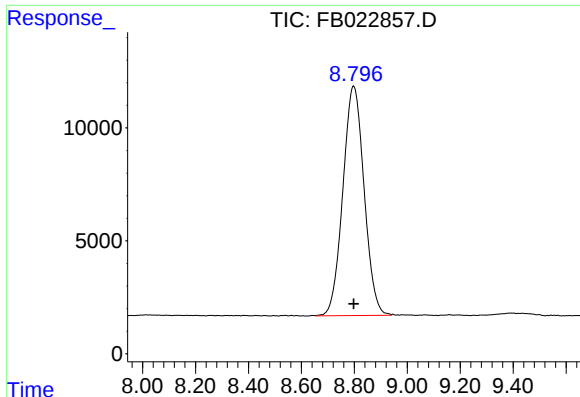


#5 AAA-TFT

R.T.: 8.798 min
Delta R.T.: 0.000 min
Response: 566701
Conc: 22.40 ng/ml

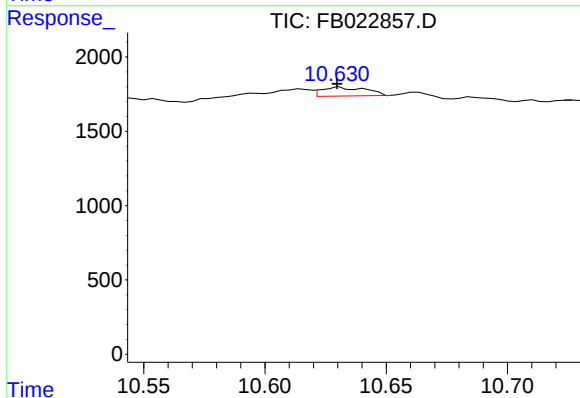


#6 Toluene

R.T.: 10.631 min
Delta R.T.: 0.002 min
Response: 751
Conc: 0.02 ng/ml

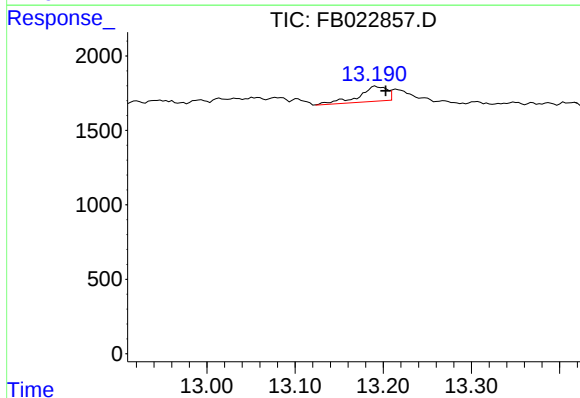


#8 m-Xylene

R.T.: 13.192 min
Delta R.T.: -0.011 min
Response: 2172
Conc: 0.06 ng/ml

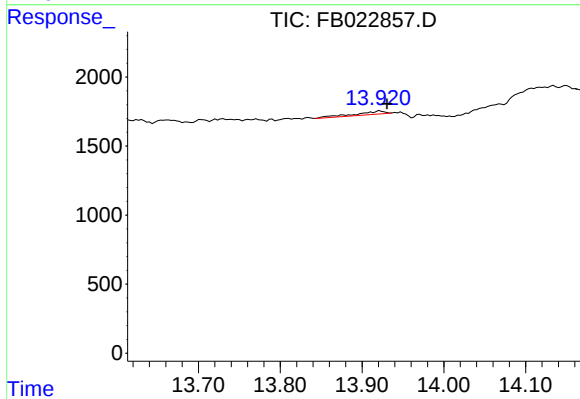

#9 O-Xylene

R.T.: 13.922 min
Delta R.T.: -0.009 min
Response: 542
Conc: 0.01 ng/ml

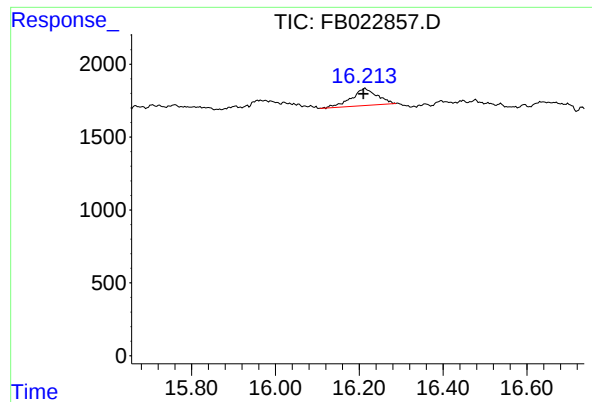

#10 1,2,4-Trimethylbenzene

R.T.: 16.214 min
Delta R.T.: 0.005 min
Response: 4906
Conc: 0.17 ng/ml