

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB103019\
 Data File : FB022852.D
 Signal(s) : FID2B.CH
 Acq On : 30 Oct 2019 14:00
 Operator : DD/AJ
 Sample : BSF1030S1
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Oct 31 00:54:41 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101619.M
 Quant Title :
 QLast Update : Wed Oct 16 15:04:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.797	550977	21.774 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.688	1040587	30.619 ng/ml
2) t	2,2,4-Trimethylpentane	7.416	1173817	32.259 ng/ml
3) t	n-Heptane	7.756	381074	10.444 ng/ml
4) t	Benzene	7.890	458662	10.388 ng/ml
6) t	Toluene	10.628	1327801	30.807 ng/ml
7) t	Ethylbenzene	13.069	419940	10.339 ng/ml
8) t	m-Xylene	13.202	791638	20.575 ng/ml
9) t	O-Xylene	13.929	753716	20.694 ng/ml
10) t	1,2,4-Trimethylbenzene	16.208	590724	20.730 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB103019\
Data File : FB022852.D
Signal(s) : FID2B.CH
Acq On : 30 Oct 2019 14:00
Operator : DD/AJ
Sample : BSF1030S1
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 31 00:54:41 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101619.M
Quant Title :
QLast Update : Wed Oct 16 15:04:00 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

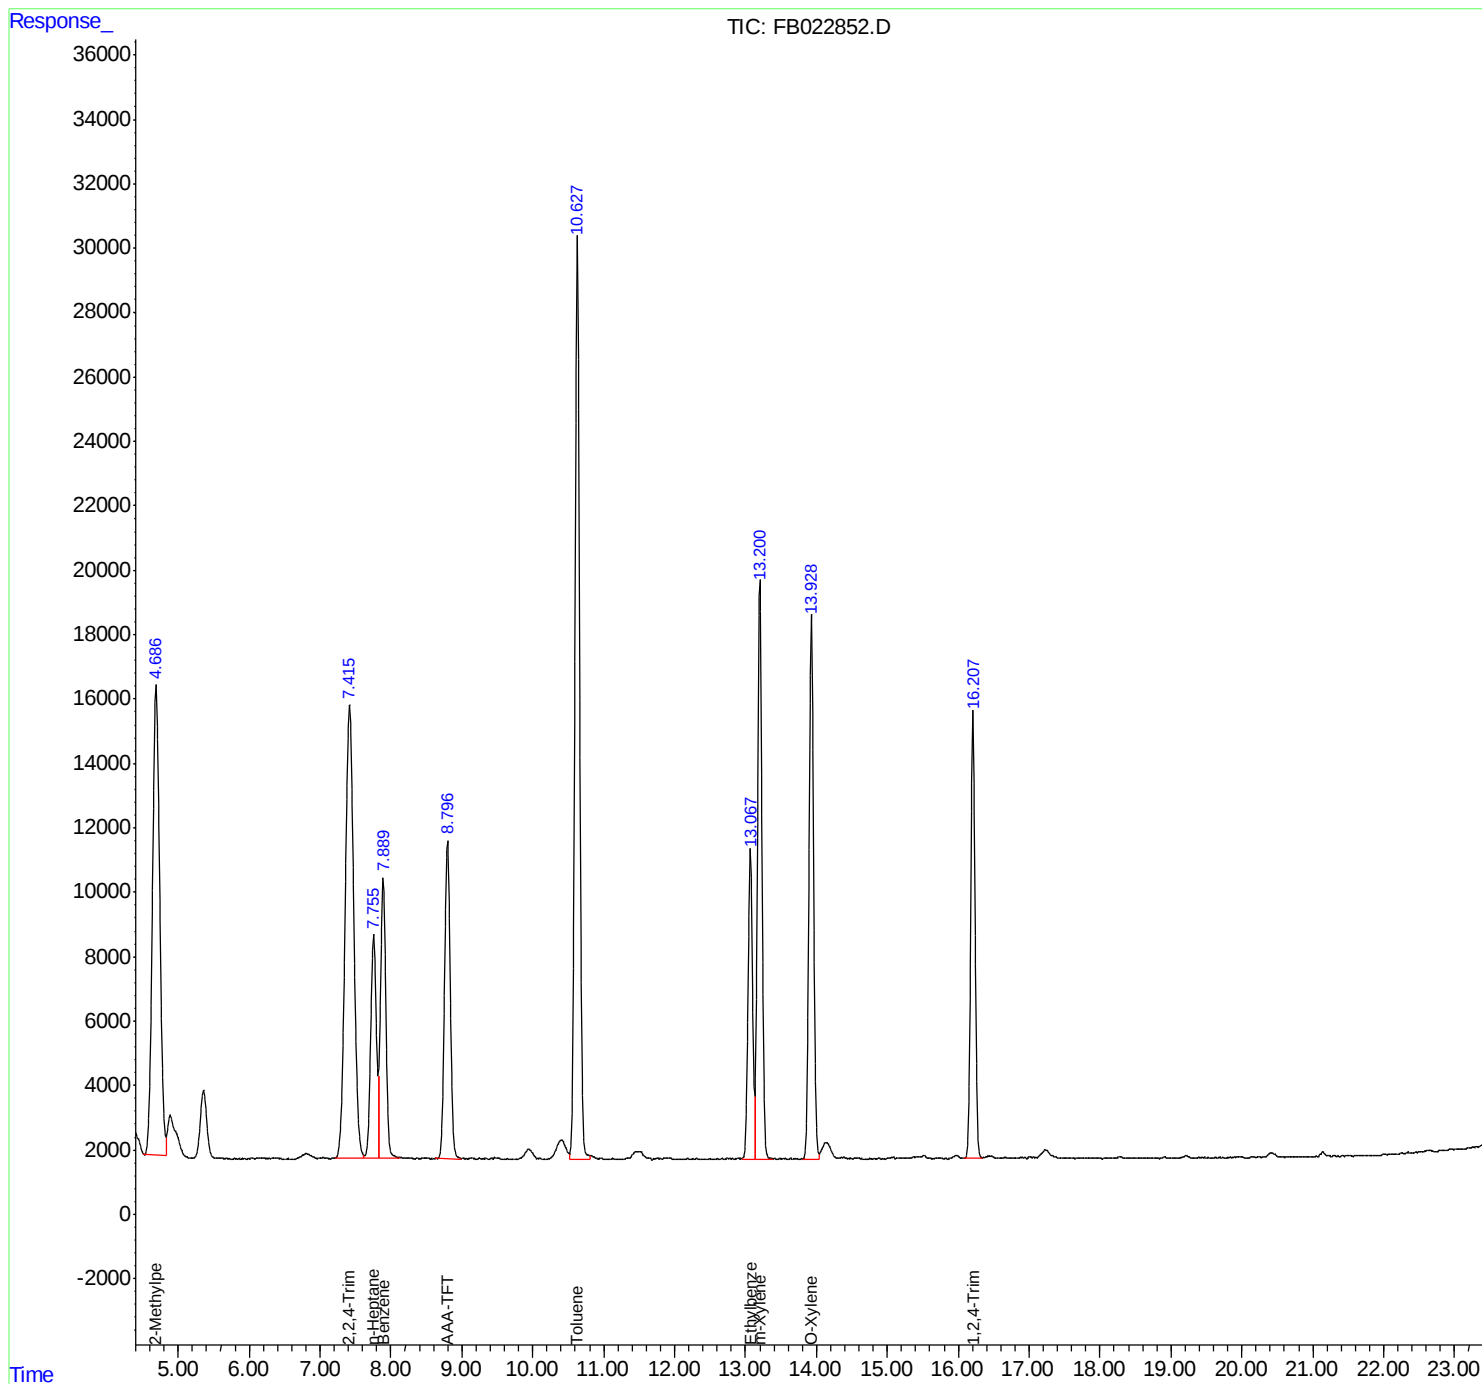

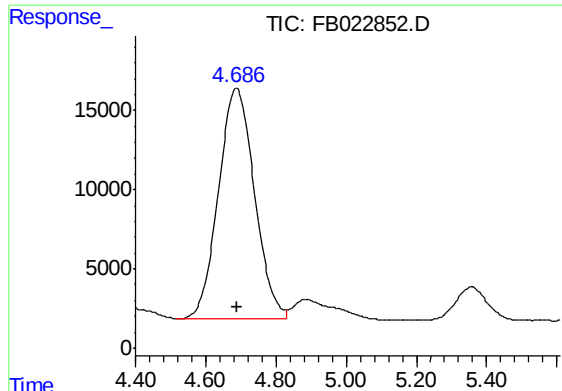


#1 2-Methylpentane

R.T.: 4.688 min
Delta R.T.: -0.002 min
Response: 1040587
Conc: 30.62 ng/ml

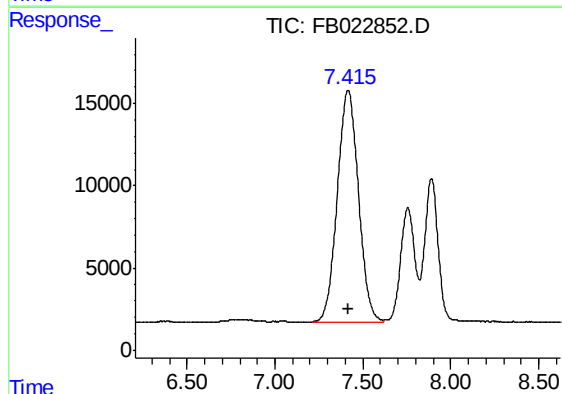


#2 2,2,4-Trimethylpentane

R.T.: 7.416 min
Delta R.T.: -0.001 min
Response: 1173817
Conc: 32.26 ng/ml

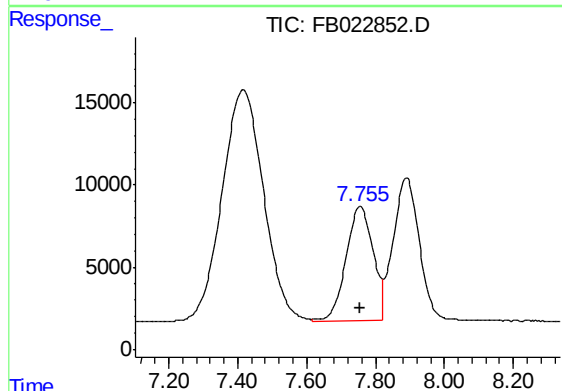


#3 n-Heptane

R.T.: 7.756 min
Delta R.T.: -0.001 min
Response: 381074
Conc: 10.44 ng/ml

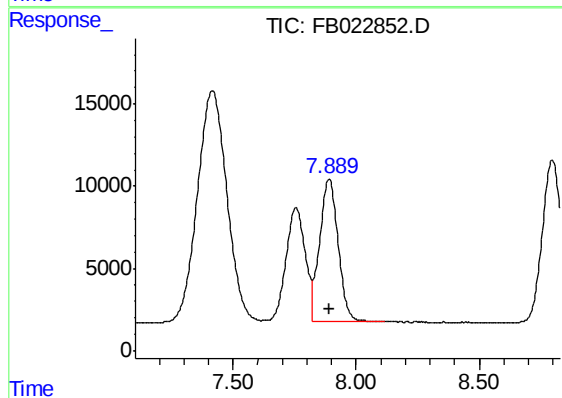


#4 Benzene

R.T.: 7.890 min
Delta R.T.: -0.001 min
Response: 458662
Conc: 10.39 ng/ml

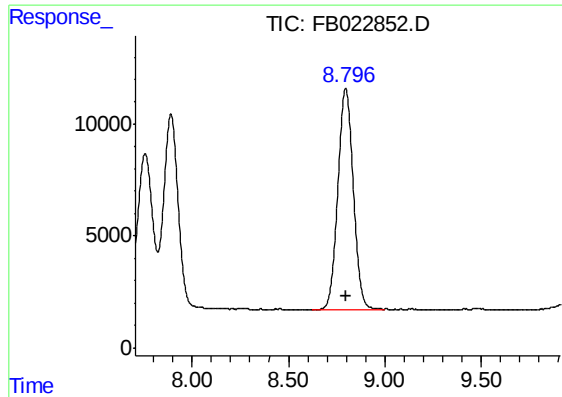


#5 AAA-TFT

R.T.: 8.797 min
Delta R.T.: -0.001 min
Response: 550977
Conc: 21.77 ng/ml

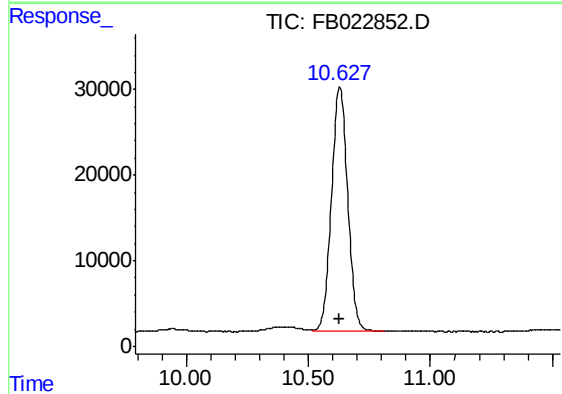


#6 Toluene

R.T.: 10.628 min
Delta R.T.: -0.001 min
Response: 1327801
Conc: 30.81 ng/ml

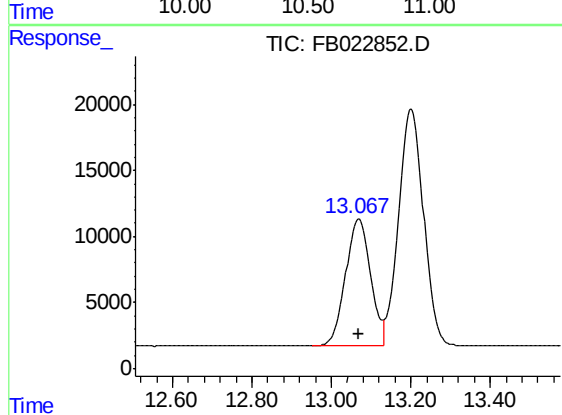


#7 Ethylbenzene

R.T.: 13.069 min
Delta R.T.: -0.001 min
Response: 419940
Conc: 10.34 ng/ml

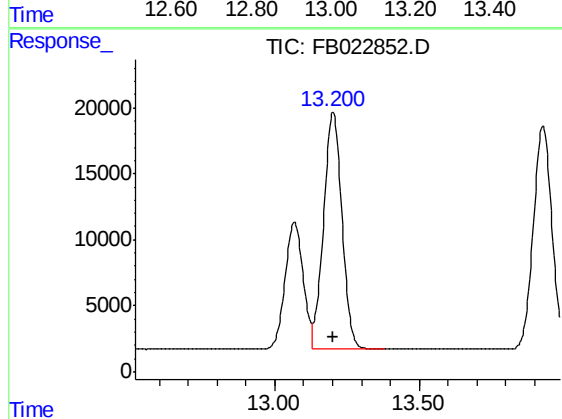


#8 m-Xylene

R.T.: 13.202 min
Delta R.T.: -0.001 min
Response: 791638
Conc: 20.57 ng/ml

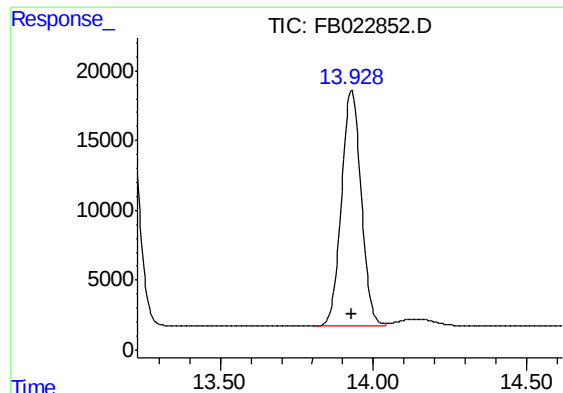

#9 O-Xylene

R.T.: 13.929 min
Delta R.T.: -0.001 min
Response: 753716
Conc: 20.69 ng/ml

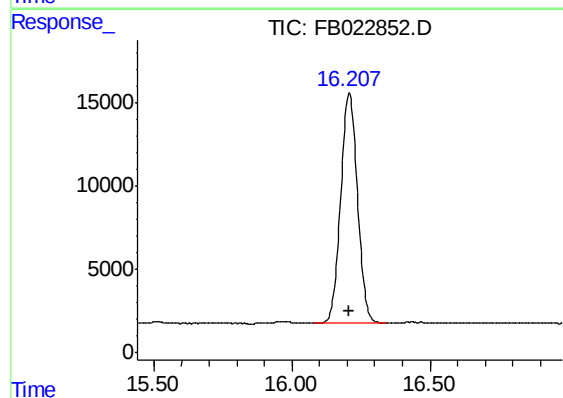

#10 1,2,4-Trimethylbenzene

R.T.: 16.208 min
Delta R.T.: -0.002 min
Response: 590724
Conc: 20.73 ng/ml