

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB103019\
 Data File : FB022855.D
 Signal(s) : FID2B.CH
 Acq On : 30 Oct 2019 15:30
 Operator : DD/AJ
 Sample : K5148-14MSD
 Misc : 5.06g/5.00ml DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Oct 31 00:55:13 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101619.M
 Quant Title :
 QLast Update : Wed Oct 16 15:04:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.797	521603	20.613 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.690	754157	22.191 ng/ml
2) t 2,2,4-Trimethylpentane	7.417	753809	20.716 ng/ml
3) t n-Heptane	7.757	243582	6.676 ng/ml
4) t Benzene	7.891	384500	8.709 ng/ml
6) t Toluene	10.629	2487403	57.712 ng/ml
7) t Ethylbenzene	13.069	489498	12.052 ng/ml
8) t m-Xylene	13.201	1198834	31.158 ng/ml
9) t O-Xylene	13.930	765805	21.026 ng/ml
10) t 1,2,4-Trimethylbenzene	16.209	466279	16.363 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB103019\
Data File : FB022855.D
Signal(s) : FID2B.CH
Acq On : 30 Oct 2019 15:30
Operator : DD/AJ
Sample : K5148-14MSD
Misc : 5.06g/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 31 00:55:13 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101619.M
Quant Title :
QLast Update : Wed Oct 16 15:04:00 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

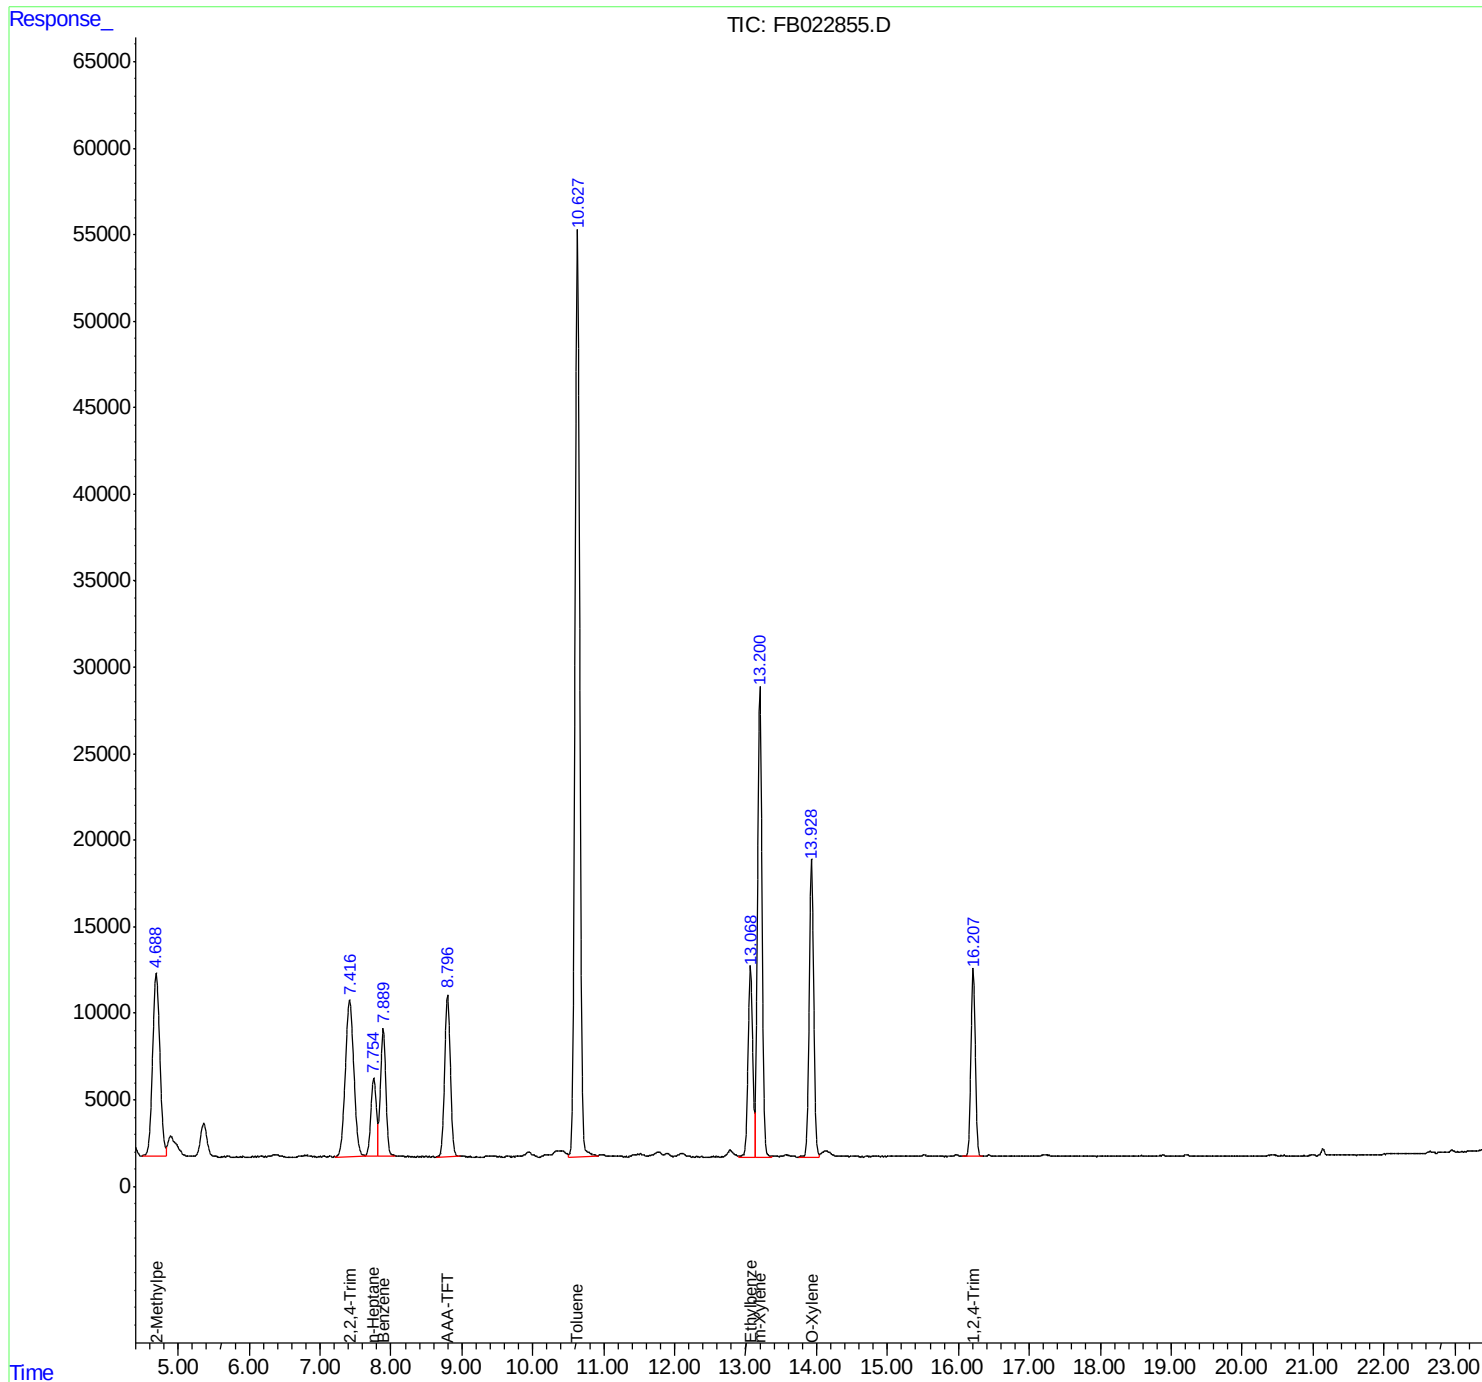

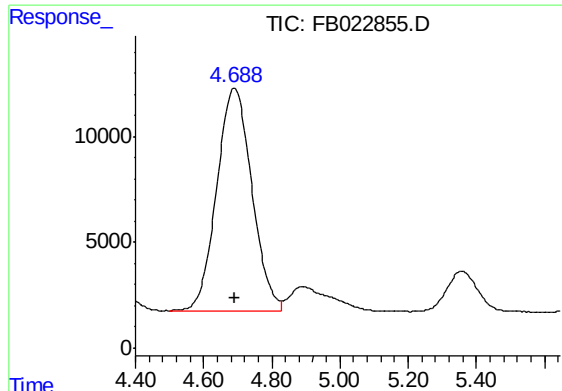


#1 2-Methylpentane

R.T.: 4.690 min
Delta R.T.: 0.000 min
Response: 754157
Conc: 22.19 ng/ml

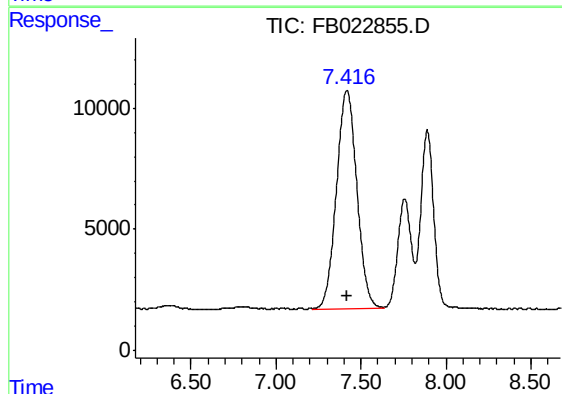


#2 2,2,4-Trimethylpentane

R.T.: 7.417 min
Delta R.T.: 0.000 min
Response: 753809
Conc: 20.72 ng/ml

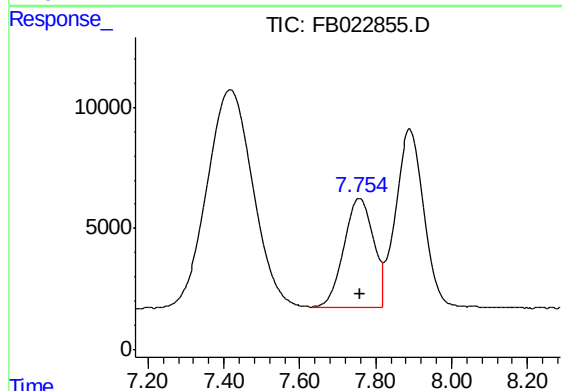


#3 n-Heptane

R.T.: 7.757 min
Delta R.T.: 0.000 min
Response: 243582
Conc: 6.68 ng/ml

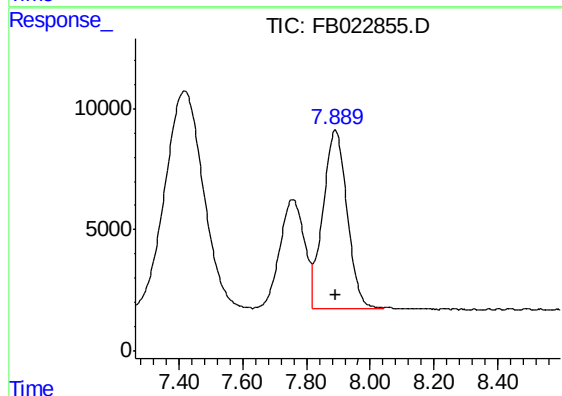


#4 Benzene

R.T.: 7.891 min
Delta R.T.: 0.000 min
Response: 384500
Conc: 8.71 ng/ml

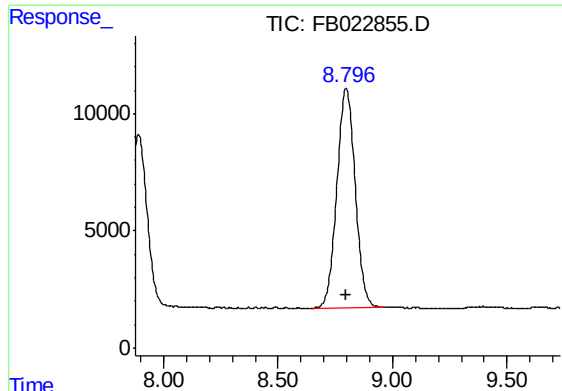


#5 AAA-TFT

R.T.: 8.797 min
Delta R.T.: 0.000 min
Response: 521603
Conc: 20.61 ng/ml

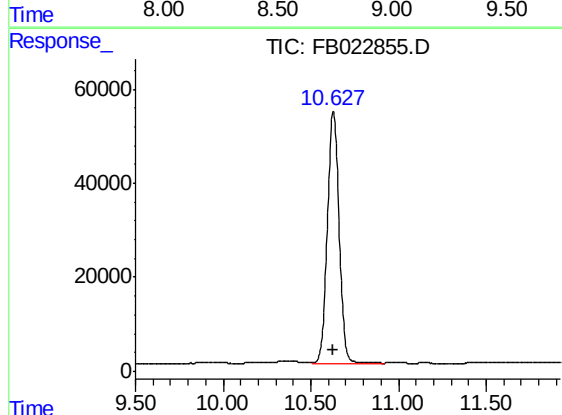


#6 Toluene

R.T.: 10.629 min
Delta R.T.: 0.000 min
Response: 2487403
Conc: 57.71 ng/ml

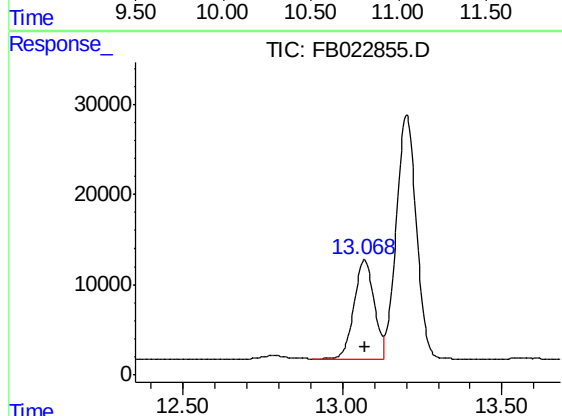


#7 Ethylbenzene

R.T.: 13.069 min
Delta R.T.: 0.000 min
Response: 489498
Conc: 12.05 ng/ml

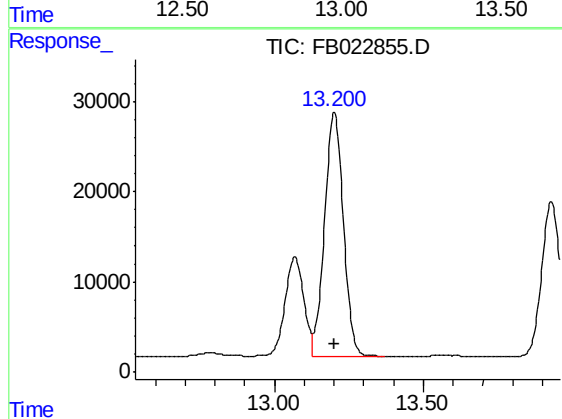


#8 m-Xylene

R.T.: 13.201 min
Delta R.T.: -0.002 min
Response: 1198834
Conc: 31.16 ng/ml

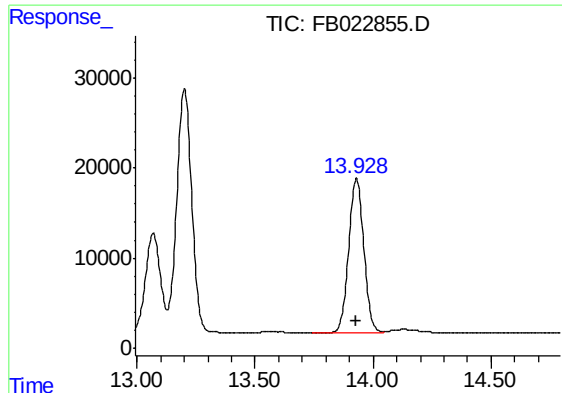

#9 O-Xylene

R.T.: 13.930 min
Delta R.T.: 0.000 min
Response: 765805
Conc: 21.03 ng/ml

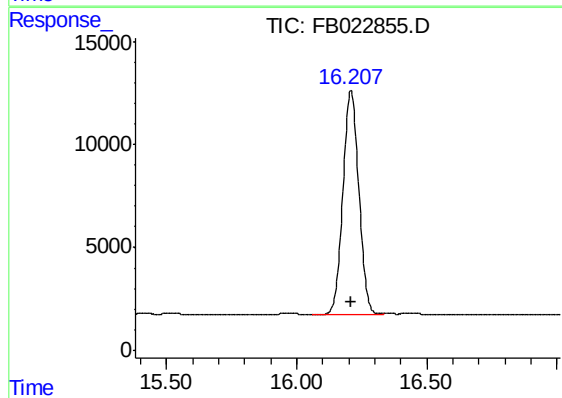

#10 1,2,4-Trimethylbenzene

R.T.: 16.209 min
Delta R.T.: 0.000 min
Response: 466279
Conc: 16.36 ng/ml