

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB103020\
 Data File : FB025168.D
 Signal(s) : FID2B.CH
 Acq On : 30 Oct 2020 10:12
 Operator : DD/AJ
 Sample : BSF1030S1
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Oct 31 00:19:33 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101920.M
 Quant Title :
 QLast Update : Mon Oct 19 13:01:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.799	461044	21.597 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.688	946635	31.124 ng/ml
2) t 2,2,4-Trimethylpentane	7.417	1004302	32.239 ng/ml
3) t n-Heptane	7.758	330322	10.744 ng/ml
4) t Benzene	7.893	392397	10.441 ng/ml
6) t Toluene	10.632	1113077	31.232 ng/ml
7) t Ethylbenzene	13.072	346711	10.651 ng/ml
8) t m-Xylene	13.205	687966	21.451 ng/ml
9) t O-Xylene	13.933	666328	21.615 ng/ml
10) t 1,2,4-Trimethylbenzene	16.211	560799	21.479 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB103020\
Data File : FB025168.D
Signal(s) : FID2B.CH
Acq On : 30 Oct 2020 10:12
Operator : DD/AJ
Sample : BSF1030S1
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 31 00:19:33 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101920.M
Quant Title :
QLast Update : Mon Oct 19 13:01:11 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

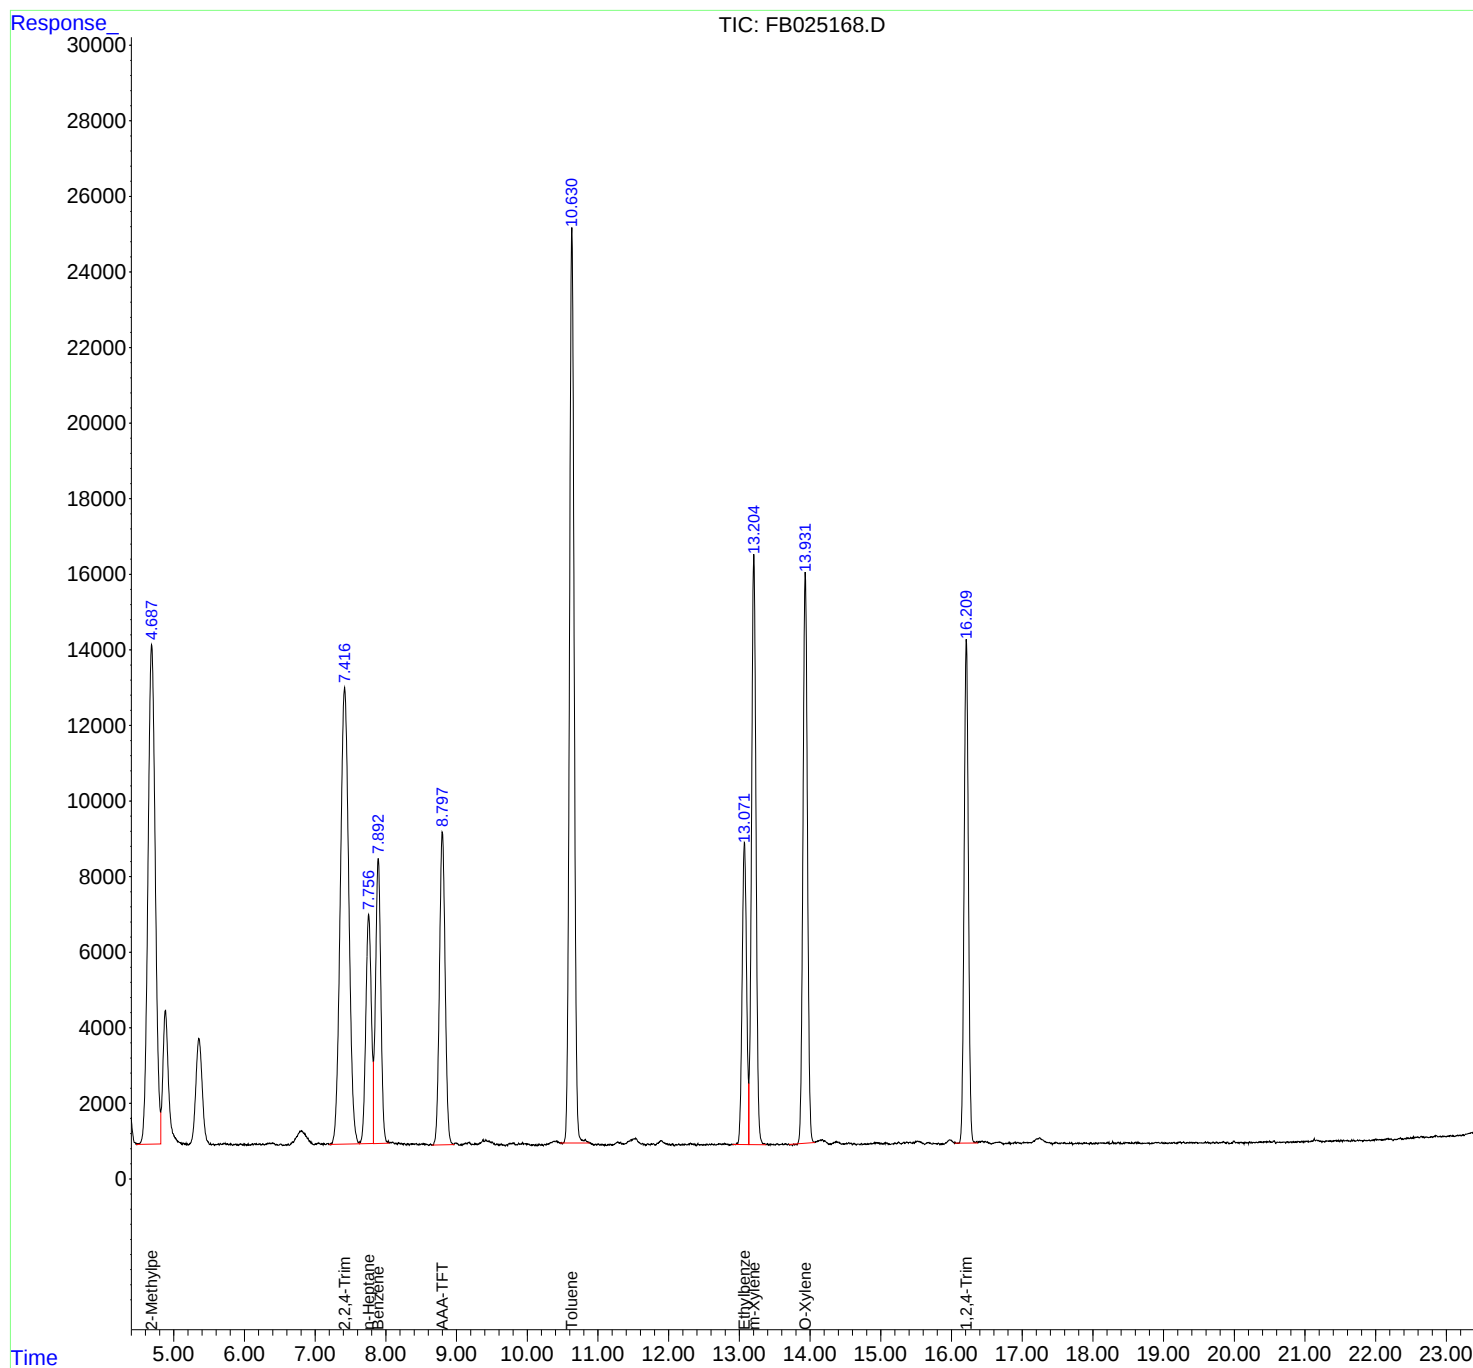

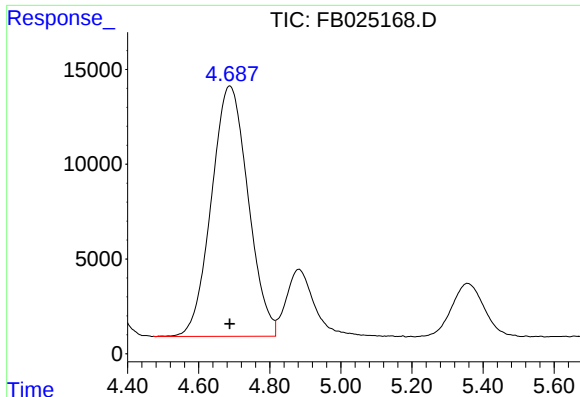


#1 2-Methylpentane

R.T.: 4.688 min
Delta R.T.: 0.000 min
Response: 946635
Conc: 31.12 ng/ml

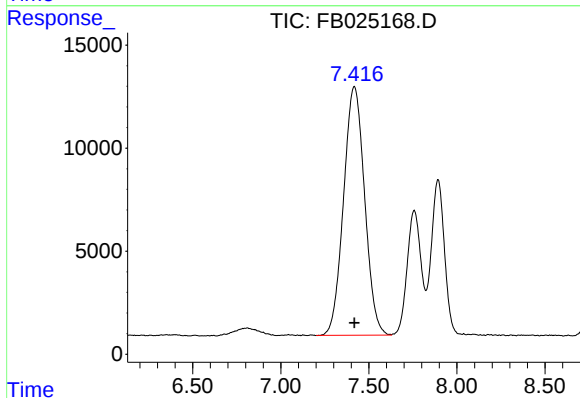


#2 2,2,4-Trimethylpentane

R.T.: 7.417 min
Delta R.T.: 0.000 min
Response: 1004302
Conc: 32.24 ng/ml

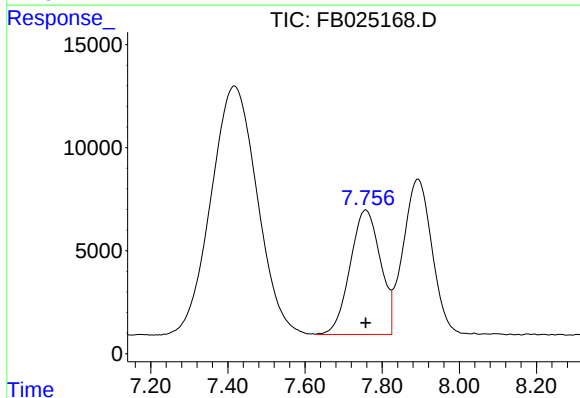


#3 n-Heptane

R.T.: 7.758 min
Delta R.T.: 0.000 min
Response: 330322
Conc: 10.74 ng/ml

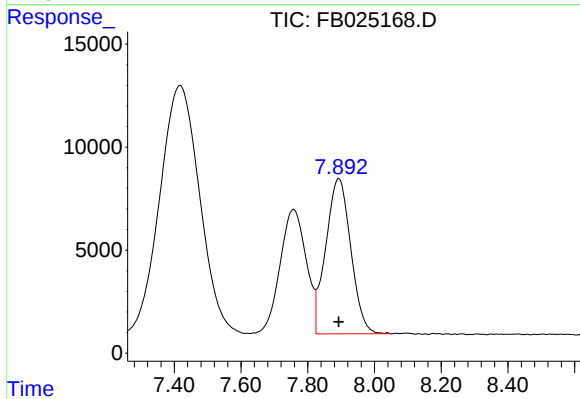


#4 Benzene

R.T.: 7.893 min
Delta R.T.: 0.000 min
Response: 392397
Conc: 10.44 ng/ml

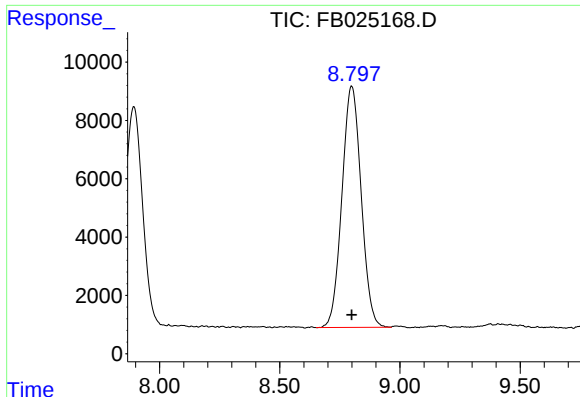


#5 AAA-TFT

R.T.: 8.799 min
Delta R.T.: 0.000 min
Response: 461044
Conc: 21.60 ng/ml

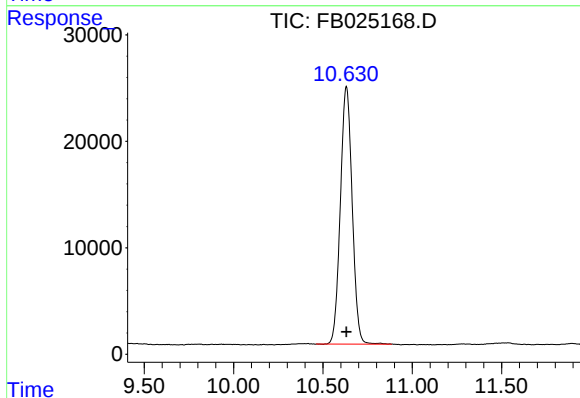


#6 Toluene

R.T.: 10.632 min
Delta R.T.: 0.000 min
Response: 1113077
Conc: 31.23 ng/ml

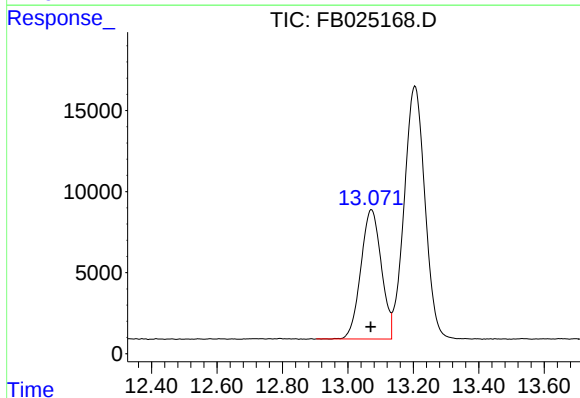


#7 Ethylbenzene

R.T.: 13.072 min
Delta R.T.: 0.002 min
Response: 346711
Conc: 10.65 ng/ml

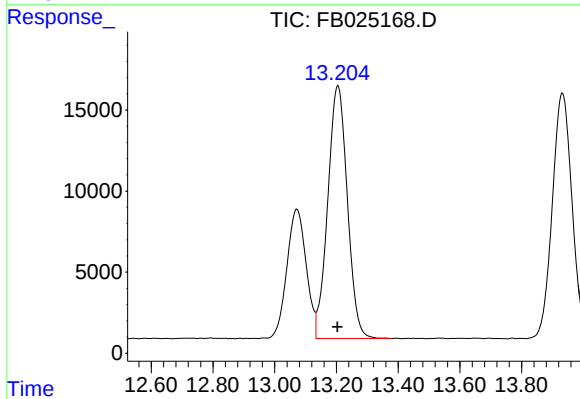


#8 m-Xylene

R.T.: 13.205 min
Delta R.T.: 0.002 min
Response: 687966
Conc: 21.45 ng/ml

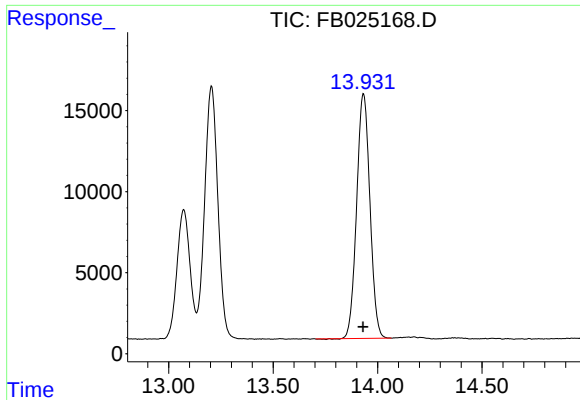

#9 O-Xylene

R.T.: 13.933 min
Delta R.T.: 0.002 min
Response: 666328
Conc: 21.62 ng/ml

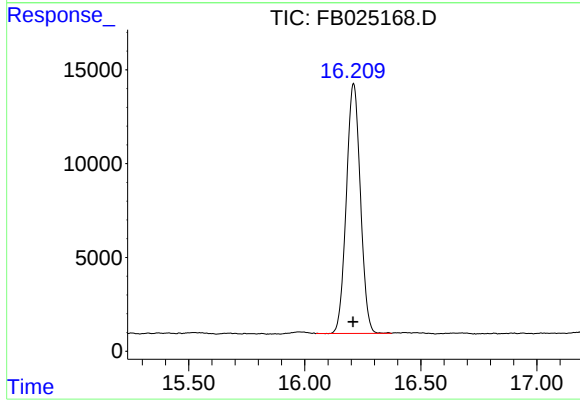

#10 1,2,4-Trimethylbenzene

R.T.: 16.211 min
Delta R.T.: 0.002 min
Response: 560799
Conc: 21.48 ng/ml