

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB103020\
 Data File : FB025171.D
 Signal(s) : FID2B.CH
 Acq On : 30 Oct 2020 12:04
 Operator : DD/AJ
 Sample : L4222-07MSD
 Misc : 5.05g/5.00ml DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Oct 31 00:19:52 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101920.M
 Quant Title :
 QLast Update : Mon Oct 19 13:01:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.799	418479	19.603 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.688	807654	26.555 ng/ml
2) t 2,2,4-Trimethylpentane	7.418	745808	23.941 ng/ml
3) t n-Heptane	7.758	232268	7.554 ng/ml
4) t Benzene	7.893	385617	10.260 ng/ml
6) t Toluene	10.631	1058978	29.714 ng/ml
7) t Ethylbenzene	13.071	313414	9.628 ng/ml
8) t m-Xylene	13.204	617592	19.257 ng/ml
9) t O-Xylene	13.932	608365	19.735 ng/ml
10) t 1,2,4-Trimethylbenzene	16.210	484179	18.545 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB103020\
Data File : FB025171.D
Signal(s) : FID2B.CH
Acq On : 30 Oct 2020 12:04
Operator : DD/AJ
Sample : L4222-07MSD
Misc : 5.05g/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 31 00:19:52 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101920.M
Quant Title :
QLast Update : Mon Oct 19 13:01:11 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

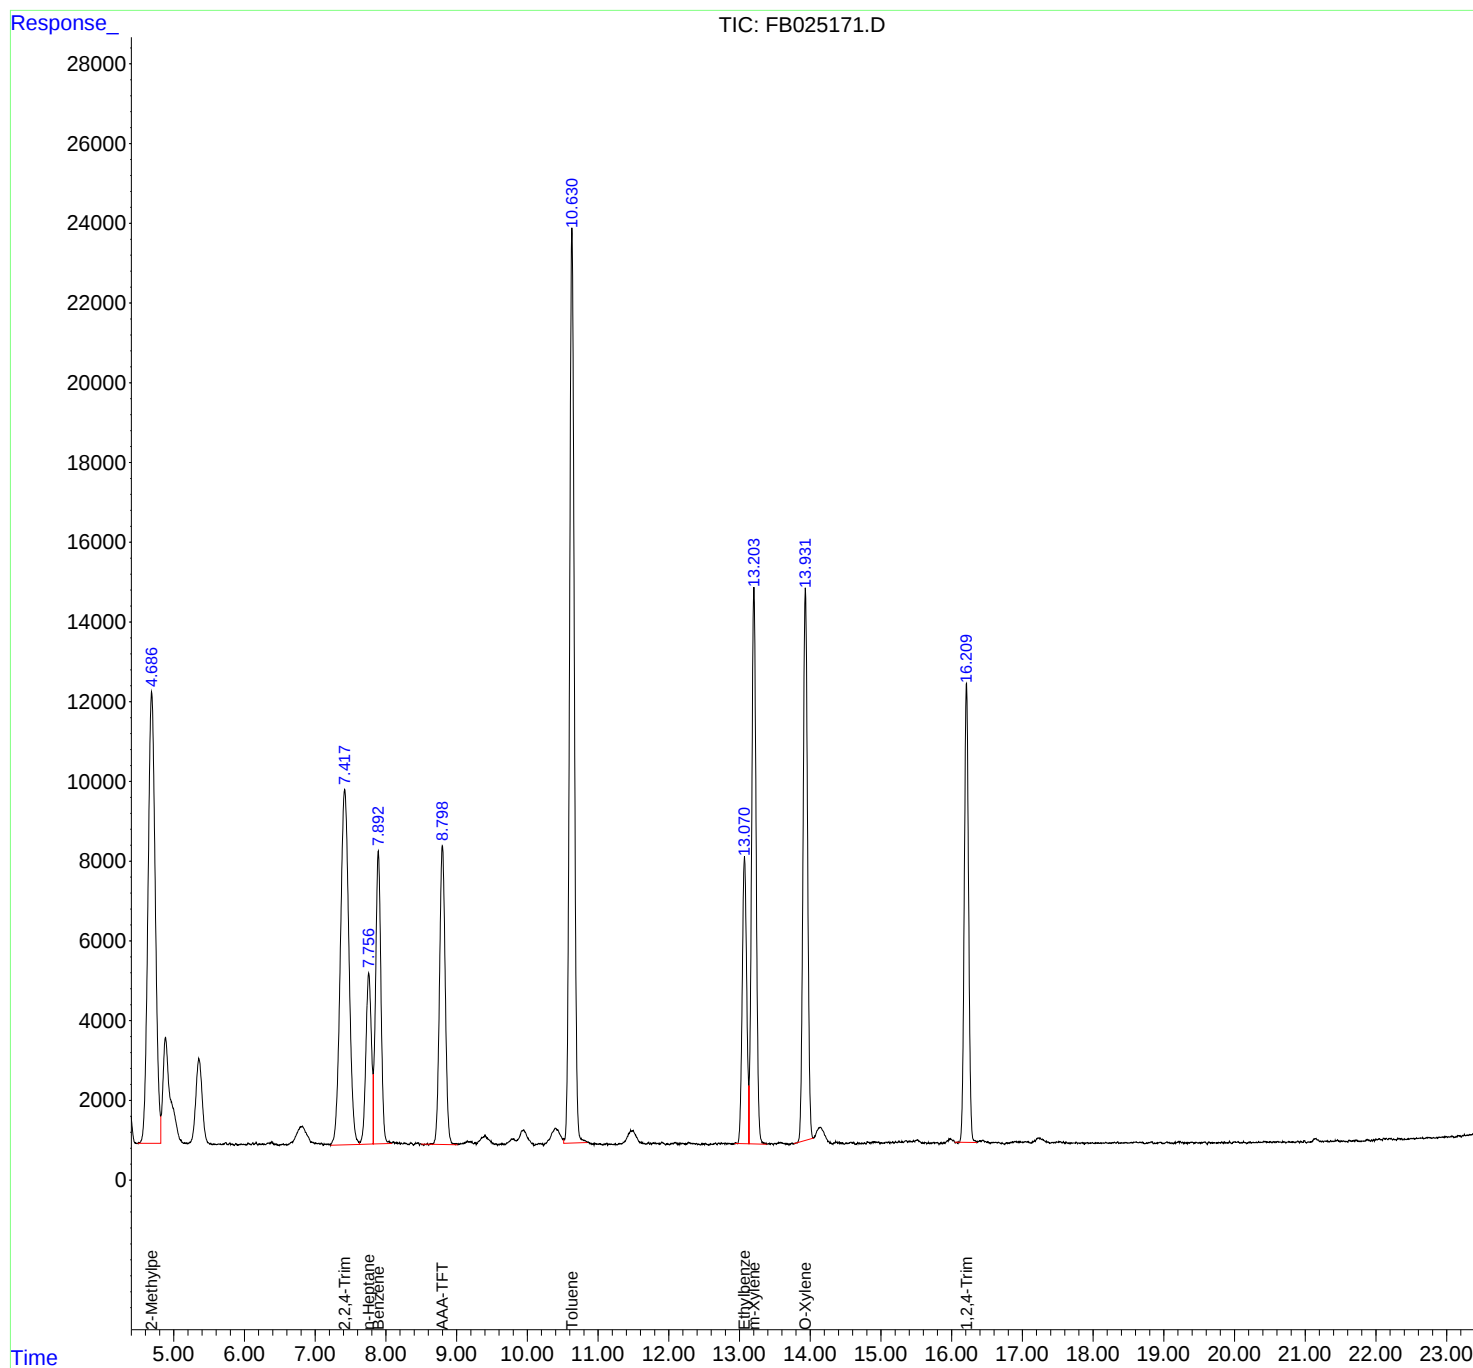

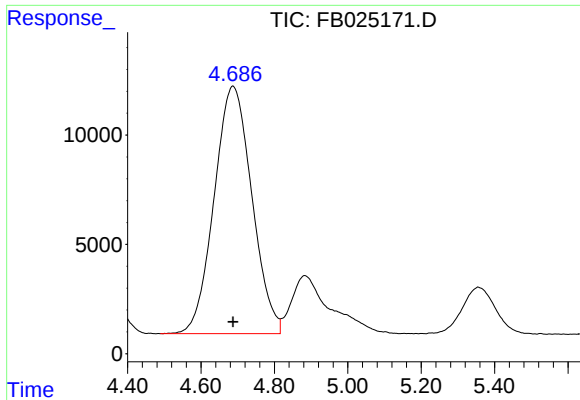


#1 2-Methylpentane

R.T.: 4.688 min
Delta R.T.: 0.000 min
Response: 807654
Conc: 26.55 ng/ml

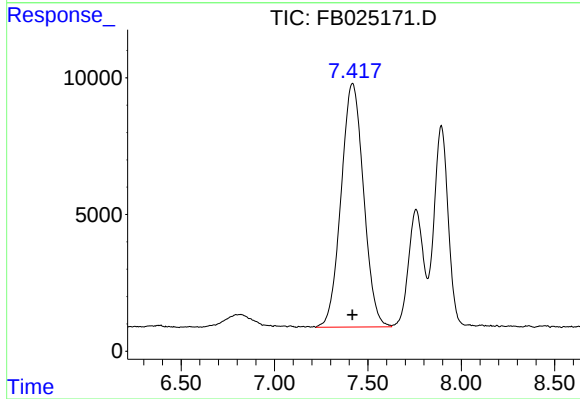


#2 2,2,4-Trimethylpentane

R.T.: 7.418 min
Delta R.T.: 0.000 min
Response: 745808
Conc: 23.94 ng/ml

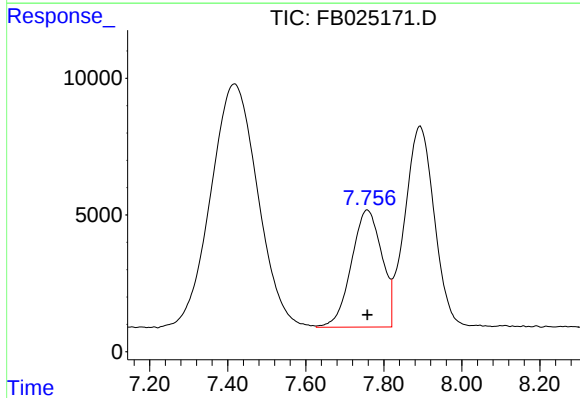


#3 n-Heptane

R.T.: 7.758 min
Delta R.T.: 0.000 min
Response: 232268
Conc: 7.55 ng/ml

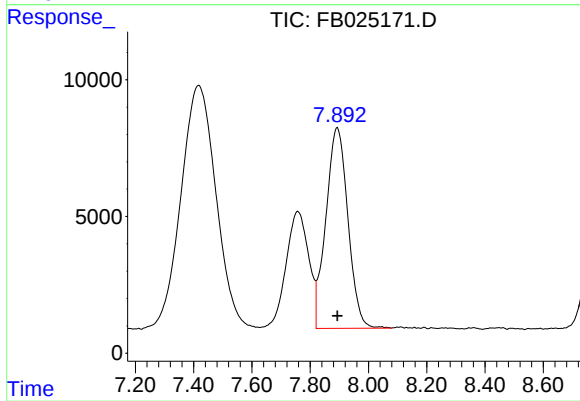


#4 Benzene

R.T.: 7.893 min
Delta R.T.: 0.000 min
Response: 385617
Conc: 10.26 ng/ml

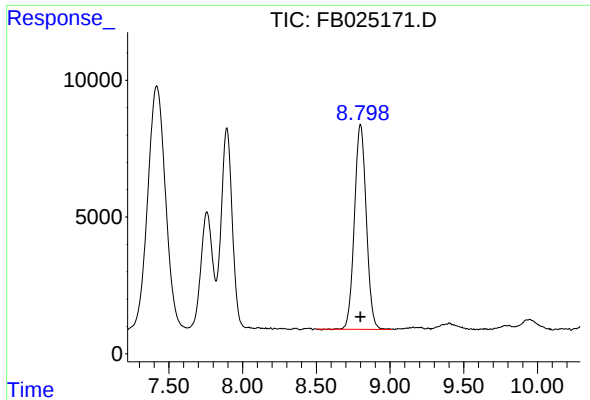


#5 AAA-TFT

R.T.: 8.799 min
Delta R.T.: 0.000 min
Response: 418479
Conc: 19.60 ng/ml

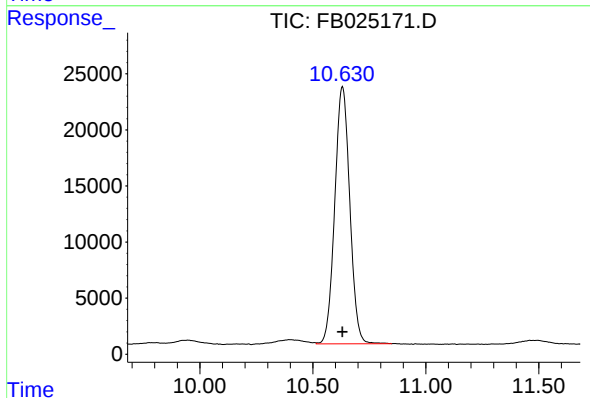


#6 Toluene

R.T.: 10.631 min
Delta R.T.: 0.000 min
Response: 1058978
Conc: 29.71 ng/ml

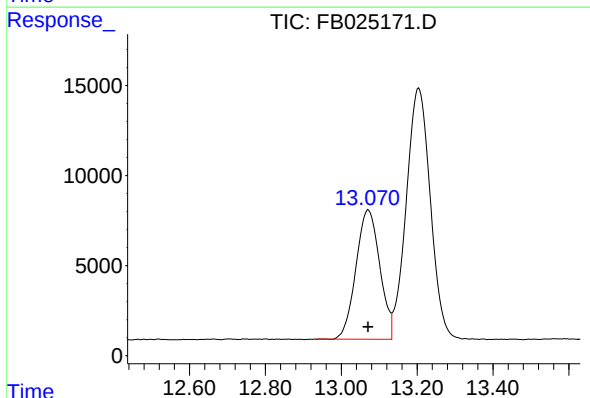


#7 Ethylbenzene

R.T.: 13.071 min
Delta R.T.: 0.000 min
Response: 313414
Conc: 9.63 ng/ml

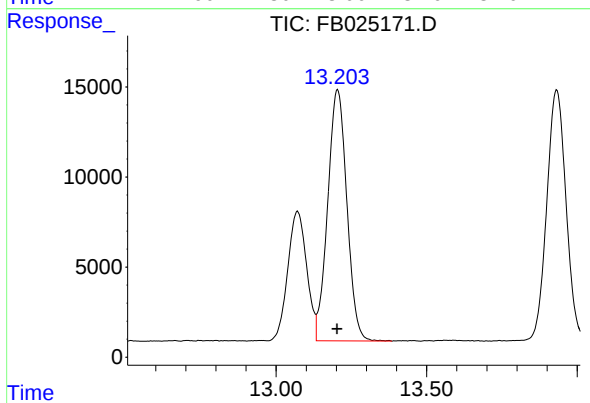


#8 m-Xylene

R.T.: 13.204 min
Delta R.T.: 0.001 min
Response: 617592
Conc: 19.26 ng/ml

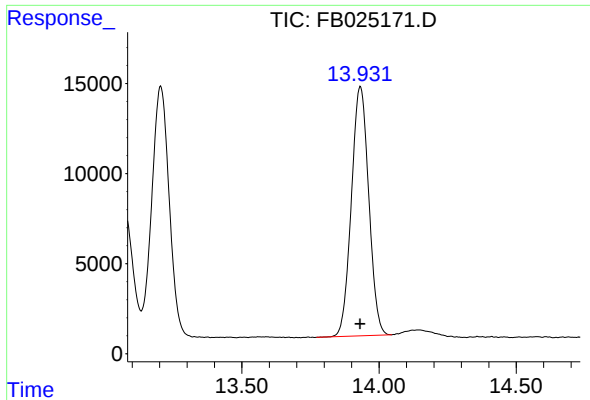

#9 O-Xylene

R.T.: 13.932 min
Delta R.T.: 0.001 min
Response: 608365
Conc: 19.73 ng/ml

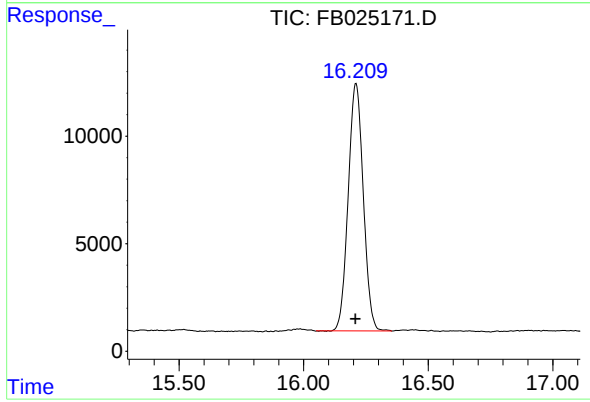

#10 1,2,4-Trimethylbenzene

R.T.: 16.210 min
Delta R.T.: 0.002 min
Response: 484179
Conc: 18.54 ng/ml