

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB103024\
 Data File : FB031093.D
 Signal(s) : FID2B.CH
 Acq On : 30 Oct 2024 13:03
 Operator : YP/AJ
 Sample : BSF1030S2
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1030S2

Integration File: Calibration.e
 Quant Time: Nov 01 03:45:19 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102824.M
 Quant Title :
 QLast Update : Mon Oct 28 12:19:57 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.793	499449	18.094 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.721	1345373	34.256 ng/ml
2) t 2,2,4-Trimethylpentane	7.426	1583249	33.804 ng/ml
3) t n-Heptane	7.754	508506	11.220 ng/ml
4) t Benzene	7.893	608606	11.385 ng/ml
6) t Toluene	10.621	1661273	33.268 ng/ml
7) t Ethylbenzene	13.058	482135	10.771 ng/ml
8) t m-Xylene	13.192	1038410	21.350 ng/ml
9) t O-Xylene	13.919	966793	21.210 ng/ml
10) t 1,2,4-Trimethylbenzene	16.195	739903	19.885 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB103024\
Data File : FB031093.D
Signal(s) : FID2B.CH
Acq On : 30 Oct 2024 13:03
Operator : YP/AJ
Sample : BSF1030S2
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1030S2

Integration File: Calibration.e
Quant Time: Nov 01 03:45:19 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102824.M
Quant Title :
QLast Update : Mon Oct 28 12:19:57 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

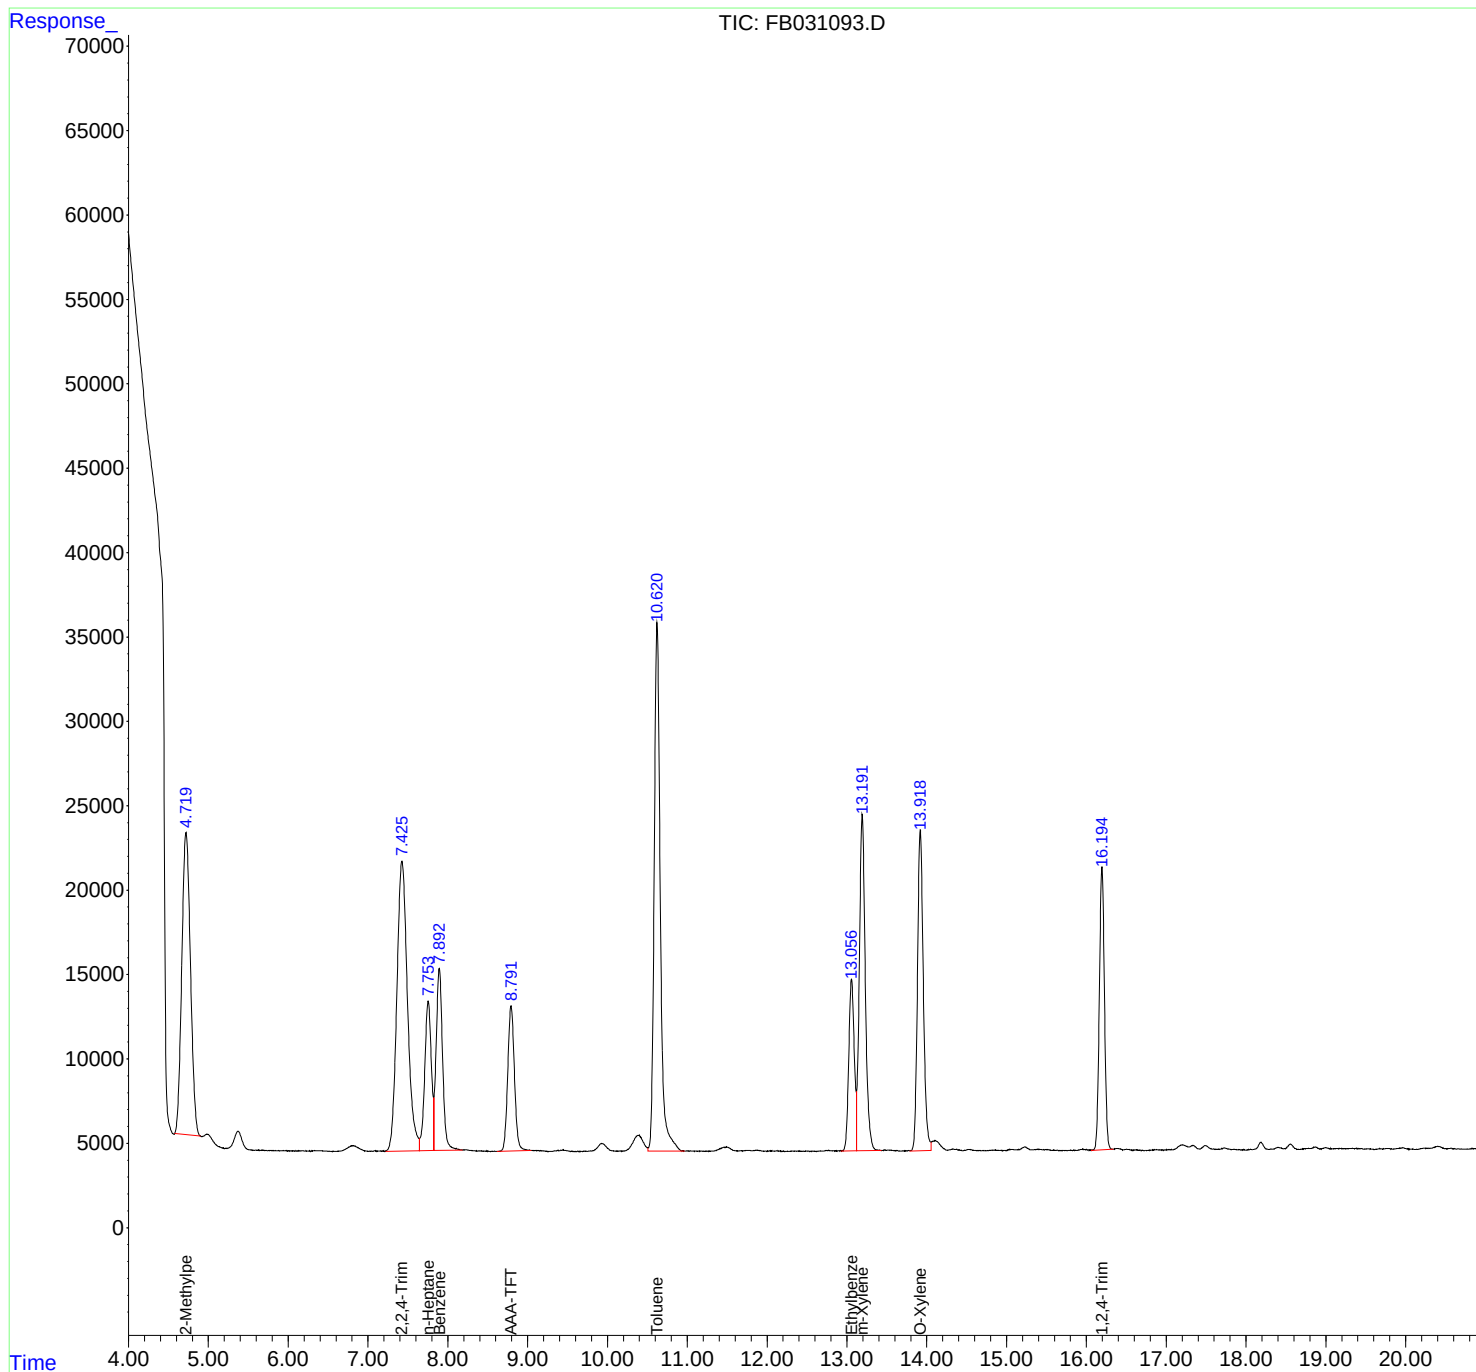


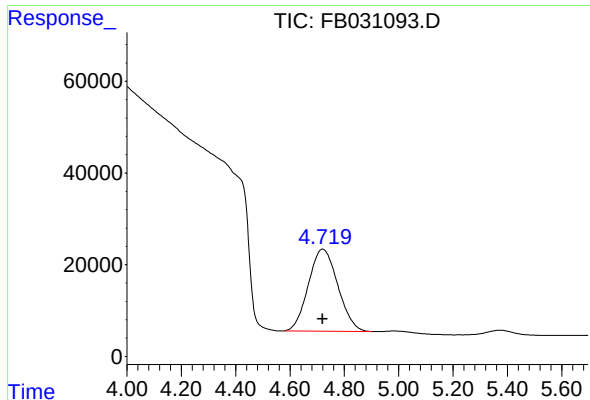

#1 2-Methylpentane


R.T.: 4.721 min
Delta R.T.: 0.000 min
Response: 1345373
Conc: 34.26 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1030S2

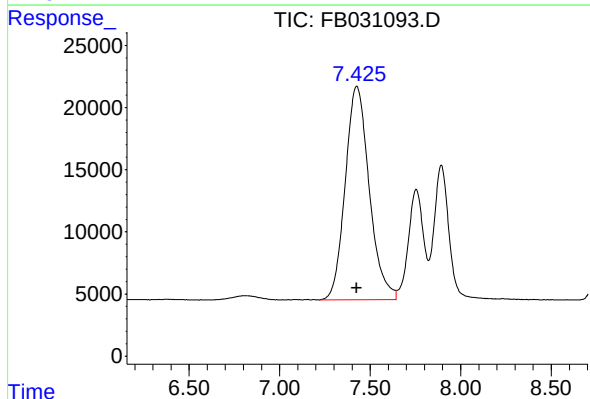


#2 2,2,4-Trimethylpentane

R.T.: 7.426 min
Delta R.T.: 0.001 min
Response: 1583249
Conc: 33.80 ng/ml

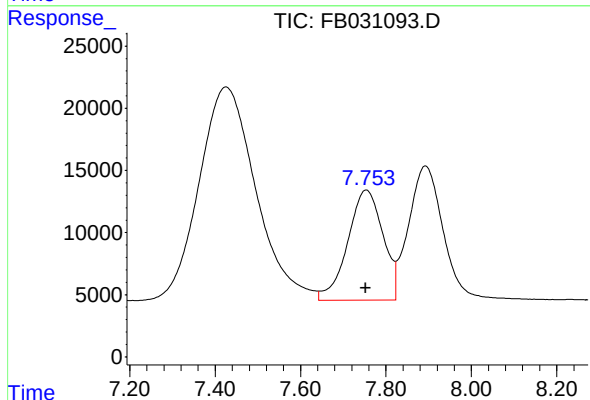


#3 n-Heptane

R.T.: 7.754 min
Delta R.T.: 0.002 min
Response: 508506
Conc: 11.22 ng/ml

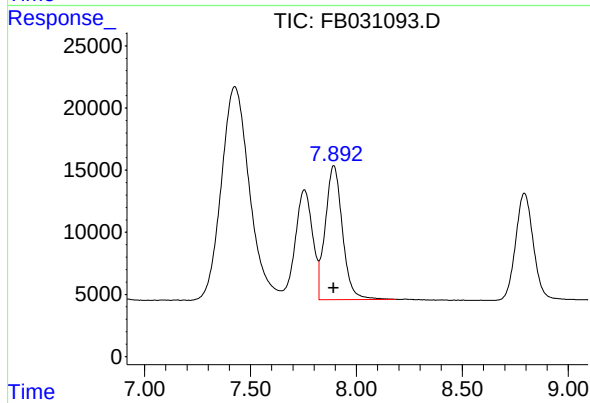

#4 Benzene


R.T.: 7.893 min
Delta R.T.: 0.002 min
Response: 608606
Conc: 11.39 ng/ml

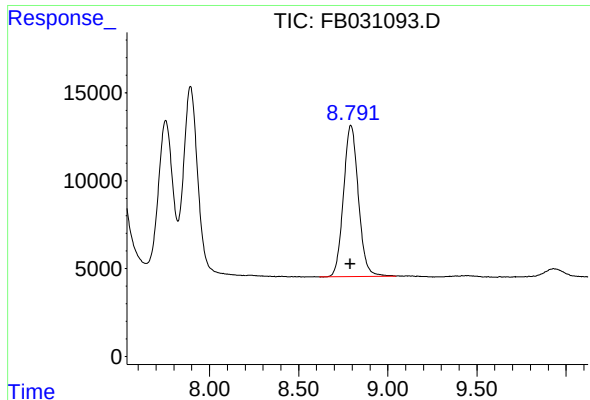

#5 AAA-TFT


R.T.: 8.793 min
Delta R.T.: 0.002 min
Response: 499449
Conc: 18.09 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1030S2

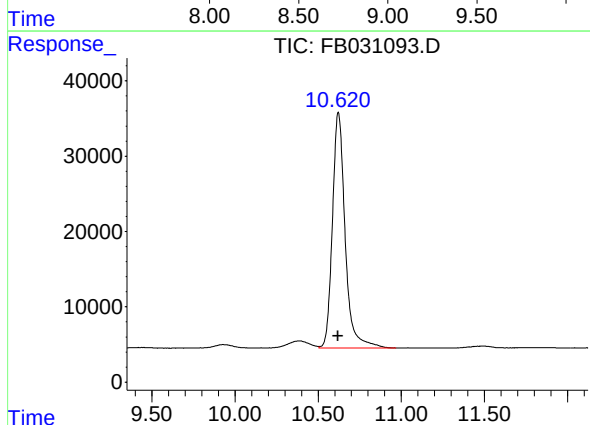


#6 Toluene

R.T.: 10.621 min
Delta R.T.: 0.002 min
Response: 1661273
Conc: 33.27 ng/ml

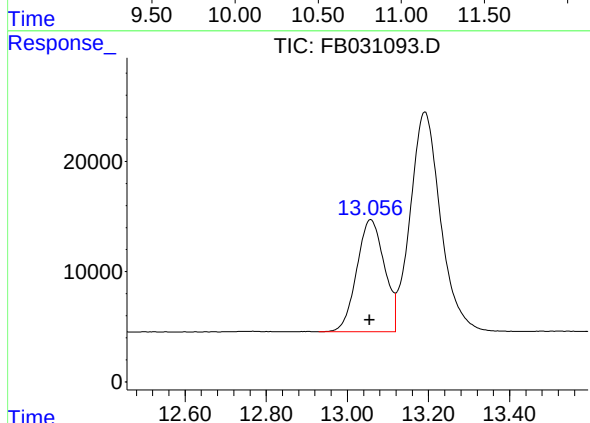


#7 Ethylbenzene

R.T.: 13.058 min
Delta R.T.: 0.003 min
Response: 482135
Conc: 10.77 ng/ml

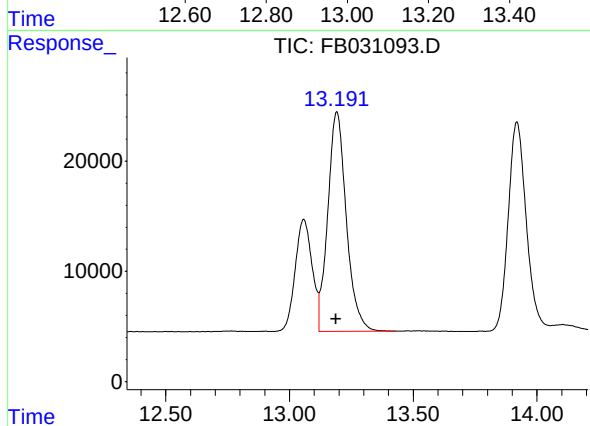

#8 m-Xylene


R.T.: 13.192 min
Delta R.T.: 0.004 min
Response: 1038410
Conc: 21.35 ng/ml

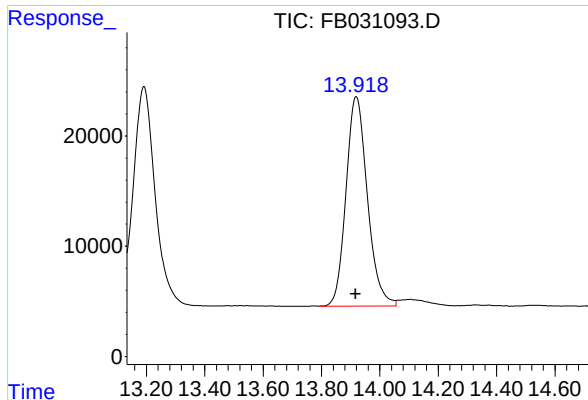

#9 O-Xylene

R.T.: 13.919 min
Delta R.T.: 0.003 min
Response: 966793
Conc: 21.21 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1030S2

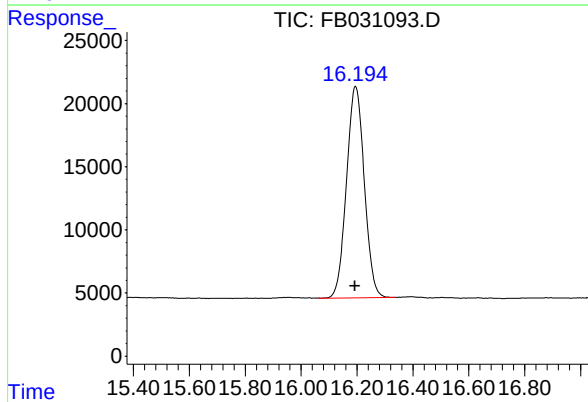

#10 1,2,4-Trimethylbenzene

R.T.: 16.195 min
Delta R.T.: 0.003 min
Response: 739903
Conc: 19.89 ng/ml