

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB103024\
 Data File : FB031102.D
 Signal(s) : FID2B.CH
 Acq On : 30 Oct 2024 17:18
 Operator : YP/AJ
 Sample : BSF1030S3
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1030S3

Integration File: Calibration.e
 Quant Time: Nov 01 03:46:29 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102824.M
 Quant Title :
 QLast Update : Mon Oct 28 12:19:57 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.794	567915	20.574 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.721	1271628	32.378 ng/ml
2) t 2,2,4-Trimethylpentane	7.428	1479527	31.589 ng/ml
3) t n-Heptane	7.754	493002	10.878 ng/ml
4) t Benzene	7.894	586426	10.970 ng/ml
6) t Toluene	10.623	1741213	34.868 ng/ml
7) t Ethylbenzene	13.060	525850	11.748 ng/ml
8) t m-Xylene	13.193	1258531	25.875 ng/ml
9) t O-Xylene	13.921	1053314	23.108 ng/ml
10) t 1,2,4-Trimethylbenzene	16.196	1106904	29.749 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB103024\
Data File : FB031102.D
Signal(s) : FID2B.CH
Acq On : 30 Oct 2024 17:18
Operator : YP/AJ
Sample : BSF1030S3
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1030S3

Integration File: Calibration.e
Quant Time: Nov 01 03:46:29 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102824.M
Quant Title :
QLast Update : Mon Oct 28 12:19:57 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

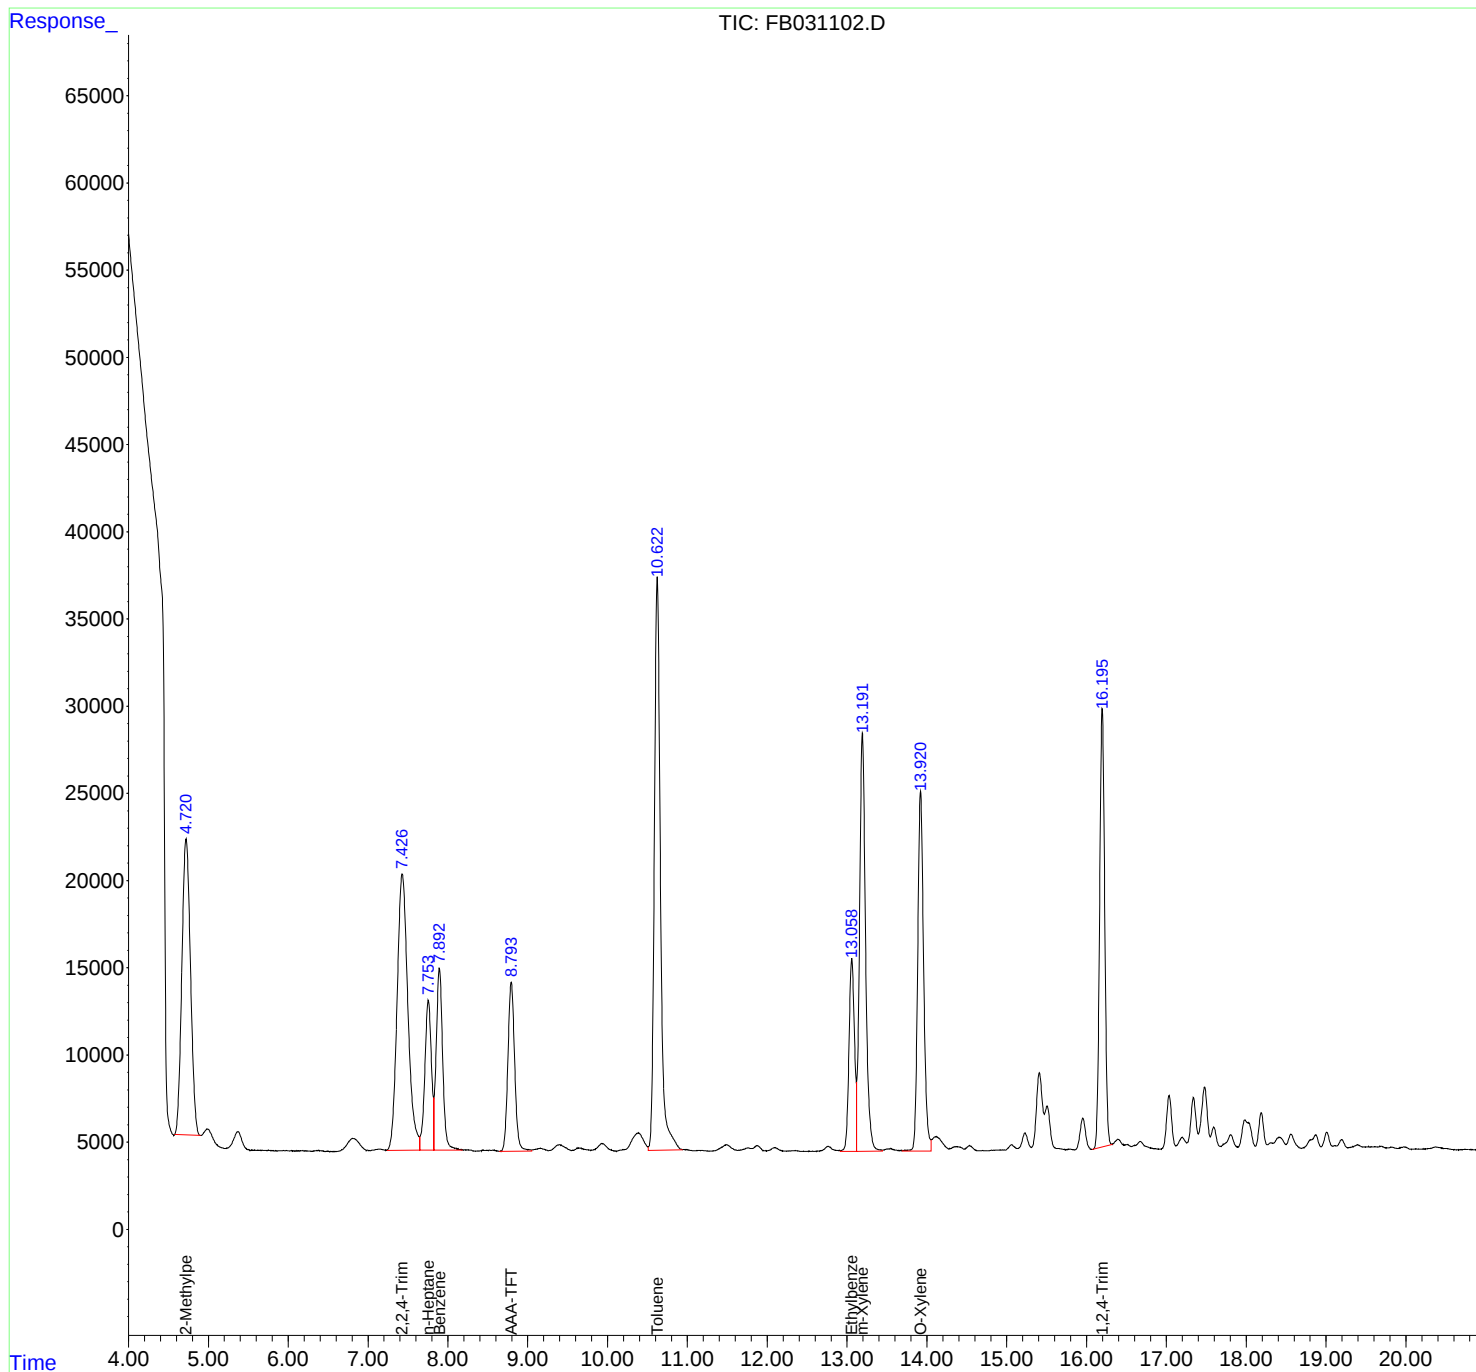


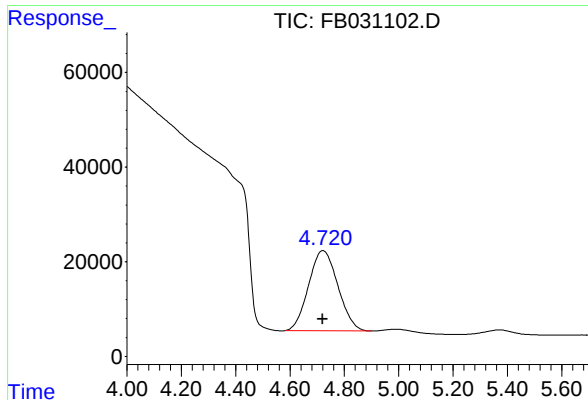

#1 2-Methylpentane


R.T.: 4.721 min
Delta R.T.: 0.001 min
Response: 1271628
Conc: 32.38 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1030S3

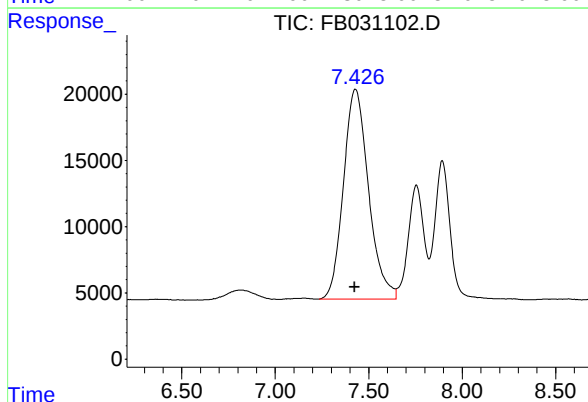


#2 2,2,4-Trimethylpentane

R.T.: 7.428 min
Delta R.T.: 0.003 min
Response: 1479527
Conc: 31.59 ng/ml

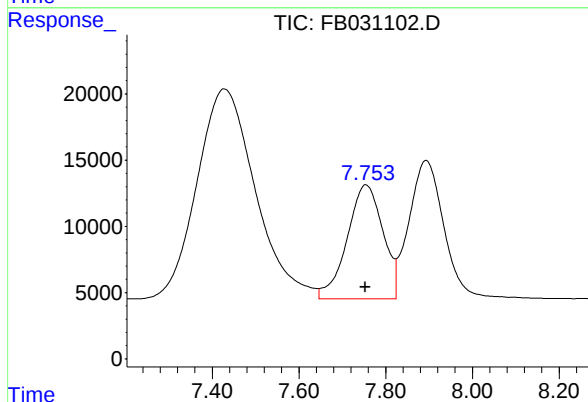


#3 n-Heptane

R.T.: 7.754 min
Delta R.T.: 0.002 min
Response: 493002
Conc: 10.88 ng/ml

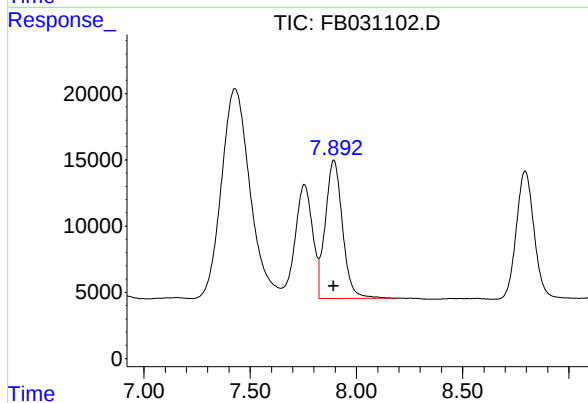

#4 Benzene

R.T.: 7.894 min
Delta R.T.: 0.002 min
Response: 586426
Conc: 10.97 ng/ml

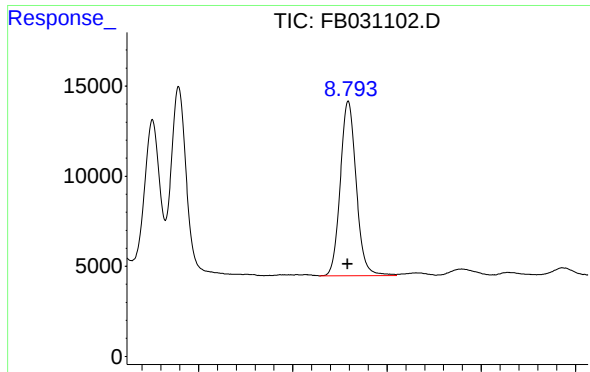

#5 AAA-TFT

R.T.: 8.794 min
Delta R.T.: 0.003 min
Response: 567915
Conc: 20.57 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1030S3

#6 Toluene


R.T.: 10.623 min
Delta R.T.: 0.004 min
Response: 1741213
Conc: 34.87 ng/ml

#7 Ethylbenzene

R.T.: 13.060 min
Delta R.T.: 0.005 min
Response: 525850
Conc: 11.75 ng/ml

#8 m-Xylene


R.T.: 13.193 min
Delta R.T.: 0.004 min
Response: 1258531
Conc: 25.88 ng/ml

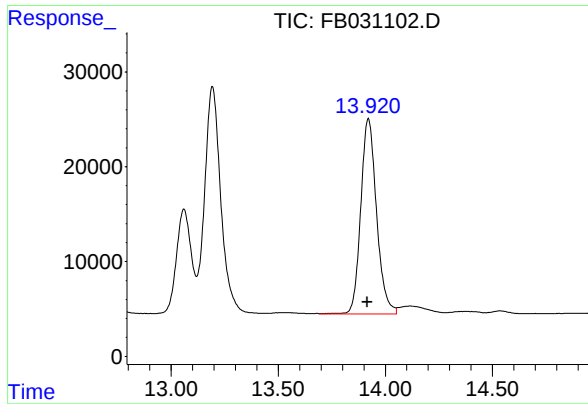

#9 O-Xylene

R.T.: 13.921 min
Delta R.T.: 0.004 min
Response: 1053314
Conc: 23.11 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1030S3

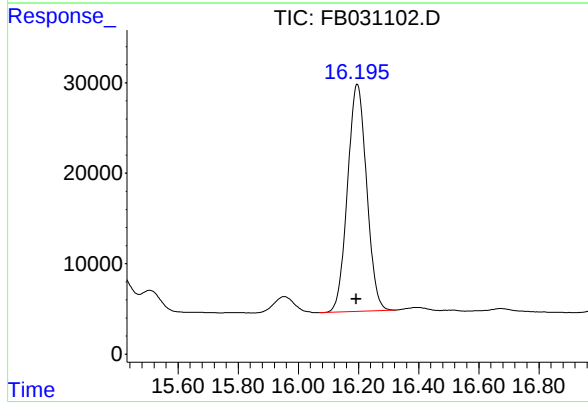

#10 1,2,4-Trimethylbenzene

R.T.: 16.196 min
Delta R.T.: 0.004 min
Response: 1106904
Conc: 29.75 ng/ml