

Data Path : \\74.0.250.170\Terastorage\pestpcbsrv\HPCHEM1\FID_B\Data\FB103118\
 Data File : FB018380.D
 Signal(s) : FID2B.CH
 Acq On : 31 Oct 2018 9:15
 Operator : MJ/SJ
 Sample : BSF1031S1
 Misc : 5.03g/5.00mL DI Water
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Oct 31 17:28:09 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101218.M
 Quant Title :
 QLast Update : Fri Oct 12 08:04:31 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.109	188372	21.871 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.961	473390	30.952 ng/ml
2) t 2,2,4-Trimethylpentane	7.727	491025	33.230 ng/ml
3) t n-Heptane	8.063	156450	11.040 ng/ml
4) t Benzene	8.204	196885	10.569 ng/ml
6) t Toluene	10.958	484196	31.770 ng/ml
7) t Ethylbenzene	13.408	166230	10.477 ng/ml
8) t m-Xylene	13.541	356826	21.445 ng/ml
9) t O-Xylene	14.272	378314	21.218 ng/ml
10) t 1,2,4-Trimethylbenzene	16.555	436740	21.468 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : \\74.0.250.170\Terastorage\pestpcbsrv\HPCHEM1\FID_B\Data\FB103118\
Data File : FB018380.D
Signal(s) : FID2B.CH
Acq On : 31 Oct 2018 9:15
Operator : MJ/SJ
Sample : BSF1031S1
Misc : 5.03g/5.00mL DI Water
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 31 17:28:09 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101218.M
Quant Title :
QLast Update : Fri Oct 12 08:04:31 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

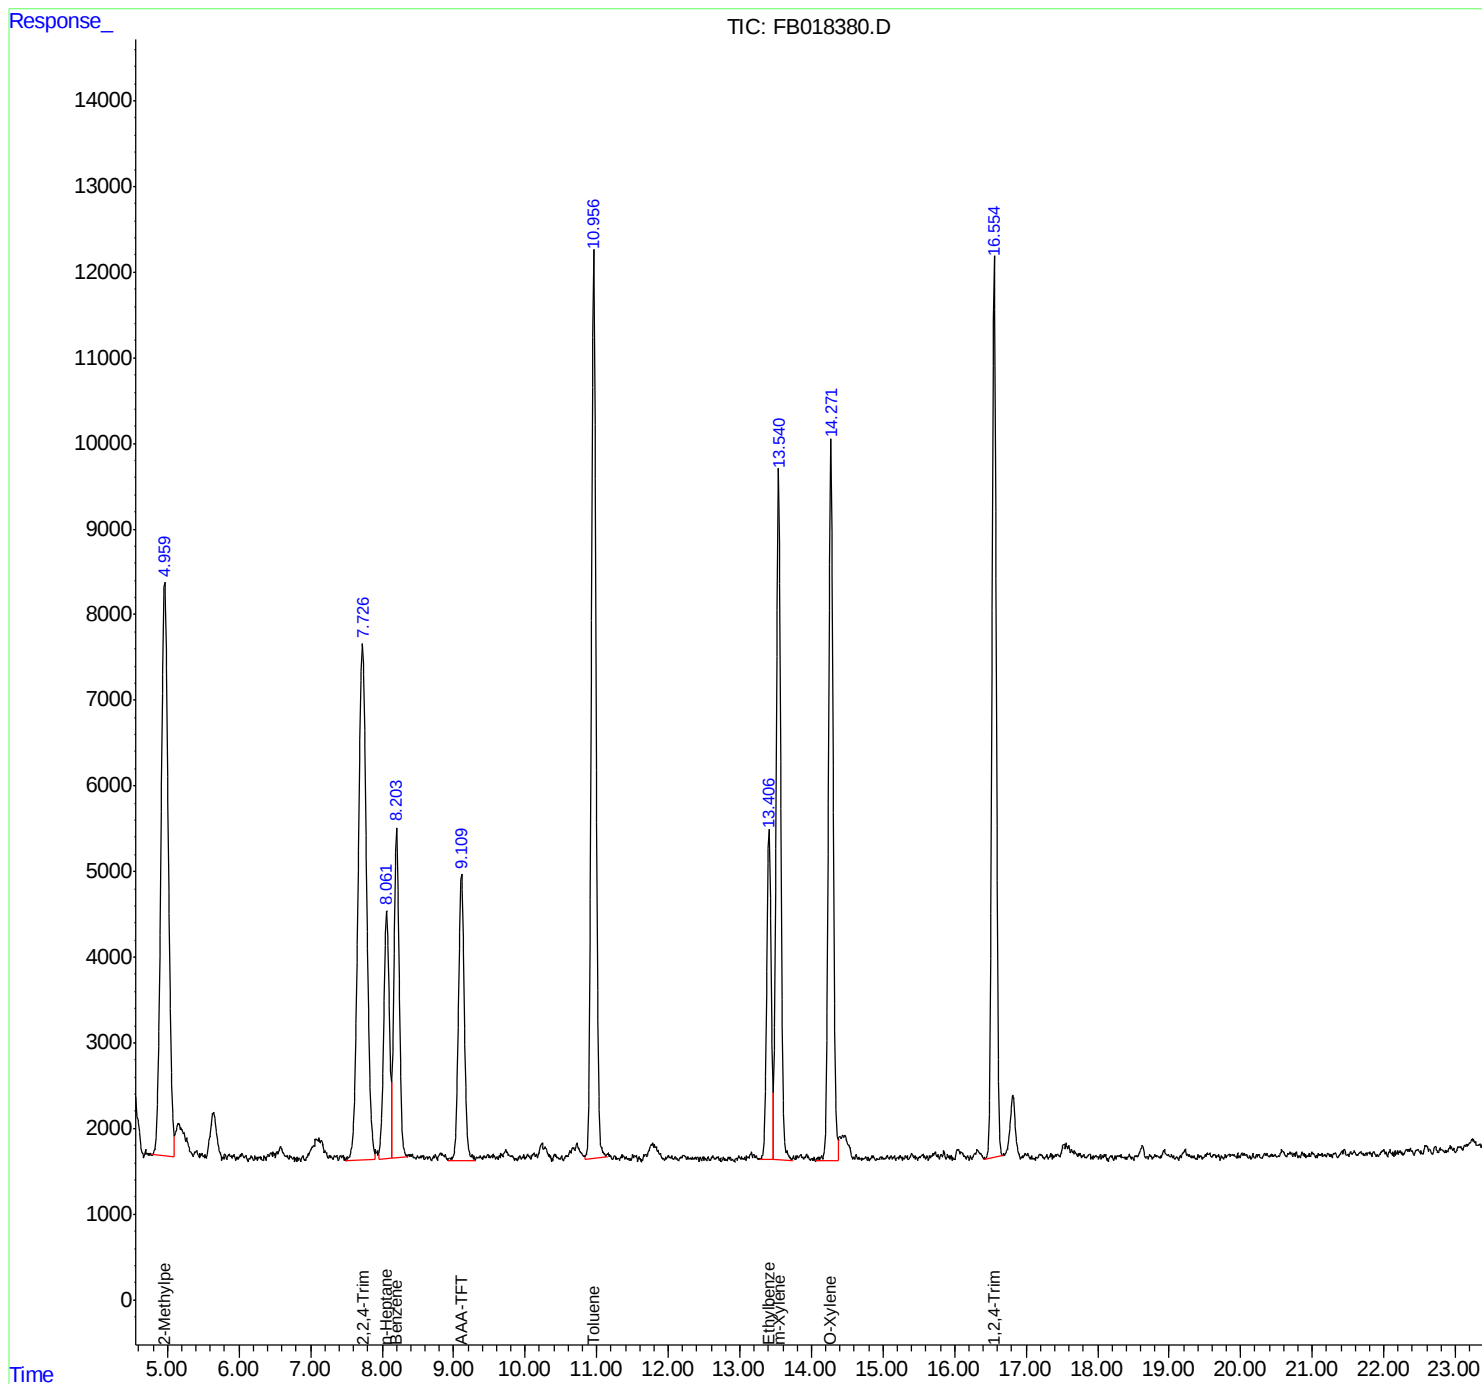

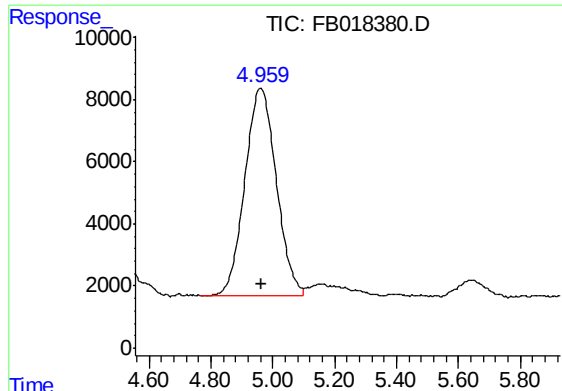


#1 2-Methylpentane

R.T.: 4.961 min
Delta R.T.: -0.004 min
Response: 473390
Conc: 30.95 ng/ml

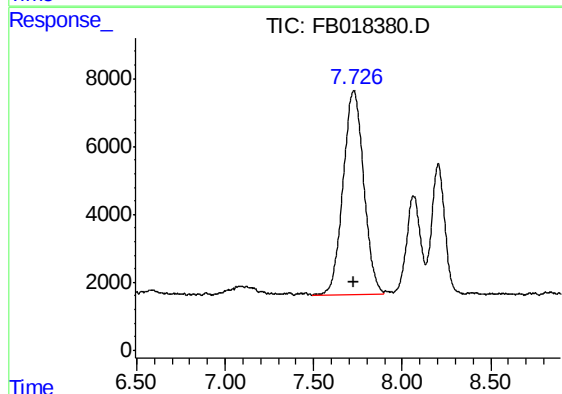


#2 2,2,4-Trimethylpentane

R.T.: 7.727 min
Delta R.T.: -0.001 min
Response: 491025
Conc: 33.23 ng/ml

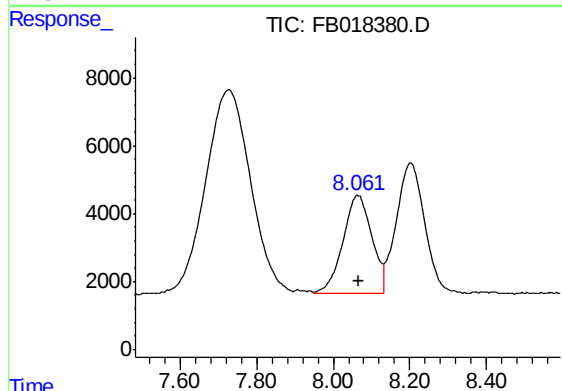


#3 n-Heptane

R.T.: 8.063 min
Delta R.T.: -0.005 min
Response: 156450
Conc: 11.04 ng/ml

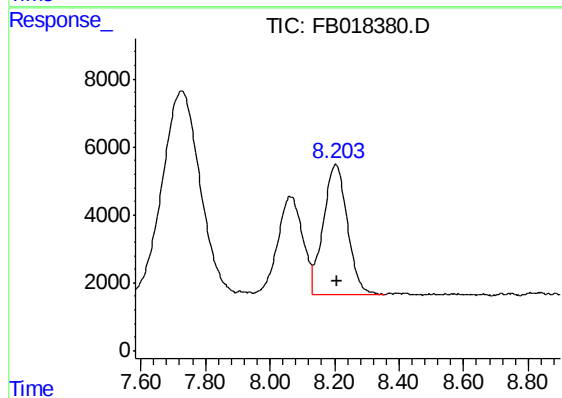


#4 Benzene

R.T.: 8.204 min
Delta R.T.: -0.002 min
Response: 196885
Conc: 10.57 ng/ml

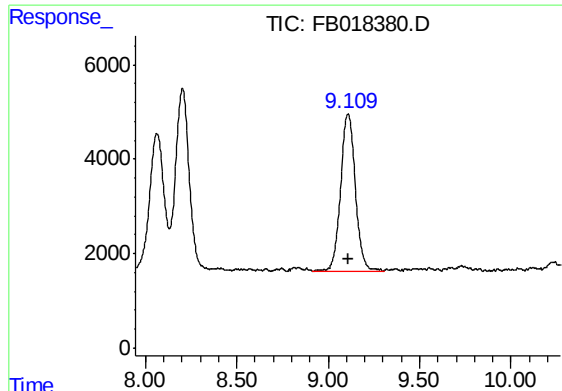


#5 AAA-TFT

R.T.: 9.109 min
Delta R.T.: -0.003 min
Response: 188372
Conc: 21.87 ng/ml

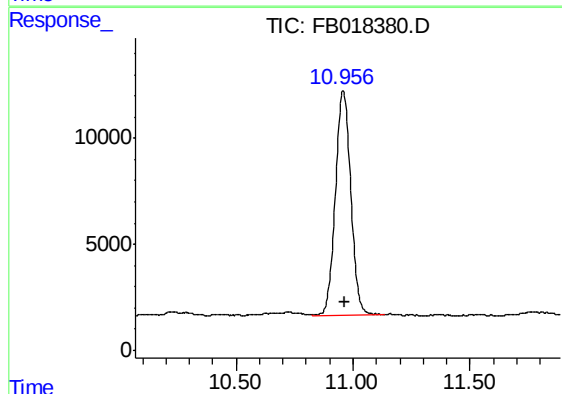


#6 Toluene

R.T.: 10.958 min
Delta R.T.: -0.004 min
Response: 484196
Conc: 31.77 ng/ml

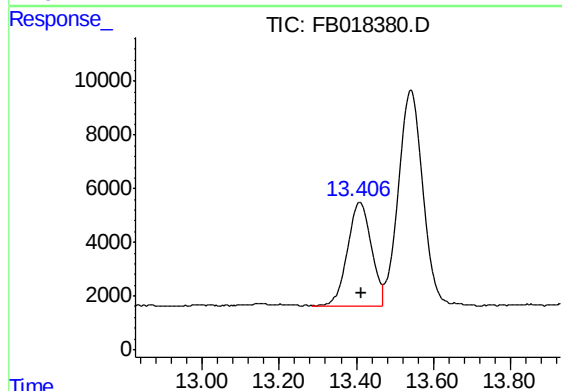


#7 Ethylbenzene

R.T.: 13.408 min
Delta R.T.: -0.004 min
Response: 166230
Conc: 10.48 ng/ml

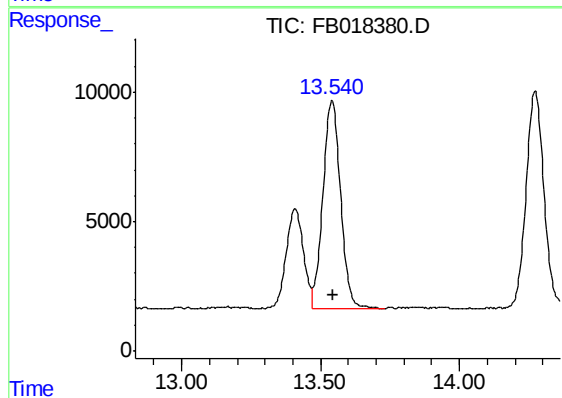


#8 m-Xylene

R.T.: 13.541 min
Delta R.T.: -0.003 min
Response: 356826
Conc: 21.45 ng/ml

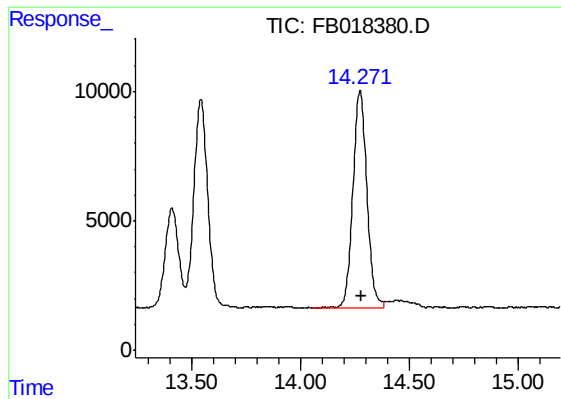

#9 O-Xylene

R.T.: 14.272 min
Delta R.T.: -0.004 min
Response: 378314
Conc: 21.22 ng/ml

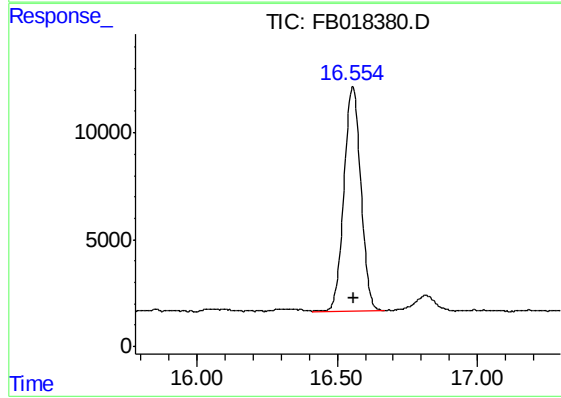

#10 1,2,4-Trimethylbenzene

R.T.: 16.555 min
Delta R.T.: -0.004 min
Response: 436740
Conc: 21.47 ng/ml