

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB103122\
 Data File : FB028795.D
 Signal(s) : FID2B.CH
 Acq On : 31 Oct 2022 11:13
 Operator : AJ/MA
 Sample : BSF1031S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1031S1

Integration File: Calibration.e
 Quant Time: Nov 01 06:39:14 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100522.M
 Quant Title :
 QLast Update : Wed Oct 05 12:47:25 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.791	264354	20.434 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.709	478551	29.253 ng/ml
2) t 2,2,4-Trimethylpentane	7.420	507305	28.071 ng/ml
3) t n-Heptane	7.749	171673	10.135 ng/ml
4) t Benzene	7.886	198181	9.023 ng/ml
6) t Toluene	10.619	580627	27.702 ng/ml
7) t Ethylbenzene	13.055	180957	9.118 ng/ml
8) t m-Xylene	13.188	360530	18.300 ng/ml
9) t O-Xylene	13.915	353470	18.169 ng/ml
10) t 1,2,4-Trimethylbenzene	16.190	360916	18.643 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB103122\
Data File : FB028795.D
Signal(s) : FID2B.CH
Acq On : 31 Oct 2022 11:13
Operator : AJ/MA
Sample : BSF1031S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1031S1

Integration File: Calibration.e
Quant Time: Nov 01 06:39:14 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100522.M
Quant Title :
QLast Update : Wed Oct 05 12:47:25 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

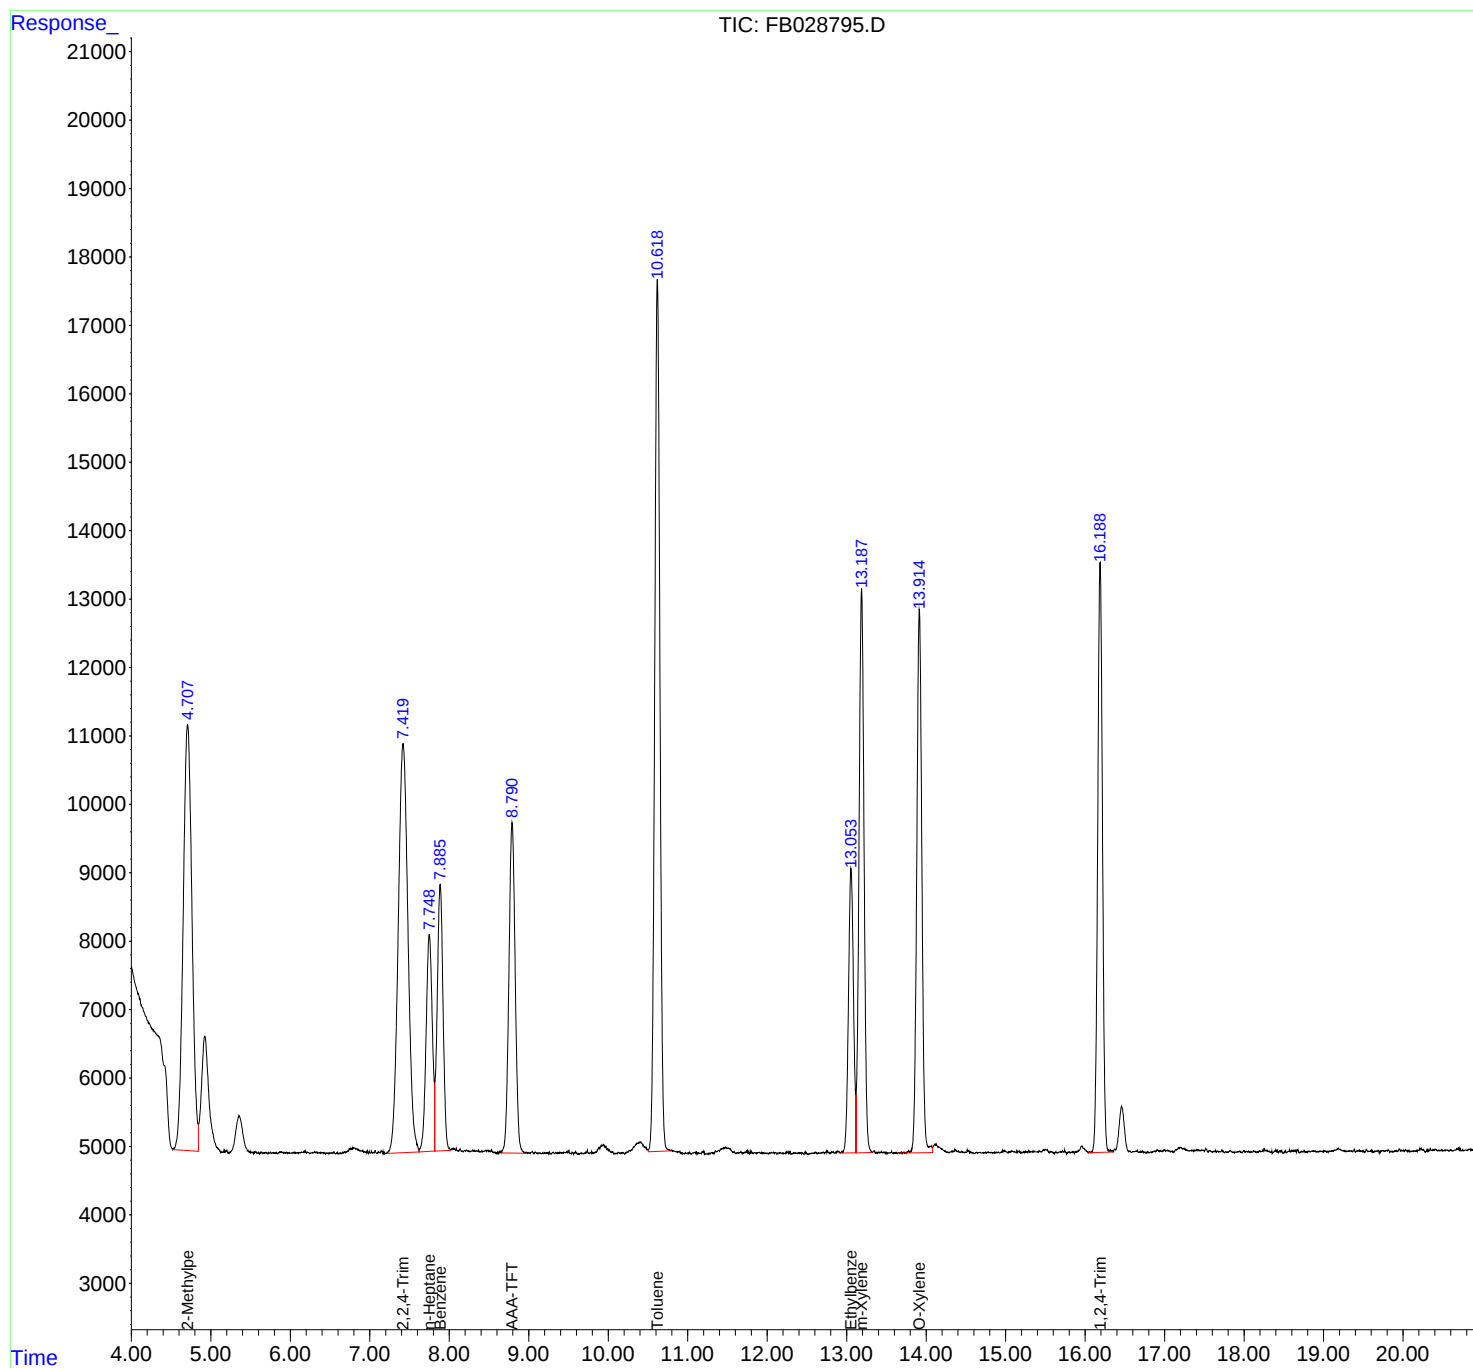


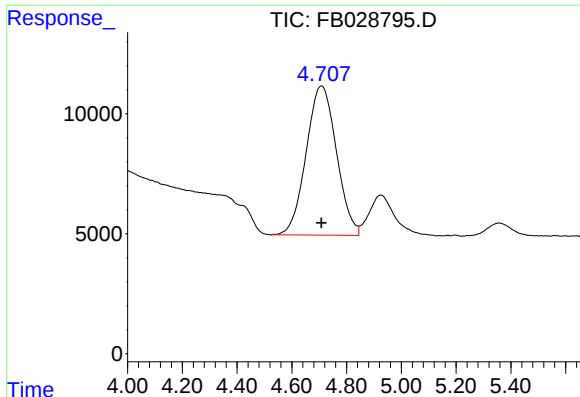

#1 2-Methylpentane


R.T.: 4.709 min
Delta R.T.: 0.000 min
Response: 478551
Conc: 29.25 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1031S1

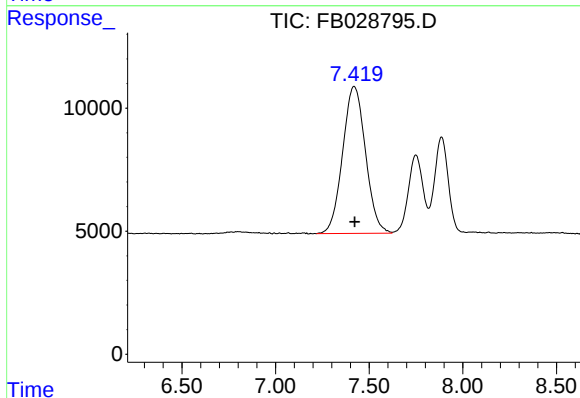


#2 2,2,4-Trimethylpentane

R.T.: 7.420 min
Delta R.T.: -0.004 min
Response: 507305
Conc: 28.07 ng/ml

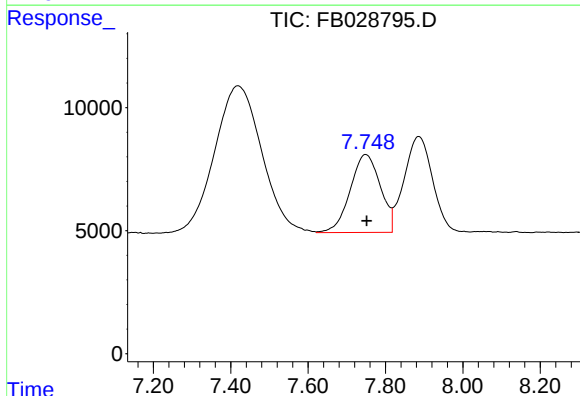


#3 n-Heptane

R.T.: 7.749 min
Delta R.T.: -0.002 min
Response: 171673
Conc: 10.14 ng/ml

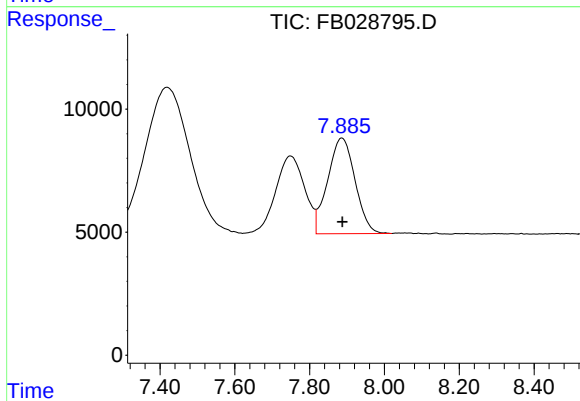

#4 Benzene


R.T.: 7.886 min
Delta R.T.: -0.001 min
Response: 198181
Conc: 9.02 ng/ml

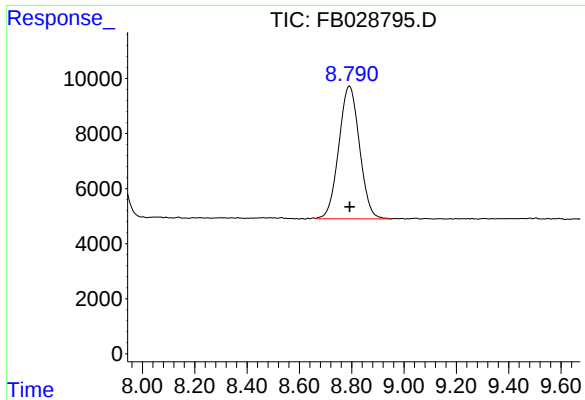

#5 AAA-TFT


R.T.: 8.791 min
Delta R.T.: -0.001 min
Response: 264354
Conc: 20.43 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1031S1

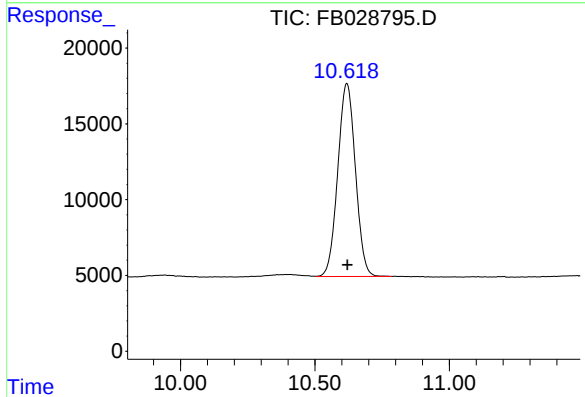


#6 Toluene

R.T.: 10.619 min
Delta R.T.: -0.002 min
Response: 580627
Conc: 27.70 ng/ml

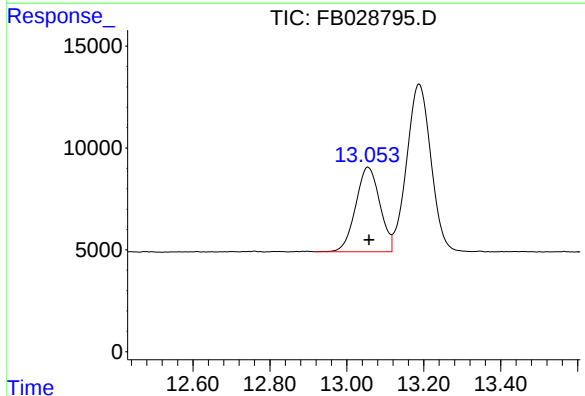


#7 Ethylbenzene

R.T.: 13.055 min
Delta R.T.: -0.003 min
Response: 180957
Conc: 9.12 ng/ml

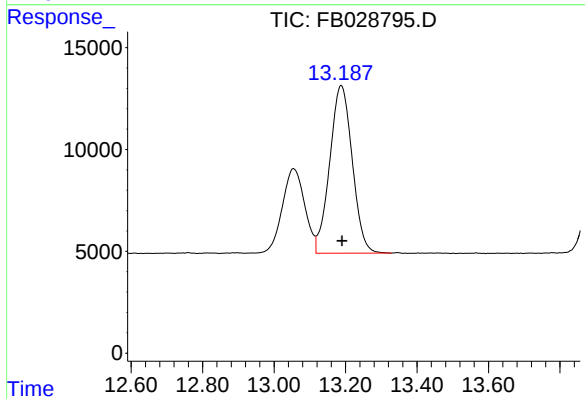

#8 m-Xylene


R.T.: 13.188 min
Delta R.T.: -0.002 min
Response: 360530
Conc: 18.30 ng/ml

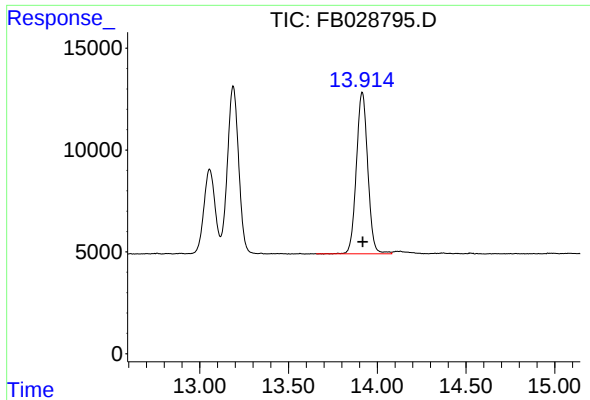

#9 O-Xylene

R.T.: 13.915 min
Delta R.T.: -0.002 min
Response: 353470
Conc: 18.17 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1031S1

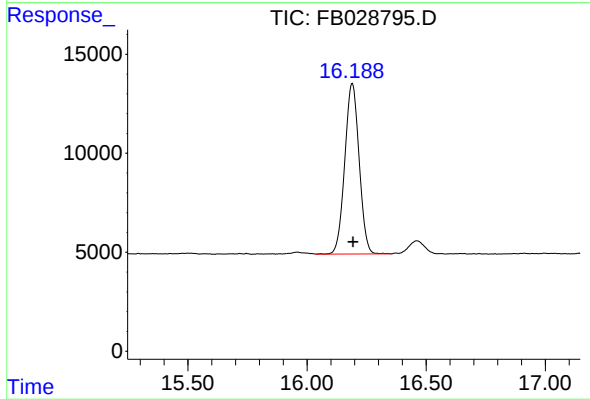

#10 1,2,4-Trimethylbenzene

R.T.: 16.190 min
Delta R.T.: -0.003 min
Response: 360916
Conc: 18.64 ng/ml