

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB103122\
 Data File : FB028804.D
 Signal(s) : FID2B.CH
 Acq On : 31 Oct 2022 18:53
 Operator : AJ/MA
 Sample : N5336-07MSD 50X
 Misc : 5.10G/5.00 ML MEOH
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 SB-02-COMPMSD

Integration File: Calibration.e
 Quant Time: Nov 01 06:40:21 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100522.M
 Quant Title :
 QLast Update : Wed Oct 05 12:47:25 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.796	298563	23.078 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.709	471716	28.835 ng/ml
2) t 2,2,4-Trimethylpentane	7.428	531989	29.437 ng/ml
3) t n-Heptane	7.752	186297	10.999 ng/ml
4) t Benzene	7.890	223899	10.194 ng/ml
6) t Toluene	10.624	646576	30.848 ng/ml
7) t Ethylbenzene	13.061	197635	9.958 ng/ml
8) t m-Xylene	13.194	389658	19.779 ng/ml
9) t O-Xylene	13.921	365340	18.779 ng/ml
10) t 1,2,4-Trimethylbenzene	16.196	338526	17.487 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.





Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB103122\
Data File : FB028804.D
Signal(s) : FID2B.CH
Acq On : 31 Oct 2022 18:53
Operator : AJ/MA
Sample : N5336-07MSD 50X
Misc : 5.10G/5.00 ML MEOH
ALS Vial : 13 Sample Multiplier: 1


Instrument :
FID_B
ClientSampleId :
SB-02-COMPMSD

Integration File: Calibration.e
Quant Time: Nov 01 06:40:21 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100522.M
Quant Title :
QLast Update : Wed Oct 05 12:47:25 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

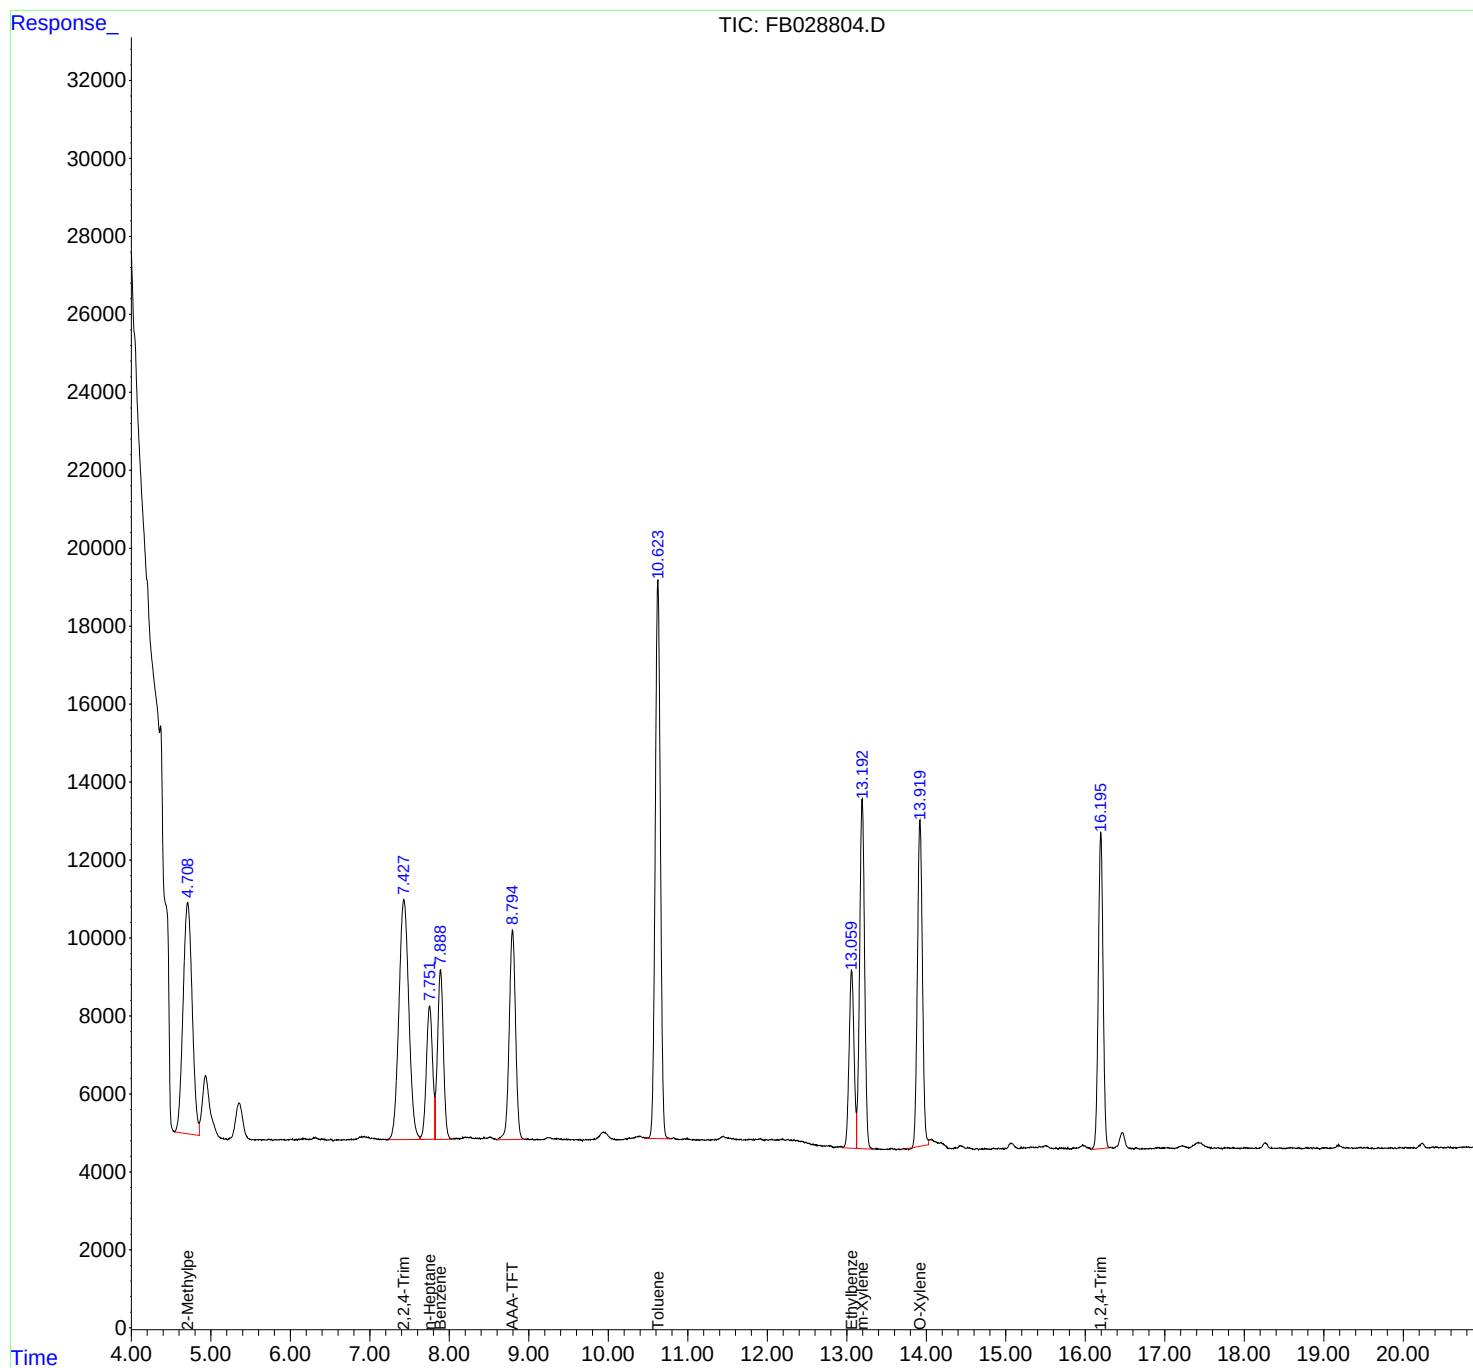




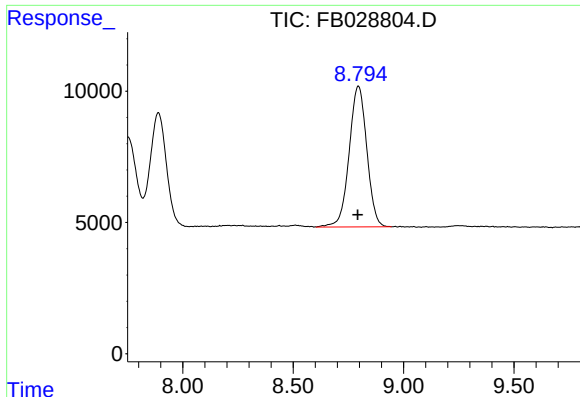

#5 AAA-TFT


R.T.: 8.796 min
Delta R.T.: 0.003 min
Response: 298563
Conc: 23.08 ng/ml

Instrument :
FID_B
ClientSampleId :
SB-02-COMPMSD

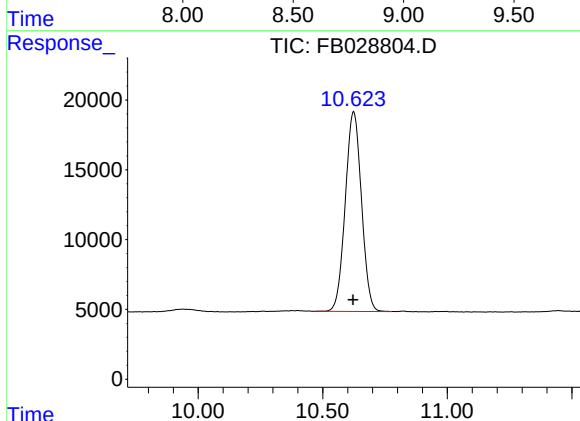


#6 Toluene

R.T.: 10.624 min
Delta R.T.: 0.003 min
Response: 646576
Conc: 30.85 ng/ml

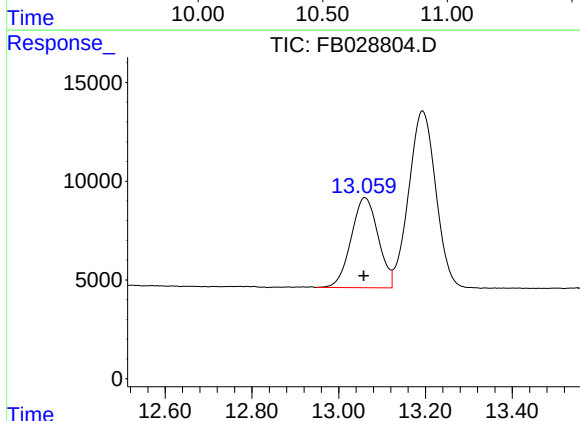


#7 Ethylbenzene

R.T.: 13.061 min
Delta R.T.: 0.003 min
Response: 197635
Conc: 9.96 ng/ml

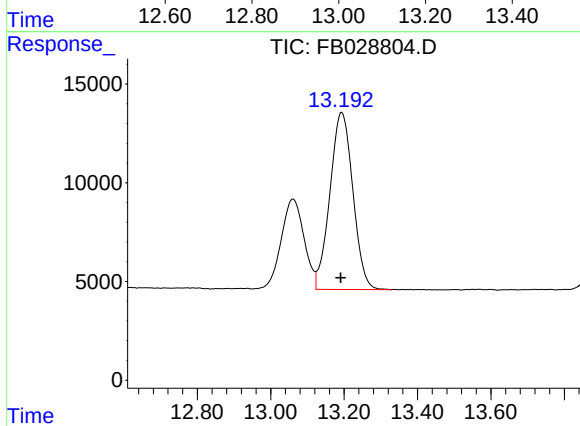

#8 m-Xylene


R.T.: 13.194 min
Delta R.T.: 0.003 min
Response: 389658
Conc: 19.78 ng/ml

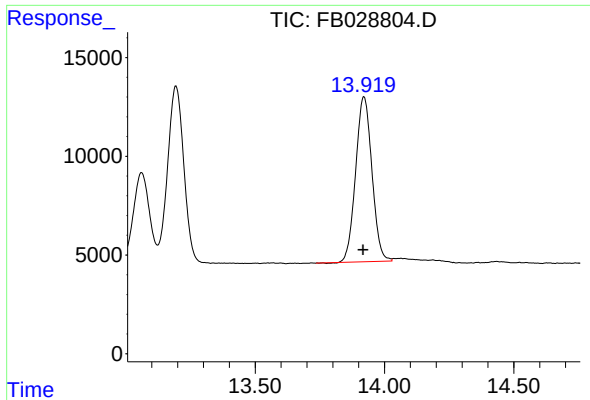

#9 O-Xylene

R.T.: 13.921 min
Delta R.T.: 0.003 min
Response: 365340
Conc: 18.78 ng/ml

Instrument :
FID_B
ClientSampleId :
SB-02-COMPMSD

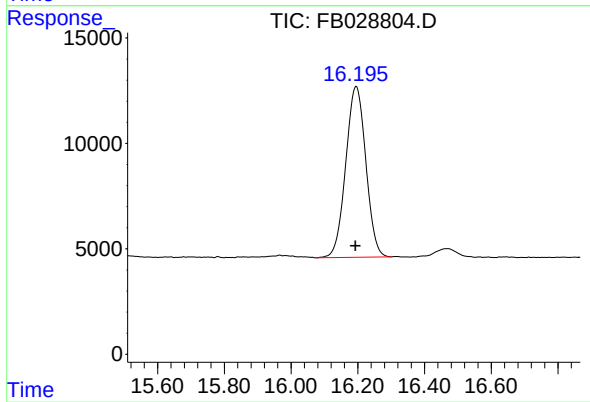

#10 1,2,4-Trimethylbenzene

R.T.: 16.196 min
Delta R.T.: 0.003 min
Response: 338526
Conc: 17.49 ng/ml