

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB103122\
 Data File : FB028799.D
 Signal(s) : FID2B.CH
 Acq On : 31 Oct 2022 15:45
 Operator : AJ/MA
 Sample : BSF1031S2
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1031S2

Integration File: Calibration.e
 Quant Time: Nov 01 06:39:44 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100522.M
 Quant Title :
 QLast Update : Wed Oct 05 12:47:25 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.799	294945	22.798 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.722	486925	29.765 ng/ml
2) t 2,2,4-Trimethylpentane	7.435	540892	29.930 ng/ml
3) t n-Heptane	7.758	180707	10.669 ng/ml
4) t Benzene	7.894	212272	9.664 ng/ml
6) t Toluene	10.627	614187	29.303 ng/ml
7) t Ethylbenzene	13.063	192547	9.702 ng/ml
8) t m-Xylene	13.196	382123	19.396 ng/ml
9) t O-Xylene	13.923	370253	19.032 ng/ml
10) t 1,2,4-Trimethylbenzene	16.198	358489	18.518 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB103122\
Data File : FB028799.D
Signal(s) : FID2B.CH
Acq On : 31 Oct 2022 15:45
Operator : AJ/MA
Sample : BSF1031S2
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1031S2

Integration File: Calibration.e
Quant Time: Nov 01 06:39:44 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100522.M
Quant Title :
QLast Update : Wed Oct 05 12:47:25 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

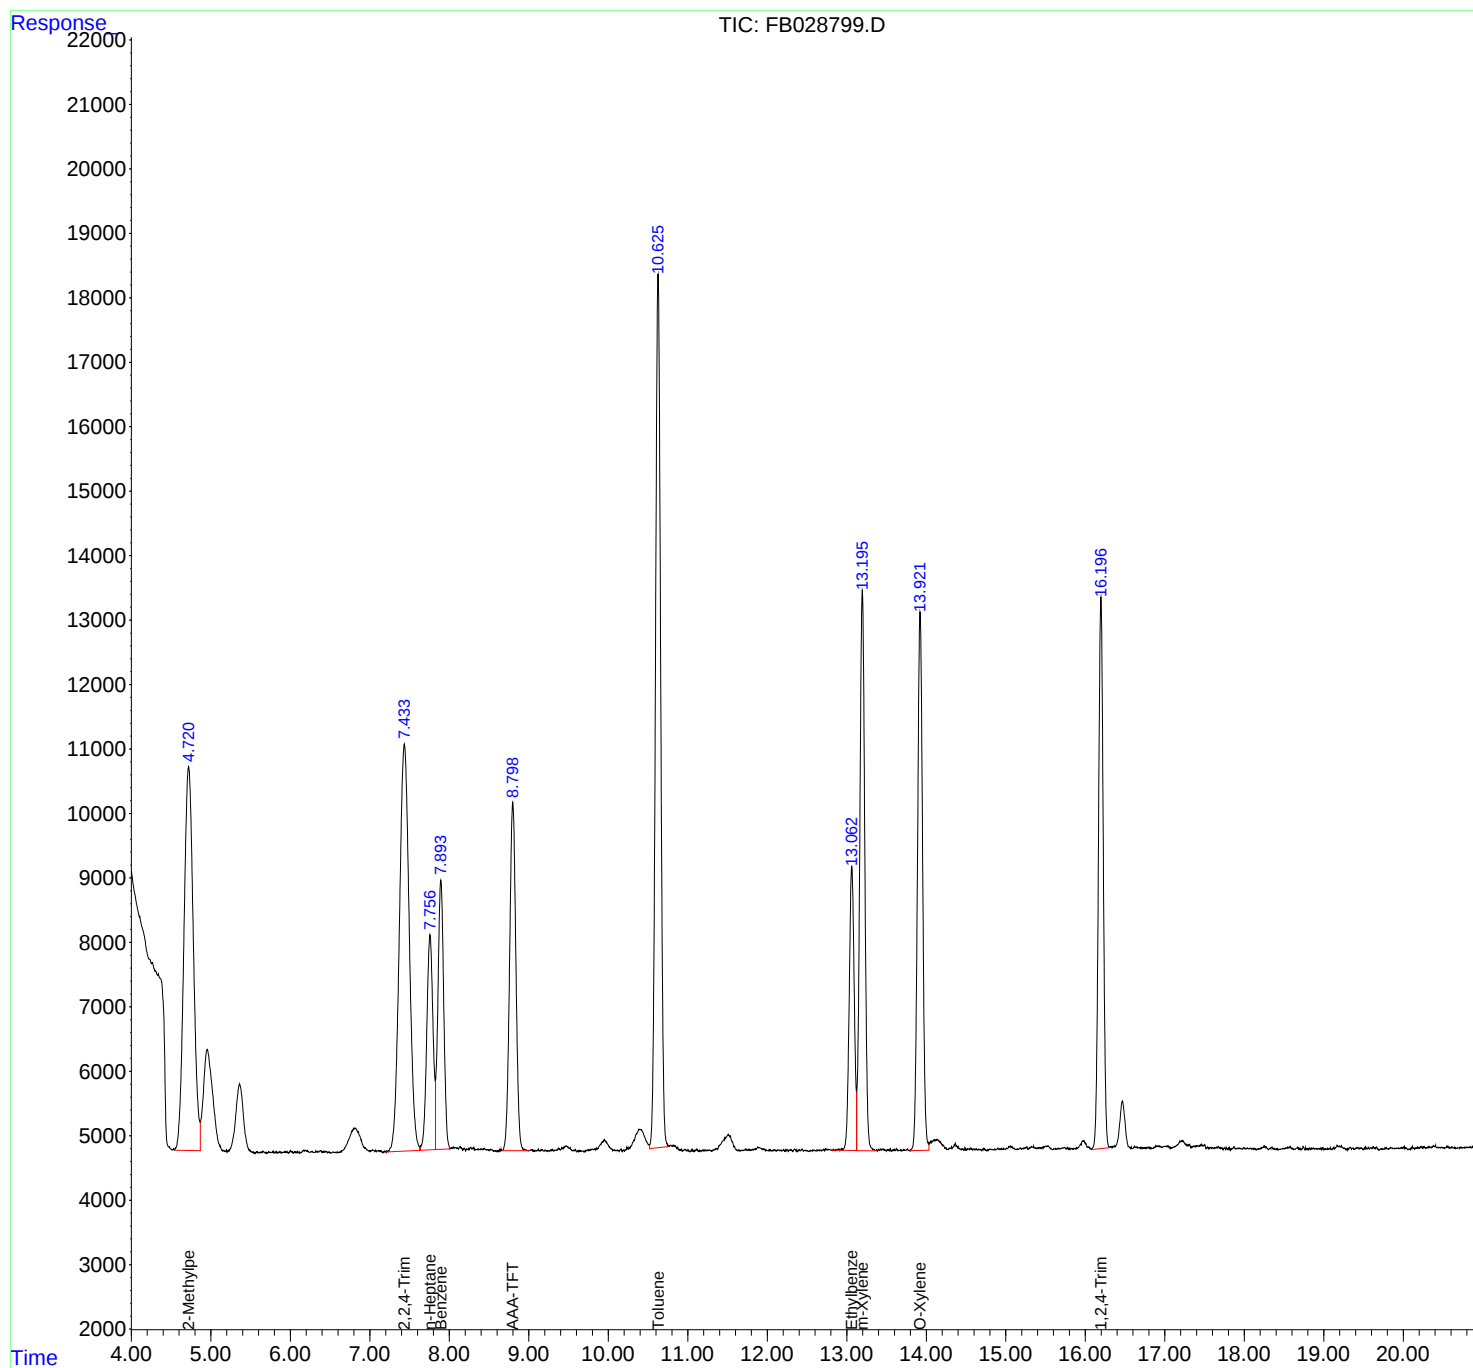


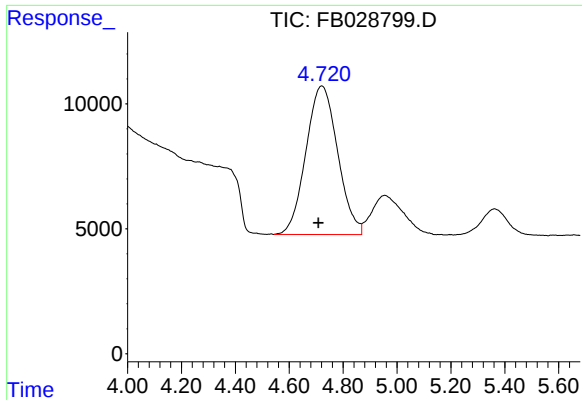

#1 2-Methylpentane


R.T.: 4.722 min
Delta R.T.: 0.014 min
Response: 486925
Conc: 29.76 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1031S2

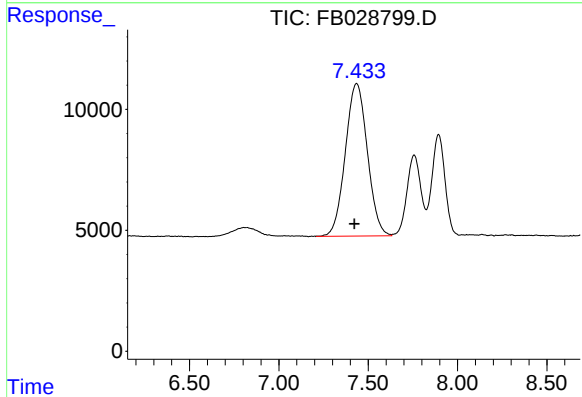


#2 2,2,4-Trimethylpentane

R.T.: 7.435 min
Delta R.T.: 0.011 min
Response: 540892
Conc: 29.93 ng/ml

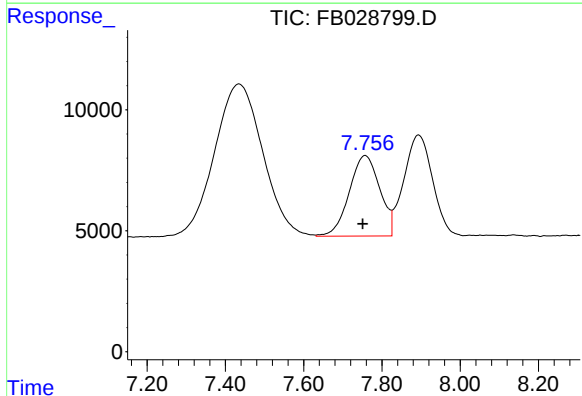


#3 n-Heptane

R.T.: 7.758 min
Delta R.T.: 0.006 min
Response: 180707
Conc: 10.67 ng/ml

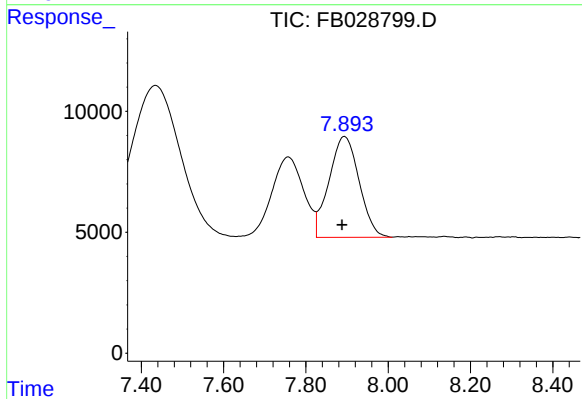

#4 Benzene


R.T.: 7.894 min
Delta R.T.: 0.006 min
Response: 212272
Conc: 9.66 ng/ml

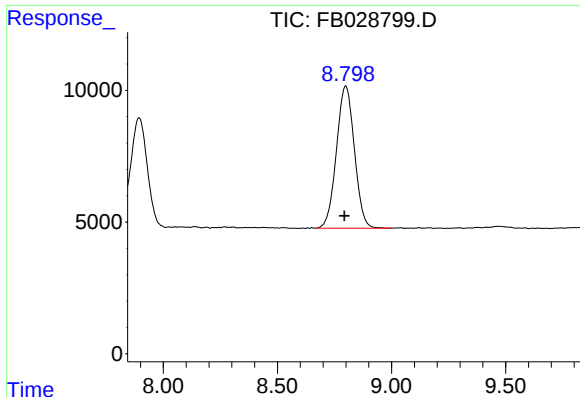

#5 AAA-TFT


R.T.: 8.799 min
Delta R.T.: 0.007 min
Response: 294945
Conc: 22.80 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1031S2

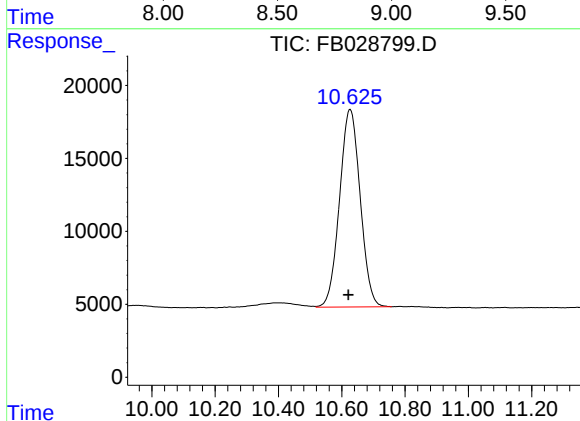


#6 Toluene

R.T.: 10.627 min
Delta R.T.: 0.006 min
Response: 614187
Conc: 29.30 ng/ml

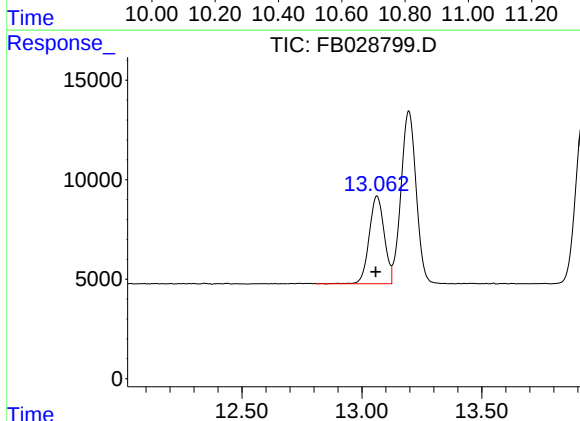


#7 Ethylbenzene

R.T.: 13.063 min
Delta R.T.: 0.005 min
Response: 192547
Conc: 9.70 ng/ml

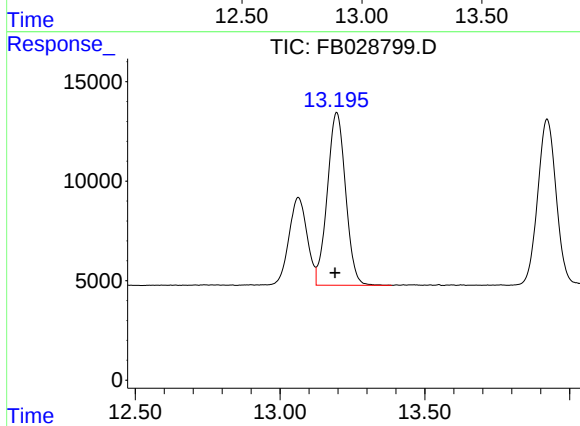

#8 m-Xylene


R.T.: 13.196 min
Delta R.T.: 0.006 min
Response: 382123
Conc: 19.40 ng/ml

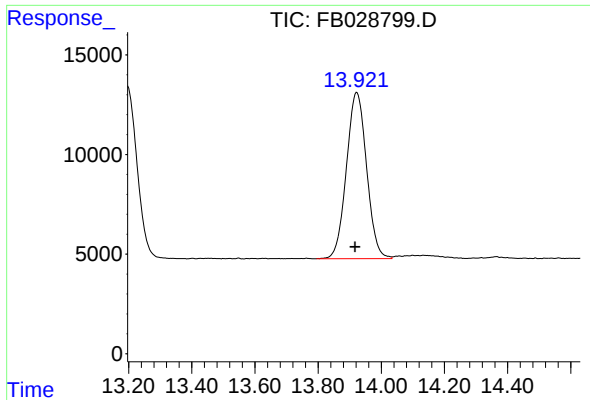

#9 O-Xylene

R.T.: 13.923 min
Delta R.T.: 0.005 min
Response: 370253
Conc: 19.03 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1031S2

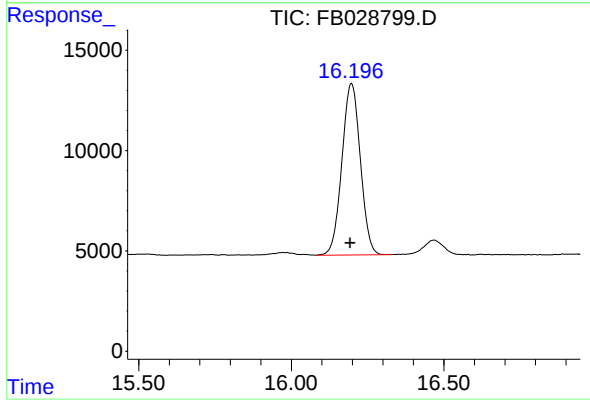

#10 1,2,4-Trimethylbenzene

R.T.: 16.198 min
Delta R.T.: 0.005 min
Response: 358489
Conc: 18.52 ng/ml