

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB103122\
 Data File : FB028806.D
 Signal(s) : FID2B.CH
 Acq On : 31 Oct 2022 20:08
 Operator : AJ/MA
 Sample : BSF1031S3
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1031S3

Integration File: Calibration.e
 Quant Time: Nov 01 06:40:35 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100522.M
 Quant Title :
 QLast Update : Wed Oct 05 12:47:25 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.798	285709	22.084 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.716	497018	30.382 ng/ml
2) t 2,2,4-Trimethylpentane	7.432	550355	30.453 ng/ml
3) t n-Heptane	7.758	178505	10.539 ng/ml
4) t Benzene	7.893	213563	9.723 ng/ml
6) t Toluene	10.625	616260	29.402 ng/ml
7) t Ethylbenzene	13.062	193121	9.731 ng/ml
8) t m-Xylene	13.194	383010	19.441 ng/ml
9) t O-Xylene	13.921	373060	19.176 ng/ml
10) t 1,2,4-Trimethylbenzene	16.195	368620	19.041 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB103122\
Data File : FB028806.D
Signal(s) : FID2B.CH
Acq On : 31 Oct 2022 20:08
Operator : AJ/MA
Sample : BSF1031S3
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1031S3

Integration File: Calibration.e
Quant Time: Nov 01 06:40:35 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100522.M
Quant Title :
QLast Update : Wed Oct 05 12:47:25 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

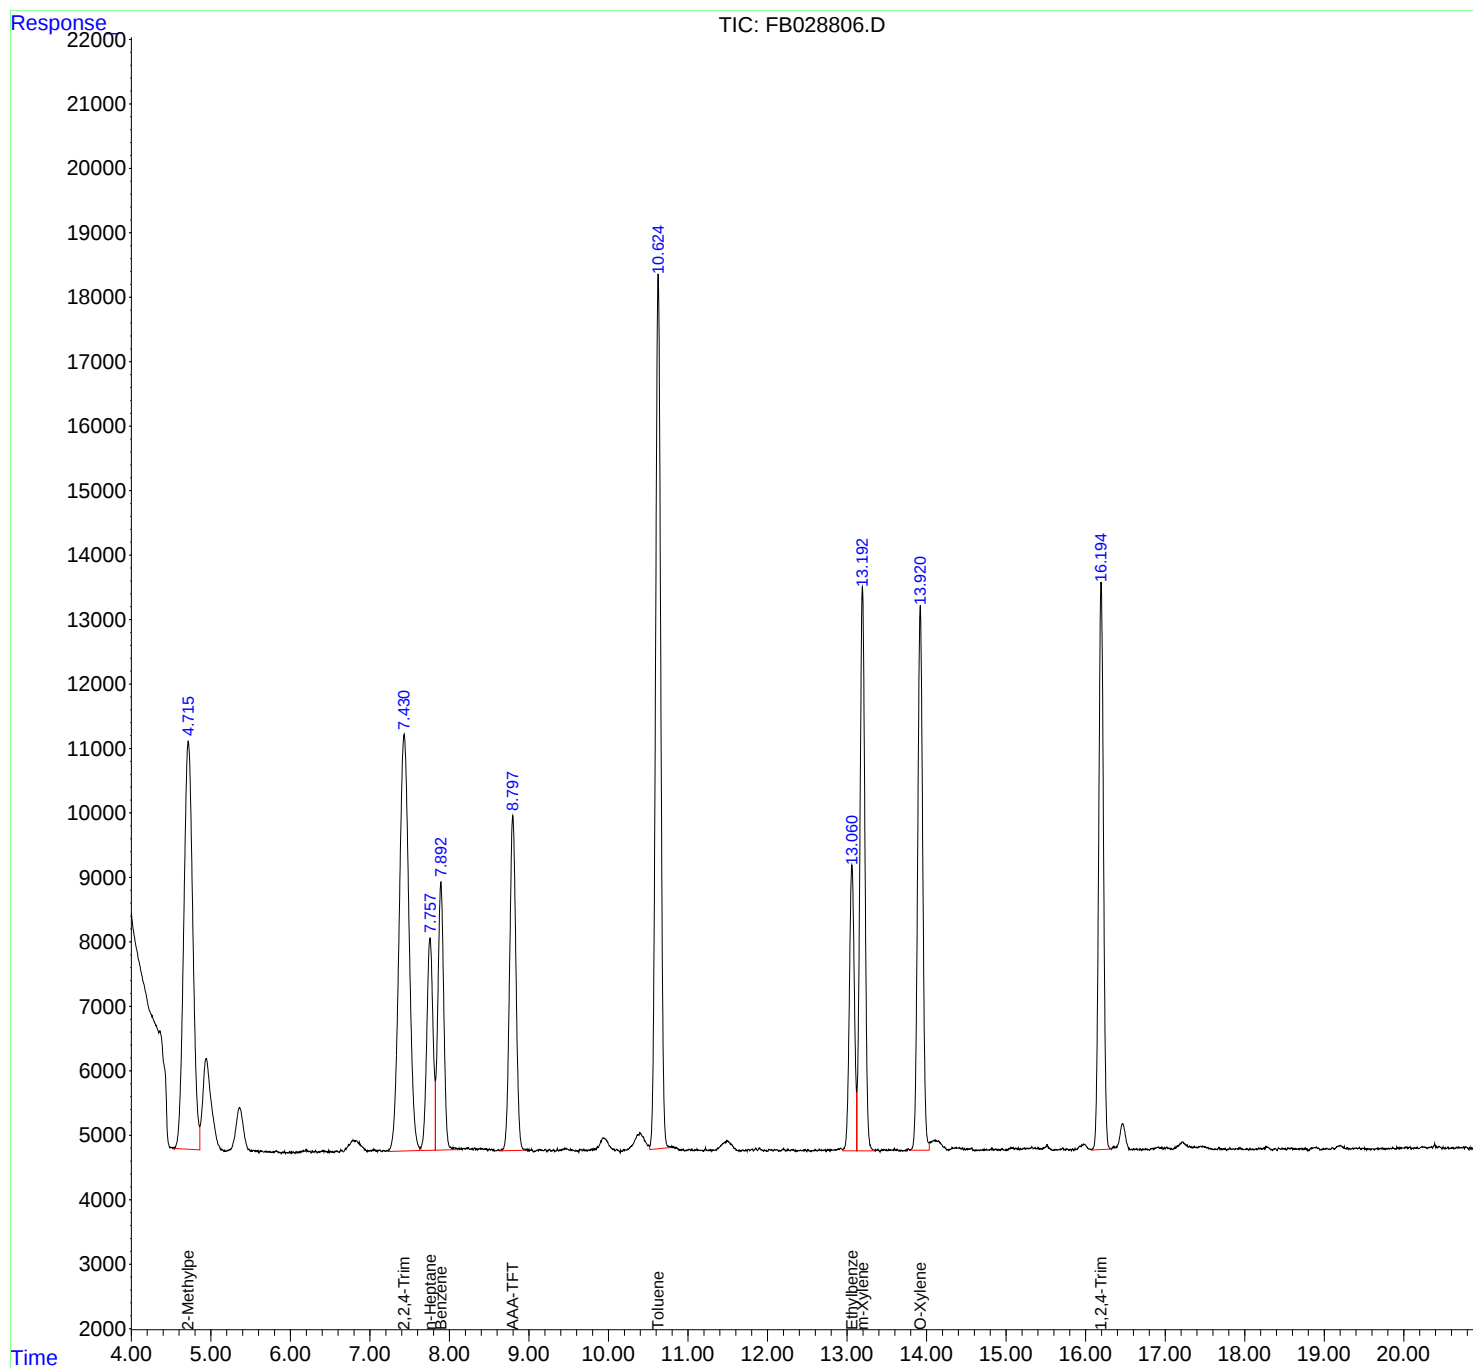


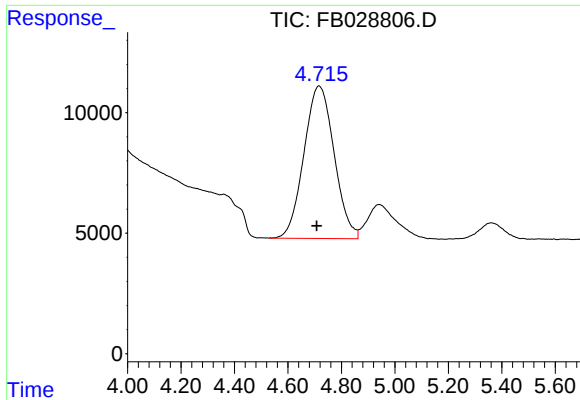

#1 2-Methylpentane


R.T.: 4.716 min
Delta R.T.: 0.008 min
Response: 497018
Conc: 30.38 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1031S3

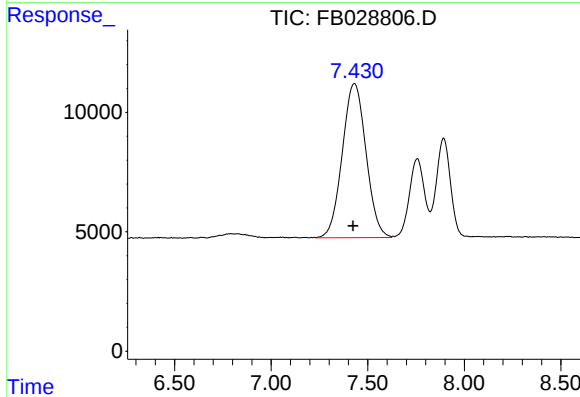


#2 2,2,4-Trimethylpentane

R.T.: 7.432 min
Delta R.T.: 0.008 min
Response: 550355
Conc: 30.45 ng/ml

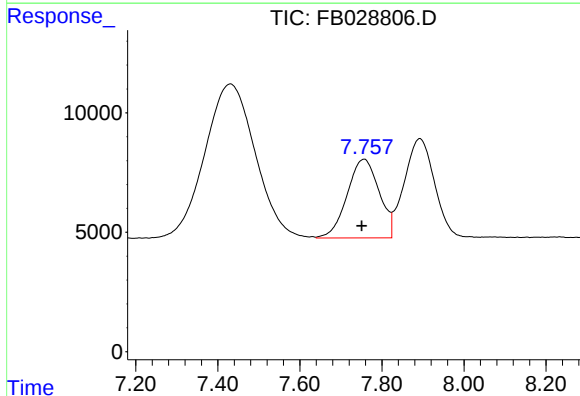


#3 n-Heptane

R.T.: 7.758 min
Delta R.T.: 0.007 min
Response: 178505
Conc: 10.54 ng/ml

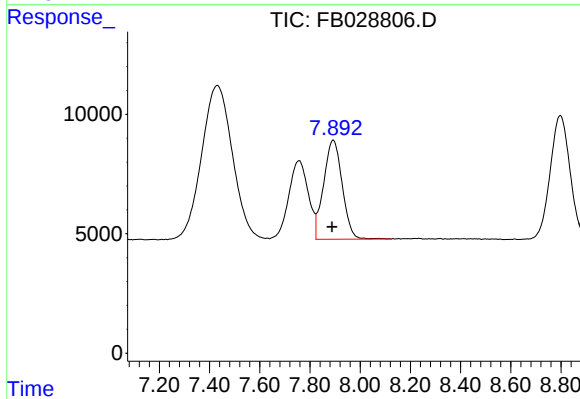

#4 Benzene


R.T.: 7.893 min
Delta R.T.: 0.005 min
Response: 213563
Conc: 9.72 ng/ml

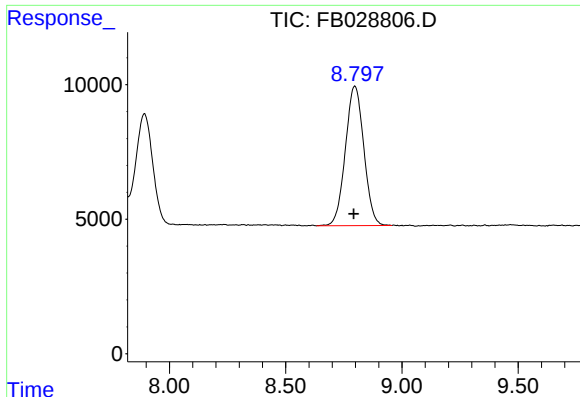

#5 AAA-TFT


R.T.: 8.798 min
Delta R.T.: 0.005 min
Response: 285709
Conc: 22.08 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1031S3

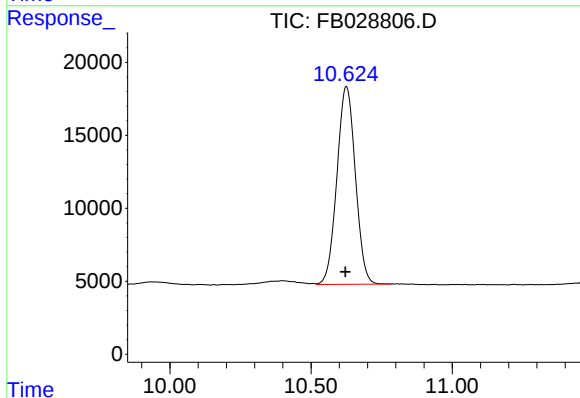


#6 Toluene

R.T.: 10.625 min
Delta R.T.: 0.004 min
Response: 616260
Conc: 29.40 ng/ml

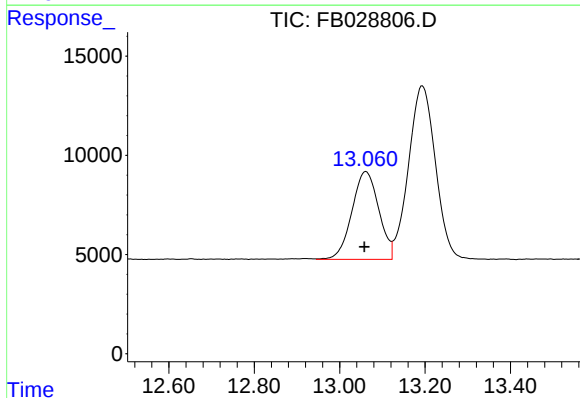


#7 Ethylbenzene

R.T.: 13.062 min
Delta R.T.: 0.004 min
Response: 193121
Conc: 9.73 ng/ml

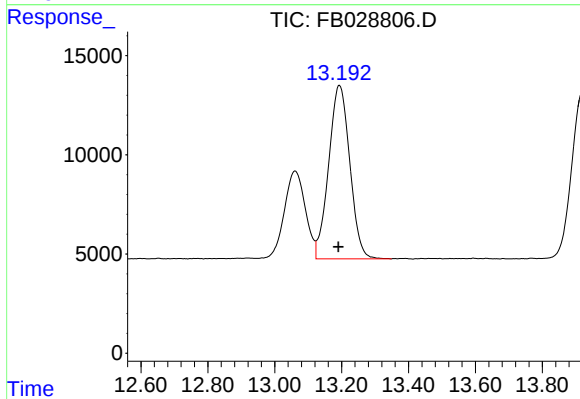

#8 m-Xylene


R.T.: 13.194 min
Delta R.T.: 0.003 min
Response: 383010
Conc: 19.44 ng/ml

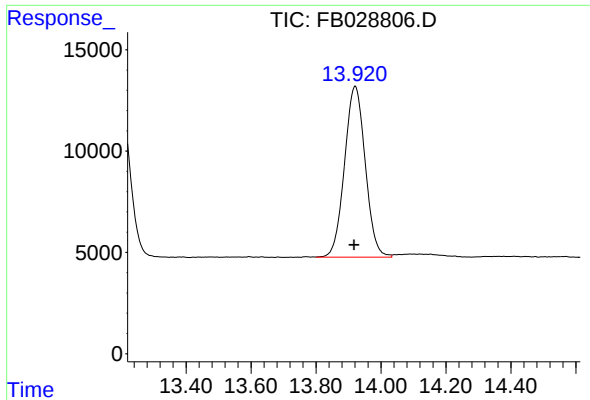

#9 O-Xylene

R.T.: 13.921 min
Delta R.T.: 0.004 min
Response: 373060
Conc: 19.18 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1031S3

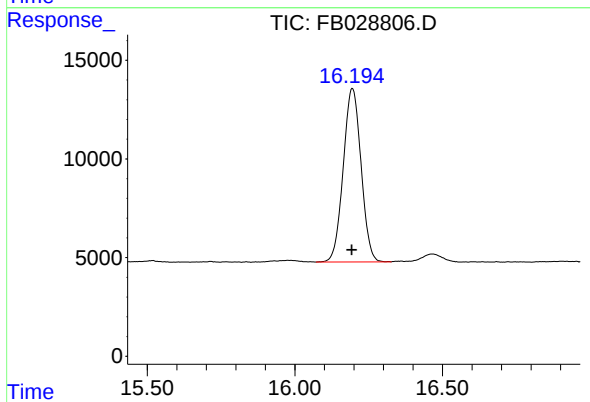

#10 1,2,4-Trimethylbenzene

R.T.: 16.195 min
Delta R.T.: 0.003 min
Response: 368620
Conc: 19.04 ng/ml