

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110122\
Data File : FB028808.D
Signal(s) : FID2B.CH
Acq On : 1 Nov 2022 9:16
Operator : AJ/MA
Sample : 5 GRO STD
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
5 GRO STD

Integration File: Calibration.e
Quant Time: Nov 01 10:48:13 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110122.M
Quant Title :
QLast Update : Tue Nov 01 10:44:43 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.789	68060	5.321 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.704	117733	6.954 ng/ml
2) t 2,2,4-Trimethylpentane	7.414	119619	6.563 ng/ml
3) t n-Heptane	7.746	41124	2.229 ng/ml
4) t Benzene	7.887	45382	2.118 ng/ml
6) t Toluene	10.618	137040	6.530 ng/ml
7) t Ethylbenzene	13.056	45127	2.279 ng/ml
8) t m-Xylene	13.188	88168	4.468 ng/ml
9) t O-Xylene	13.914	88587	4.674 ng/ml
10) t 1,2,4-Trimethylbenzene	16.189	94824	5.047 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110122\
Data File : FB028808.D
Signal(s) : FID2B.CH
Acq On : 1 Nov 2022 9:16
Operator : AJ/MA
Sample : 5 GRO STD
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
5 GRO STD

Integration File: Calibration.e
Quant Time: Nov 01 10:48:13 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110122.M
Quant Title :
QLast Update : Tue Nov 01 10:44:43 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

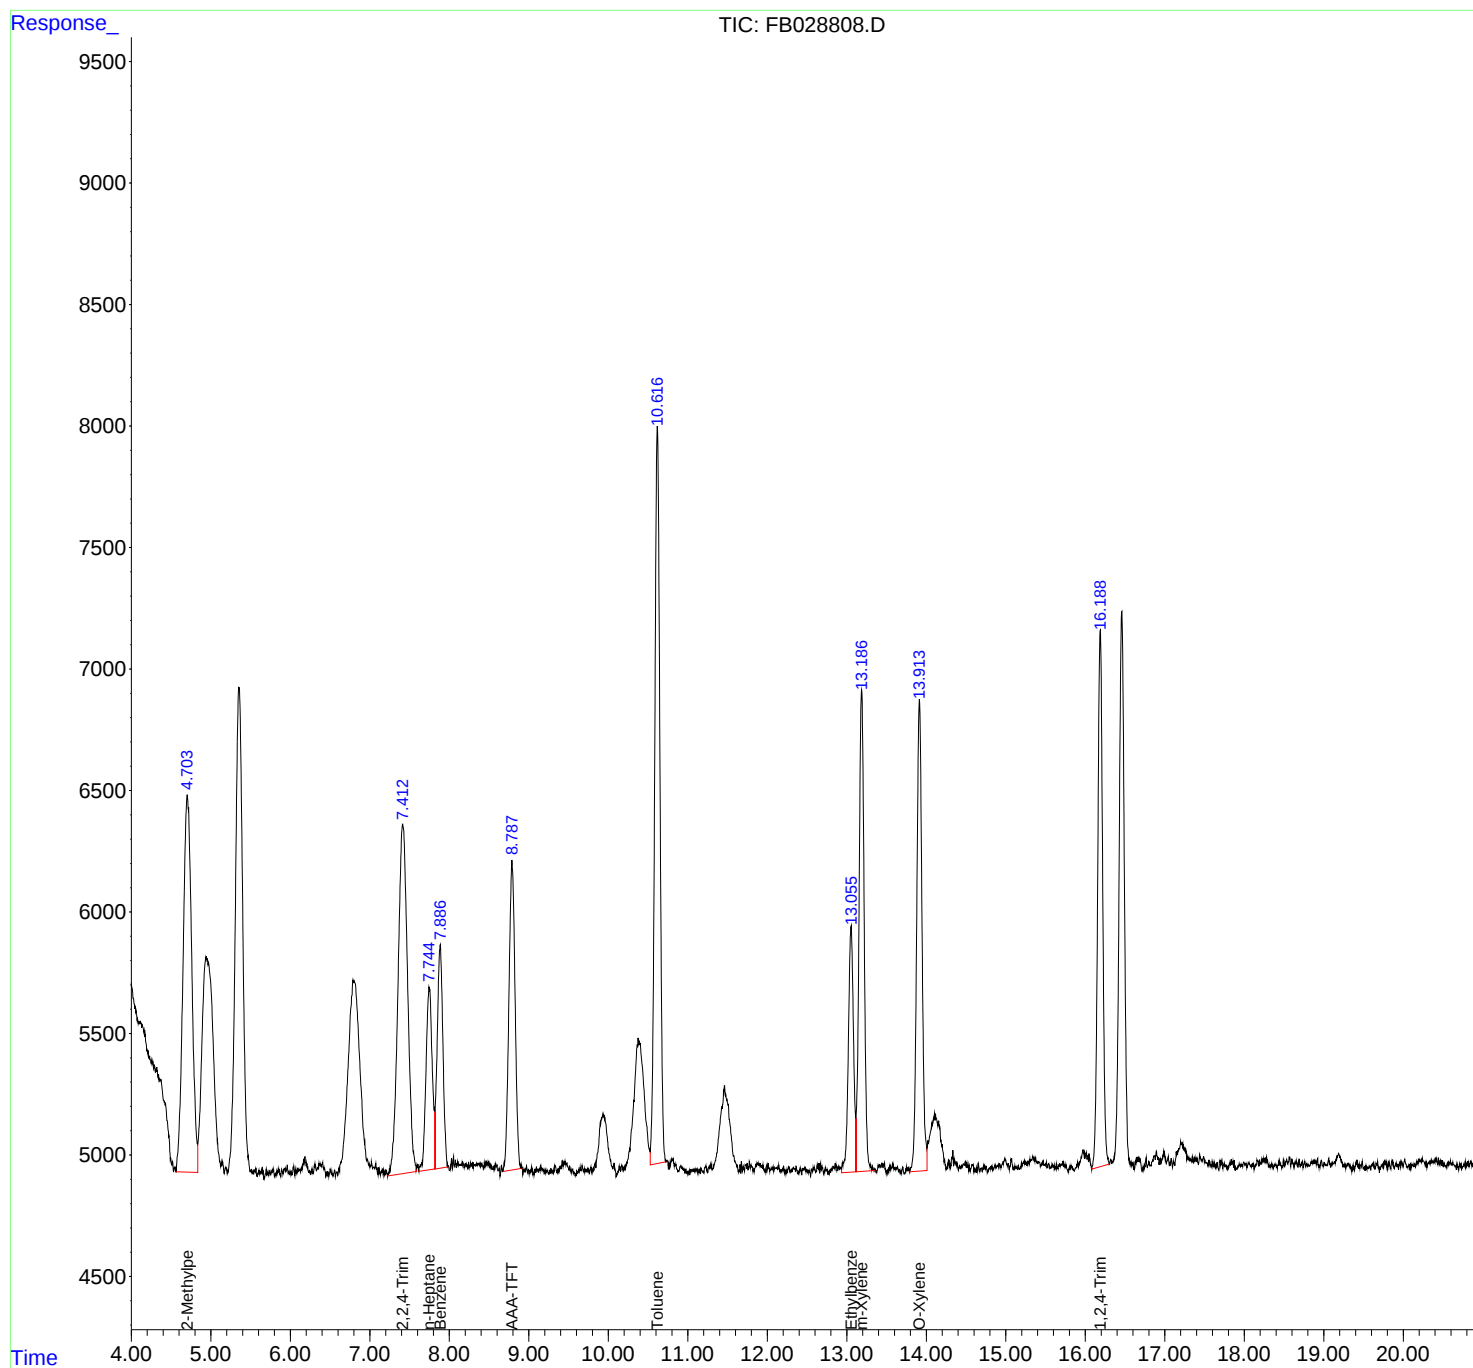


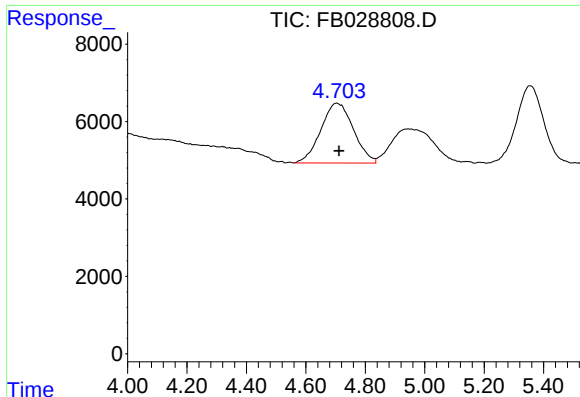

#1 2-Methylpentane


R.T.: 4.704 min
Delta R.T.: -0.008 min
Response: 117733
Conc: 6.95 ng/ml

Instrument :
FID_B
ClientSampleId :
5 GRO STD

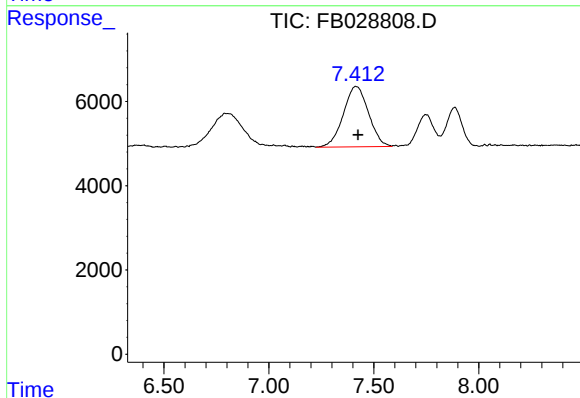


#2 2,2,4-Trimethylpentane

R.T.: 7.414 min
Delta R.T.: -0.011 min
Response: 119619
Conc: 6.56 ng/ml

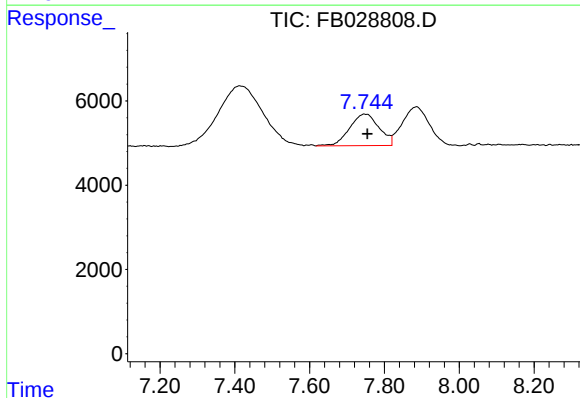


#3 n-Heptane

R.T.: 7.746 min
Delta R.T.: -0.008 min
Response: 41124
Conc: 2.23 ng/ml

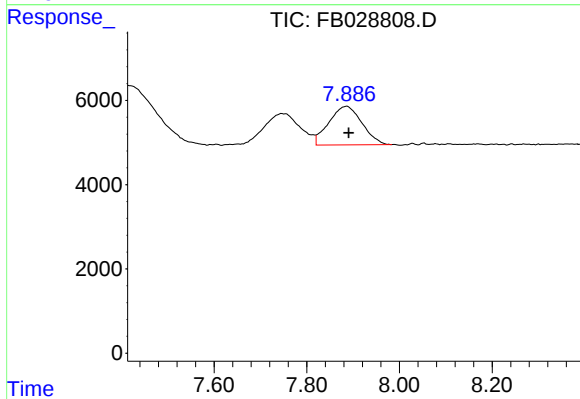

#4 Benzene


R.T.: 7.887 min
Delta R.T.: -0.003 min
Response: 45382
Conc: 2.12 ng/ml

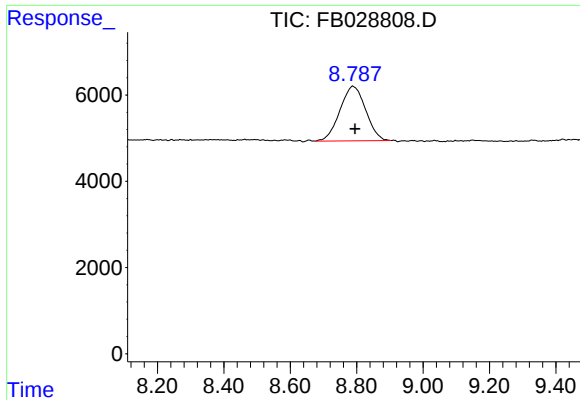

#5 AAA-TFT


R.T.: 8.789 min
Delta R.T.: -0.006 min
Response: 68060
Conc: 5.32 ng/ml

Instrument :
FID_B
ClientSampleId :
5 GRO STD

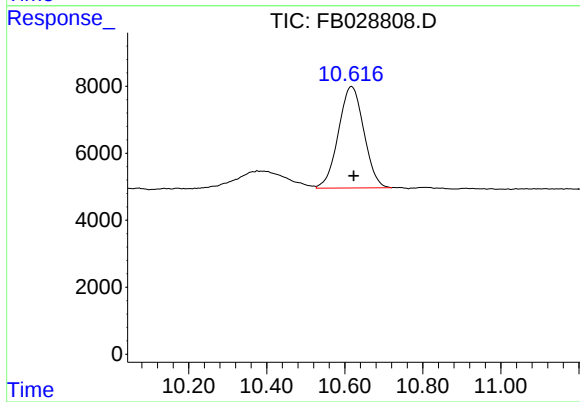


#6 Toluene

R.T.: 10.618 min
Delta R.T.: -0.005 min
Response: 137040
Conc: 6.53 ng/ml

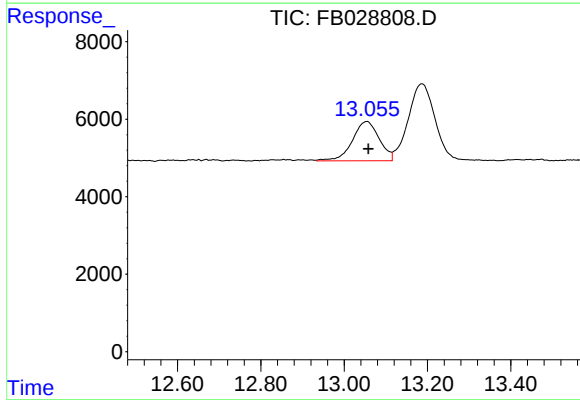


#7 Ethylbenzene

R.T.: 13.056 min
Delta R.T.: -0.002 min
Response: 45127
Conc: 2.28 ng/ml

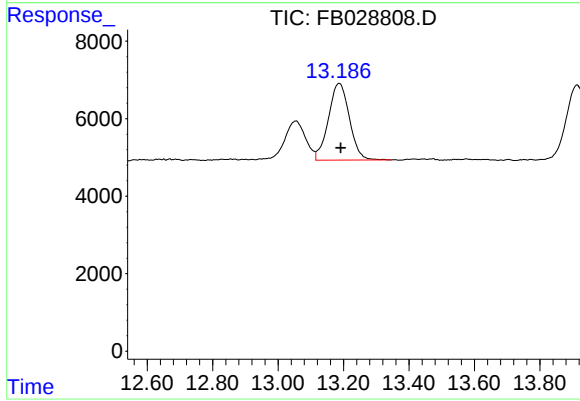

#8 m-Xylene


R.T.: 13.188 min
Delta R.T.: -0.004 min
Response: 88168
Conc: 4.47 ng/ml

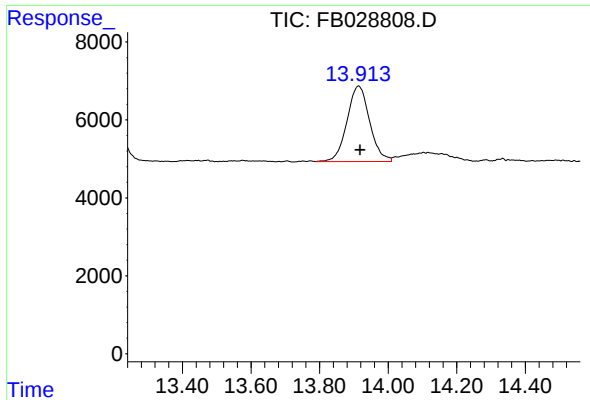

#9 O-Xylene

R.T.: 13.914 min
Delta R.T.: -0.004 min
Response: 88587
Conc: 4.67 ng/ml

Instrument :
FID_B
ClientSampleId :
5 GRO STD

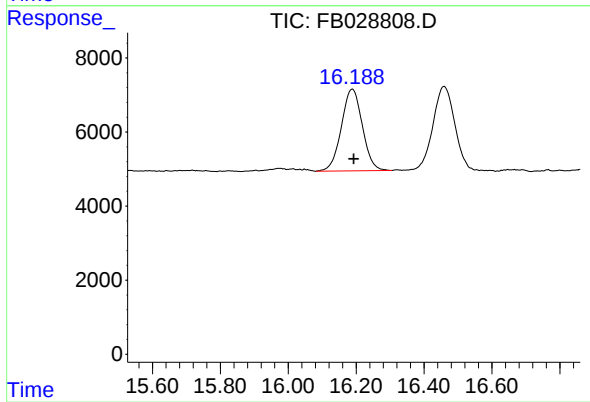

#10 1,2,4-Trimethylbenzene

R.T.: 16.189 min
Delta R.T.: -0.004 min
Response: 94824
Conc: 5.05 ng/ml