

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110122\
 Data File : FB028810.D
 Signal(s) : FID2B.CH
 Acq On : 1 Nov 2022 10:31
 Operator : AJ/MA
 Sample : 20 GRO STD
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 20 GRO STD

Integration File: Calibration.e
 Quant Time: Nov 01 10:45:00 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110122.M
 Quant Title :
 QLast Update : Tue Nov 01 10:44:43 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.795	255825	20.000 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.712	507880	30.000 ng/ml
2) t 2,2,4-Trimethylpentane	7.425	546804	30.000 ng/ml
3) t n-Heptane	7.755	184518	10.000 ng/ml
4) t Benzene	7.891	214306	10.000 ng/ml
6) t Toluene	10.623	629549	30.000 ng/ml
7) t Ethylbenzene	13.058	197988	10.000 ng/ml
8) t m-Xylene	13.191	394624	20.000 ng/ml
9) t O-Xylene	13.918	379053	20.000 ng/ml
10) t 1,2,4-Trimethylbenzene	16.193	375756	20.000 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110122\
Data File : FB028810.D
Signal(s) : FID2B.CH
Acq On : 1 Nov 2022 10:31
Operator : AJ/MA
Sample : 20 GRO STD
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
20 GRO STD

Integration File: Calibration.e
Quant Time: Nov 01 10:45:00 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110122.M
Quant Title :
QLast Update : Tue Nov 01 10:44:43 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

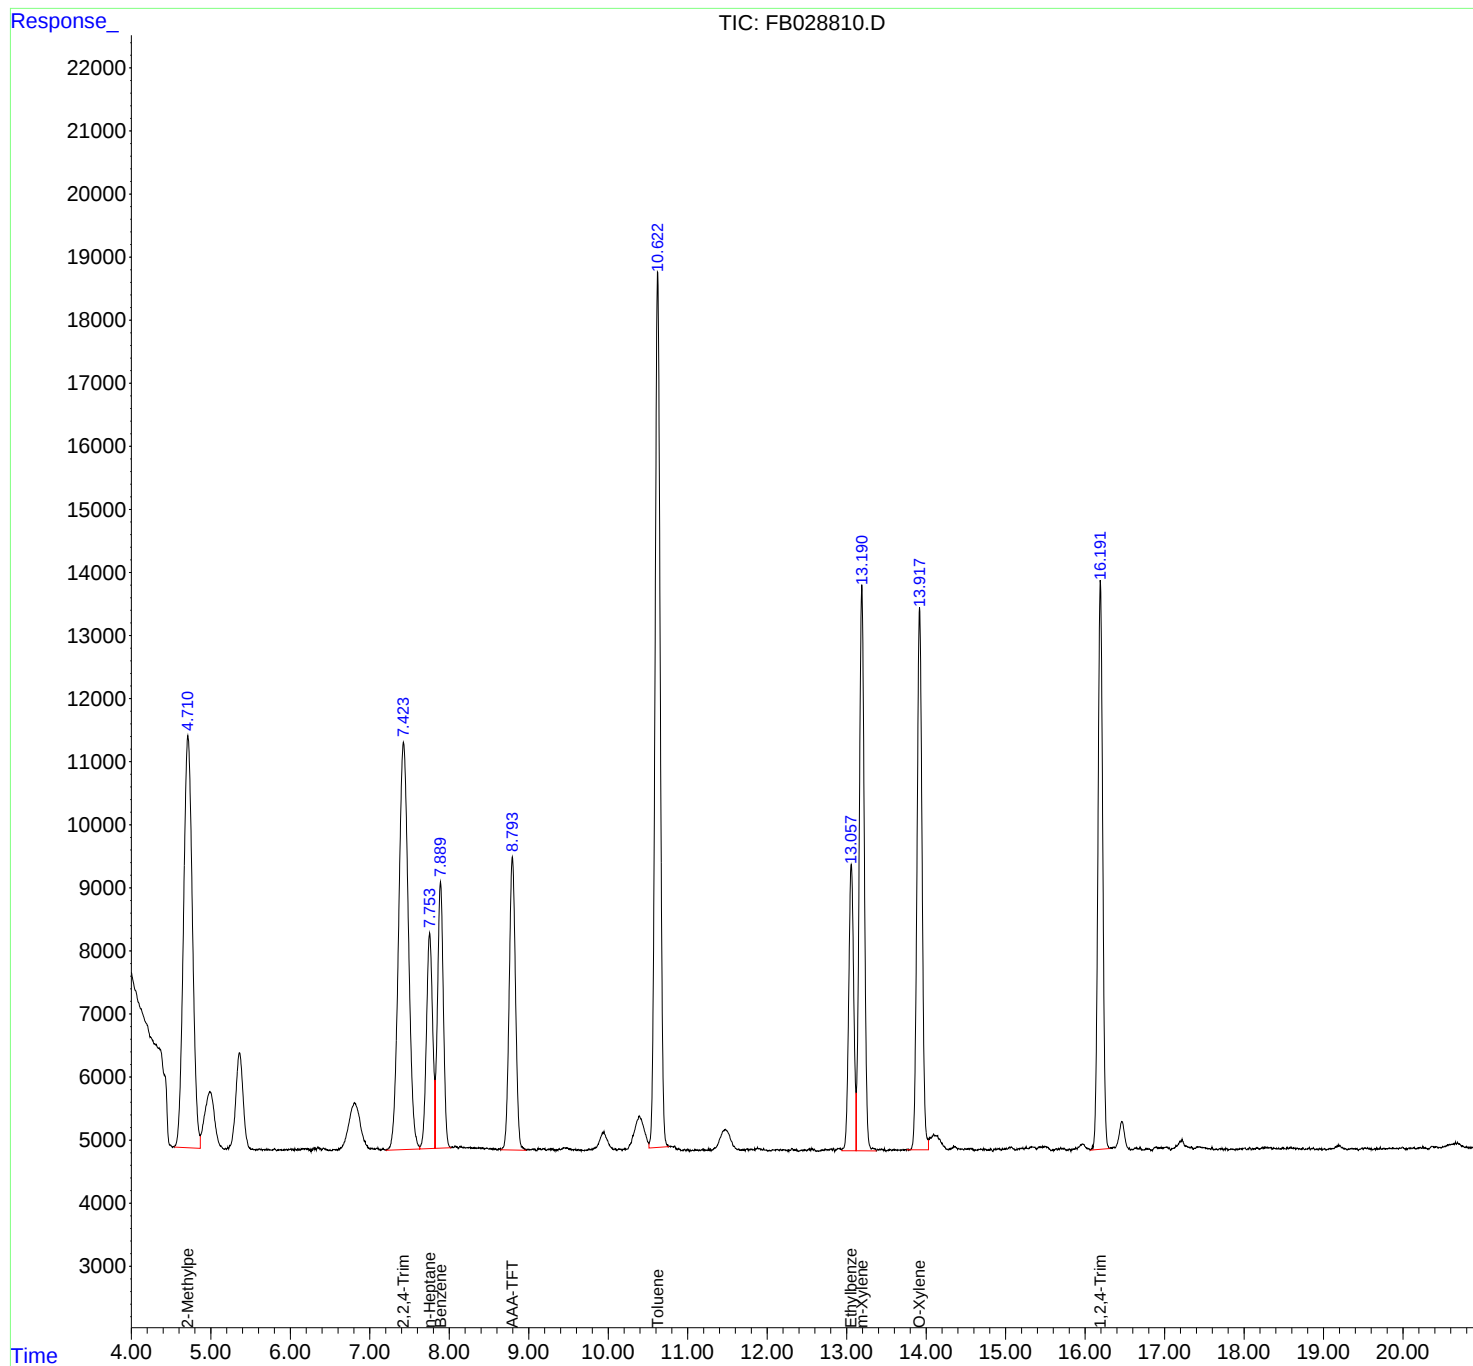


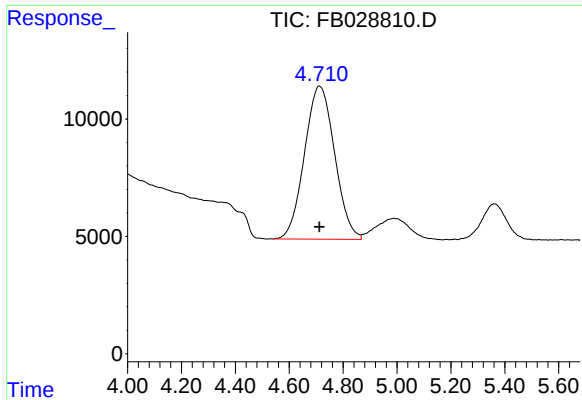

#1 2-Methylpentane


R.T.: 4.712 min
Delta R.T.: 0.000 min
Response: 507880
Conc: 30.00 ng/ml

Instrument :
FID_B
ClientSampleId :
20 GRO STD

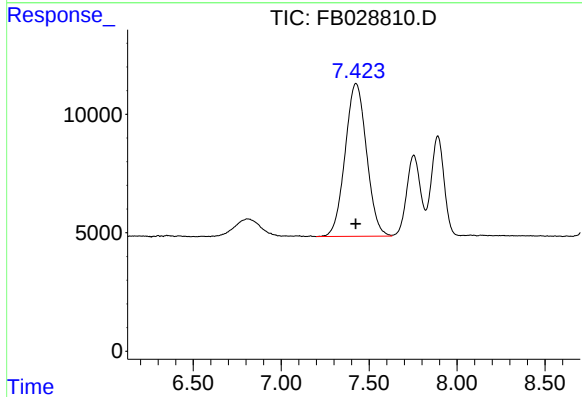


#2 2,2,4-Trimethylpentane

R.T.: 7.425 min
Delta R.T.: 0.000 min
Response: 546804
Conc: 30.00 ng/ml

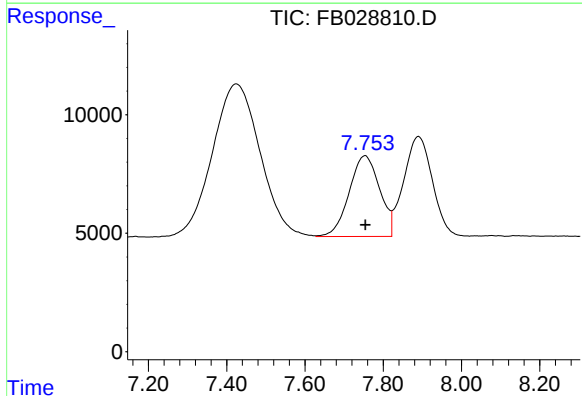


#3 n-Heptane

R.T.: 7.755 min
Delta R.T.: 0.000 min
Response: 184518
Conc: 10.00 ng/ml

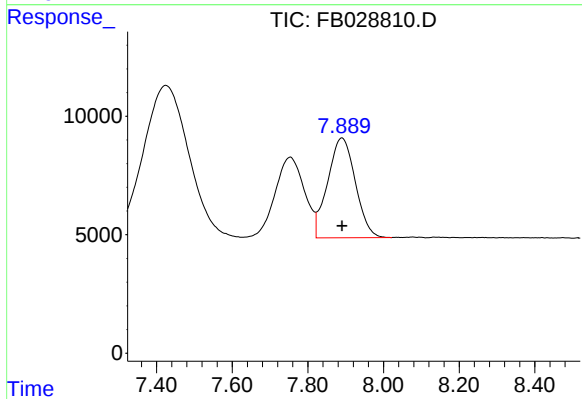

#4 Benzene


R.T.: 7.891 min
Delta R.T.: 0.000 min
Response: 214306
Conc: 10.00 ng/ml

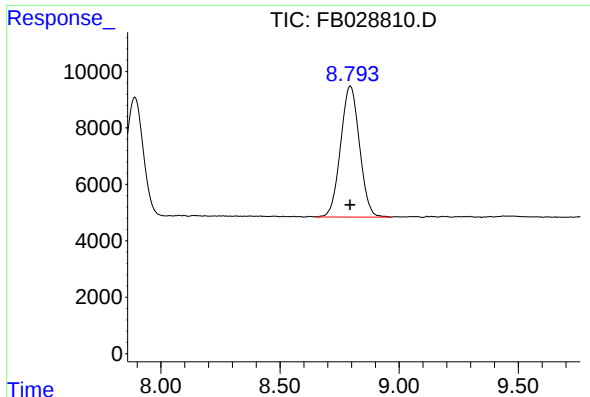

#5 AAA-TFT


R.T.: 8.795 min
Delta R.T.: 0.000 min
Response: 255825
Conc: 20.00 ng/ml

Instrument :
FID_B
ClientSampleId :
20 GRO STD

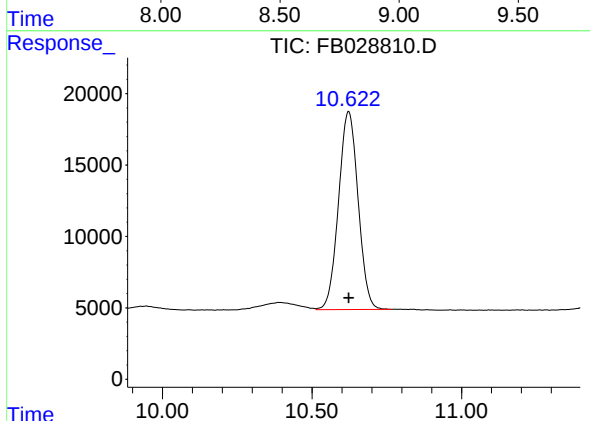


#6 Toluene

R.T.: 10.623 min
Delta R.T.: 0.000 min
Response: 629549
Conc: 30.00 ng/ml

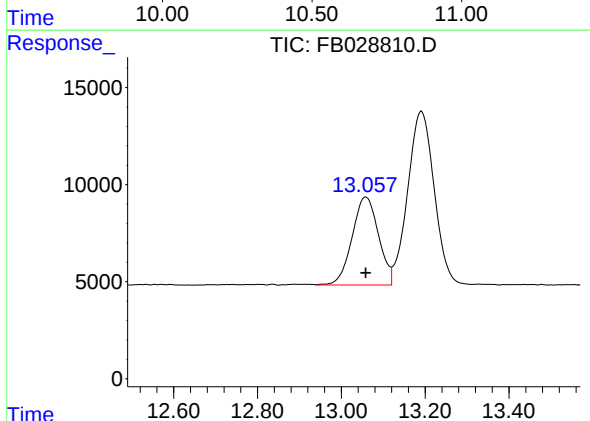


#7 Ethylbenzene

R.T.: 13.058 min
Delta R.T.: 0.000 min
Response: 197988
Conc: 10.00 ng/ml

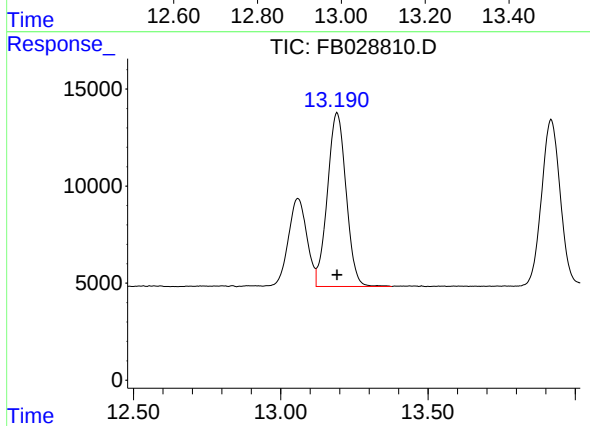

#8 m-Xylene


R.T.: 13.191 min
Delta R.T.: 0.000 min
Response: 394624
Conc: 20.00 ng/ml

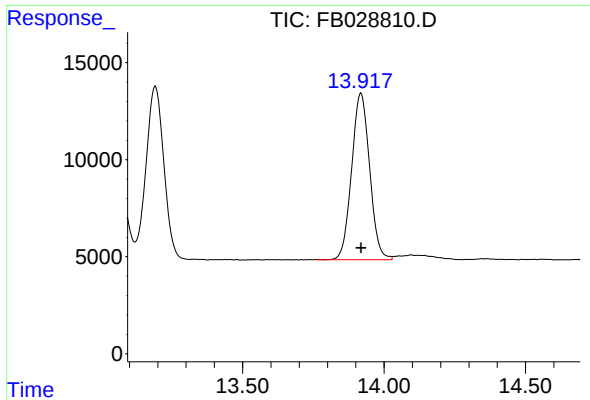

#9 O-Xylene

R.T.: 13.918 min
Delta R.T.: 0.000 min
Response: 379053
Conc: 20.00 ng/ml

Instrument :
FID_B
ClientSampleId :
20 GRO STD

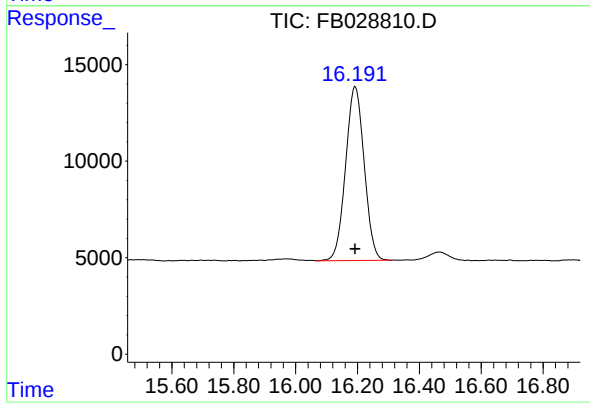

#10 1,2,4-Trimethylbenzene

R.T.: 16.193 min
Delta R.T.: 0.000 min
Response: 375756
Conc: 20.00 ng/ml