

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB110122\  
 Data File : FB028820.D  
 Signal(s) : FID2B.CH  
 Acq On : 1 Nov 2022 17:34  
 Operator : AJ/MA  
 Sample : BSF1101S2  
 Misc : 5.00G/5.00 ML DI WATER  
 ALS Vial : 13 Sample Multiplier: 1

Instrument :  
 FID\_B  
 ClientSampleId :  
 BSF1101S2

Integration File: Calibration.e  
 Quant Time: Nov 02 08:08:01 2022  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB110122.M  
 Quant Title :  
 QLast Update : Tue Nov 01 12:44:12 2022  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 5 g/ml  
 Signal Phase : RTX-502.2  
 Signal Info : 60mx0.53mmx3.00um

| Compound                     | R.T.   | Response | Conc Units   |
|------------------------------|--------|----------|--------------|
| -----                        |        |          |              |
| System Monitoring Compounds  |        |          |              |
| 5) s AAA-TFT                 | 8.800  | 264860   | 20.843 ng/ml |
| Target Compounds             |        |          |              |
| 1) t 2-Methylpentane         | 4.719  | 487744   | 29.923 ng/ml |
| 2) t 2,2,4-Trimethylpentane  | 7.434  | 534286   | 30.407 ng/ml |
| 3) t n-Heptane               | 7.759  | 176166   | 10.020 ng/ml |
| 4) t Benzene                 | 7.896  | 203827   | 9.940 ng/ml  |
| 6) t Toluene                 | 10.629 | 604721   | 30.066 ng/ml |
| 7) t Ethylbenzene            | 13.065 | 194214   | 10.240 ng/ml |
| 8) t m-Xylene                | 13.198 | 380575   | 20.229 ng/ml |
| 9) t O-Xylene                | 13.925 | 367275   | 20.020 ng/ml |
| 10) t 1,2,4-Trimethylbenzene | 16.199 | 366154   | 19.876 ng/ml |
| -----                        |        |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB110122\  
Data File : FB028820.D  
Signal(s) : FID2B.CH  
Acq On : 1 Nov 2022 17:34  
Operator : AJ/MA  
Sample : BSF1101S2  
Misc : 5.00G/5.00 ML DI WATER  
ALS Vial : 13 Sample Multiplier: 1

Instrument :  
FID\_B  
ClientSampleId :  
BSF1101S2

Integration File: Calibration.e  
Quant Time: Nov 02 08:08:01 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB110122.M  
Quant Title :  
QLast Update : Tue Nov 01 12:44:12 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

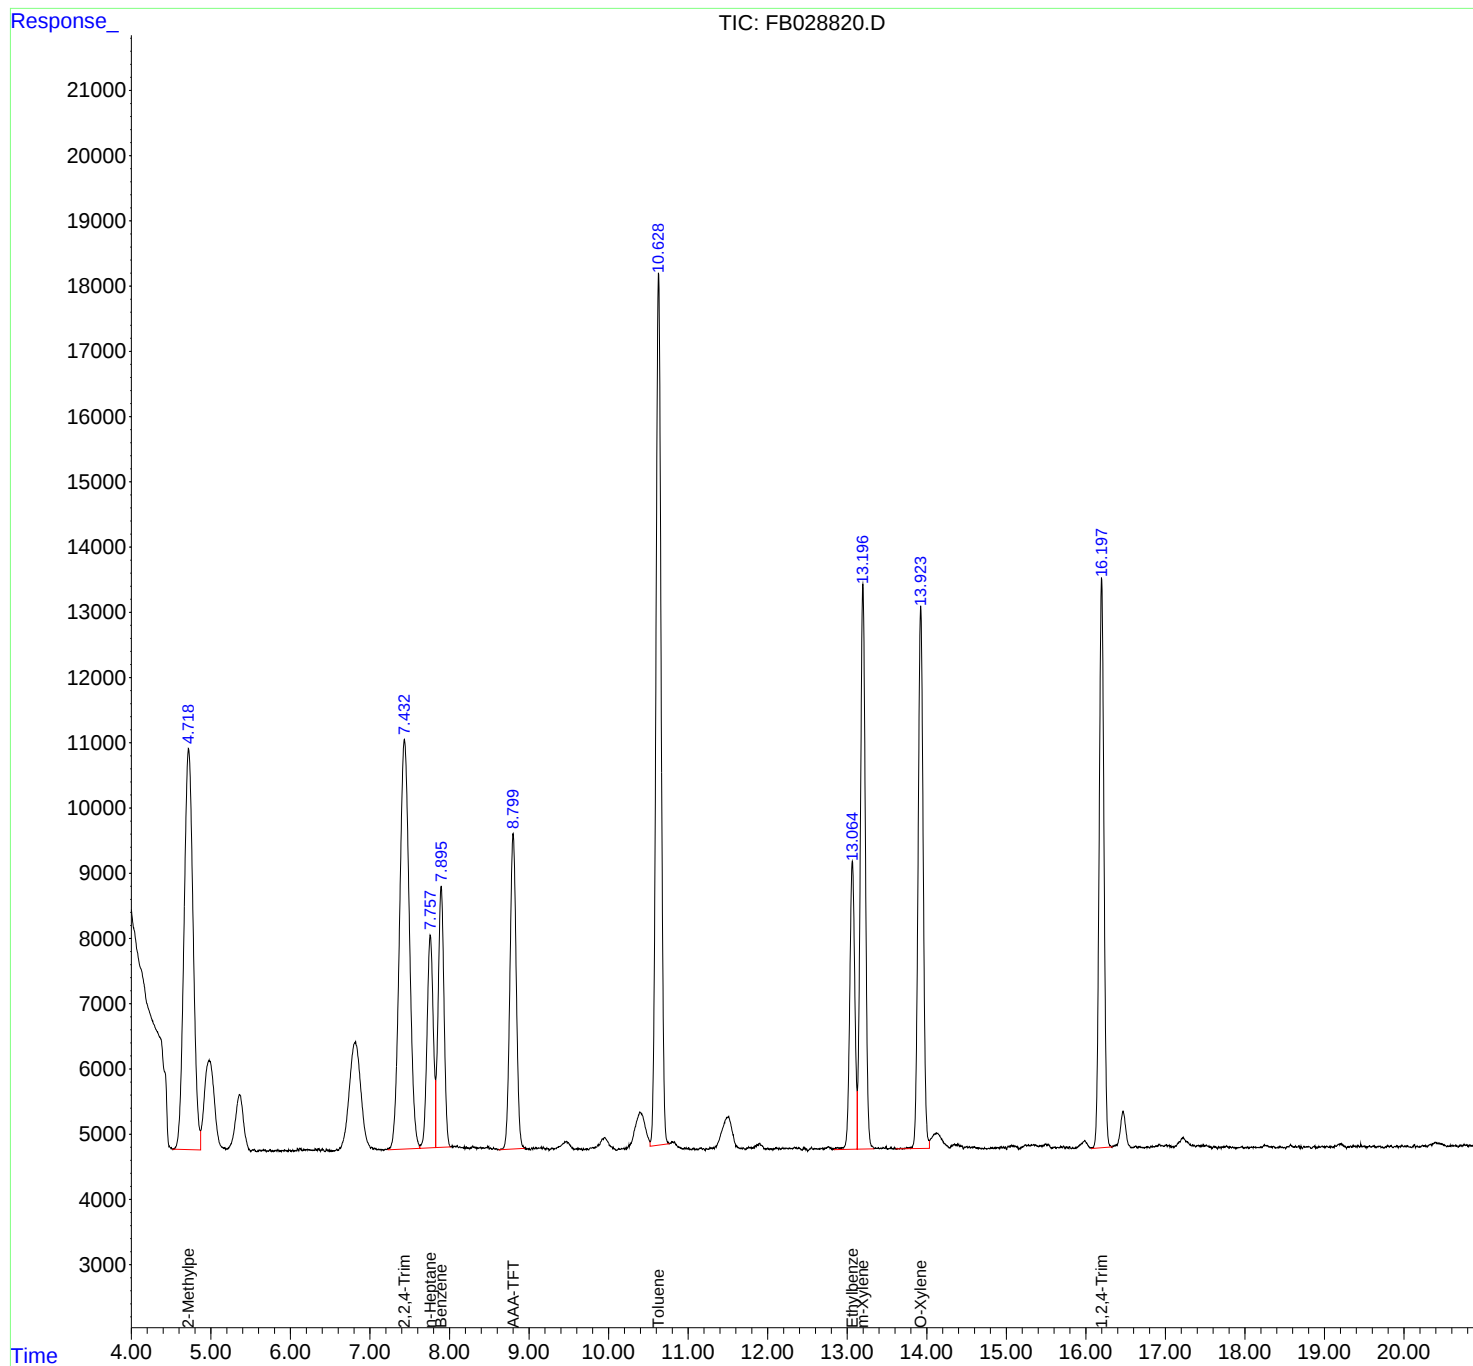


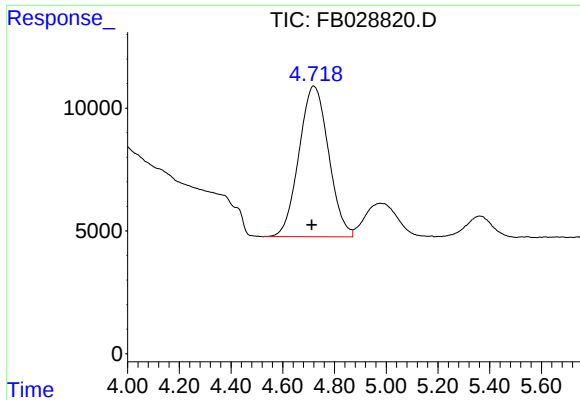

#1 2-Methylpentane


R.T.: 4.719 min  
Delta R.T.: 0.007 min  
Response: 487744  
Conc: 29.92 ng/ml

Instrument :  
FID\_B  
ClientSampleId :  
BSF1101S2

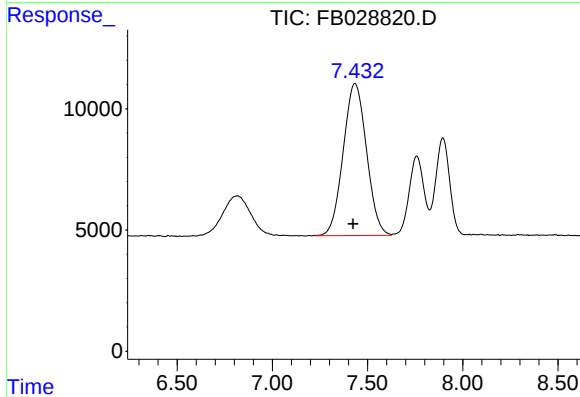


#2 2,2,4-Trimethylpentane

R.T.: 7.434 min  
Delta R.T.: 0.009 min  
Response: 534286  
Conc: 30.41 ng/ml

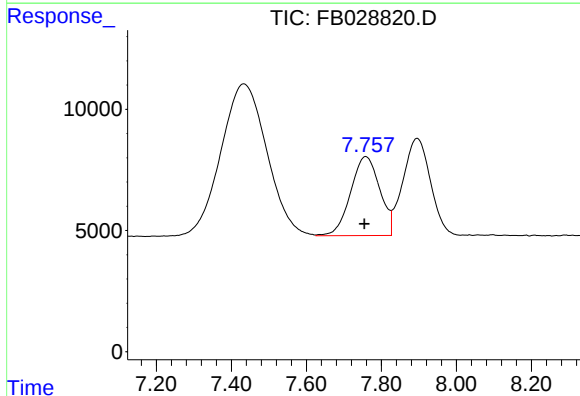


#3 n-Heptane

R.T.: 7.759 min  
Delta R.T.: 0.004 min  
Response: 176166  
Conc: 10.02 ng/ml

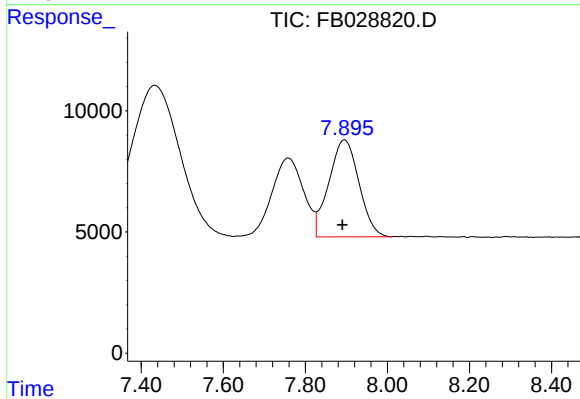

#4 Benzene


R.T.: 7.896 min  
Delta R.T.: 0.005 min  
Response: 203827  
Conc: 9.94 ng/ml

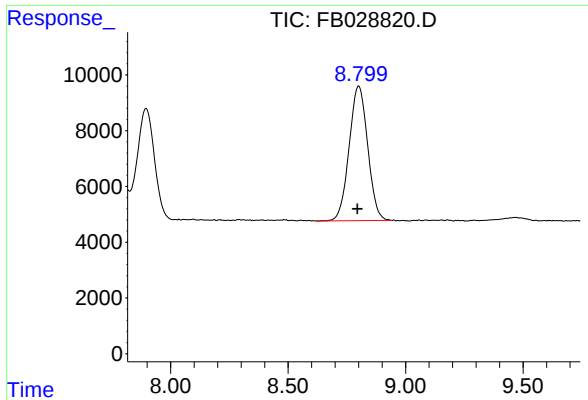

#5 AAA-TFT


R.T.: 8.800 min  
Delta R.T.: 0.006 min  
Response: 264860  
Conc: 20.84 ng/ml

Instrument :  
FID\_B  
ClientSampleId :  
BSF1101S2

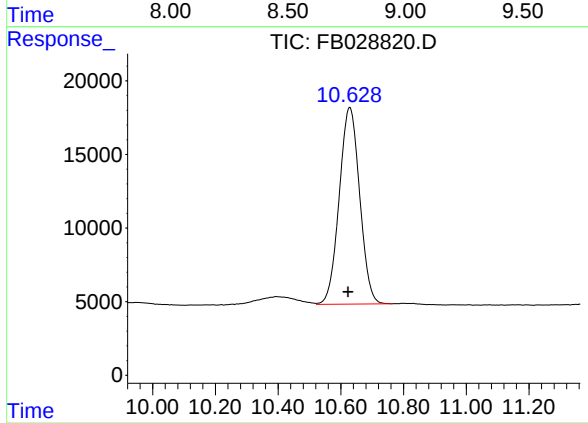


#6 Toluene

R.T.: 10.629 min  
Delta R.T.: 0.006 min  
Response: 604721  
Conc: 30.07 ng/ml

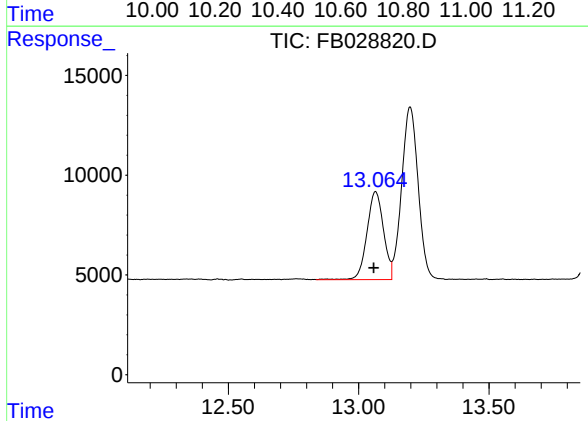


#7 Ethylbenzene

R.T.: 13.065 min  
Delta R.T.: 0.007 min  
Response: 194214  
Conc: 10.24 ng/ml

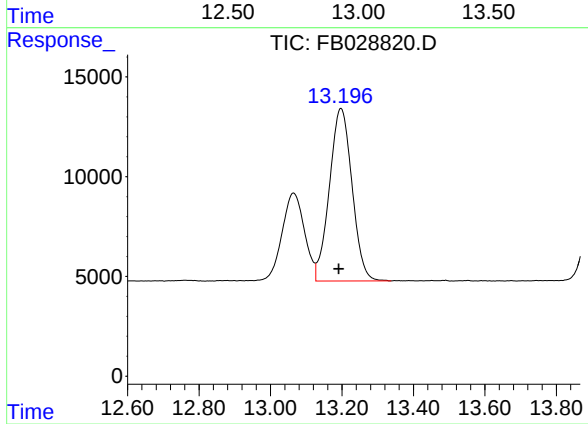

#8 m-Xylene


R.T.: 13.198 min  
Delta R.T.: 0.006 min  
Response: 380575  
Conc: 20.23 ng/ml

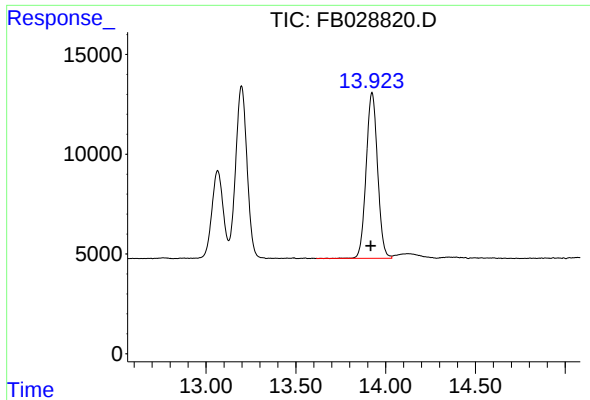

#9 O-Xylene

R.T.: 13.925 min  
Delta R.T.: 0.006 min  
Response: 367275  
Conc: 20.02 ng/ml

Instrument :  
FID\_B  
ClientSampleId :  
BSF1101S2

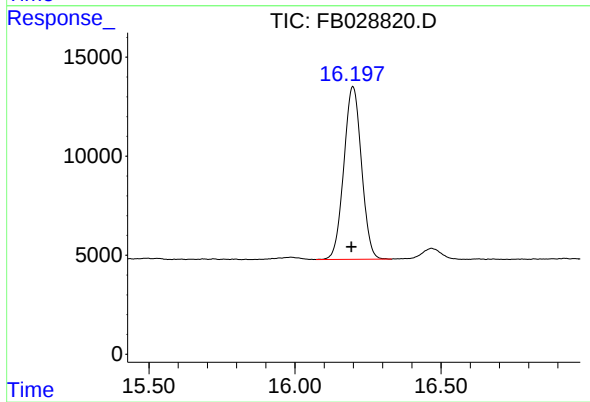

#10 1,2,4-Trimethylbenzene

R.T.: 16.199 min  
Delta R.T.: 0.006 min  
Response: 366154  
Conc: 19.88 ng/ml