

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110123\
 Data File : FB030420.D
 Signal(s) : FID2B.CH
 Acq On : 1 Nov 2023 10:38
 Operator : YP/AJ
 Sample : BSF1101S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Nov 01 23:50:57 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101023.M
 Quant Title :
 QLast Update : Tue Oct 10 11:38:40 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.784	205367	17.987 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.704	404497	28.911 ng/ml
2) t 2,2,4-Trimethylpentane	7.408	442537	26.803 ng/ml
3) t n-Heptane	7.744	147591	9.847 ng/ml
4) t Benzene	7.879	199128	9.706 ng/ml
6) t Toluene	10.611	592078	29.326 ng/ml
7) t Ethylbenzene	13.048	189822	9.510 ng/ml
8) t m-Xylene	13.180	373255	18.938 ng/ml
9) t O-Xylene	13.907	361026	18.343 ng/ml
10) t 1,2,4-Trimethylbenzene	16.182	359264	17.391 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110123\
Data File : FB030420.D
Signal(s) : FID2B.CH
Acq On : 1 Nov 2023 10:38
Operator : YP/AJ
Sample : BSF1101S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Nov 01 23:50:57 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101023.M
Quant Title :
QLast Update : Tue Oct 10 11:38:40 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

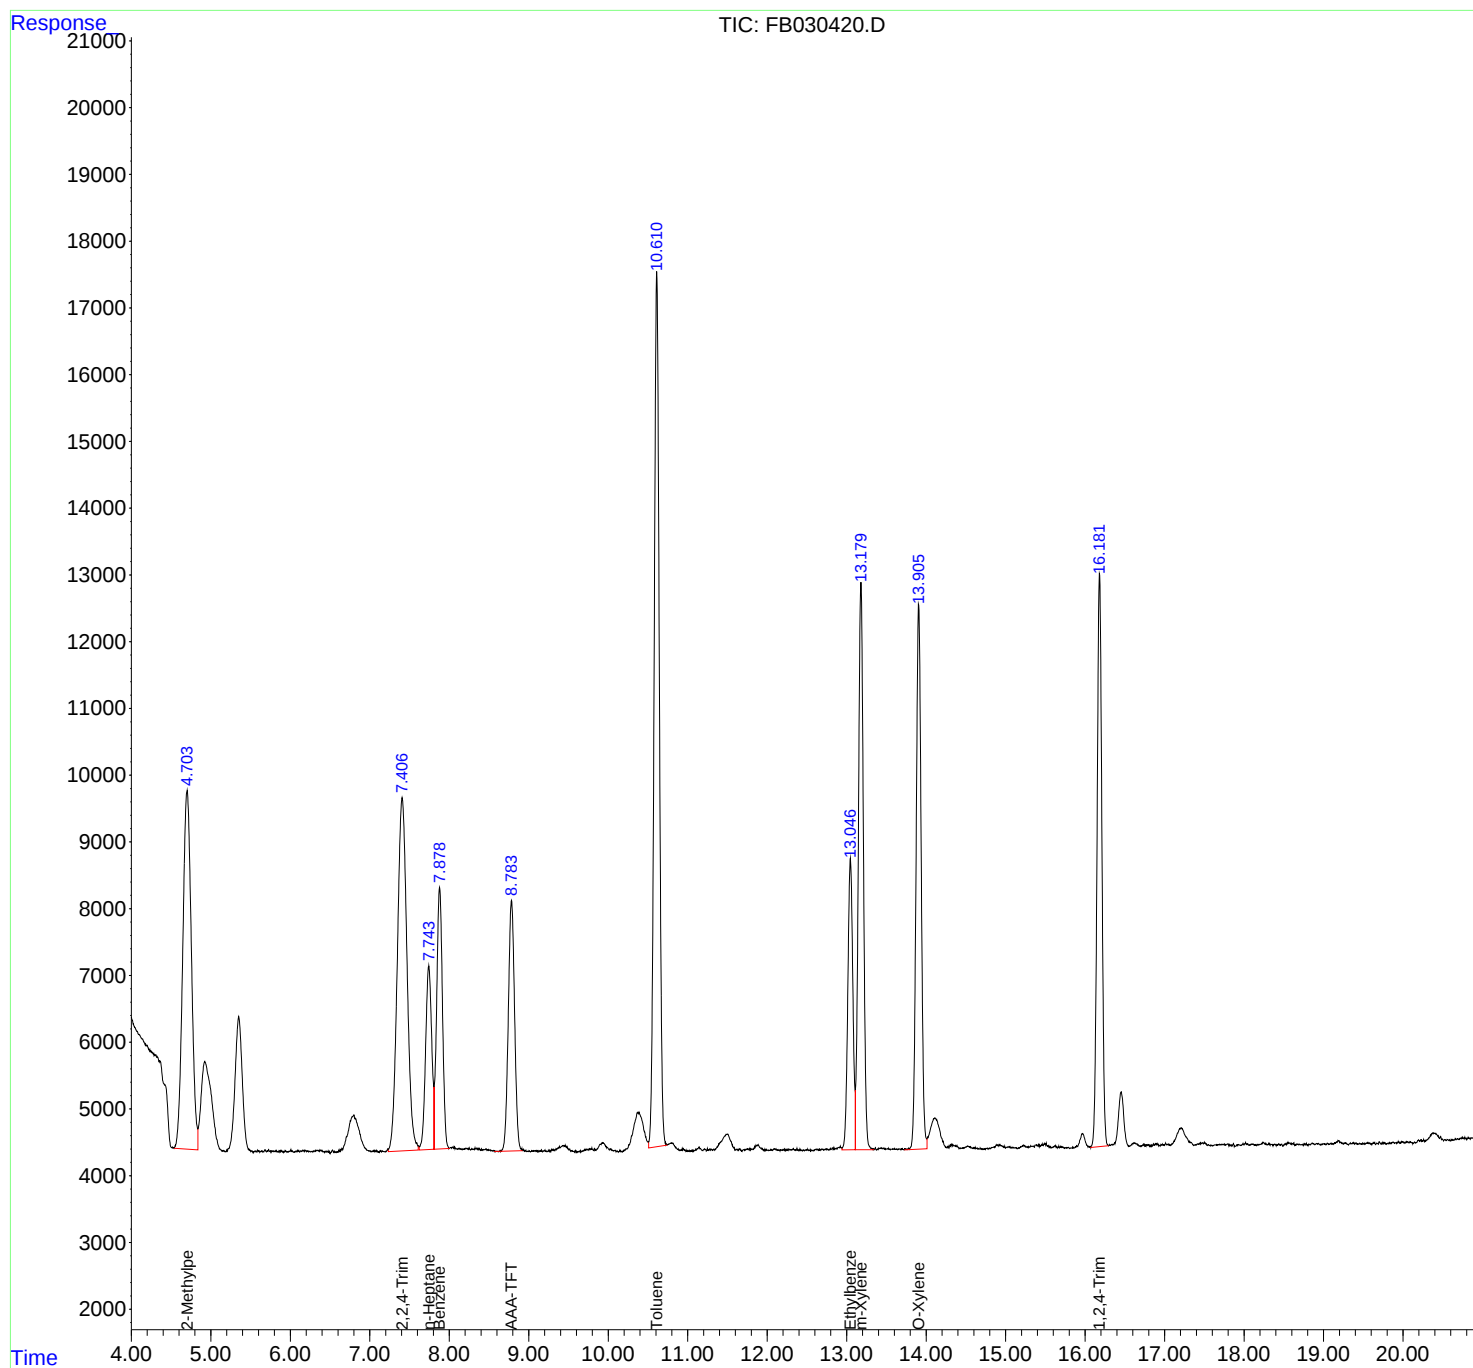

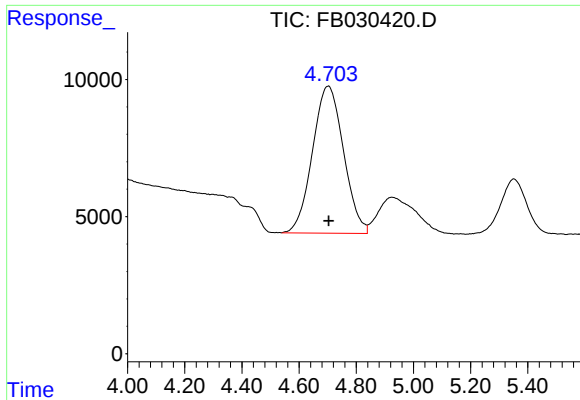


#1 2-Methylpentane

R.T.: 4.704 min
Delta R.T.: 0.000 min
Response: 404497
Conc: 28.91 ng/ml

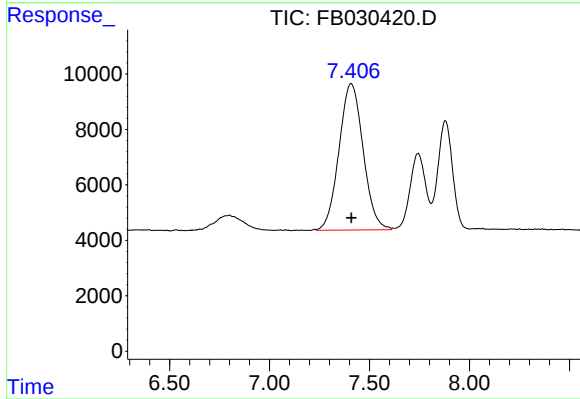


#2 2,2,4-Trimethylpentane

R.T.: 7.408 min
Delta R.T.: -0.002 min
Response: 442537
Conc: 26.80 ng/ml

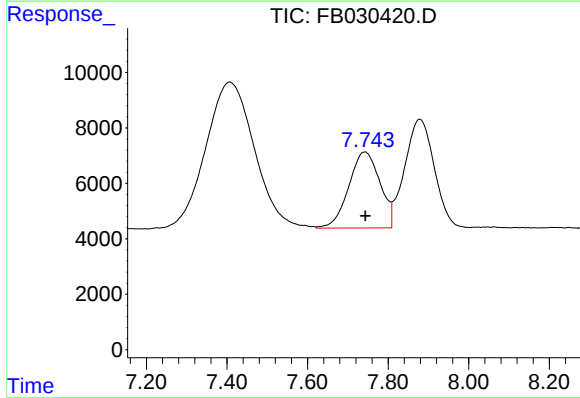


#3 n-Heptane

R.T.: 7.744 min
Delta R.T.: 0.000 min
Response: 147591
Conc: 9.85 ng/ml

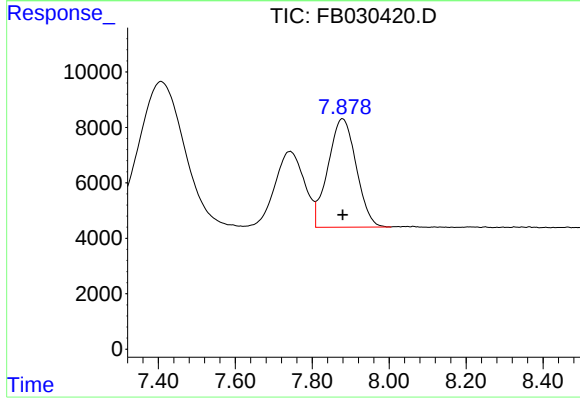


#4 Benzene

R.T.: 7.879 min
Delta R.T.: 0.000 min
Response: 199128
Conc: 9.71 ng/ml

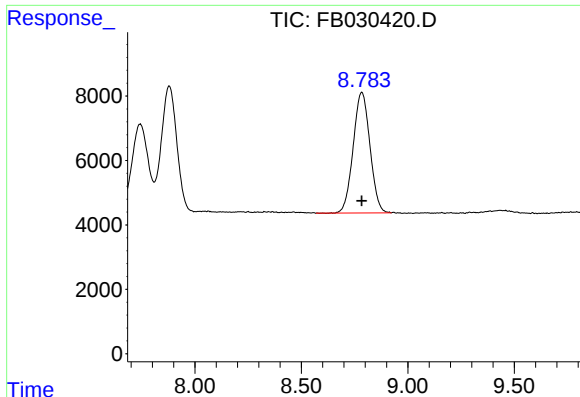


#5 AAA-TFT

R.T.: 8.784 min
Delta R.T.: 0.000 min
Response: 205367
Conc: 17.99 ng/ml

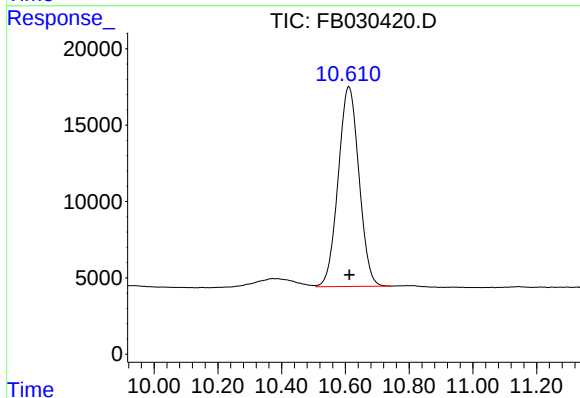


#6 Toluene

R.T.: 10.611 min
Delta R.T.: -0.001 min
Response: 592078
Conc: 29.33 ng/ml

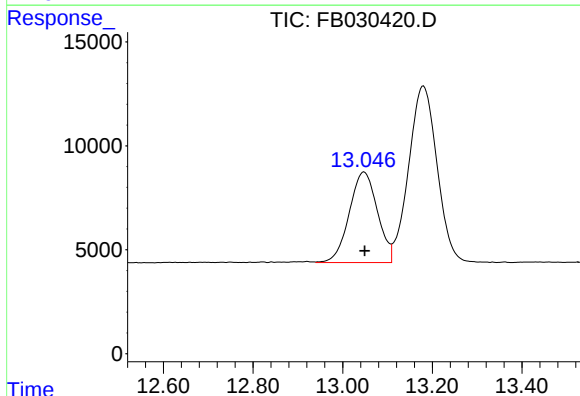


#7 Ethylbenzene

R.T.: 13.048 min
Delta R.T.: -0.002 min
Response: 189822
Conc: 9.51 ng/ml

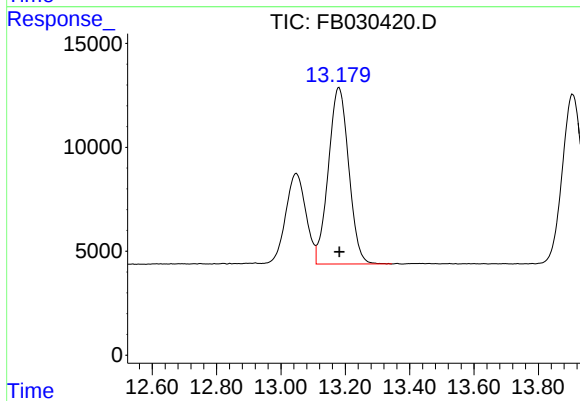


#8 m-Xylene

R.T.: 13.180 min
Delta R.T.: -0.001 min
Response: 373255
Conc: 18.94 ng/ml

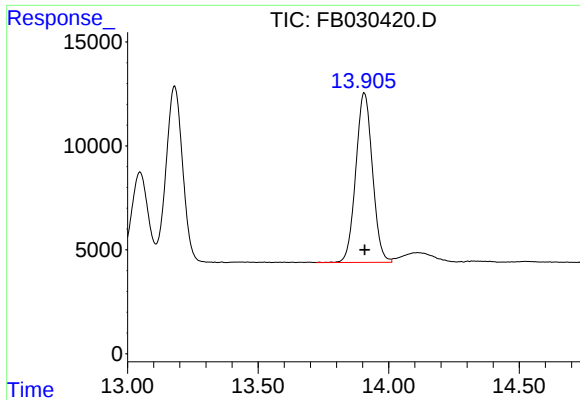

#9 O-Xylene

R.T.: 13.907 min
Delta R.T.: -0.002 min
Response: 361026
Conc: 18.34 ng/ml

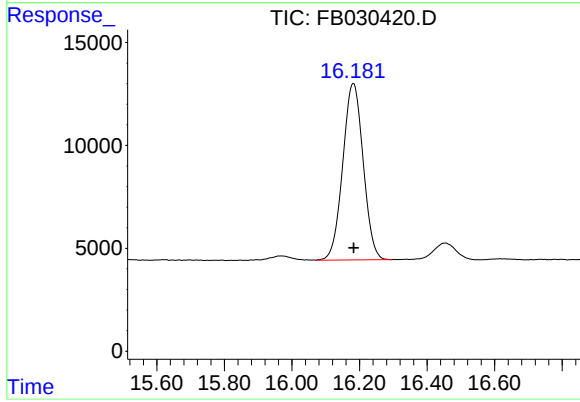

#10 1,2,4-Trimethylbenzene

R.T.: 16.182 min
Delta R.T.: -0.001 min
Response: 359264
Conc: 17.39 ng/ml