

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110123\
 Data File : FB030422.D
 Signal(s) : FID2B.CH
 Acq On : 1 Nov 2023 13:27
 Operator : YP/AJ
 Sample : BSF1101S2
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 8 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Nov 02 00:24:01 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101023.M
 Quant Title :
 QLast Update : Tue Oct 10 11:38:40 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.783	167423	14.663 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.702	468249	33.467 ng/ml
2) t 2,2,4-Trimethylpentane	7.407	522251	31.632 ng/ml
3) t n-Heptane	7.742	170754	11.392 ng/ml
4) t Benzene	7.878	234990	11.454 ng/ml
6) t Toluene	10.610	693865	34.368 ng/ml
7) t Ethylbenzene	13.045	221222	11.083 ng/mlm
8) t m-Xylene	13.179	433984	22.019 ng/ml
9) t O-Xylene	13.906	426025	21.646 ng/ml
10) t 1,2,4-Trimethylbenzene	16.181	426302	20.636 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110123\
Data File : FB030422.D
Signal(s) : FID2B.CH
Acq On : 1 Nov 2023 13:27
Operator : YP/AJ
Sample : BSF1101S2
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 8 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Nov 02 00:24:01 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101023.M
Quant Title :
QLast Update : Tue Oct 10 11:38:40 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

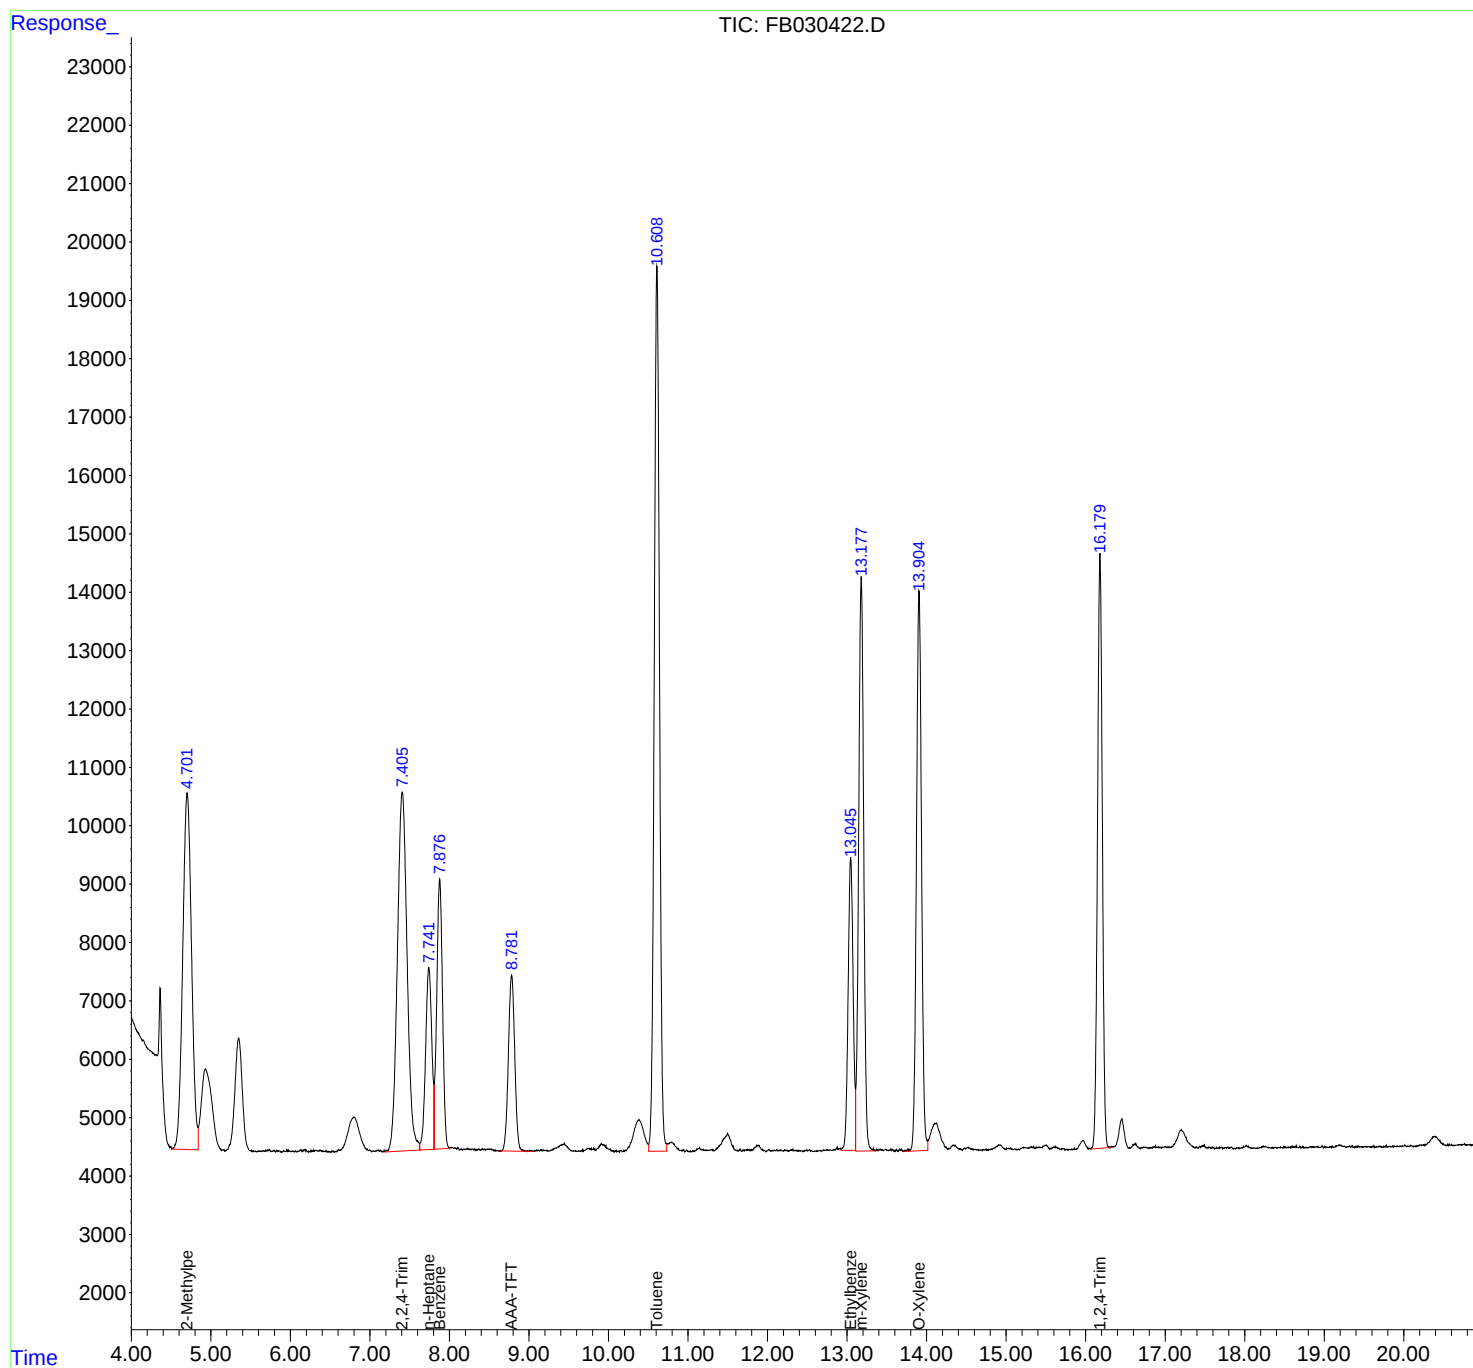

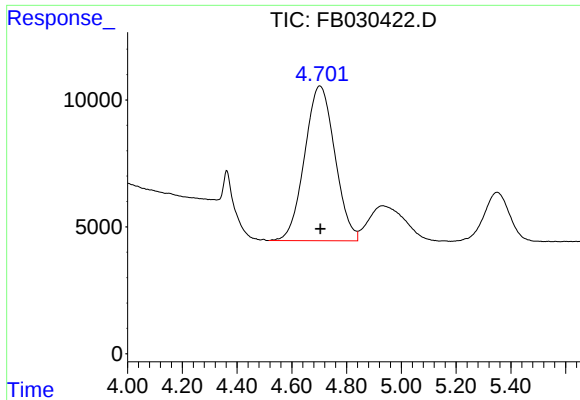


#1 2-Methylpentane

R.T.: 4.702 min
Delta R.T.: -0.002 min
Response: 468249
Conc: 33.47 ng/ml

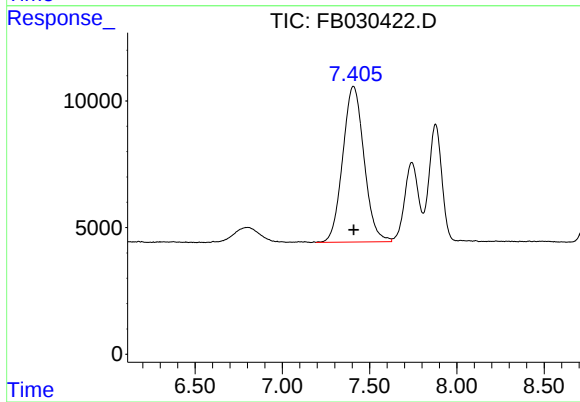


#2 2,2,4-Trimethylpentane

R.T.: 7.407 min
Delta R.T.: -0.002 min
Response: 522251
Conc: 31.63 ng/ml

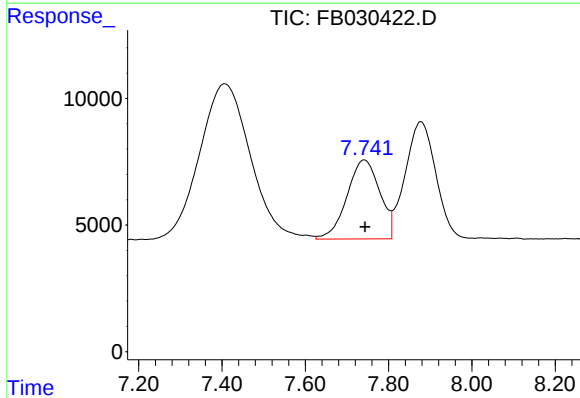


#3 n-Heptane

R.T.: 7.742 min
Delta R.T.: -0.002 min
Response: 170754
Conc: 11.39 ng/ml

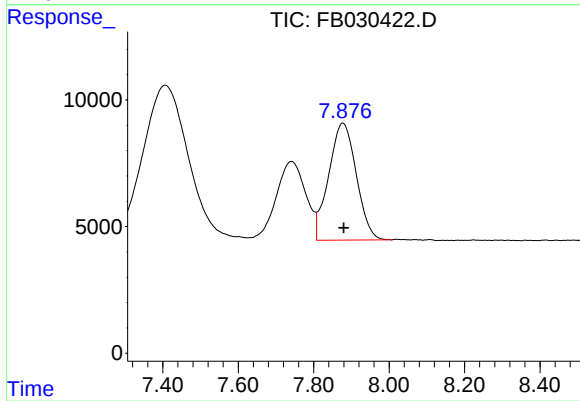


#4 Benzene

R.T.: 7.878 min
Delta R.T.: -0.002 min
Response: 234990
Conc: 11.45 ng/ml

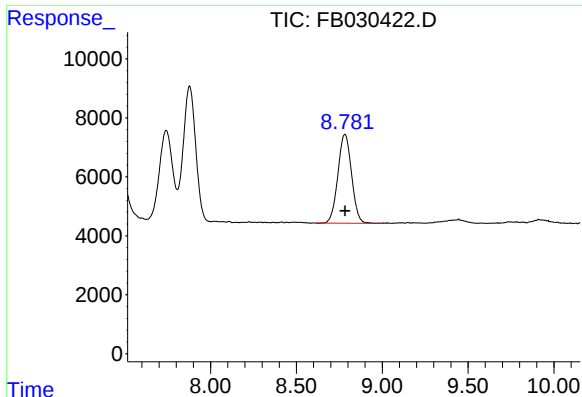


#5 AAA-TFT

R.T.: 8.783 min
Delta R.T.: -0.002 min
Response: 167423
Conc: 14.66 ng/ml

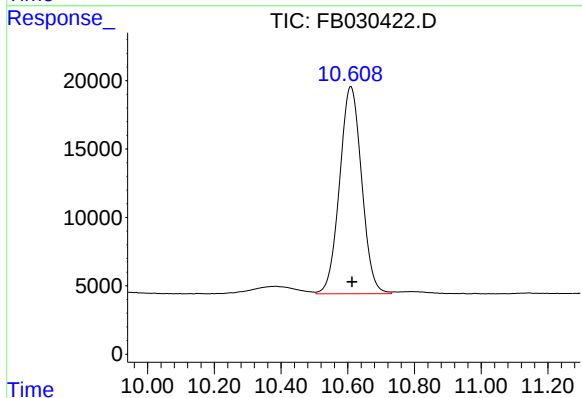


#6 Toluene

R.T.: 10.610 min
Delta R.T.: -0.003 min
Response: 693865
Conc: 34.37 ng/ml

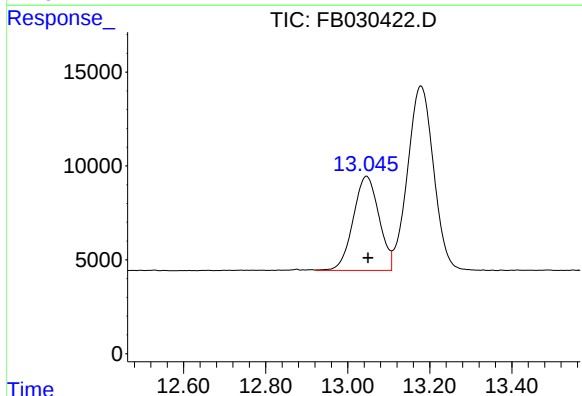


#7 Ethylbenzene

R.T.: 13.045 min
Delta R.T.: -0.004 min
Response: 221222
Conc: 11.08 ng/ml m

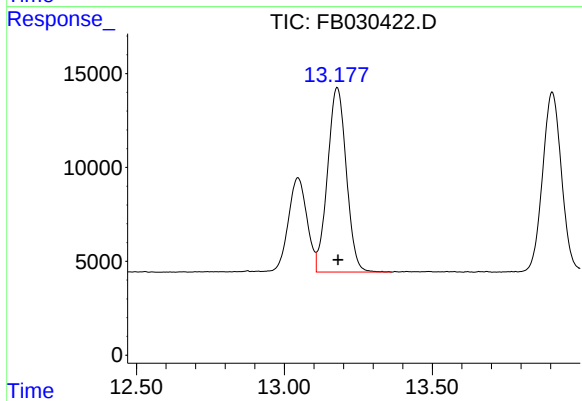


#8 m-Xylene

R.T.: 13.179 min
Delta R.T.: -0.003 min
Response: 433984
Conc: 22.02 ng/ml

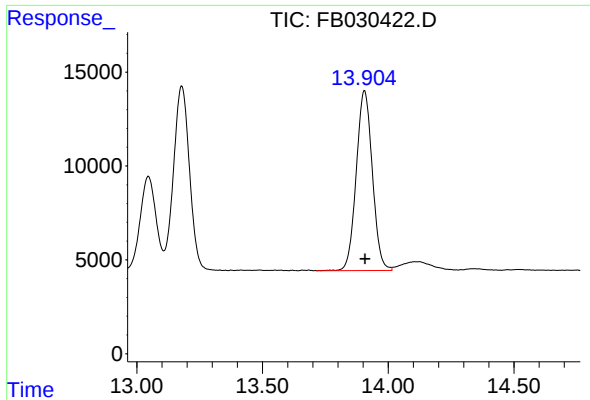

#9 O-Xylene

R.T.: 13.906 min
Delta R.T.: -0.003 min
Response: 426025
Conc: 21.65 ng/ml

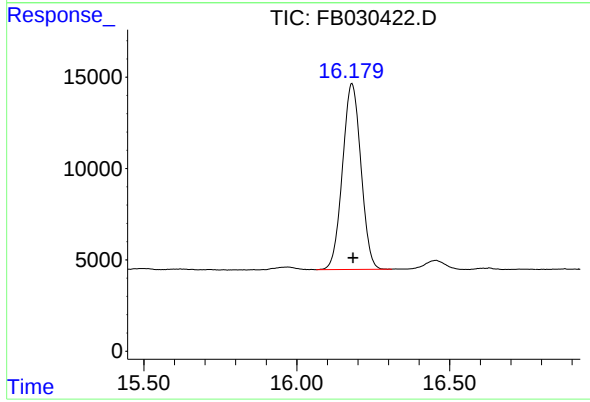

#10 1,2,4-Trimethylbenzene

R.T.: 16.181 min
Delta R.T.: -0.003 min
Response: 426302
Conc: 20.64 ng/ml