

Data Path : \\74.0.250.170\Terastorage\pestpcbsrv\HPCHEM1\FID_B\Data\FB110218\
 Data File : FB018452.D
 Signal(s) : FID2B.CH
 Acq On : 2 Nov 2018 12:03
 Operator : MJ/SJ
 Sample : BSF1102S1
 Misc : 5.01g/5.00mL DI Water
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Nov 03 01:38:21 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101218.M
 Quant Title :
 QLast Update : Fri Oct 12 08:04:31 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.112	158646	18.420 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.961	472168	30.872 ng/ml
2) t 2,2,4-Trimethylpentane	7.728	489003	33.093 ng/ml
3) t n-Heptane	8.067	155190	10.951 ng/ml
4) t Benzene	8.206	202520	10.871 ng/ml
6) t Toluene	10.961	509911	33.457 ng/ml
7) t Ethylbenzene	13.410	157502	9.927 ng/ml
8) t m-Xylene	13.543	330862	19.885 ng/ml
9) t O-Xylene	14.275	346753	19.448 ng/ml
10) t 1,2,4-Trimethylbenzene	16.558	422801	20.783 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : \\74.0.250.170\Terastorage\pestpcbsrv\HPCHEM1\FID_B\Data\FB110218\
Data File : FB018452.D
Signal(s) : FID2B.CH
Acq On : 2 Nov 2018 12:03
Operator : MJ/SJ
Sample : BSF1102S1
Misc : 5.01g/5.00mL DI Water
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Nov 03 01:38:21 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101218.M
Quant Title :
QLast Update : Fri Oct 12 08:04:31 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

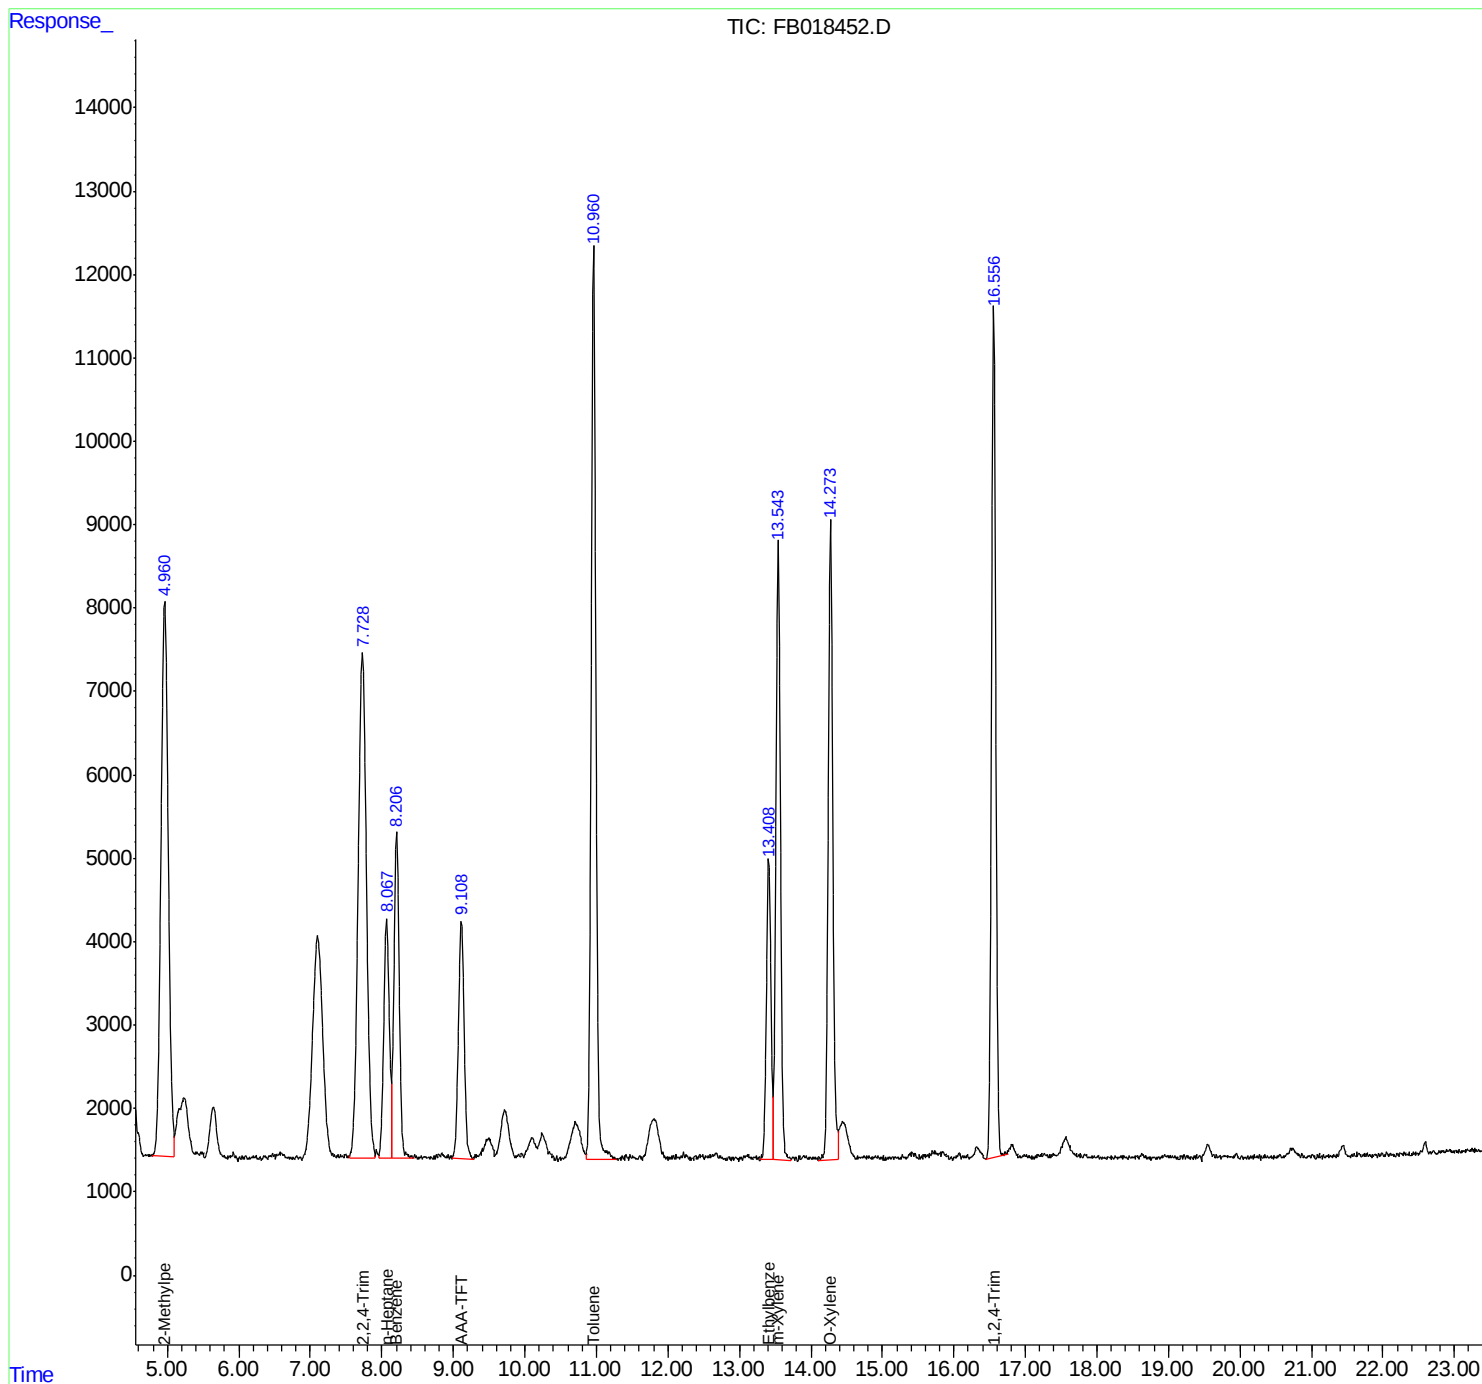

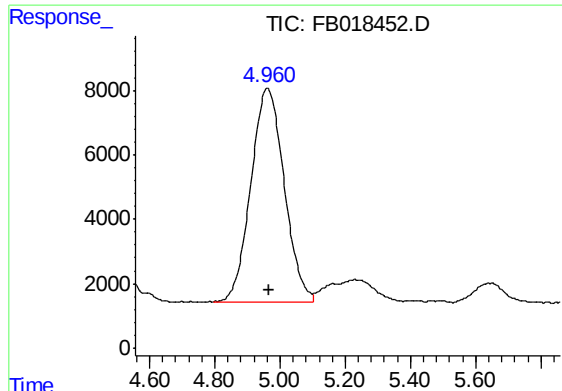


#1 2-Methylpentane

R.T.: 4.961 min
Delta R.T.: -0.004 min
Response: 472168
Conc: 30.87 ng/ml

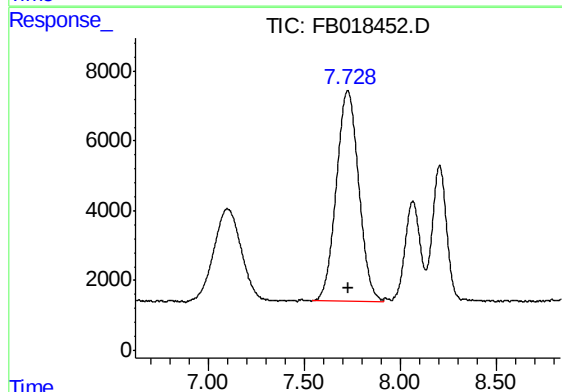


#2 2,2,4-Trimethylpentane

R.T.: 7.728 min
Delta R.T.: 0.000 min
Response: 489003
Conc: 33.09 ng/ml

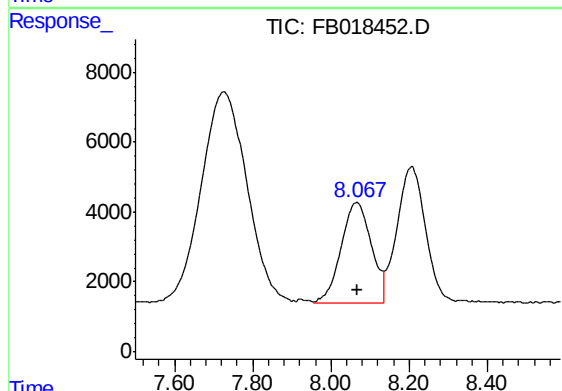


#3 n-Heptane

R.T.: 8.067 min
Delta R.T.: 0.000 min
Response: 155190
Conc: 10.95 ng/ml

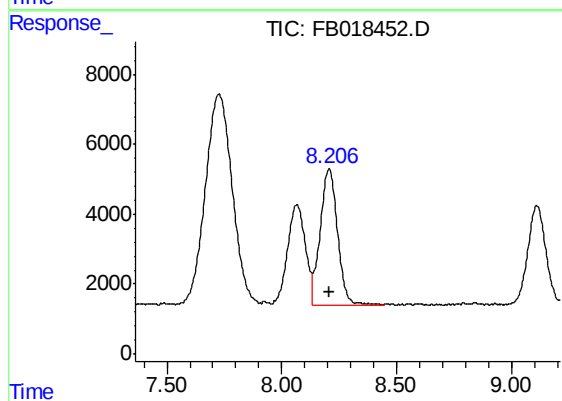


#4 Benzene

R.T.: 8.206 min
Delta R.T.: 0.000 min
Response: 202520
Conc: 10.87 ng/ml

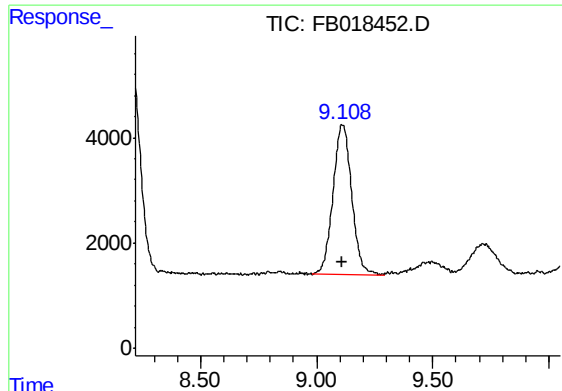


#5 AAA-TFT

R.T.: 9.112 min
Delta R.T.: 0.000 min
Response: 158646
Conc: 18.42 ng/ml

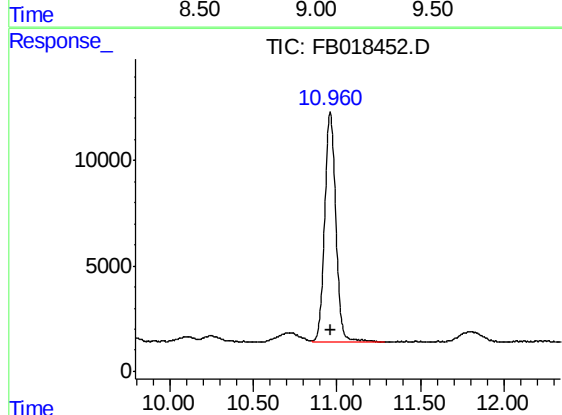


#6 Toluene

R.T.: 10.961 min
Delta R.T.: 0.000 min
Response: 509911
Conc: 33.46 ng/ml

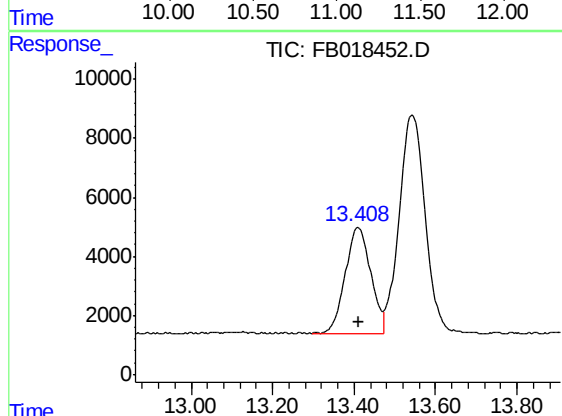


#7 Ethylbenzene

R.T.: 13.410 min
Delta R.T.: -0.002 min
Response: 157502
Conc: 9.93 ng/ml

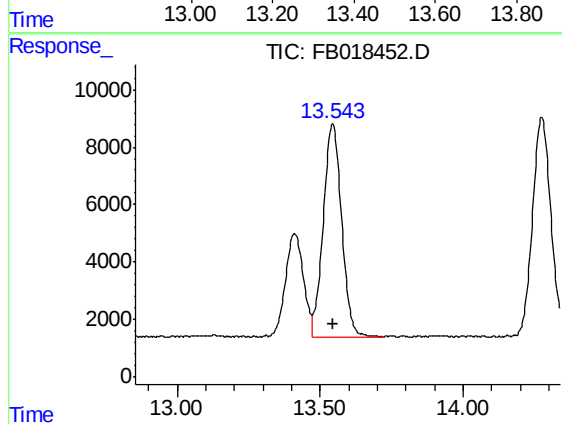


#8 m-Xylene

R.T.: 13.543 min
Delta R.T.: -0.001 min
Response: 330862
Conc: 19.88 ng/ml

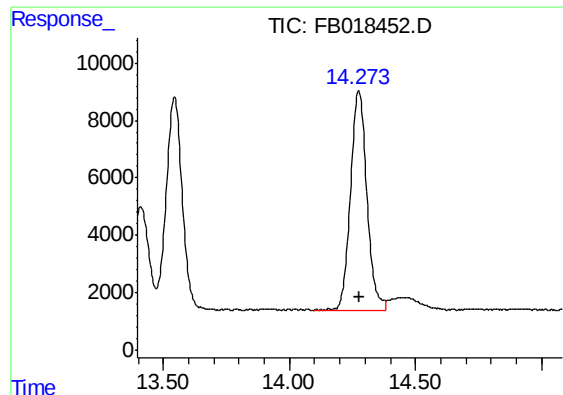

#9 O-Xylene

R.T.: 14.275 min
Delta R.T.: -0.001 min
Response: 346753
Conc: 19.45 ng/ml

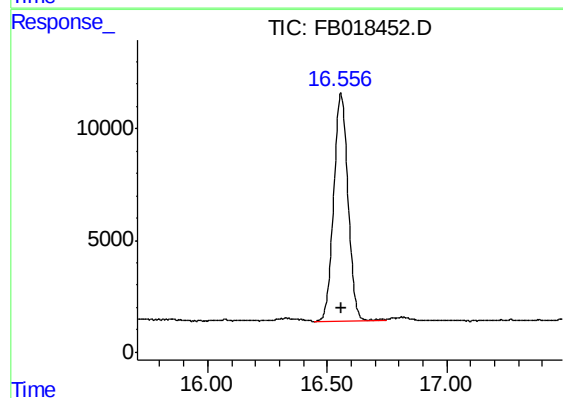

#10 1,2,4-Trimethylbenzene

R.T.: 16.558 min
Delta R.T.: -0.002 min
Response: 422801
Conc: 20.78 ng/ml