

Data Path : \\74.0.250.170\Terastorage\pestpcbsrv\HPCHEM1\FID_B\Data\FB110218\
 Data File : FB018485.D
 Signal(s) : FID2B.CH
 Acq On : 3 Nov 2018 5:42
 Operator : MJ/SJ
 Sample : J5741-32MS
 Misc : 5.00g/5.00mL DI Water
 ALS Vial : 38 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Nov 03 07:02:43 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101218.M
 Quant Title :
 QLast Update : Fri Oct 12 08:04:31 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.112	160625	18.649 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.962	408317	26.697 ng/ml
2) t 2,2,4-Trimethylpentane	7.728	424801	28.748 ng/ml
3) t n-Heptane	8.068	129166	9.115 ng/ml
4) t Benzene	8.207	167855	9.011 ng/ml
6) t Toluene	10.961	423130	27.763 ng/ml
7) t Ethylbenzene	13.411	144253	9.092 ng/ml
8) t m-Xylene	13.544	304386	18.294 ng/ml
9) t O-Xylene	14.276	329673	18.490 ng/ml
10) t 1,2,4-Trimethylbenzene	16.559	374814	18.424 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : \\74.0.250.170\Terastorage\pestpcbsrv\HPCHEM1\FID_B\Data\FB110218\
Data File : FB018485.D
Signal(s) : FID2B.CH
Acq On : 3 Nov 2018 5:42
Operator : MJ/SJ
Sample : J5741-32MS
Misc : 5.00g/5.00mL DI Water
ALS Vial : 38 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Nov 03 07:02:43 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101218.M
Quant Title :
QLast Update : Fri Oct 12 08:04:31 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

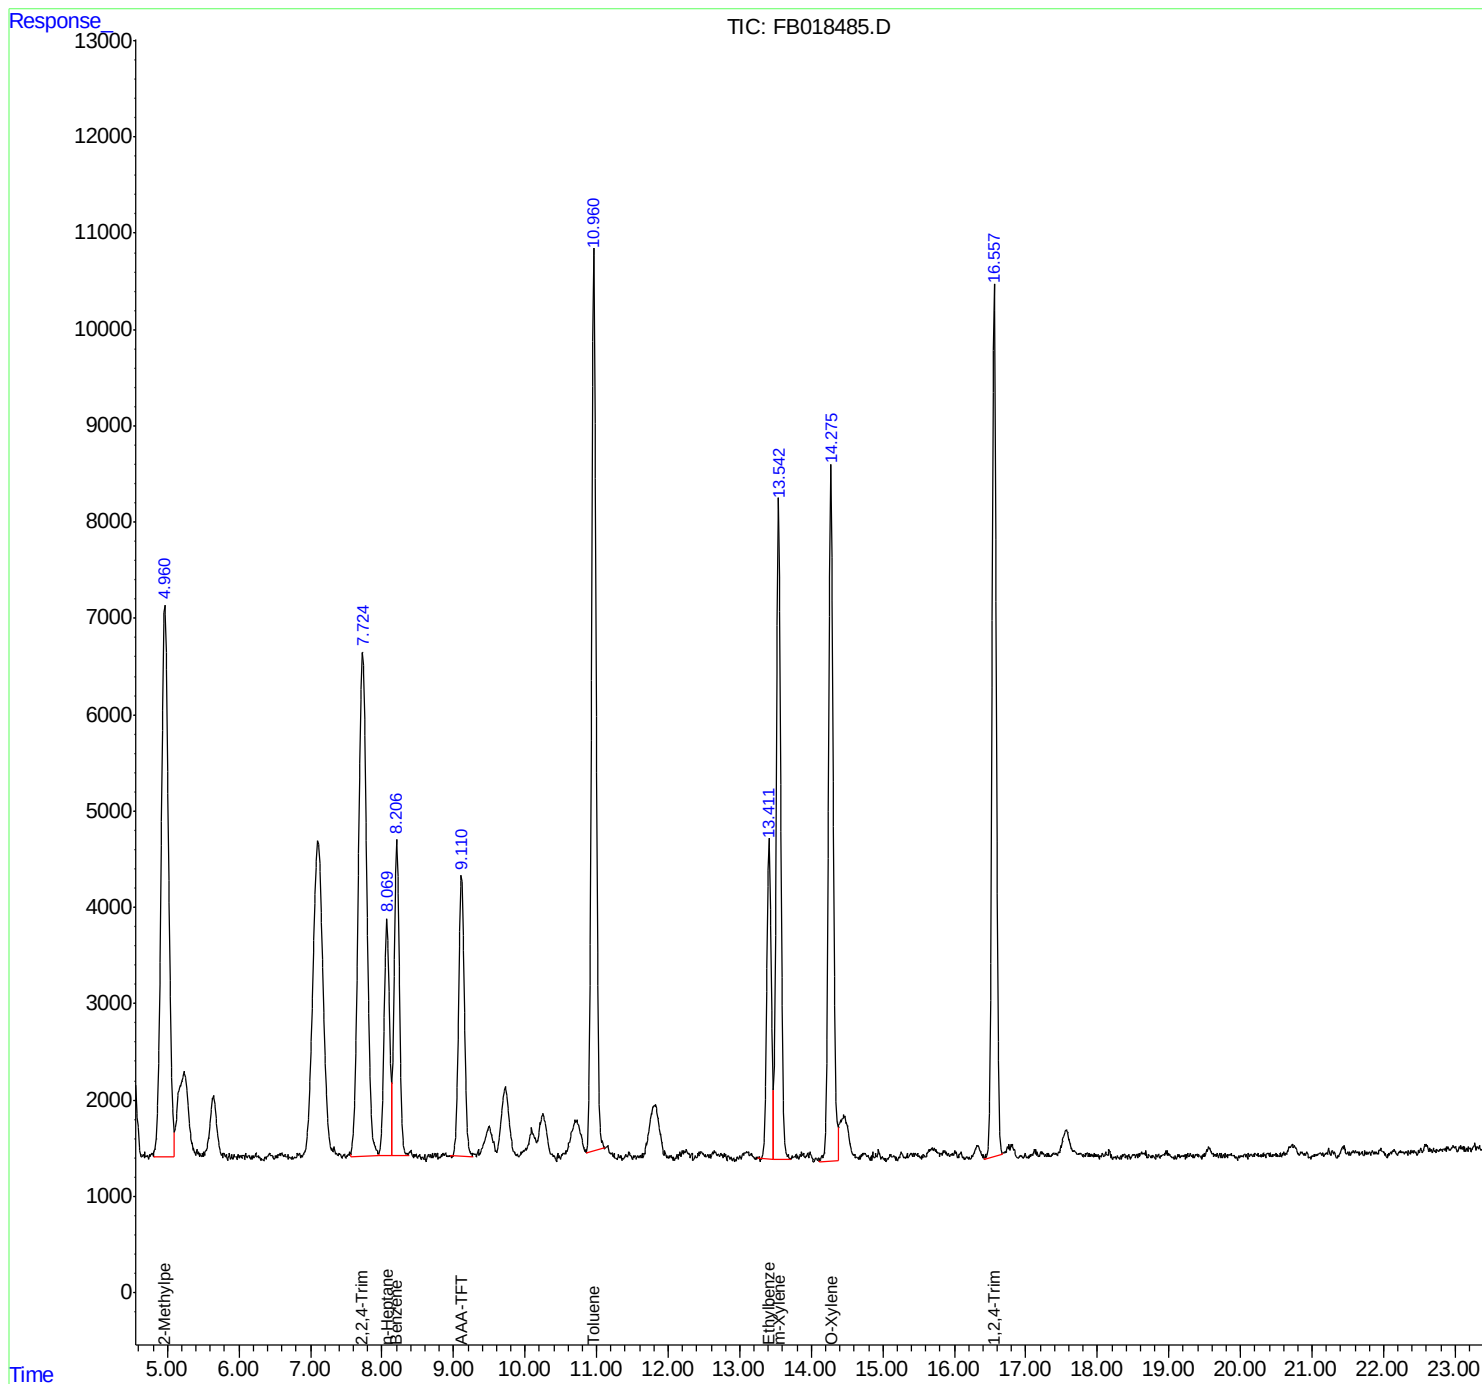

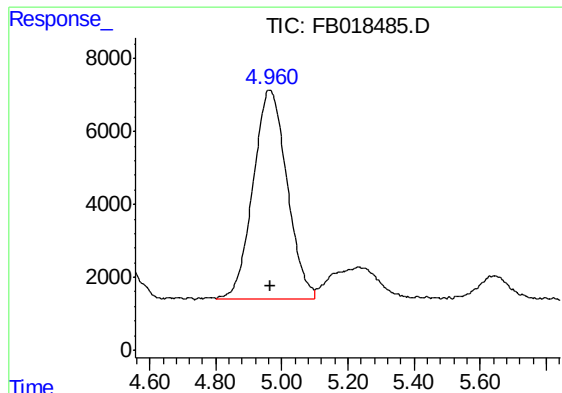


#1 2-Methylpentane

R.T.: 4.962 min
Delta R.T.: -0.003 min
Response: 408317
Conc: 26.70 ng/ml

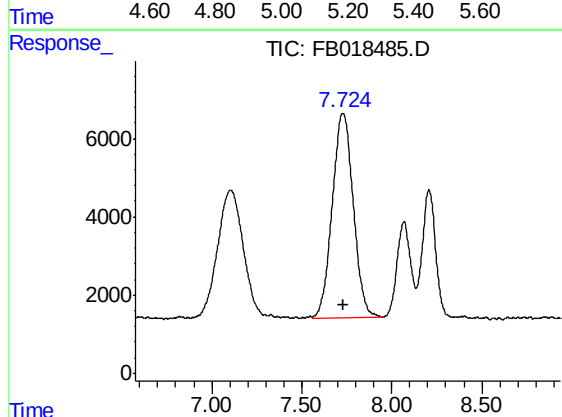


#2 2,2,4-Trimethylpentane

R.T.: 7.728 min
Delta R.T.: 0.000 min
Response: 424801
Conc: 28.75 ng/ml

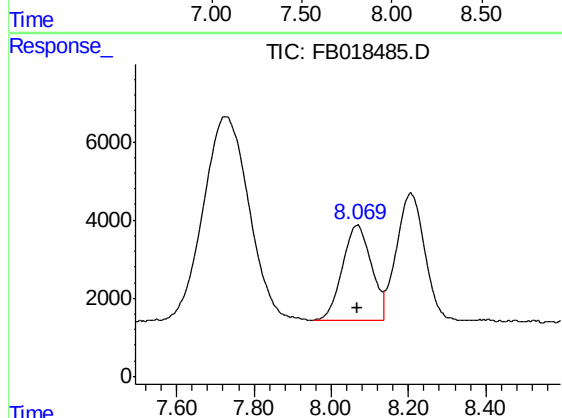


#3 n-Heptane

R.T.: 8.068 min
Delta R.T.: 0.000 min
Response: 129166
Conc: 9.11 ng/ml

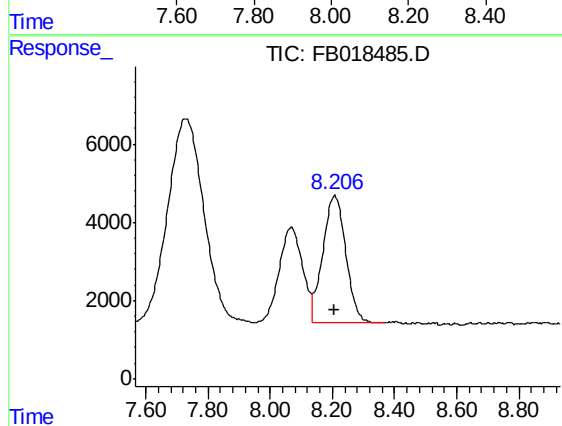


#4 Benzene

R.T.: 8.207 min
Delta R.T.: 0.000 min
Response: 167855
Conc: 9.01 ng/ml

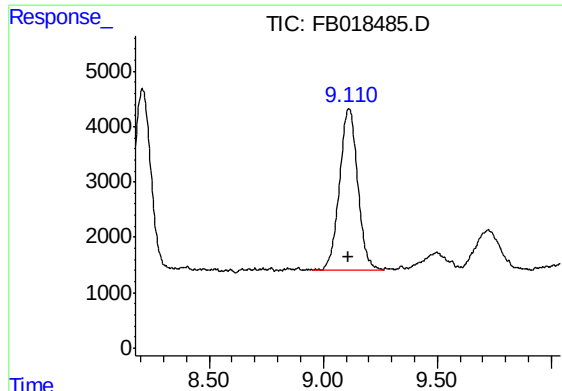


#5 AAA-TFT

R.T.: 9.112 min
Delta R.T.: 0.000 min
Response: 160625
Conc: 18.65 ng/ml

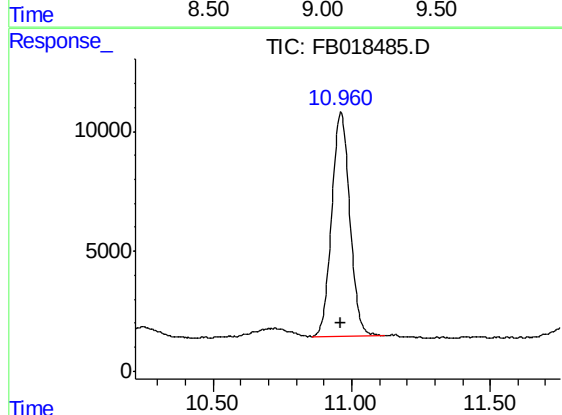


#6 Toluene

R.T.: 10.961 min
Delta R.T.: 0.000 min
Response: 423130
Conc: 27.76 ng/ml

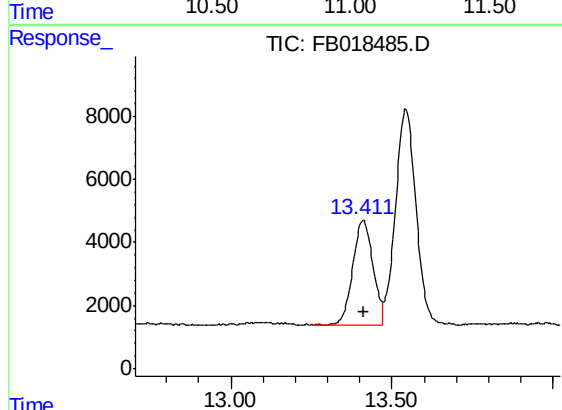


#7 Ethylbenzene

R.T.: 13.411 min
Delta R.T.: 0.000 min
Response: 144253
Conc: 9.09 ng/ml

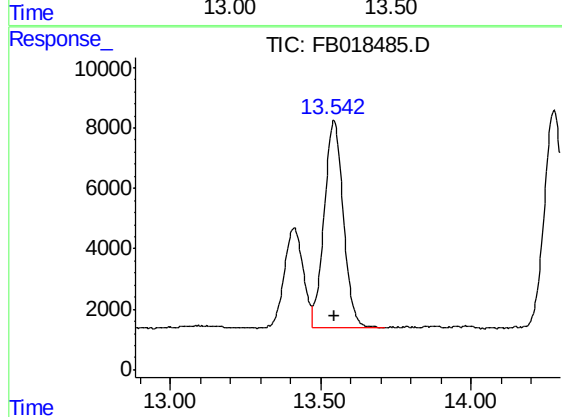


#8 m-Xylene

R.T.: 13.544 min
Delta R.T.: 0.000 min
Response: 304386
Conc: 18.29 ng/ml

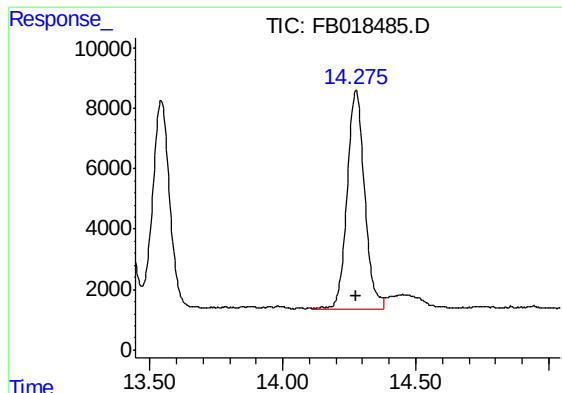

#9 O-Xylene

R.T.: 14.276 min
Delta R.T.: 0.000 min
Response: 329673
Conc: 18.49 ng/ml

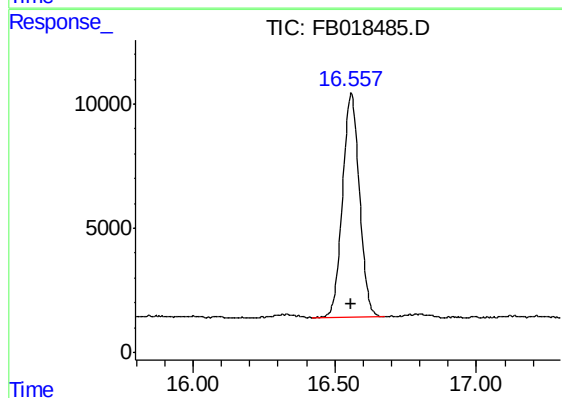

#10 1,2,4-Trimethylbenzene

R.T.: 16.559 min
Delta R.T.: 0.000 min
Response: 374814
Conc: 18.42 ng/ml