

Data Path : \\74.0.250.170\Terastorage\pestpcbsrv\HPCHEM1\FID_B\Data\FB110218\
 Data File : FB018486.D
 Signal(s) : FID2B.CH
 Acq On : 3 Nov 2018 6:11
 Operator : MJ/SJ
 Sample : J5741-32MSD
 Misc : 5.01g/5.00mL DI Water
 ALS Vial : 39 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Nov 03 07:02:54 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101218.M
 Quant Title :
 QLast Update : Fri Oct 12 08:04:31 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.111	160115	18.590 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.964	383527	25.076 ng/ml
2) t 2,2,4-Trimethylpentane	7.728	405139	27.418 ng/ml
3) t n-Heptane	8.067	120686	8.516 ng/ml
4) t Benzene	8.206	165140	8.865 ng/ml
6) t Toluene	10.961	423883	27.813 ng/ml
7) t Ethylbenzene	13.411	138364	8.721 ng/ml
8) t m-Xylene	13.543	295000	17.729 ng/ml
9) t O-Xylene	14.275	319688	17.930 ng/ml
10) t 1,2,4-Trimethylbenzene	16.558	364088	17.897 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : \\74.0.250.170\Terastorage\pestpcbsrv\HPCHEM1\FID_B\Data\FB110218\
Data File : FB018486.D
Signal(s) : FID2B.CH
Acq On : 3 Nov 2018 6:11
Operator : MJ/SJ
Sample : J5741-32MSD
Misc : 5.01g/5.00mL DI Water
ALS Vial : 39 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Nov 03 07:02:54 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101218.M
Quant Title :
QLast Update : Fri Oct 12 08:04:31 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

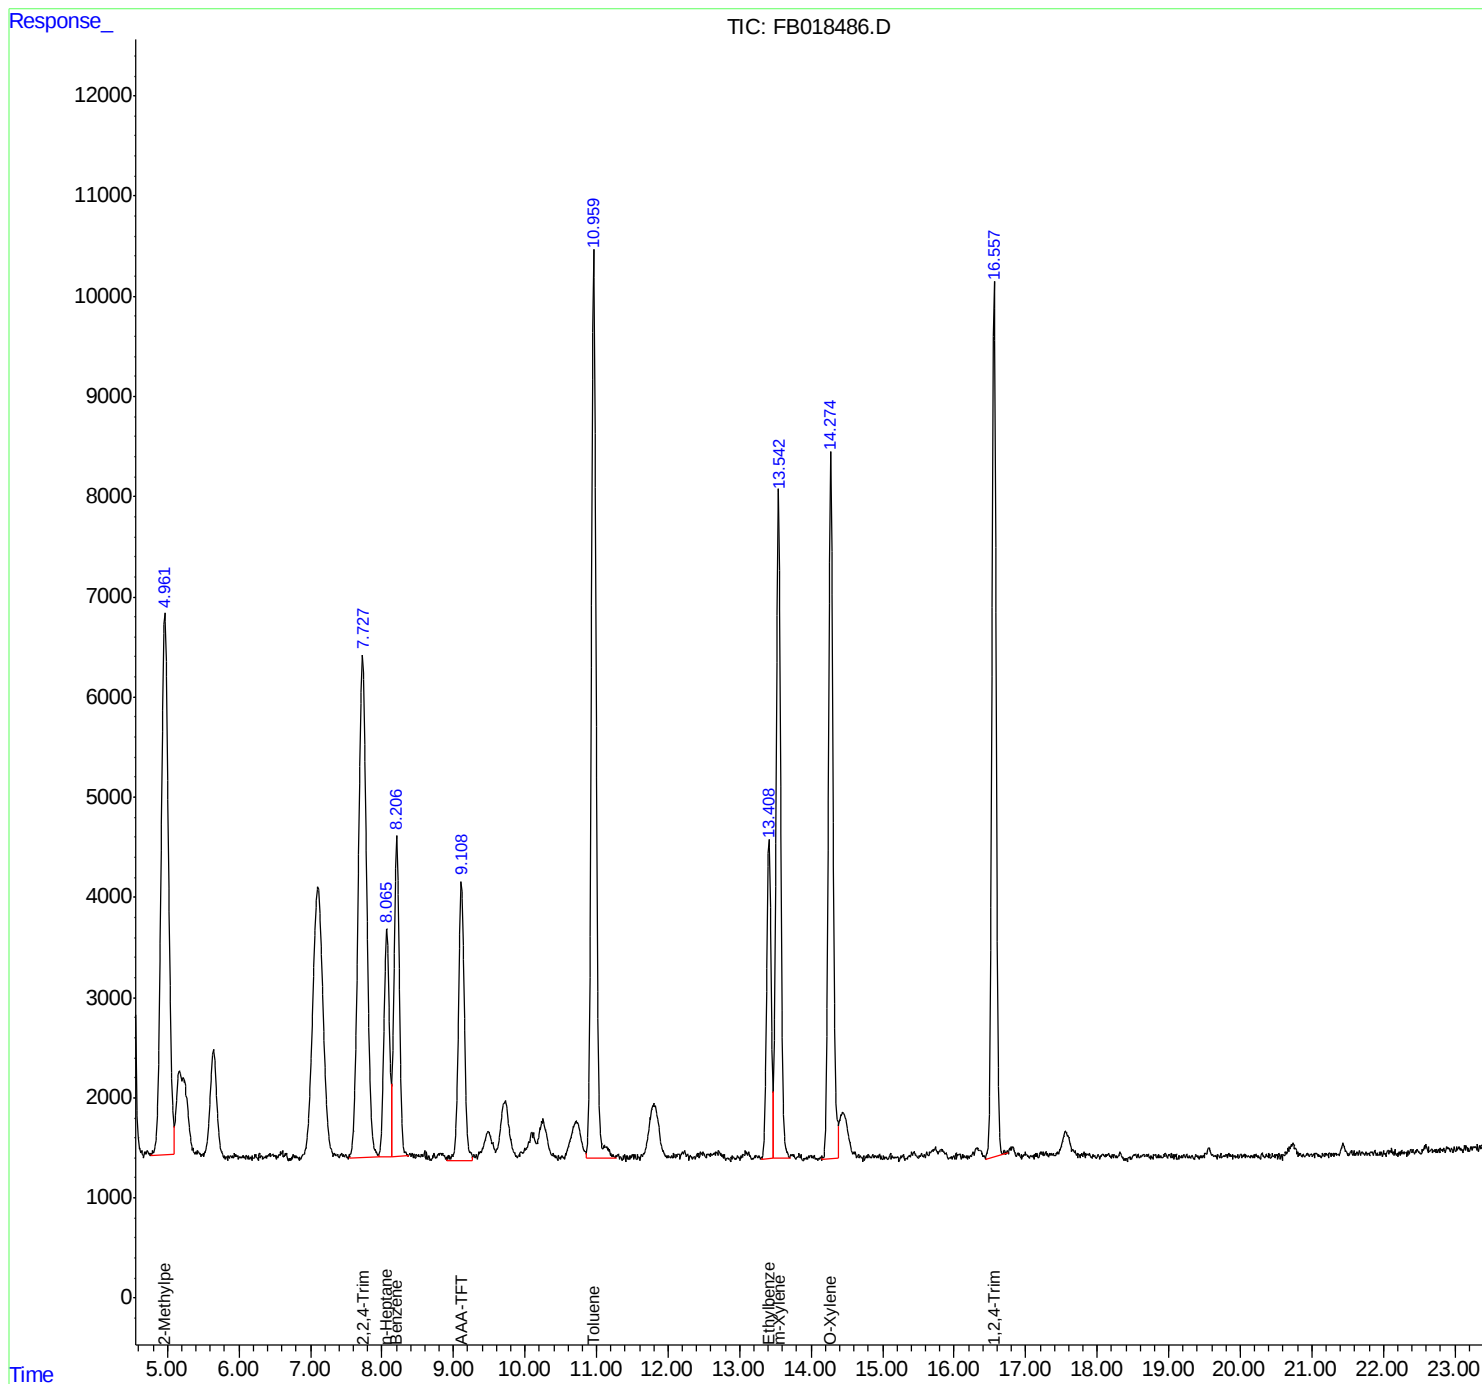

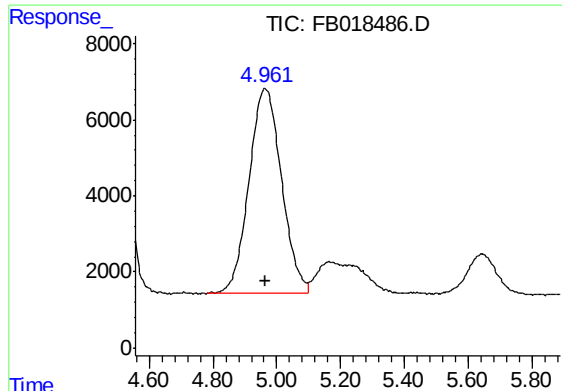


#1 2-Methylpentane

R.T.: 4.964 min
Delta R.T.: -0.001 min
Response: 383527
Conc: 25.08 ng/ml

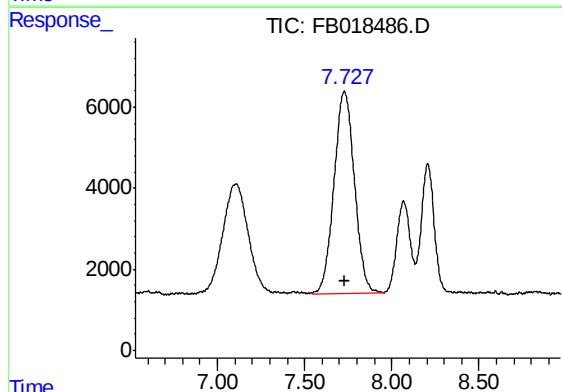


#2 2,2,4-Trimethylpentane

R.T.: 7.728 min
Delta R.T.: 0.000 min
Response: 405139
Conc: 27.42 ng/ml

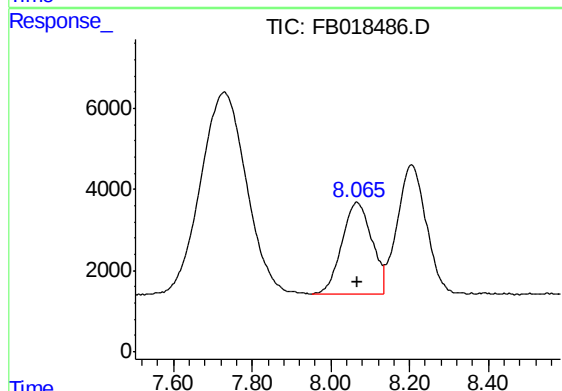


#3 n-Heptane

R.T.: 8.067 min
Delta R.T.: 0.000 min
Response: 120686
Conc: 8.52 ng/ml

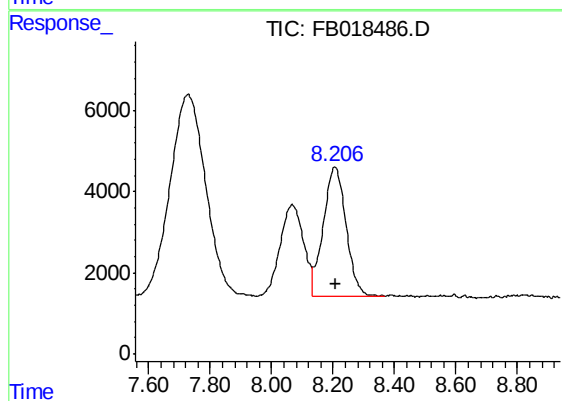


#4 Benzene

R.T.: 8.206 min
Delta R.T.: 0.000 min
Response: 165140
Conc: 8.86 ng/ml

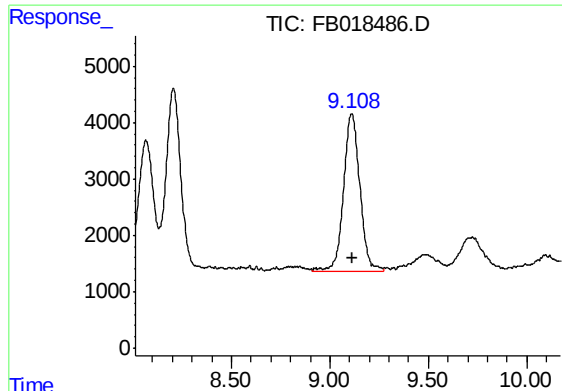


#5 AAA-TFT

R.T.: 9.111 min
Delta R.T.: -0.001 min
Response: 160115
Conc: 18.59 ng/ml

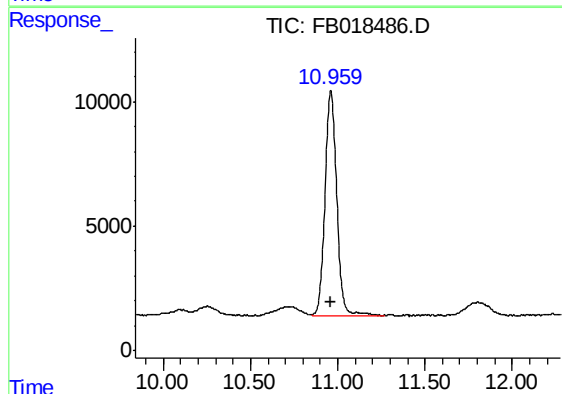


#6 Toluene

R.T.: 10.961 min
Delta R.T.: -0.001 min
Response: 423883
Conc: 27.81 ng/ml

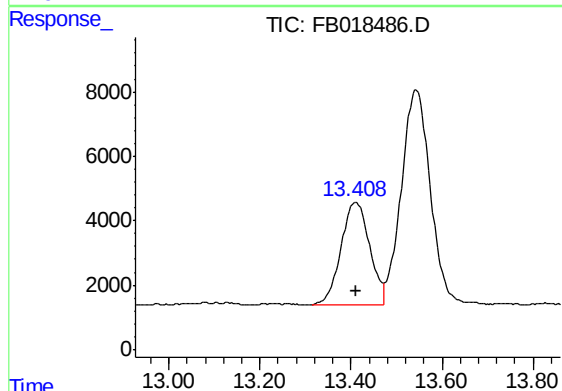


#7 Ethylbenzene

R.T.: 13.411 min
Delta R.T.: -0.001 min
Response: 138364
Conc: 8.72 ng/ml

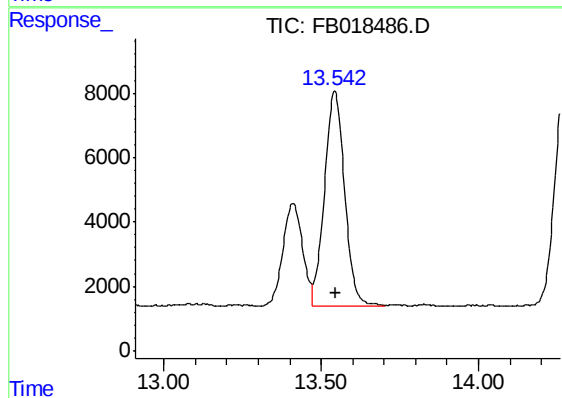


#8 m-Xylene

R.T.: 13.543 min
Delta R.T.: 0.000 min
Response: 295000
Conc: 17.73 ng/ml

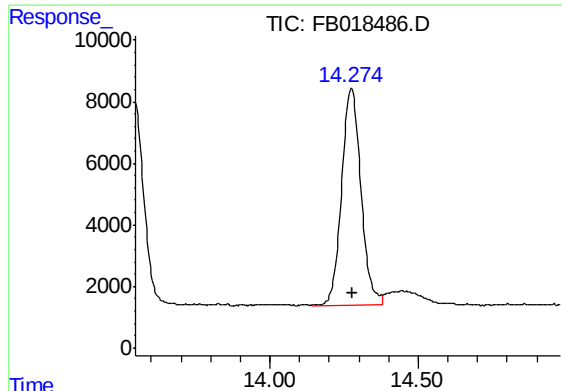

#9 O-Xylene

R.T.: 14.275 min
Delta R.T.: -0.001 min
Response: 319688
Conc: 17.93 ng/ml

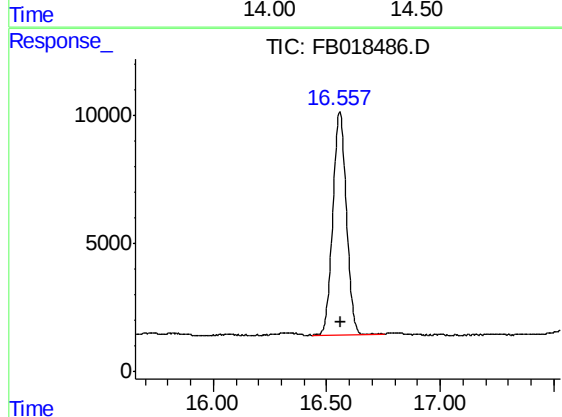

#10 1,2,4-Trimethylbenzene

R.T.: 16.558 min
Delta R.T.: -0.002 min
Response: 364088
Conc: 17.90 ng/ml