

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110222\
 Data File : FB028832.D
 Signal(s) : FID2B.CH
 Acq On : 2 Nov 2022 14:11
 Operator : AJ/MA
 Sample : N5406-06MS
 Misc : 2.15G/5.00 ML DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 SB-03-COMPMS

Integration File: SAMPLE.e
 Quant Time: Nov 03 05:36:54 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110122.M
 Quant Title :
 QLast Update : Tue Nov 01 12:44:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.792	315417	24.822 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.705	477356	29.286 ng/ml
2) t 2,2,4-Trimethylpentane	7.423	532100	30.282 ng/ml
3) t n-Heptane	7.748	185397	10.545 ng/ml
4) t Benzene	7.886	226632	11.052 ng/ml
6) t Toluene	10.621	658606	32.745 ng/ml
7) t Ethylbenzene	13.058	202216	10.662 ng/ml
8) t m-Xylene	13.190	399098	21.214 ng/ml
9) t O-Xylene	13.917	382941	20.874 ng/ml
10) t 1,2,4-Trimethylbenzene	16.192	347919	18.886 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110222\
Data File : FB028832.D
Signal(s) : FID2B.CH
Acq On : 2 Nov 2022 14:11
Operator : AJ/MA
Sample : N5406-06MS
Misc : 2.15G/5.00 ML DI WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
SB-03-COMPMS

Integration File: SAMPLE.e
Quant Time: Nov 03 05:36:54 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110122.M
Quant Title :
QLast Update : Tue Nov 01 12:44:12 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

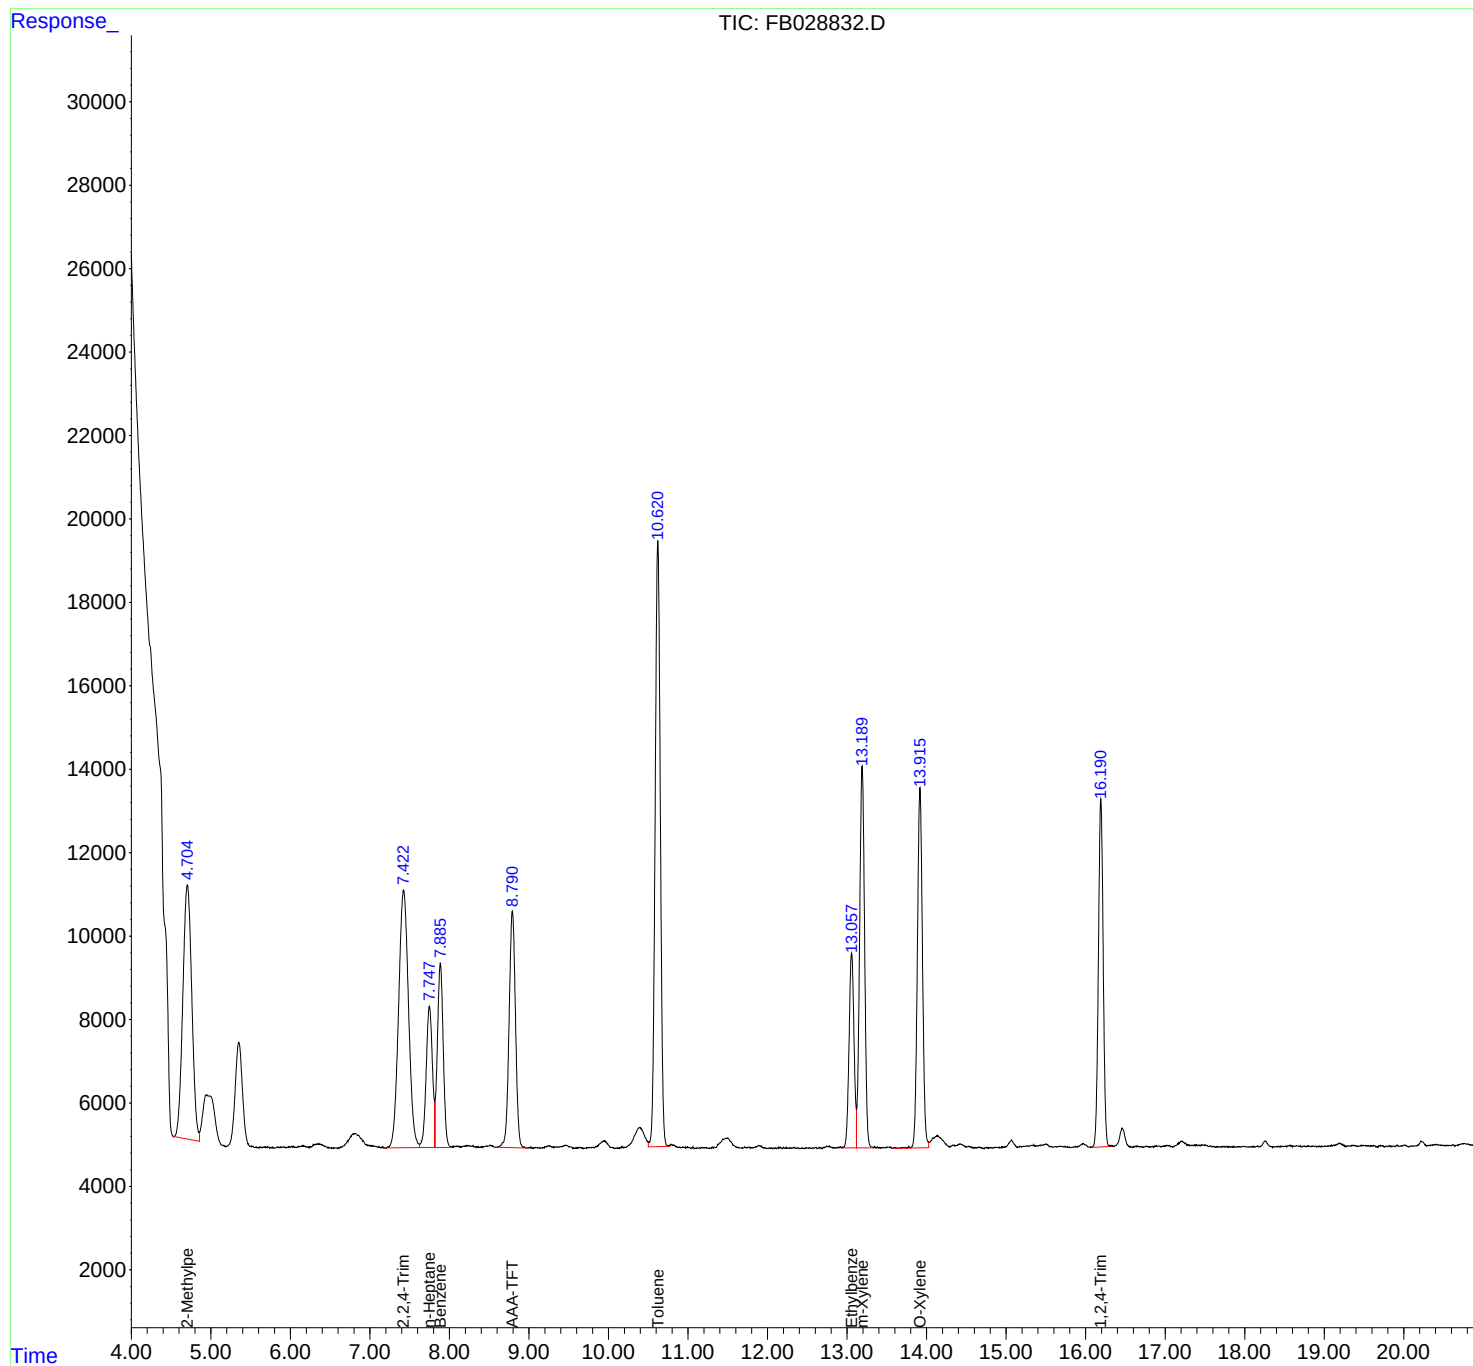


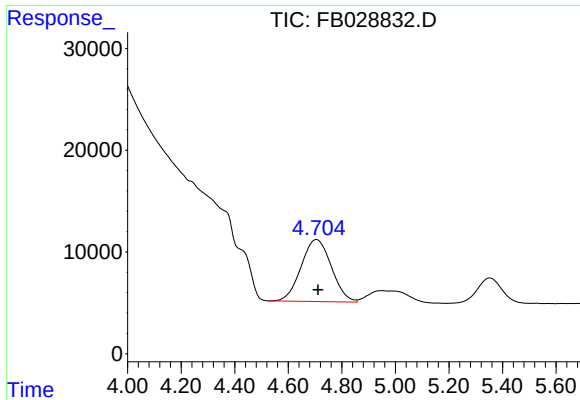

#1 2-Methylpentane


R.T.: 4.705 min
Delta R.T.: -0.007 min
Response: 477356
Conc: 29.29 ng/ml

Instrument :
FID_B
ClientSampleId :
SB-03-COMPMS

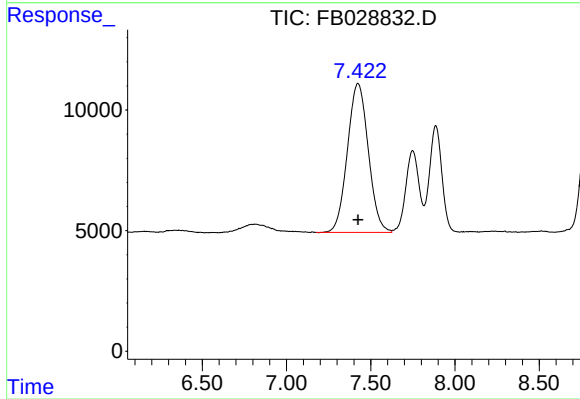


#2 2,2,4-Trimethylpentane

R.T.: 7.423 min
Delta R.T.: -0.001 min
Response: 532100
Conc: 30.28 ng/ml

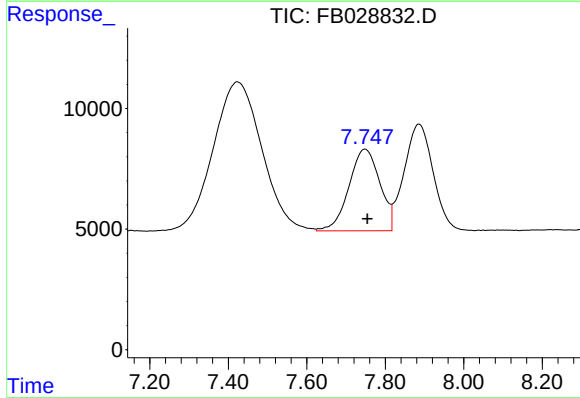


#3 n-Heptane

R.T.: 7.748 min
Delta R.T.: -0.006 min
Response: 185397
Conc: 10.54 ng/ml

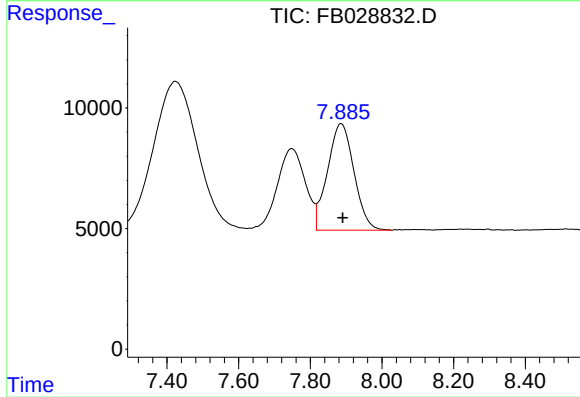

#4 Benzene


R.T.: 7.886 min
Delta R.T.: -0.004 min
Response: 226632
Conc: 11.05 ng/ml

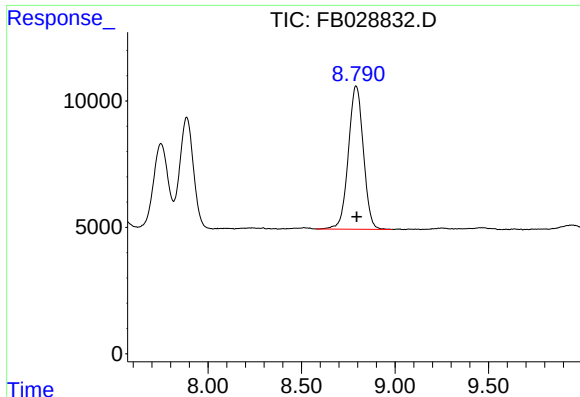

#5 AAA-TFT


R.T.: 8.792 min
Delta R.T.: -0.003 min
Response: 315417
Conc: 24.82 ng/ml

Instrument :
FID_B
ClientSampleId :
SB-03-COMPMS

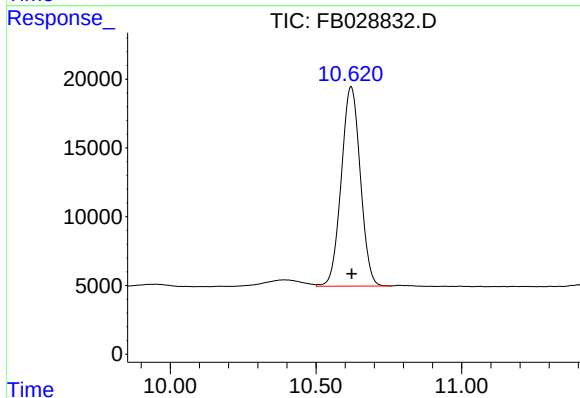


#6 Toluene

R.T.: 10.621 min
Delta R.T.: -0.002 min
Response: 658606
Conc: 32.75 ng/ml

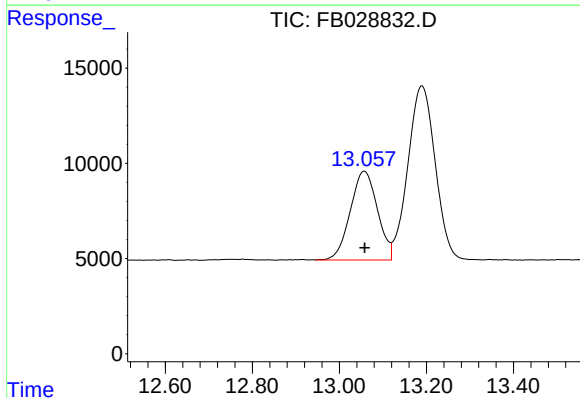


#7 Ethylbenzene

R.T.: 13.058 min
Delta R.T.: 0.000 min
Response: 202216
Conc: 10.66 ng/ml

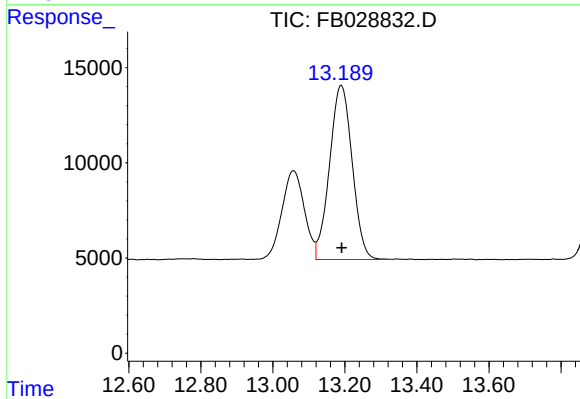

#8 m-Xylene


R.T.: 13.190 min
Delta R.T.: -0.001 min
Response: 399098
Conc: 21.21 ng/ml

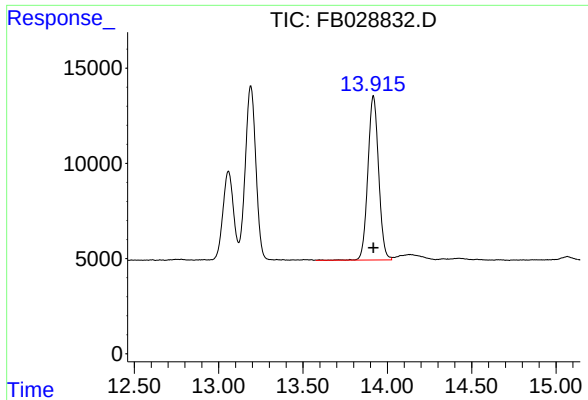

#9 O-Xylene

R.T.: 13.917 min
Delta R.T.: -0.001 min
Response: 382941
Conc: 20.87 ng/ml

Instrument :
FID_B
ClientSampleId :
SB-03-COMPMS

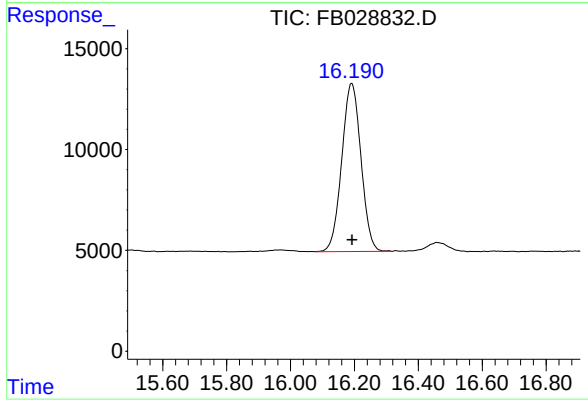

#10 1,2,4-Trimethylbenzene

R.T.: 16.192 min
Delta R.T.: 0.000 min
Response: 347919
Conc: 18.89 ng/ml