

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110222\
 Data File : FB028834.D
 Signal(s) : FID2B.CH
 Acq On : 2 Nov 2022 15:26
 Operator : AJ/MA
 Sample : BSF1102S2
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1102S2

Integration File: SAMPLE.e
 Quant Time: Nov 03 05:37:04 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110122.M
 Quant Title :
 QLast Update : Tue Nov 01 12:44:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.796	315600	24.836 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.716	496073	30.434 ng/ml
2) t 2,2,4-Trimethylpentane	7.431	544930	31.013 ng/ml
3) t n-Heptane	7.754	183116	10.415 ng/ml
4) t Benzene	7.892	218567	10.659 ng/ml
6) t Toluene	10.624	637567	31.699 ng/ml
7) t Ethylbenzene	13.060	197373	10.407 ng/ml
8) t m-Xylene	13.193	394473	20.968 ng/ml
9) t O-Xylene	13.920	382569	20.854 ng/ml
10) t 1,2,4-Trimethylbenzene	16.194	360264	19.556 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110222\
Data File : FB028834.D
Signal(s) : FID2B.CH
Acq On : 2 Nov 2022 15:26
Operator : AJ/MA
Sample : BSF1102S2
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1102S2

Integration File: SAMPLE.e
Quant Time: Nov 03 05:37:04 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110122.M
Quant Title :
QLast Update : Tue Nov 01 12:44:12 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

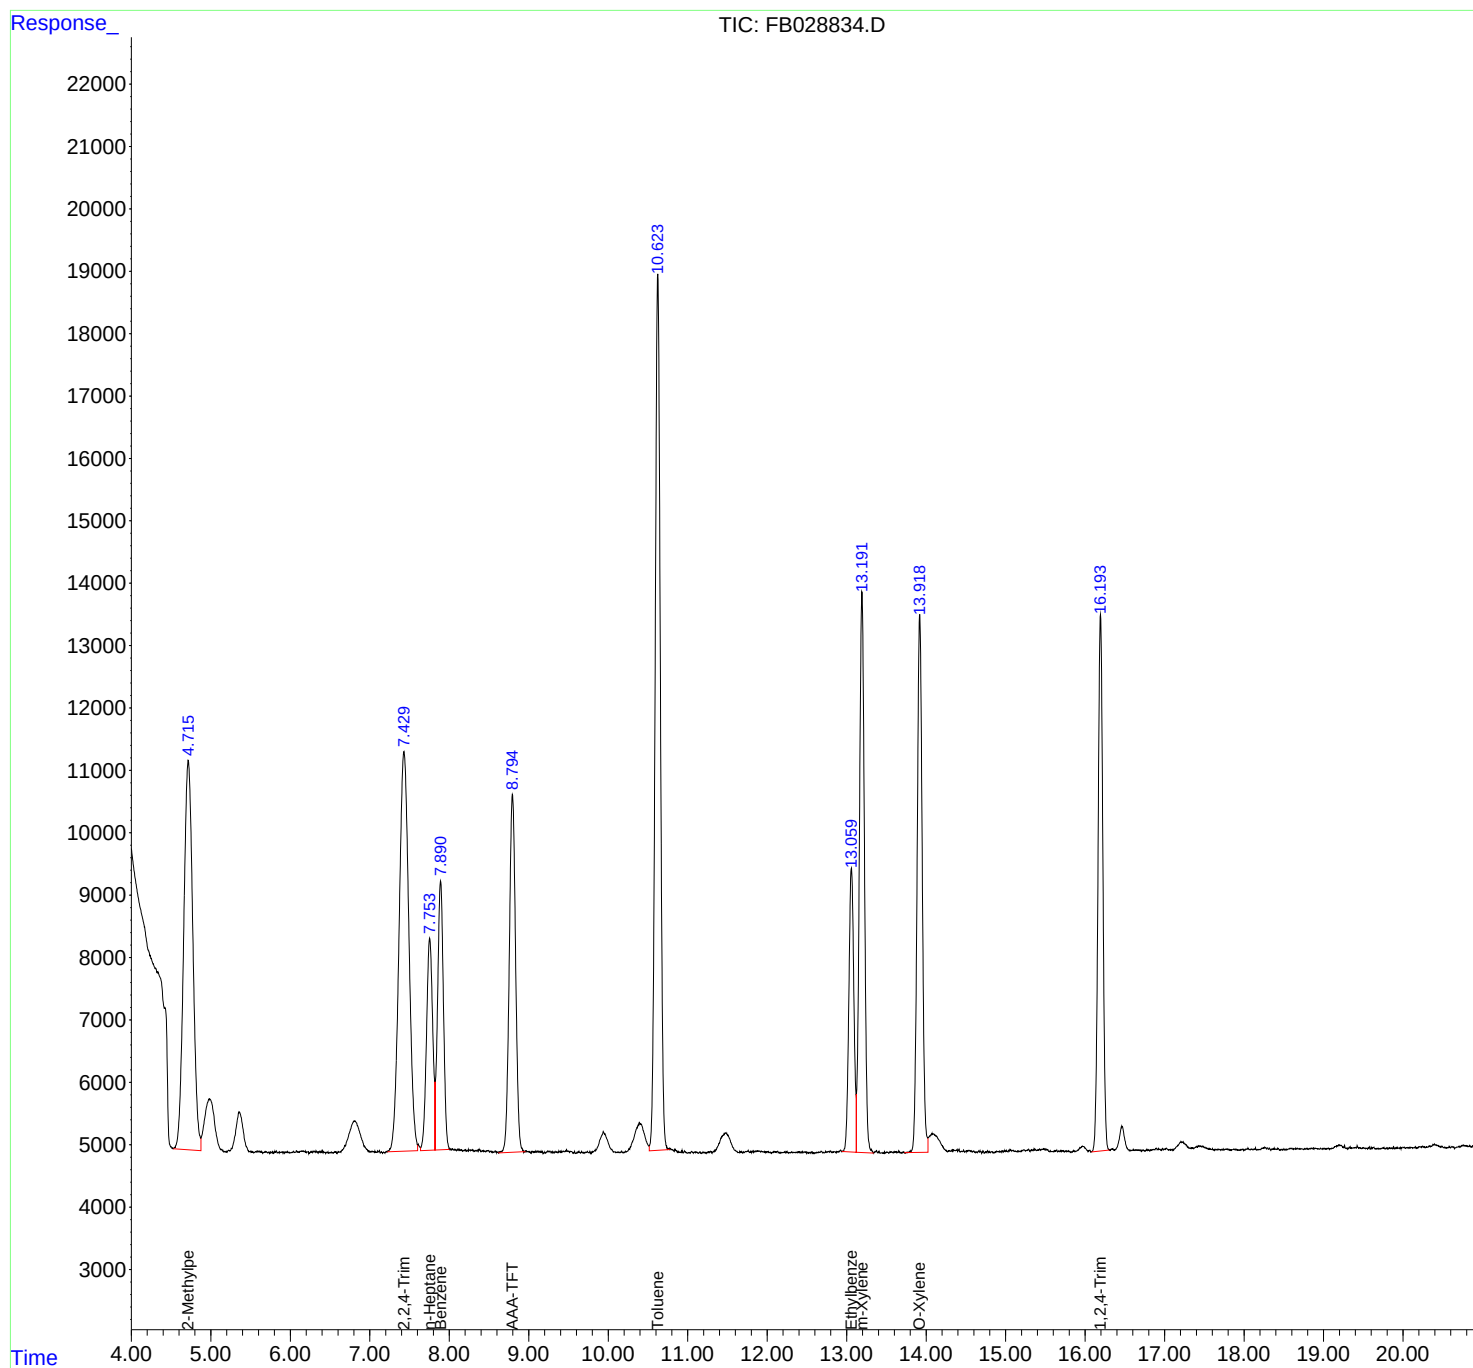


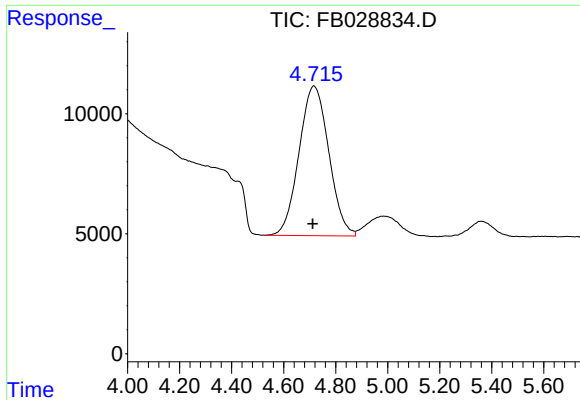

#1 2-Methylpentane


R.T.: 4.716 min
Delta R.T.: 0.004 min
Response: 496073
Conc: 30.43 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1102S2

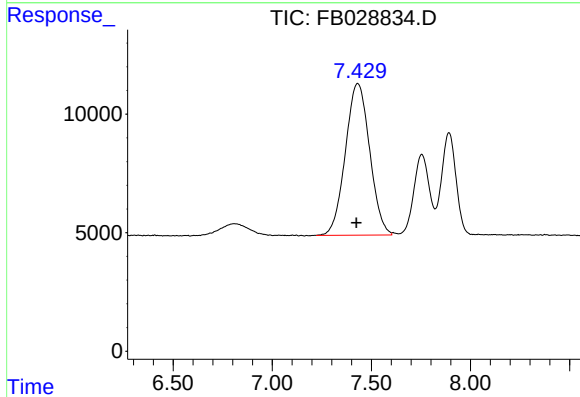


#2 2,2,4-Trimethylpentane

R.T.: 7.431 min
Delta R.T.: 0.006 min
Response: 544930
Conc: 31.01 ng/ml

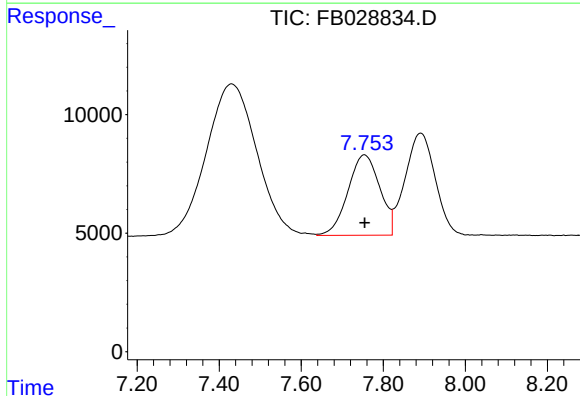


#3 n-Heptane

R.T.: 7.754 min
Delta R.T.: 0.000 min
Response: 183116
Conc: 10.41 ng/ml

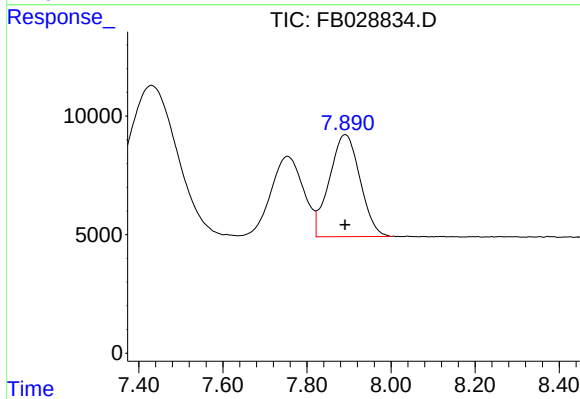

#4 Benzene


R.T.: 7.892 min
Delta R.T.: 0.001 min
Response: 218567
Conc: 10.66 ng/ml

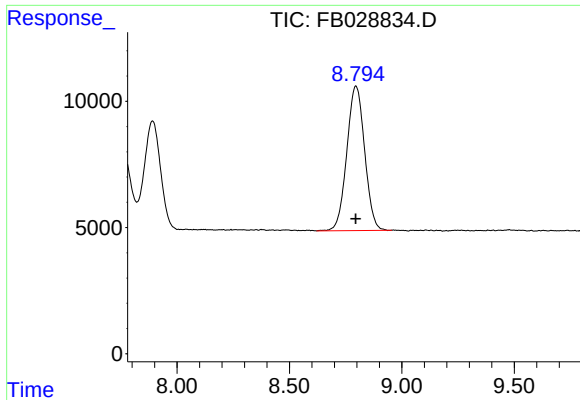

#5 AAA-TFT


R.T.: 8.796 min
Delta R.T.: 0.000 min
Response: 315600
Conc: 24.84 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1102S2

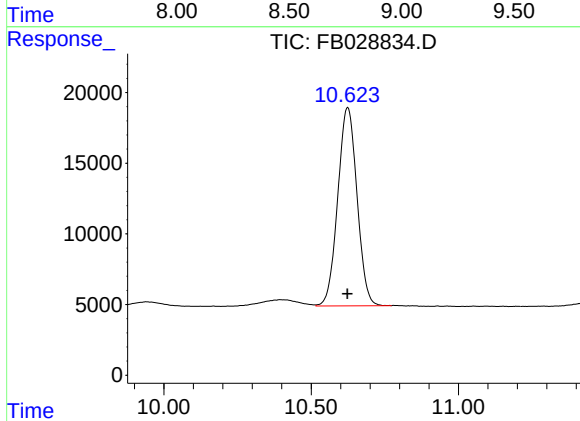


#6 Toluene

R.T.: 10.624 min
Delta R.T.: 0.001 min
Response: 637567
Conc: 31.70 ng/ml

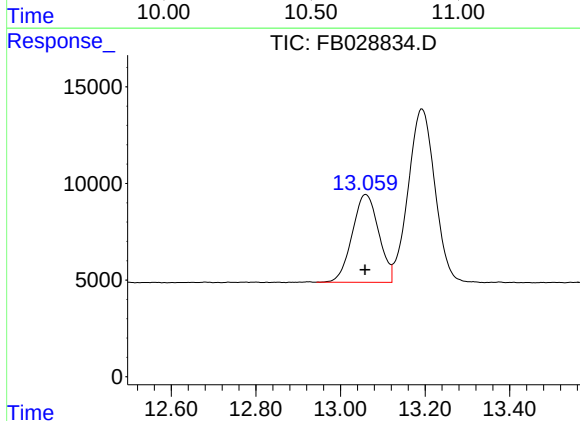


#7 Ethylbenzene

R.T.: 13.060 min
Delta R.T.: 0.002 min
Response: 197373
Conc: 10.41 ng/ml

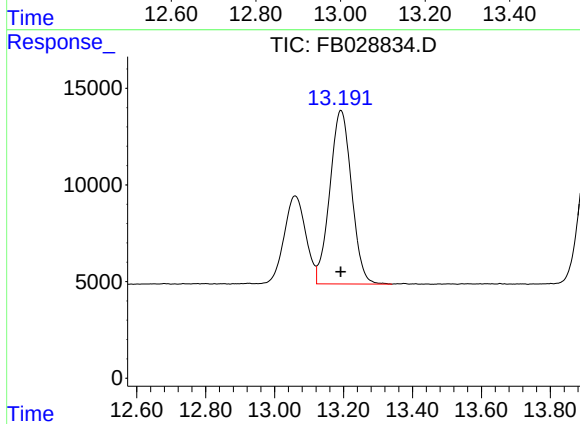

#8 m-Xylene


R.T.: 13.193 min
Delta R.T.: 0.002 min
Response: 394473
Conc: 20.97 ng/ml

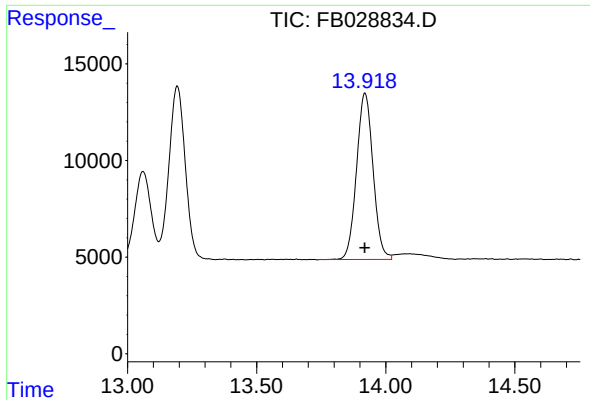

#9 O-Xylene

R.T.: 13.920 min
Delta R.T.: 0.002 min
Response: 382569
Conc: 20.85 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1102S2

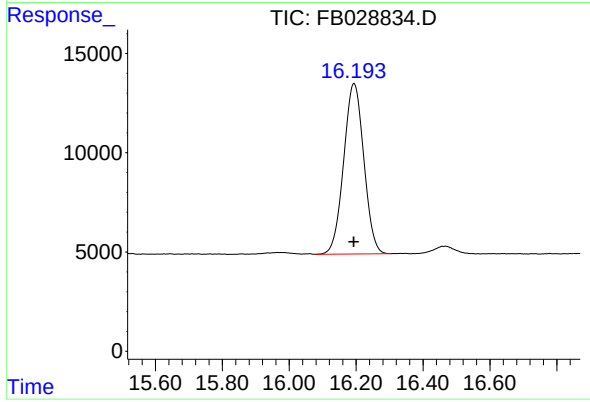

#10 1,2,4-Trimethylbenzene

R.T.: 16.194 min
Delta R.T.: 0.002 min
Response: 360264
Conc: 19.56 ng/ml