

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110419\
 Data File : FB022874.D
 Signal(s) : FID2B.CH
 Acq On : 4 Nov 2019 13:44
 Operator : DD/AJ
 Sample : K5609-15 200X
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Nov 05 00:56:28 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
 Quant Title :
 QLast Update : Thu Oct 31 14:57:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.813	783997	34.826 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.681	501277	15.583 ng/ml
2) t 2,2,4-Trimethylpentane	7.375	706260	20.007 ng/ml
3) t n-Heptane	7.752	1313574	37.762 ng/ml
4) t Benzene	7.885	454591	10.495 ng/ml
6) t Toluene	10.626	4910971	113.916 ng/ml
7) t Ethylbenzene	13.065	1233994	30.910 ng/ml
8) t m-Xylene	13.197	4693784	124.282 ng/ml
9) t O-Xylene	13.927	1698536	47.657 ng/ml
10) t 1,2,4-Trimethylbenzene	16.205	1598190	56.356 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110419\
Data File : FB022874.D
Signal(s) : FID2B.CH
Acq On : 4 Nov 2019 13:44
Operator : DD/AJ
Sample : K5609-15 200X
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Nov 05 00:56:28 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
Quant Title :
QLast Update : Thu Oct 31 14:57:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

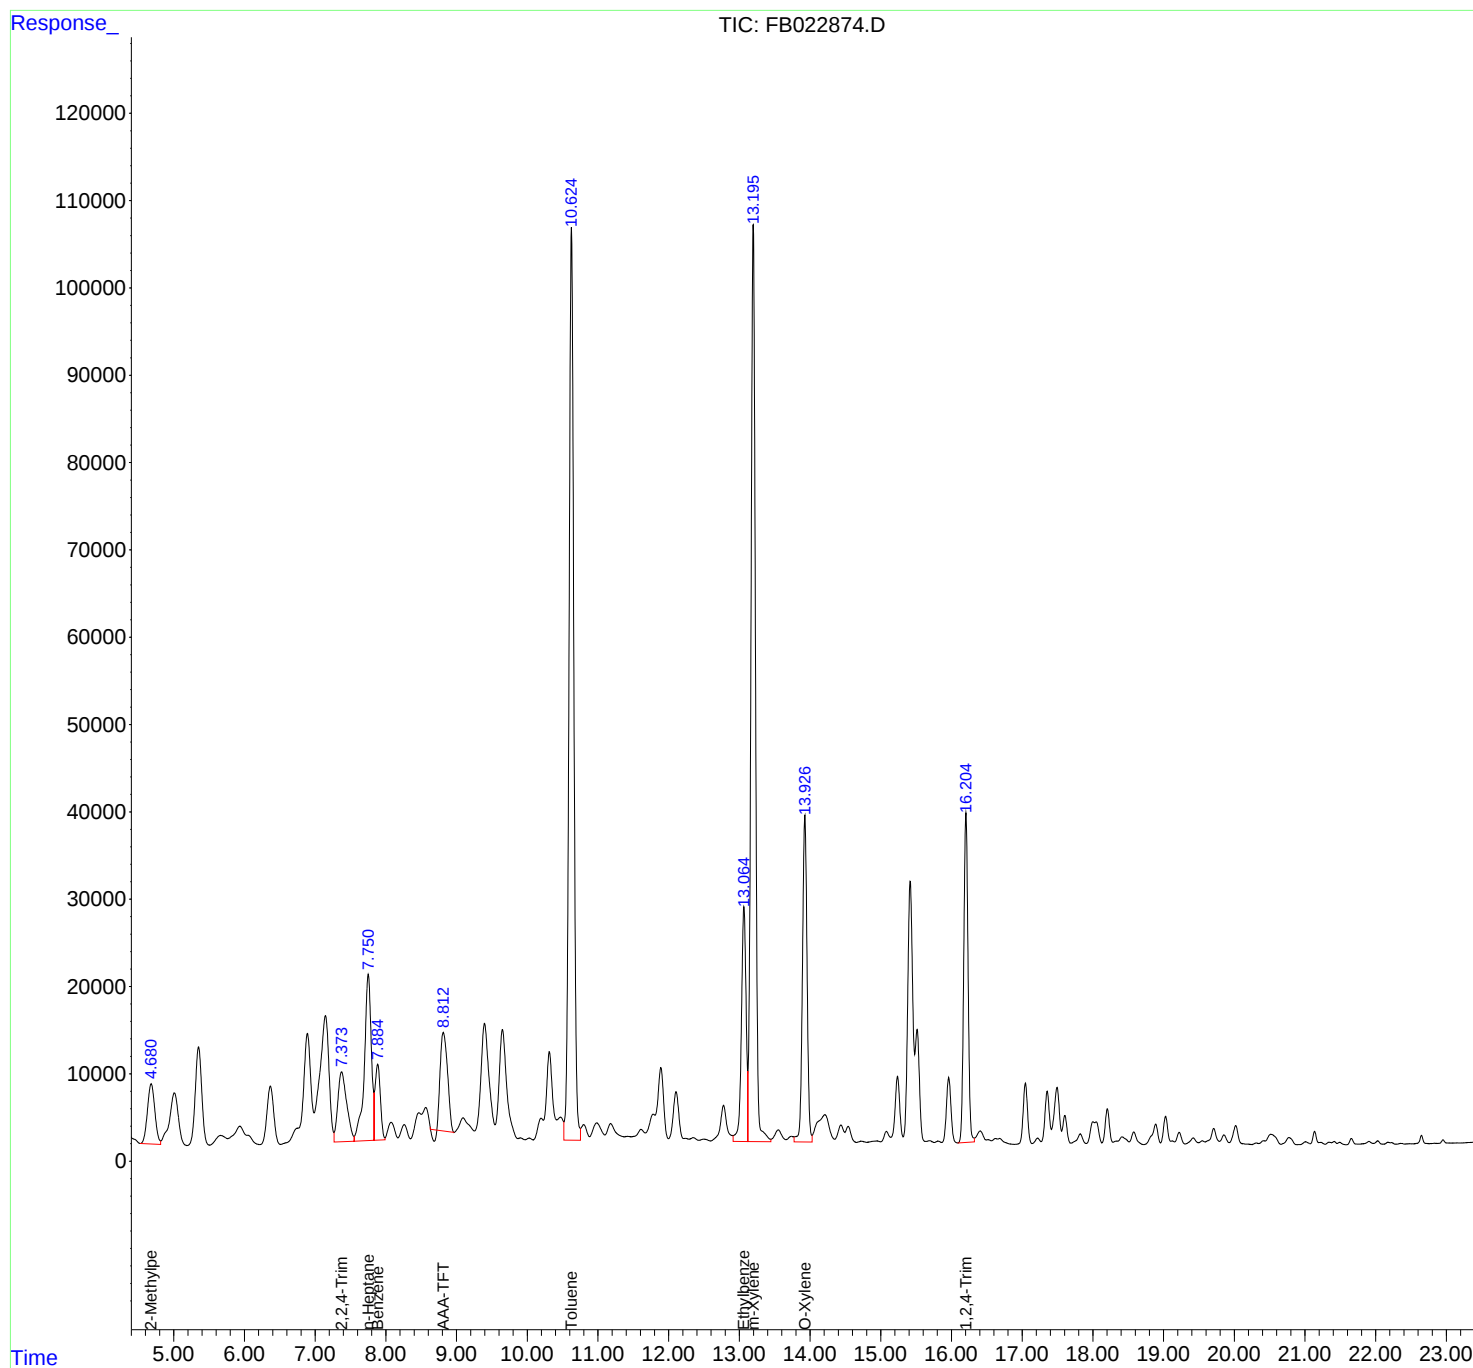


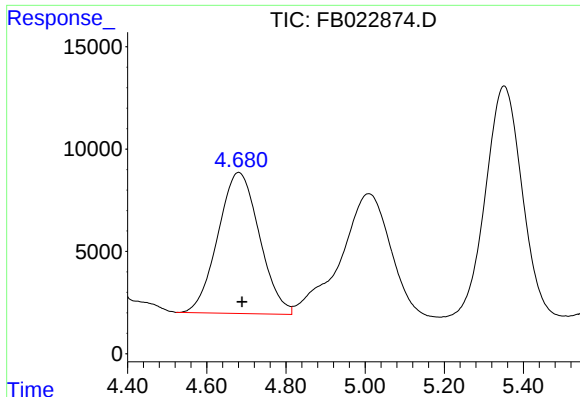

#1 2-Methylpentane


R.T.: 4.681 min
Delta R.T.: -0.008 min
Response: 501277
Conc: 15.58 ng/ml

Instrument :
FID_B
ClientSampleId :

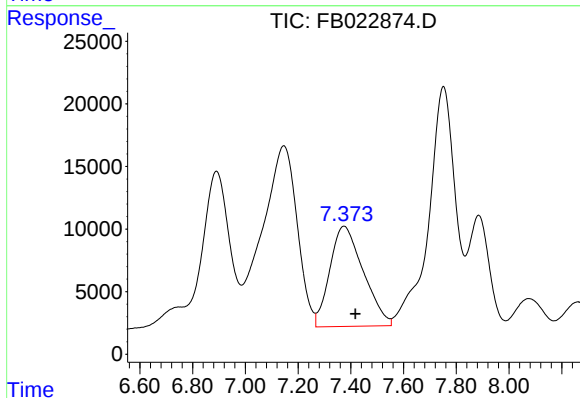


#2 2,2,4-Trimethylpentane

R.T.: 7.375 min
Delta R.T.: -0.043 min
Response: 706260
Conc: 20.01 ng/ml

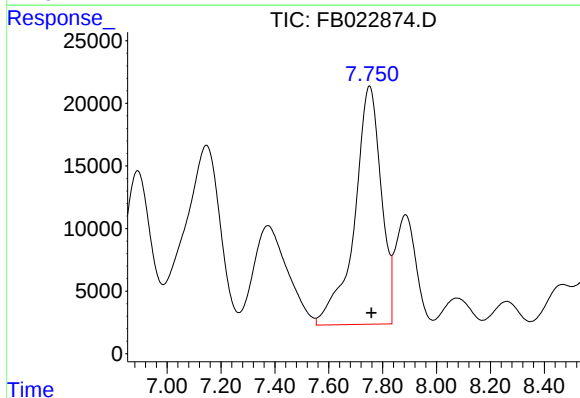


#3 n-Heptane

R.T.: 7.752 min
Delta R.T.: -0.007 min
Response: 1313574
Conc: 37.76 ng/ml

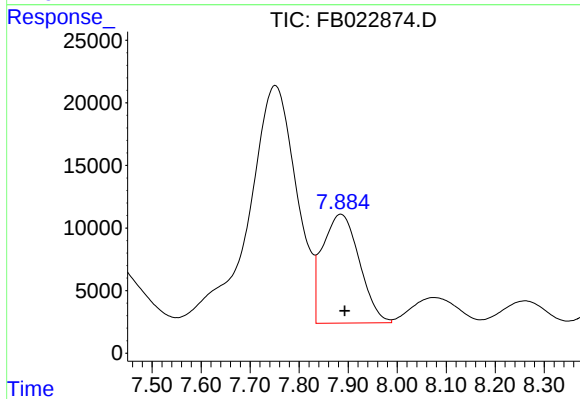

#4 Benzene


R.T.: 7.885 min
Delta R.T.: -0.008 min
Response: 454591
Conc: 10.50 ng/ml

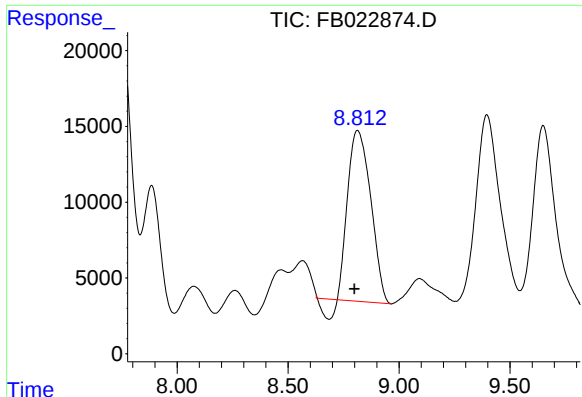

#5 AAA-TFT


R.T.: 8.813 min
Delta R.T.: 0.014 min
Response: 783997
Conc: 34.83 ng/ml

Instrument :
FID_B
ClientSampleId :

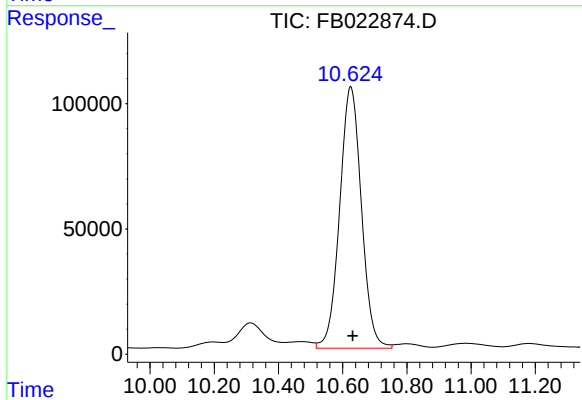


#6 Toluene

R.T.: 10.626 min
Delta R.T.: -0.006 min
Response: 4910971
Conc: 113.92 ng/ml

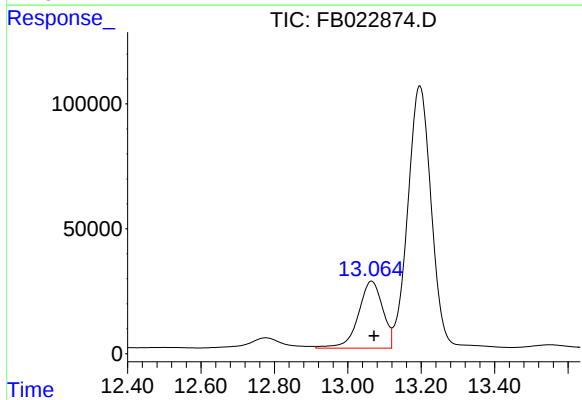


#7 Ethylbenzene

R.T.: 13.065 min
Delta R.T.: -0.006 min
Response: 1233994
Conc: 30.91 ng/ml

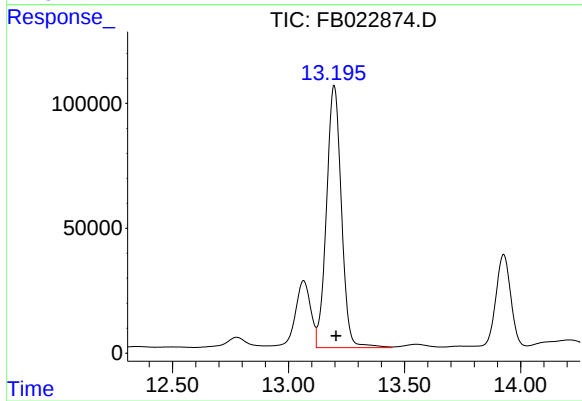

#8 m-Xylene


R.T.: 13.197 min
Delta R.T.: -0.008 min
Response: 4693784
Conc: 124.28 ng/ml

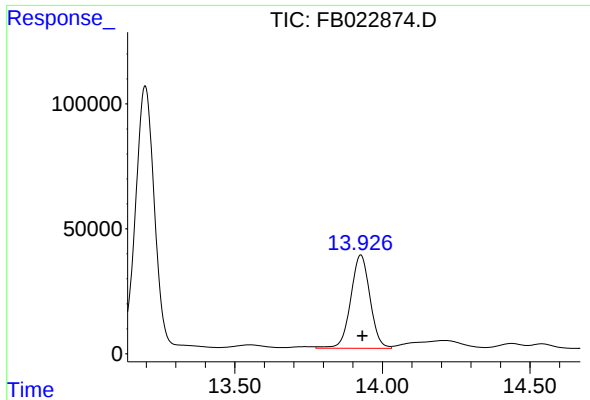

#9 O-Xylene

R.T.: 13.927 min
Delta R.T.: -0.006 min
Response: 1698536
Conc: 47.66 ng/ml

Instrument :
FID_B
ClientSampleId :

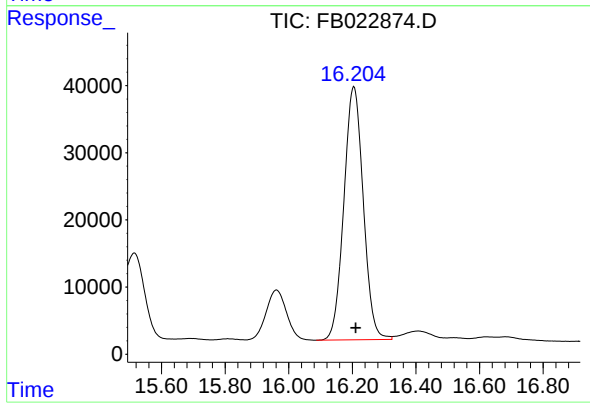

#10 1,2,4-Trimethylbenzene

R.T.: 16.205 min
Delta R.T.: -0.006 min
Response: 1598190
Conc: 56.36 ng/ml