

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110419\
 Data File : FB022875.D
 Signal(s) : FID2B.CH
 Acq On : 4 Nov 2019 14:43
 Operator : DD/AJ
 Sample : K5609-15 100X AJ
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Nov 05 13:39:07 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
 Quant Title :
 QLast Update : Thu Oct 31 14:57:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.839	1367391	60.741 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.680	1325817	41.216 ng/ml
2) t 2,2,4-Trimethylpentane	7.373	1834100	51.957 ng/ml
3) t n-Heptane	7.751	3384955	97.310 ng/ml
4) t Benzene	7.885	1162615	26.841 ng/ml
6) t Toluene	10.627	12596831	292.199 ng/ml
7) t Ethylbenzene	13.066	3200653	80.172 ng/ml
8) t m-Xylene	13.198	12188969	322.739 ng/ml
9) t O-Xylene	13.927	4402969	123.538 ng/ml
10) t 1,2,4-Trimethylbenzene	16.206	3870130	136.471 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110419\
Data File : FB022875.D
Signal(s) : FID2B.CH
Acq On : 4 Nov 2019 14:43
Operator : DD/AJ
Sample : K5609-15 100X AJ
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Nov 05 13:39:07 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
Quant Title :
QLast Update : Thu Oct 31 14:57:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

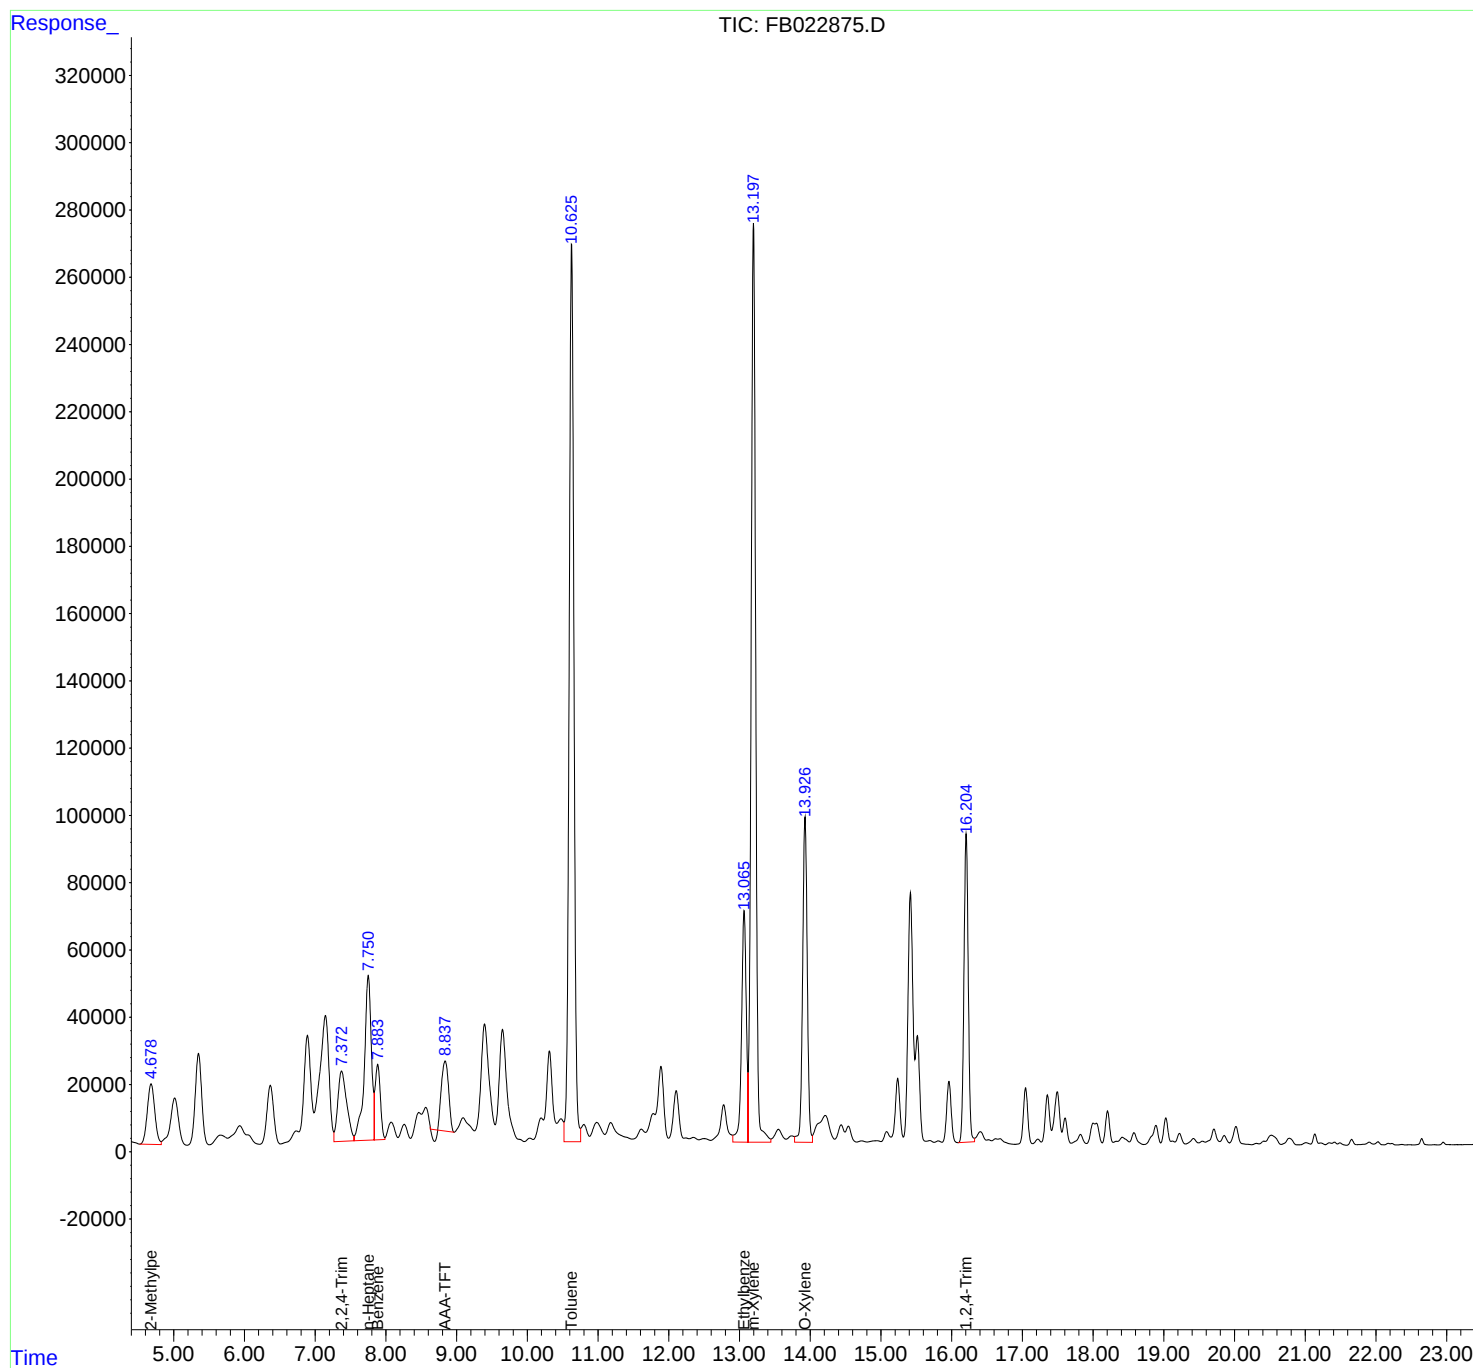


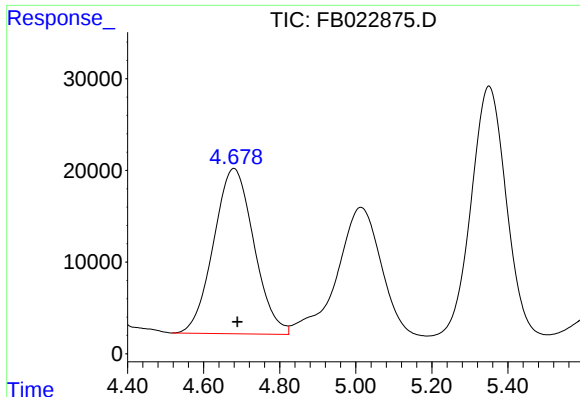

#1 2-Methylpentane


R.T.: 4.680 min
Delta R.T.: -0.009 min
Response: 1325817
Conc: 41.22 ng/ml

Instrument :
FID_B
ClientSampleId :

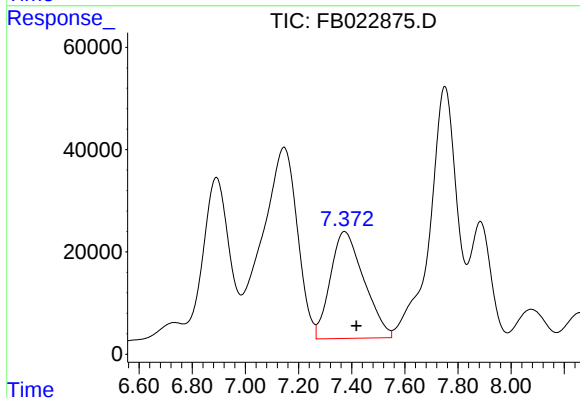


#2 2,2,4-Trimethylpentane

R.T.: 7.373 min
Delta R.T.: -0.045 min
Response: 1834100
Conc: 51.96 ng/ml

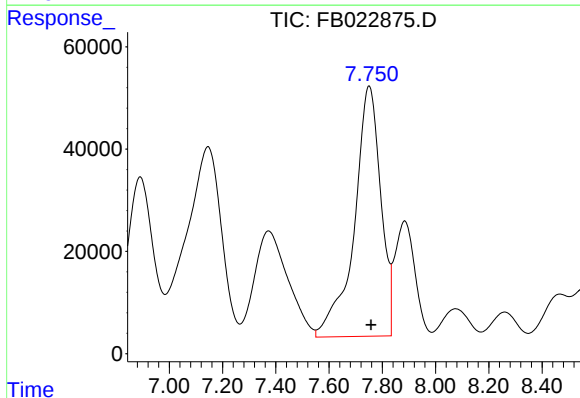


#3 n-Heptane

R.T.: 7.751 min
Delta R.T.: -0.007 min
Response: 3384955
Conc: 97.31 ng/ml

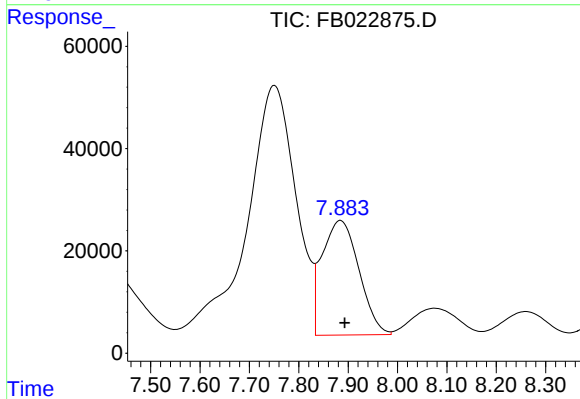

#4 Benzene


R.T.: 7.885 min
Delta R.T.: -0.008 min
Response: 1162615
Conc: 26.84 ng/ml

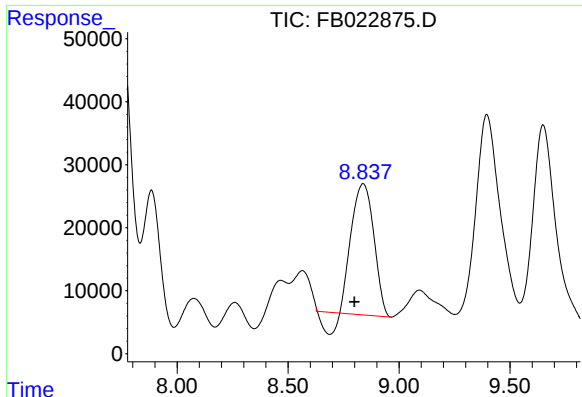

#5 AAA-TFT


R.T.: 8.839 min
Delta R.T.: 0.039 min
Response: 1367391
Conc: 60.74 ng/ml

Instrument :
FID_B
ClientSampleId :

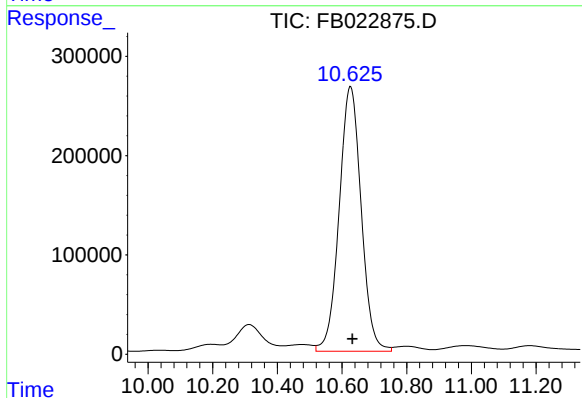


#6 Toluene

R.T.: 10.627 min
Delta R.T.: -0.005 min
Response: 12596831
Conc: 292.20 ng/ml

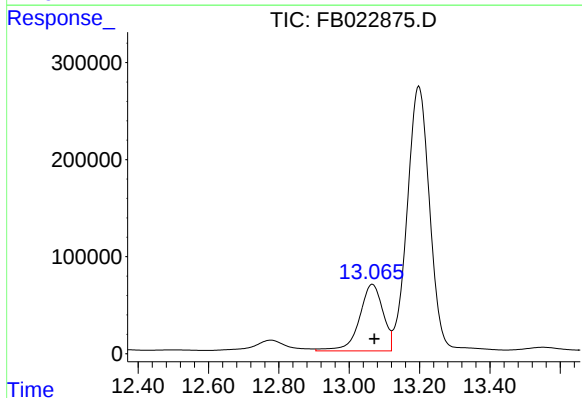


#7 Ethylbenzene

R.T.: 13.066 min
Delta R.T.: -0.006 min
Response: 3200653
Conc: 80.17 ng/ml

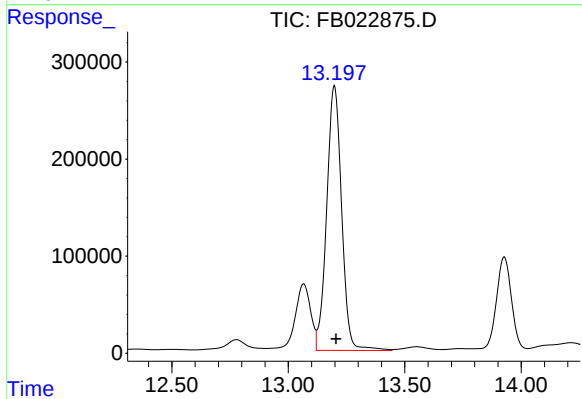

#8 m-Xylene

R.T.: 13.198 min
Delta R.T.: -0.007 min
Response: 12188969
Conc: 322.74 ng/ml

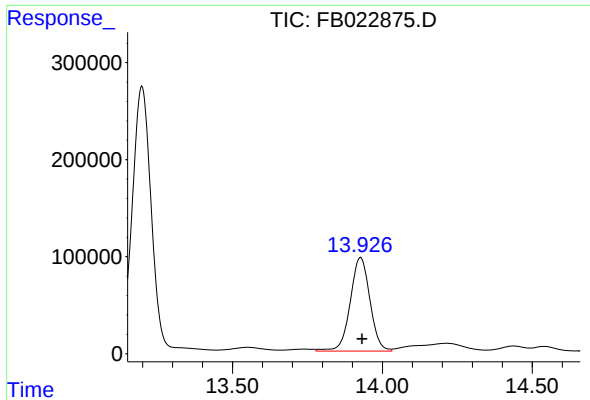

#9 O-Xylene


R.T.: 13.927 min

Delta R.T.: -0.005 min

Response: 4402969

Conc: 123.54 ng/ml

Instrument :
FID_B
ClientSampleId :

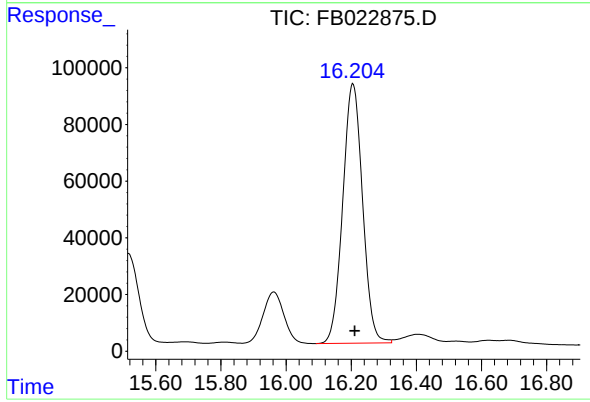

#10 1,2,4-Trimethylbenzene

R.T.: 16.206 min

Delta R.T.: -0.005 min

Response: 3870130

Conc: 136.47 ng/ml