

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110419\
 Data File : FB022877.D
 Signal(s) : FID2B.CH
 Acq On : 4 Nov 2019 16:42
 Operator : DD/AJ
 Sample : K5609-15 250X DD
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Nov 05 00:56:58 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
 Quant Title :
 QLast Update : Thu Oct 31 14:57:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.812	705649	31.346 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.683	425334	13.222 ng/ml
2) t 2,2,4-Trimethylpentane	7.376	605934	17.165 ng/ml
3) t n-Heptane	7.753	1124077	32.315 ng/ml
4) t Benzene	7.887	388857	8.978 ng/ml
6) t Toluene	10.627	4174175	96.825 ng/ml
7) t Ethylbenzene	13.067	1040273	26.057 ng/ml
8) t m-Xylene	13.198	3850541	101.955 ng/ml
9) t O-Xylene	13.928	1400872	39.305 ng/ml
10) t 1,2,4-Trimethylbenzene	16.207	1319891	46.543 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110419\
Data File : FB022877.D
Signal(s) : FID2B.CH
Acq On : 4 Nov 2019 16:42
Operator : DD/AJ
Sample : K5609-15 250X DD
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Nov 05 00:56:58 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
Quant Title :
QLast Update : Thu Oct 31 14:57:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

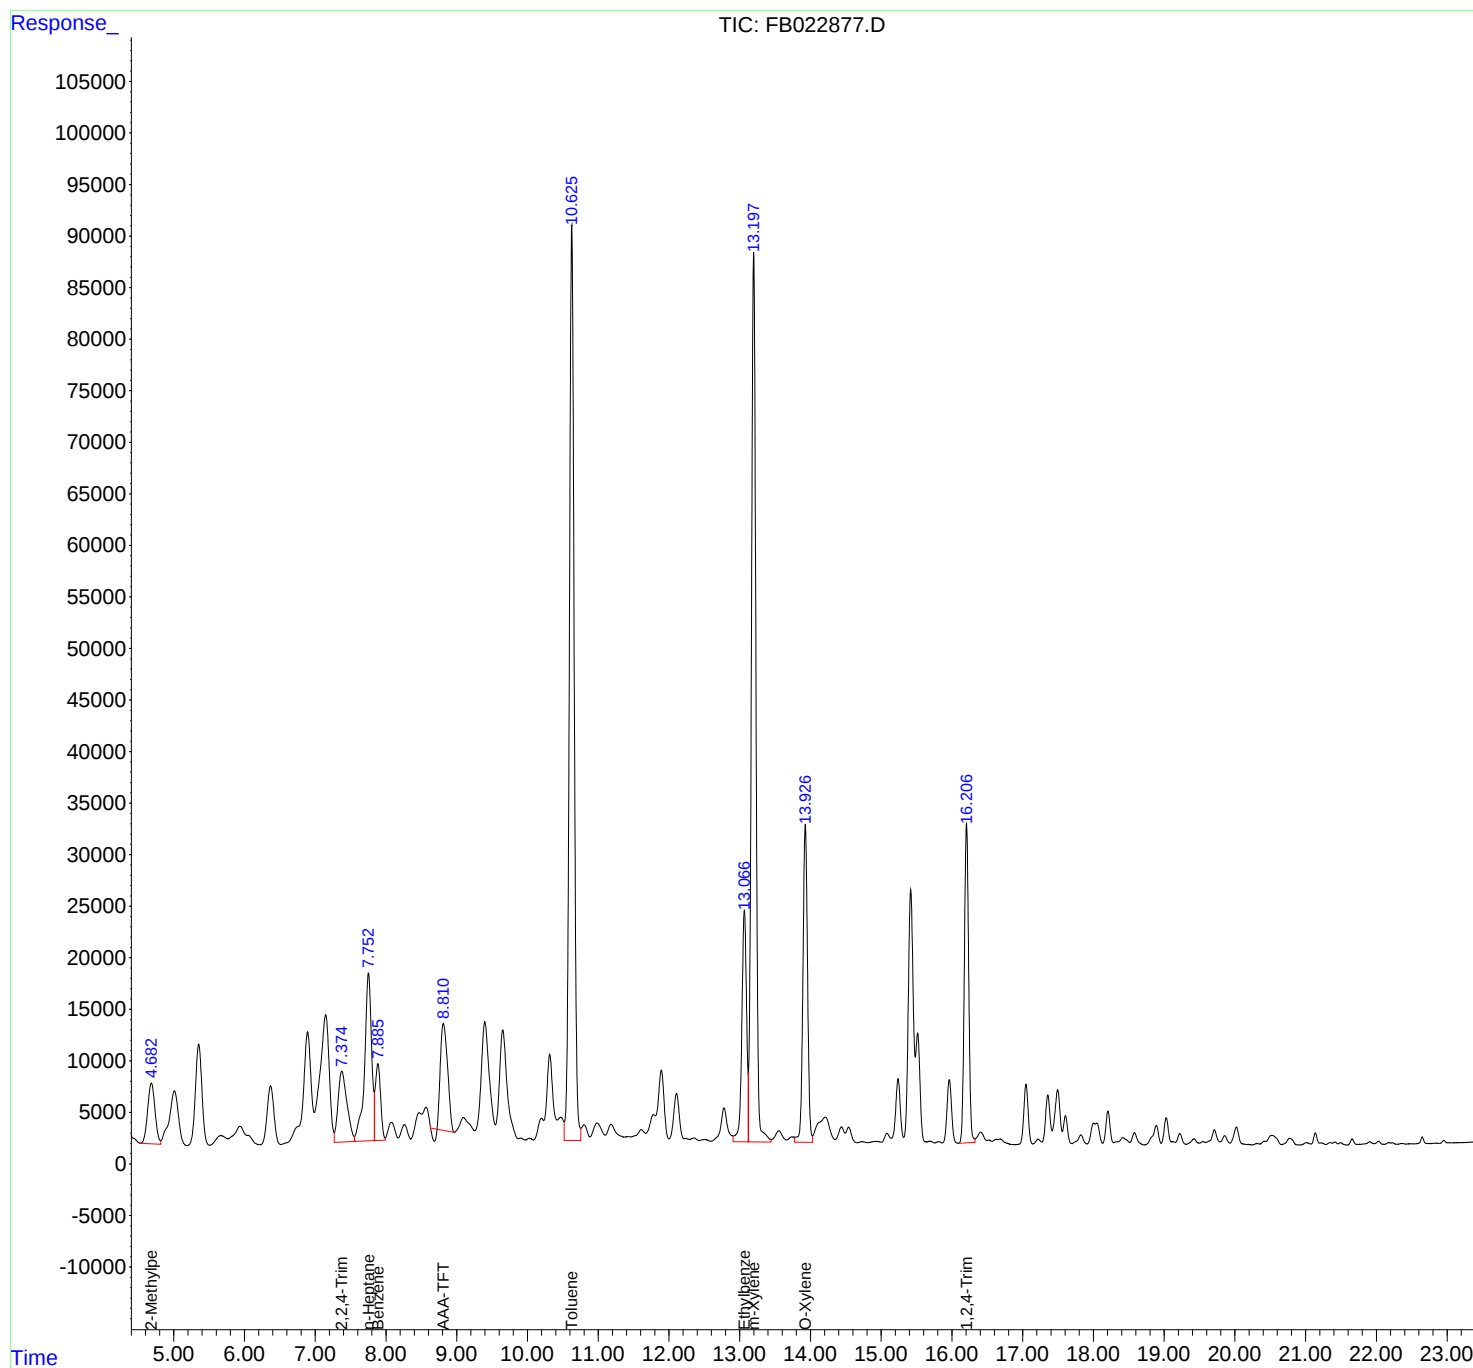


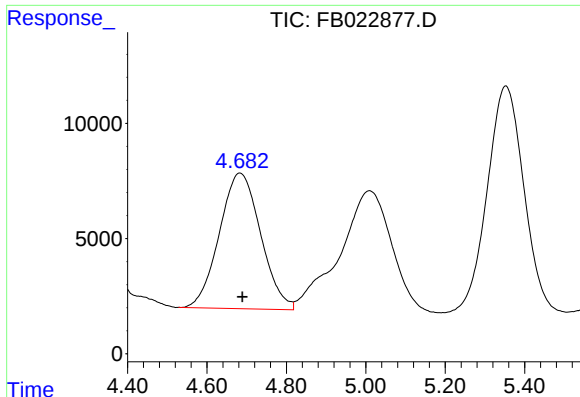

#1 2-Methylpentane


R.T.: 4.683 min
Delta R.T.: -0.006 min
Response: 425334
Conc: 13.22 ng/ml

Instrument :
FID_B
ClientSampleId :

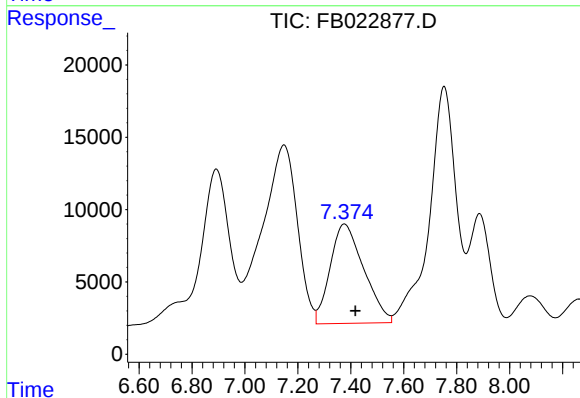


#2 2,2,4-Trimethylpentane

R.T.: 7.376 min
Delta R.T.: -0.042 min
Response: 605934
Conc: 17.17 ng/ml

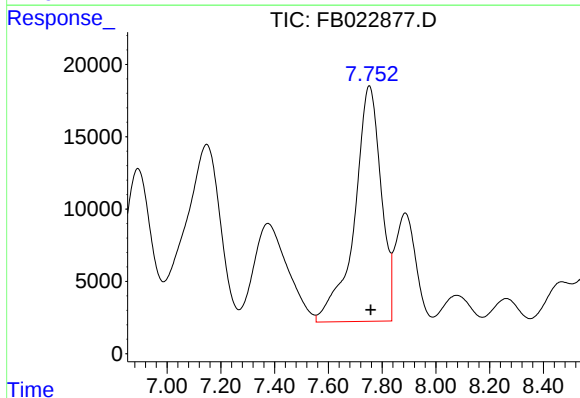


#3 n-Heptane

R.T.: 7.753 min
Delta R.T.: -0.005 min
Response: 1124077
Conc: 32.31 ng/ml

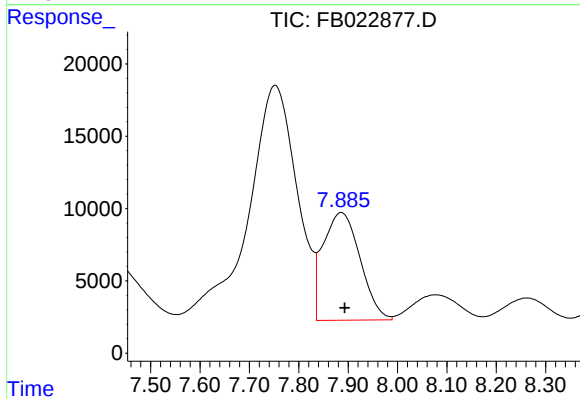

#4 Benzene


R.T.: 7.887 min
Delta R.T.: -0.006 min
Response: 388857
Conc: 8.98 ng/ml

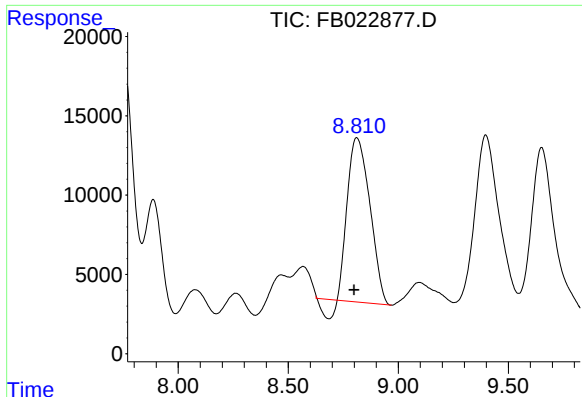

#5 AAA-TFT


R.T.: 8.812 min
Delta R.T.: 0.012 min
Response: 705649
Conc: 31.35 ng/ml

Instrument :
FID_B
ClientSampleId :

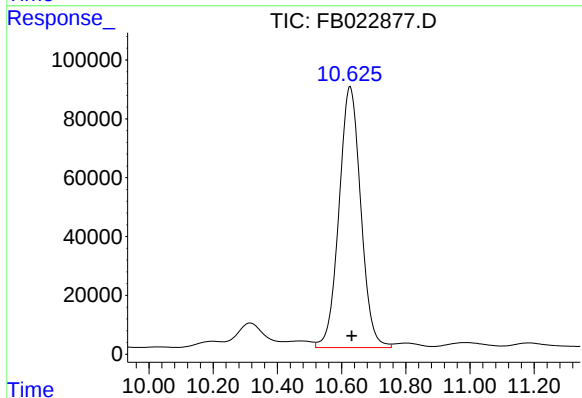


#6 Toluene

R.T.: 10.627 min
Delta R.T.: -0.005 min
Response: 4174175
Conc: 96.83 ng/ml

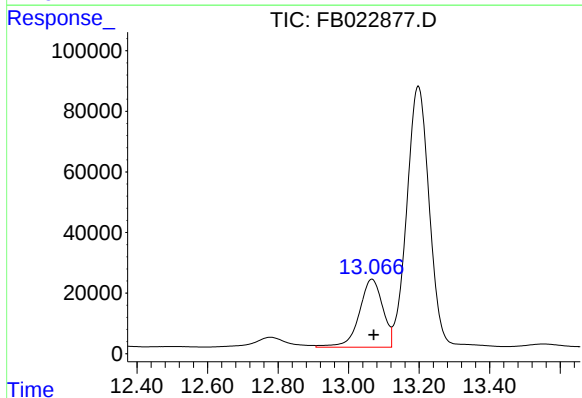


#7 Ethylbenzene

R.T.: 13.067 min
Delta R.T.: -0.005 min
Response: 1040273
Conc: 26.06 ng/ml

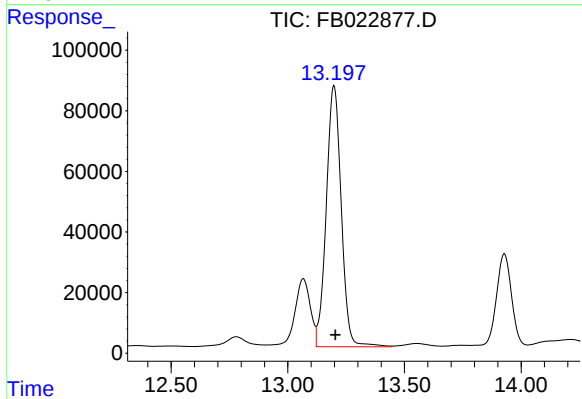

#8 m-Xylene


R.T.: 13.198 min
Delta R.T.: -0.007 min
Response: 3850541
Conc: 101.95 ng/ml

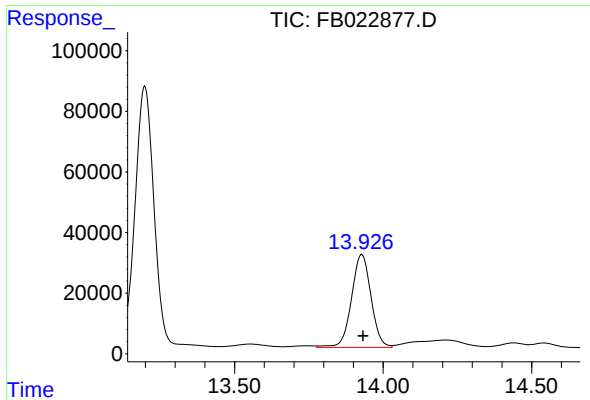

#9 O-Xylene

R.T.: 13.928 min
Delta R.T.: -0.004 min
Response: 1400872
Conc: 39.31 ng/ml

Instrument :
FID_B
ClientSampleId :

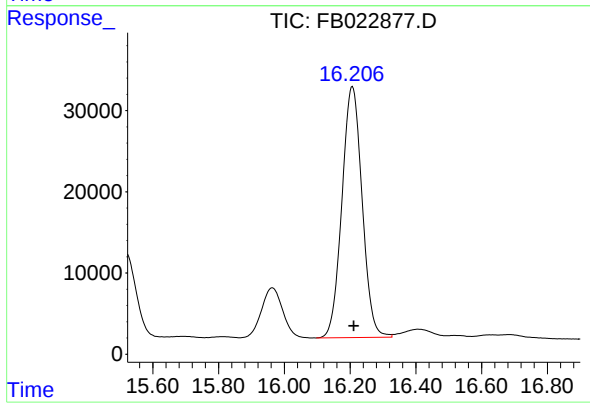

#10 1,2,4-Trimethylbenzene

R.T.: 16.207 min
Delta R.T.: -0.004 min
Response: 1319891
Conc: 46.54 ng/ml