

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110419\
Data File : FB022880.D
Signal(s) : FID2B.CH
Acq On : 4 Nov 2019 20:11
Operator : DD/AJ
Sample : K5676-02
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Nov 05 00:57:27 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
Quant Title :
QLast Update : Thu Oct 31 14:57:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.795	459780	20.424 ng/ml
Target Compounds			
6) t Toluene	10.632	1290	0.030 ng/ml
8) t m-Xylene	13.206	1566	0.041 ng/ml
10) t 1,2,4-Trimethylbenzene	16.198	1580	0.056 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110419\
Data File : FB022880.D
Signal(s) : FID2B.CH
Acq On : 4 Nov 2019 20:11
Operator : DD/AJ
Sample : K5676-02
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Nov 05 00:57:27 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
Quant Title :
QLast Update : Thu Oct 31 14:57:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

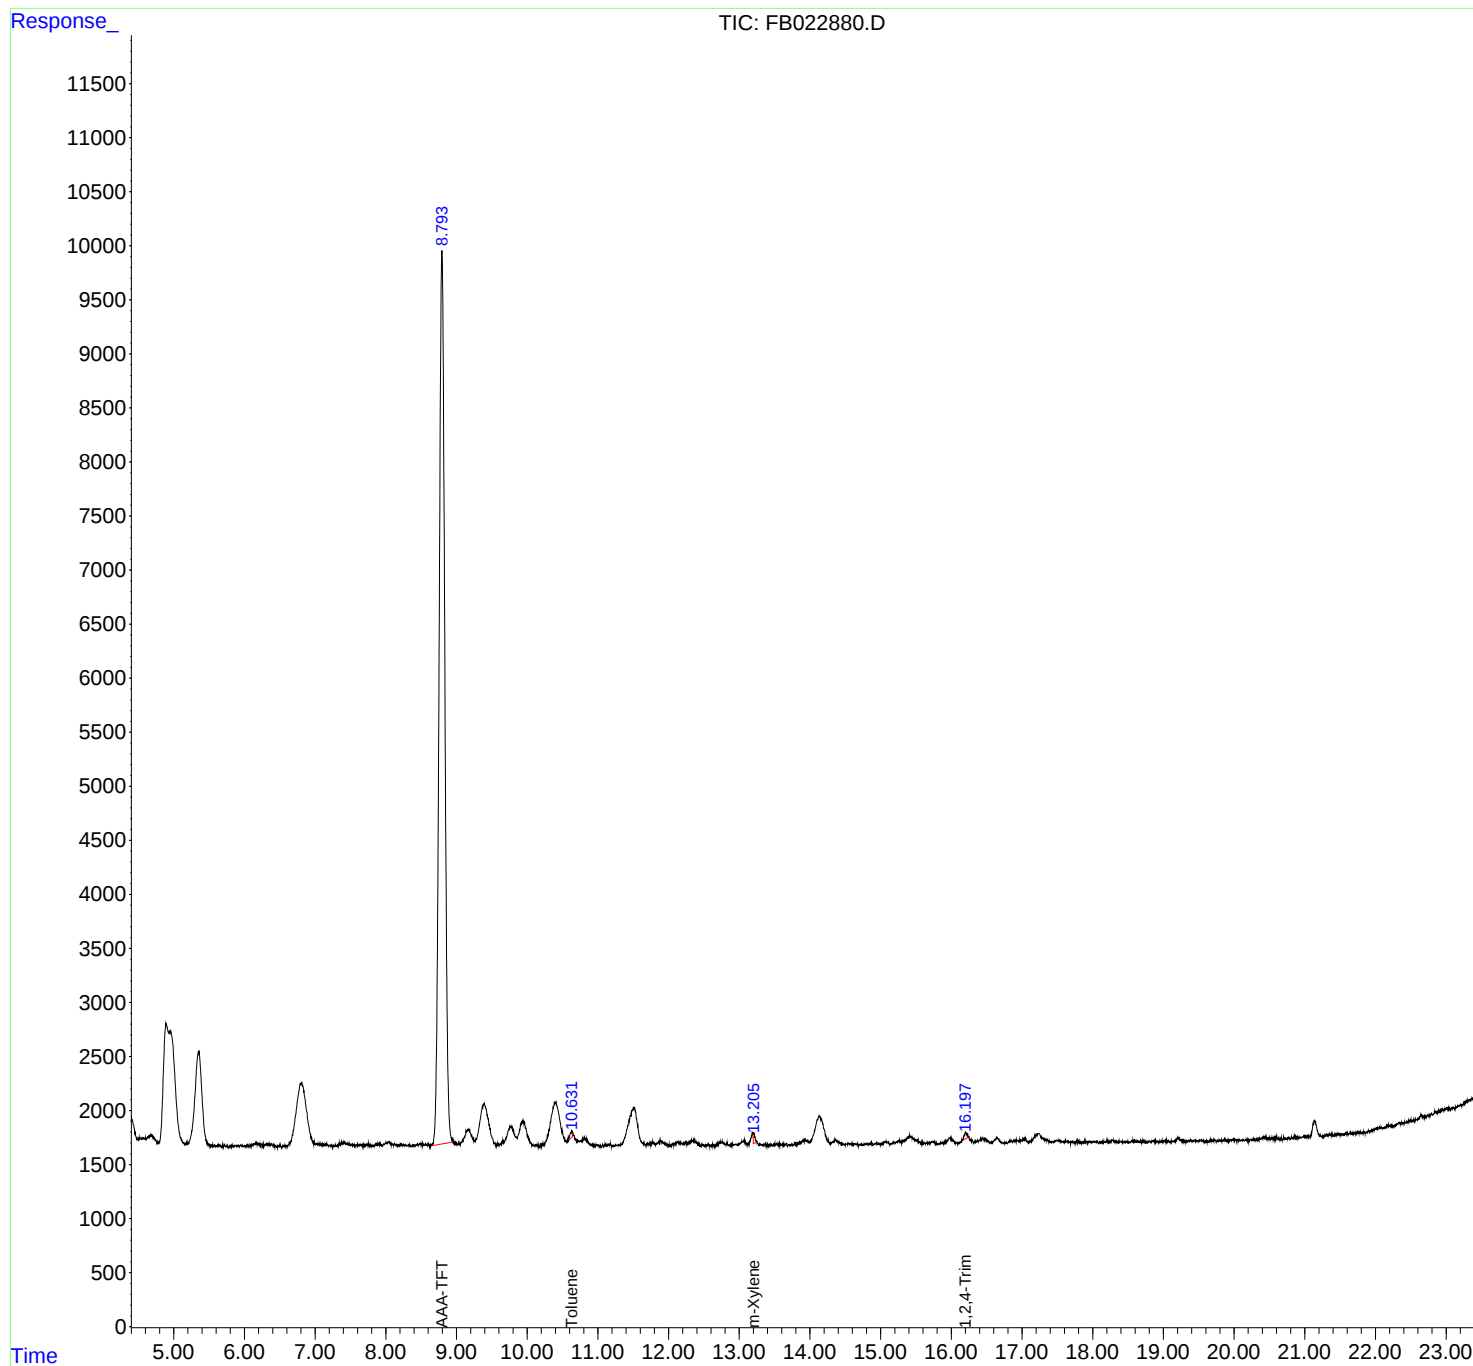


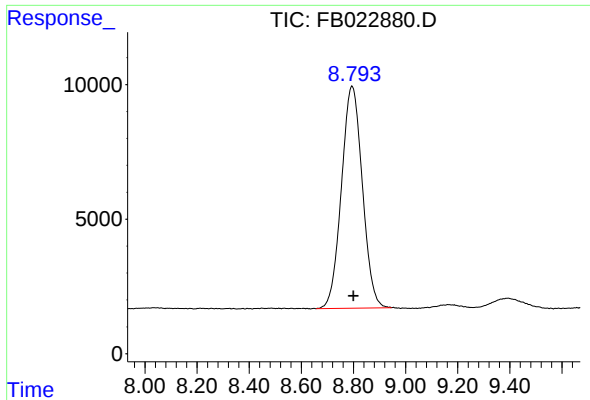

#5 AAA-TFT


R.T.: 8.795 min
Delta R.T.: -0.005 min
Response: 459780
Conc: 20.42 ng/ml

Instrument :
FID_B
ClientSampleId :

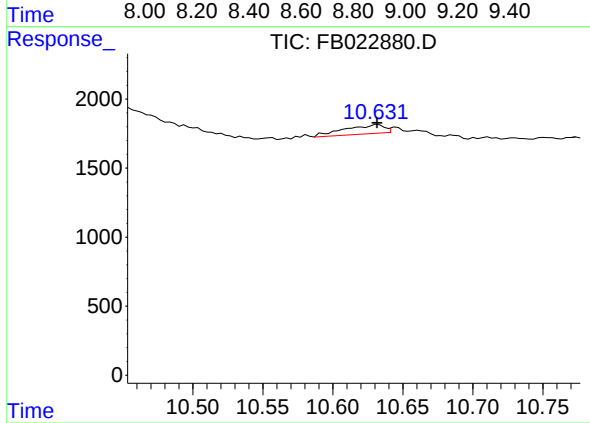


#6 Toluene

R.T.: 10.632 min
Delta R.T.: 0.000 min
Response: 1290
Conc: 0.03 ng/ml

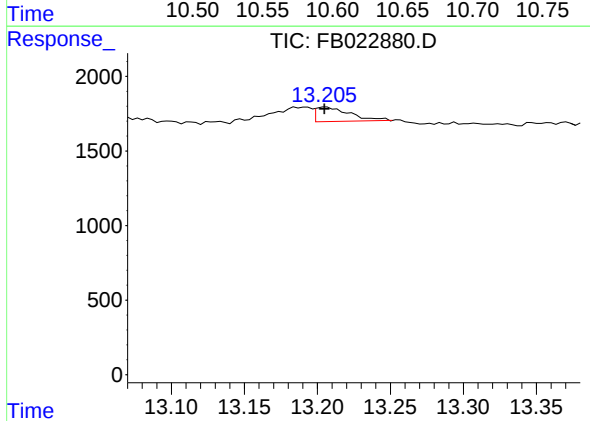

#8 m-Xylene

R.T.: 13.206 min
Delta R.T.: 0.001 min
Response: 1566
Conc: 0.04 ng/ml

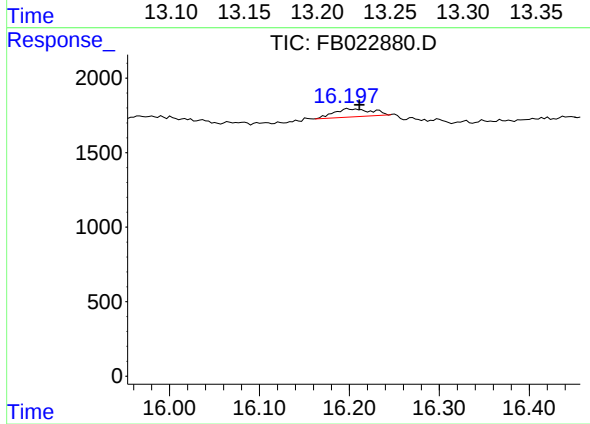

#10 1,2,4-Trimethylbenzene

R.T.: 16.198 min
Delta R.T.: -0.013 min
Response: 1580
Conc: 0.06 ng/ml