

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110419\
 Data File : FB022882.D
 Signal(s) : FID2B.CH
 Acq On : 4 Nov 2019 21:10
 Operator : DD/AJ
 Sample : K5676-02MSD
 Misc : 5.04g/5.00ml DI WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Nov 05 00:57:46 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
 Quant Title :
 QLast Update : Thu Oct 31 14:57:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.796	439534	19.525 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.686	867609	26.972 ng/ml
2) t 2,2,4-Trimethylpentane	7.414	893194	25.303 ng/ml
3) t n-Heptane	7.754	284838	8.188 ng/ml
4) t Benzene	7.889	412647	9.527 ng/ml
6) t Toluene	10.627	1212214	28.119 ng/ml
7) t Ethylbenzene	13.067	351919	8.815 ng/ml
8) t m-Xylene	13.200	656792	17.391 ng/ml
9) t O-Xylene	13.928	627089	17.595 ng/ml
10) t 1,2,4-Trimethylbenzene	16.207	487334	17.185 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110419\
Data File : FB022882.D
Signal(s) : FID2B.CH
Acq On : 4 Nov 2019 21:10
Operator : DD/AJ
Sample : K5676-02MSD
Misc : 5.04g/5.00ml DI WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Nov 05 00:57:46 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
Quant Title :
QLast Update : Thu Oct 31 14:57:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

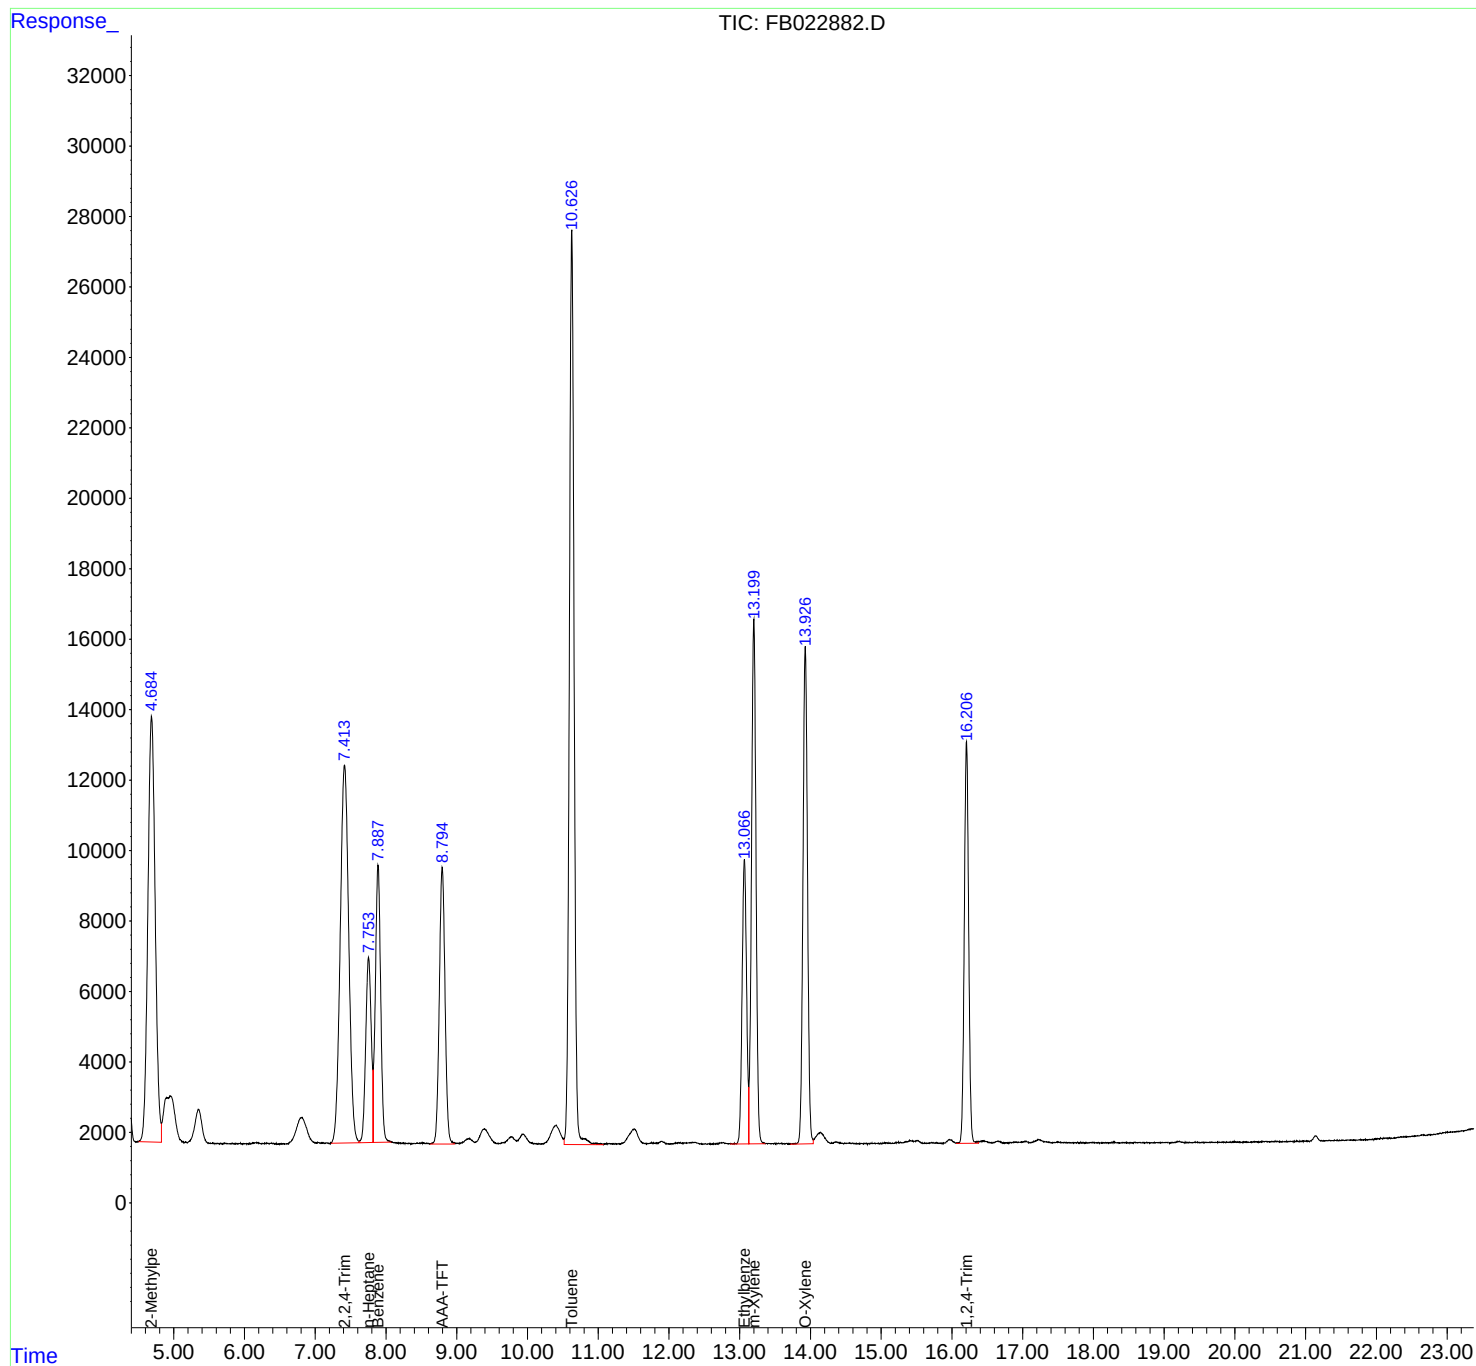


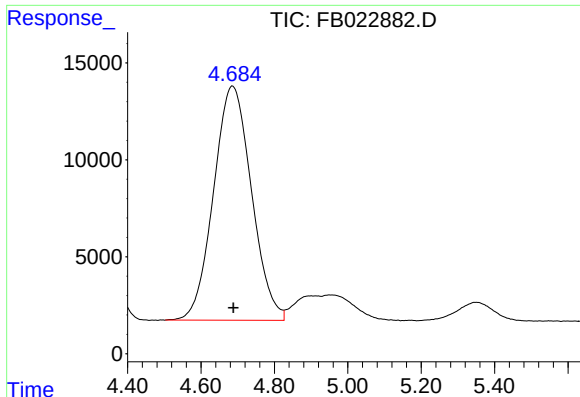

#1 2-Methylpentane


R.T.: 4.686 min
Delta R.T.: -0.003 min
Response: 867609
Conc: 26.97 ng/ml

Instrument :
FID_B
ClientSampleId :

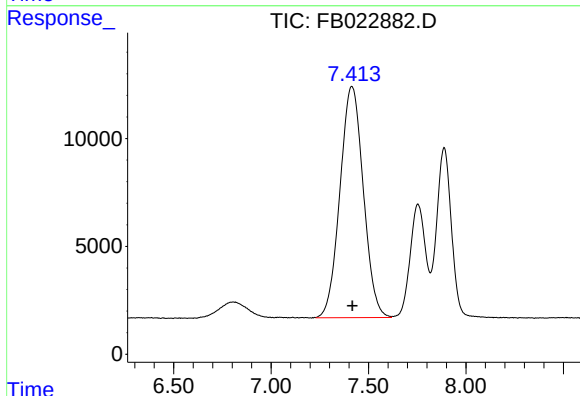


#2 2,2,4-Trimethylpentane

R.T.: 7.414 min
Delta R.T.: -0.004 min
Response: 893194
Conc: 25.30 ng/ml

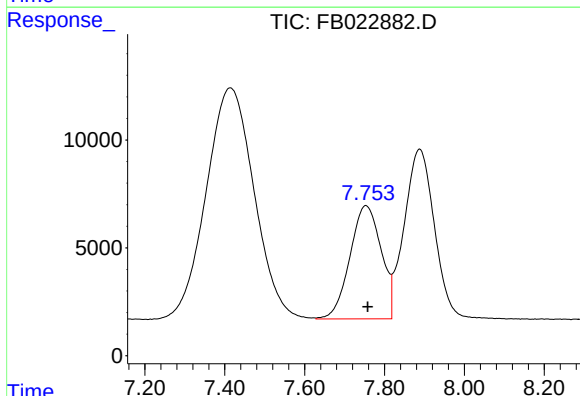


#3 n-Heptane

R.T.: 7.754 min
Delta R.T.: -0.004 min
Response: 284838
Conc: 8.19 ng/ml

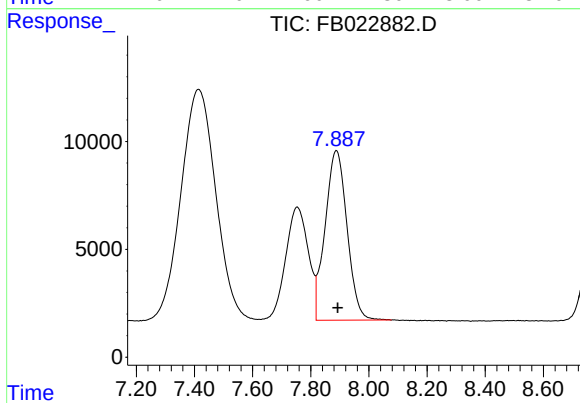

#4 Benzene


R.T.: 7.889 min
Delta R.T.: -0.004 min
Response: 412647
Conc: 9.53 ng/ml

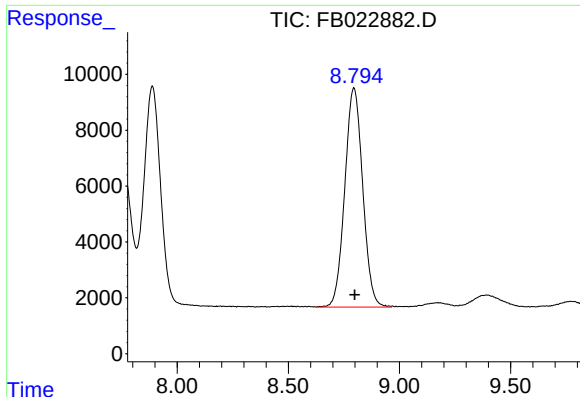

#5 AAA-TFT


R.T.: 8.796 min
Delta R.T.: -0.004 min
Response: 439534
Conc: 19.52 ng/ml

Instrument :
FID_B
ClientSampleId :

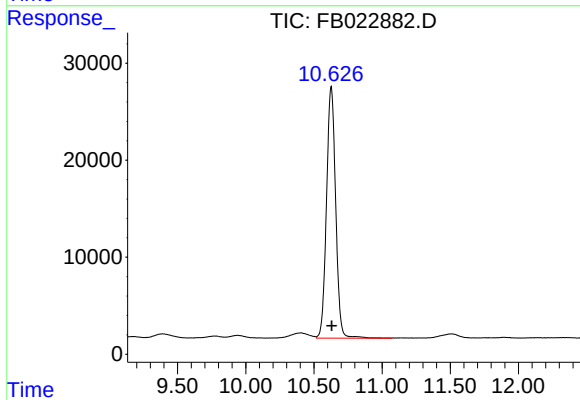


#6 Toluene

R.T.: 10.627 min
Delta R.T.: -0.005 min
Response: 1212214
Conc: 28.12 ng/ml

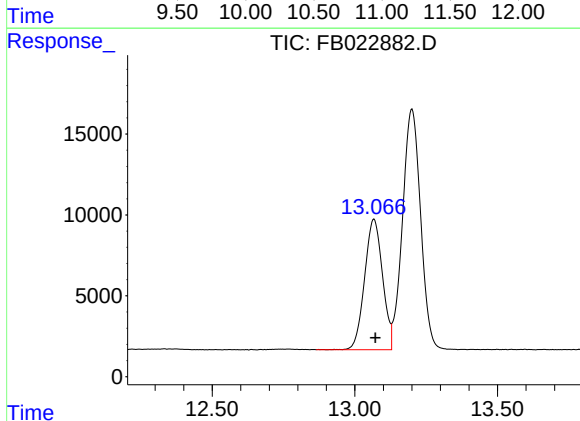


#7 Ethylbenzene

R.T.: 13.067 min
Delta R.T.: -0.005 min
Response: 351919
Conc: 8.82 ng/ml

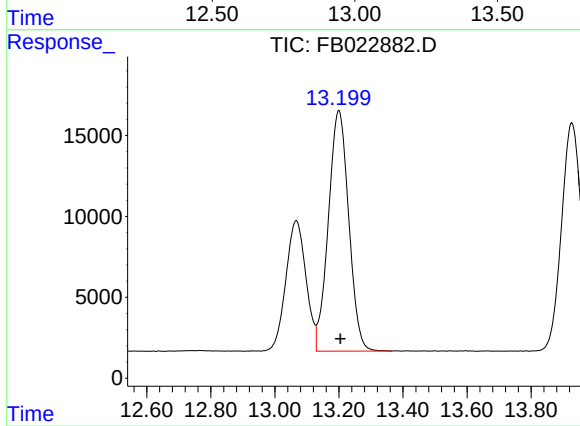

#8 m-Xylene


R.T.: 13.200 min
Delta R.T.: -0.005 min
Response: 656792
Conc: 17.39 ng/ml

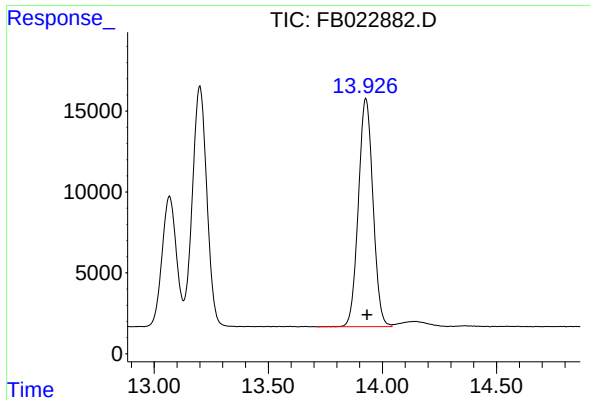

#9 O-Xylene

R.T.: 13.928 min
Delta R.T.: -0.005 min
Response: 627089
Conc: 17.59 ng/ml

Instrument :
FID_B
ClientSampleId :

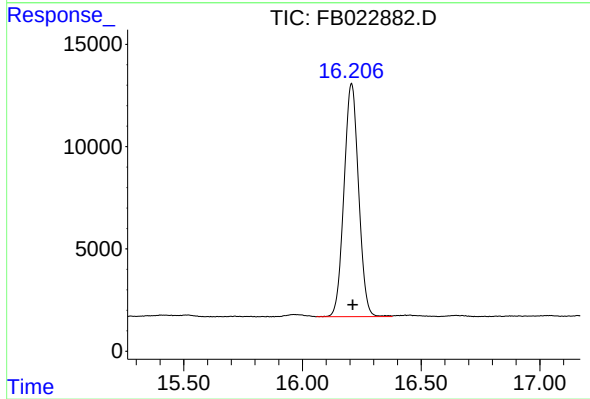

#10 1,2,4-Trimethylbenzene

R.T.: 16.207 min
Delta R.T.: -0.004 min
Response: 487334
Conc: 17.18 ng/ml