

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110419\
 Data File : FB022870.D
 Signal(s) : FID2B.CH
 Acq On : 4 Nov 2019 10:29
 Operator : DD/AJ
 Sample : BSF1101S1
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1101S1

Integration File: Calibration.e
 Quant Time: Nov 05 00:55:48 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
 Quant Title :
 QLast Update : Thu Oct 31 14:57:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.793	448426	19.920 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.682	990666	30.797 ng/ml
2) t 2,2,4-Trimethylpentane	7.411	1117036	31.644 ng/ml
3) t n-Heptane	7.751	369015	10.608 ng/ml
4) t Benzene	7.886	439962	10.157 ng/ml
6) t Toluene	10.625	1299809	30.151 ng/ml
7) t Ethylbenzene	13.066	411004	10.295 ng/ml
8) t m-Xylene	13.198	776274	20.554 ng/ml
9) t O-Xylene	13.926	728936	20.452 ng/ml
10) t 1,2,4-Trimethylbenzene	16.205	600868	21.188 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110419\
Data File : FB022870.D
Signal(s) : FID2B.CH
Acq On : 4 Nov 2019 10:29
Operator : DD/AJ
Sample : BSF1101S1
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1101S1

Integration File: Calibration.e
Quant Time: Nov 05 00:55:48 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
Quant Title :
QLast Update : Thu Oct 31 14:57:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

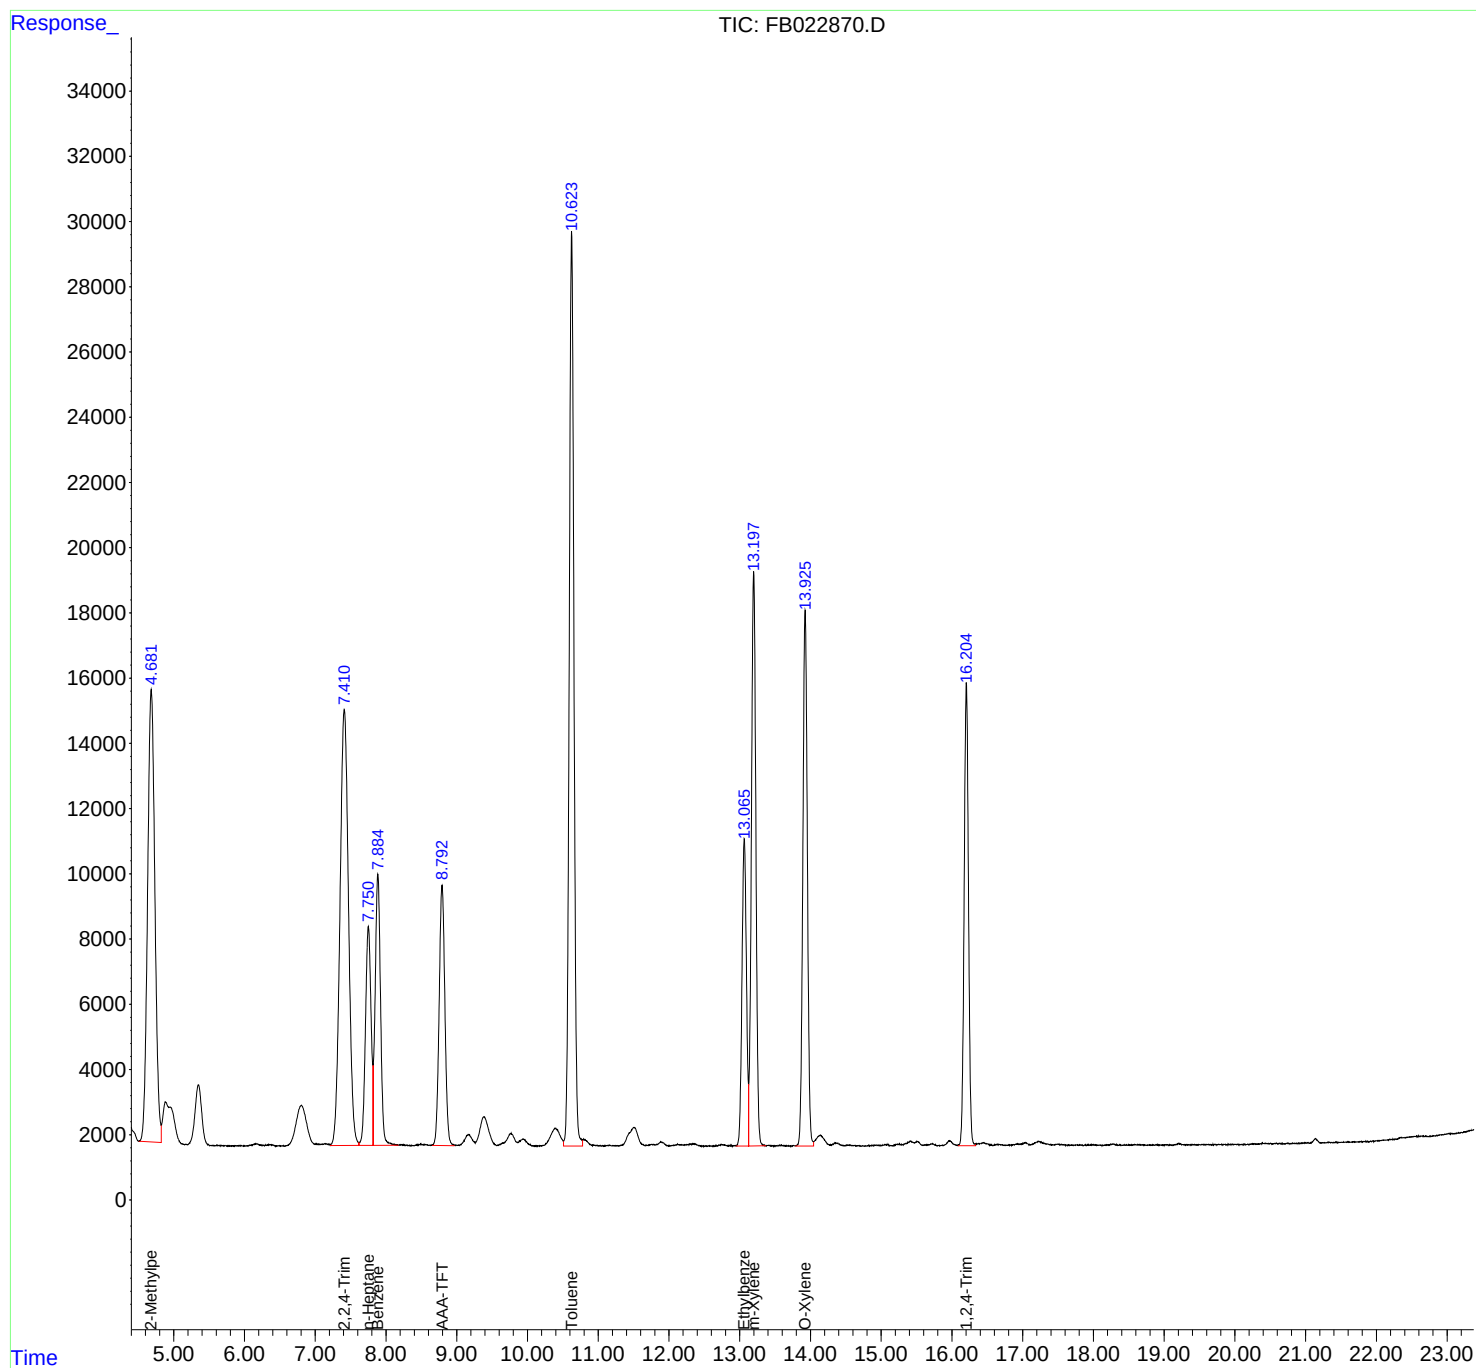


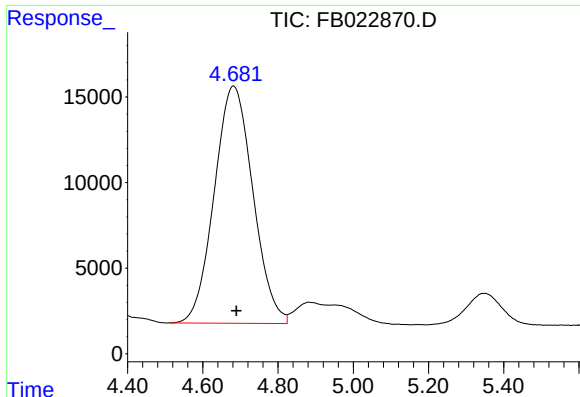

#1 2-Methylpentane


R.T.: 4.682 min
Delta R.T.: -0.007 min
Response: 990666
Conc: 30.80 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1101S1

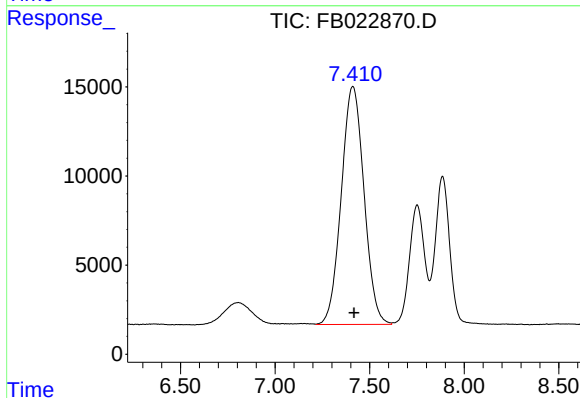


#2 2,2,4-Trimethylpentane

R.T.: 7.411 min
Delta R.T.: -0.007 min
Response: 1117036
Conc: 31.64 ng/ml

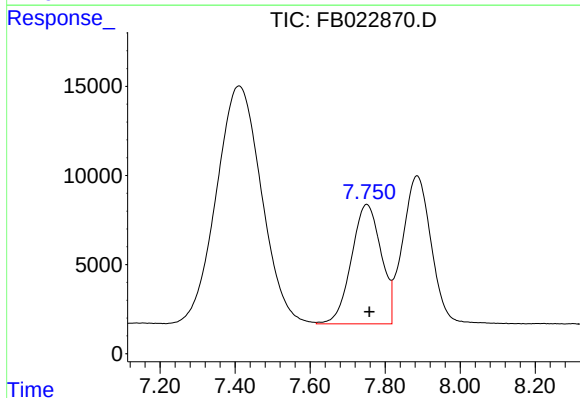


#3 n-Heptane

R.T.: 7.751 min
Delta R.T.: -0.007 min
Response: 369015
Conc: 10.61 ng/ml

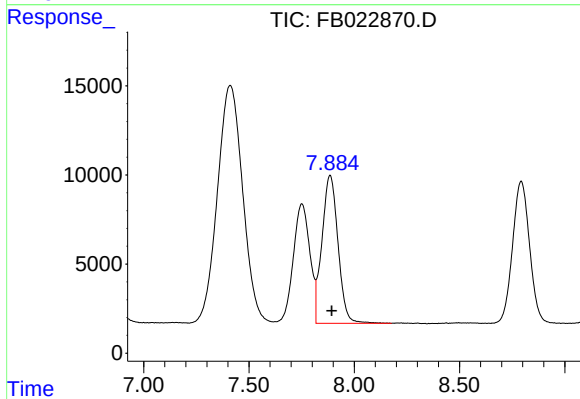

#4 Benzene


R.T.: 7.886 min
Delta R.T.: -0.007 min
Response: 439962
Conc: 10.16 ng/ml

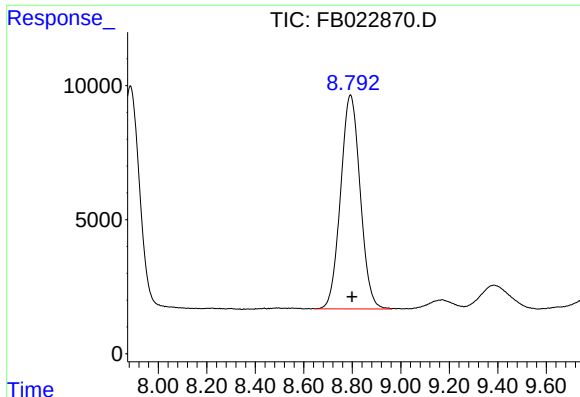

#5 AAA-TFT


R.T.: 8.793 min
Delta R.T.: -0.006 min
Response: 448426
Conc: 19.92 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1101S1

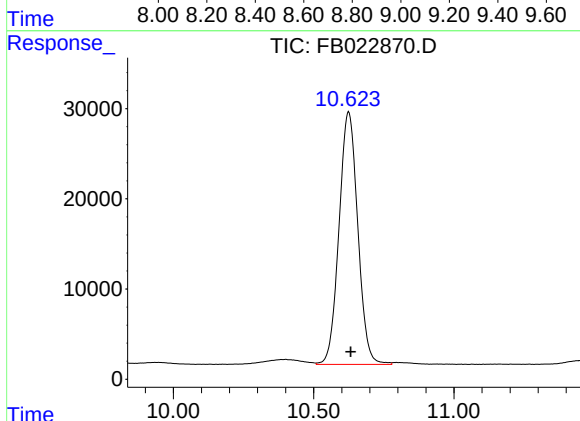


#6 Toluene

R.T.: 10.625 min
Delta R.T.: -0.007 min
Response: 1299809
Conc: 30.15 ng/ml

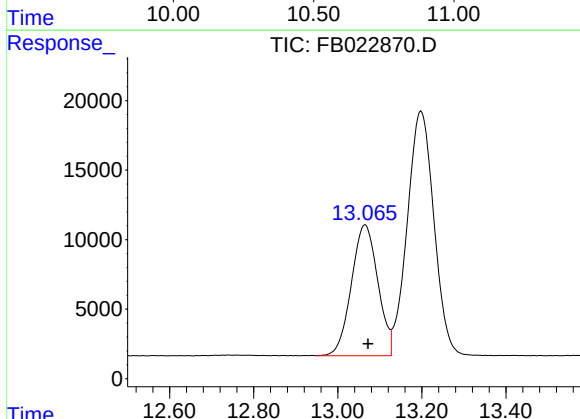


#7 Ethylbenzene

R.T.: 13.066 min
Delta R.T.: -0.006 min
Response: 411004
Conc: 10.30 ng/ml

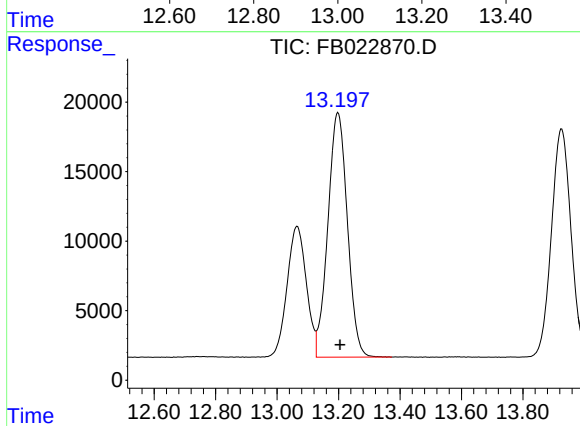

#8 m-Xylene


R.T.: 13.198 min
Delta R.T.: -0.007 min
Response: 776274
Conc: 20.55 ng/ml

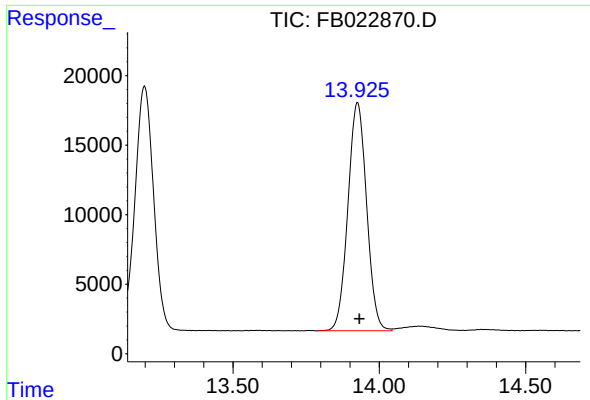

#9 O-Xylene

R.T.: 13.926 min
Delta R.T.: -0.006 min
Response: 728936
Conc: 20.45 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1101S1

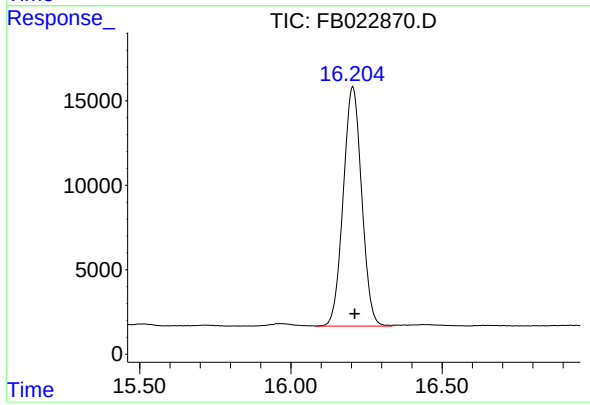

#10 1,2,4-Trimethylbenzene

R.T.: 16.205 min
Delta R.T.: -0.006 min
Response: 600868
Conc: 21.19 ng/ml