

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110419\
 Data File : FB022881.D
 Signal(s) : FID2B.CH
 Acq On : 4 Nov 2019 20:41
 Operator : DD/AJ
 Sample : K5676-02MS
 Misc : 5.06g/5.00ml DI WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 SU-02-110119MS

Integration File: Calibration.e
 Quant Time: Nov 05 00:57:36 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
 Quant Title :
 QLast Update : Thu Oct 31 14:57:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.795	377002	16.747 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.686	768154	23.880 ng/ml
2) t 2,2,4-Trimethylpentane	7.414	826937	23.426 ng/ml
3) t n-Heptane	7.752	263345	7.571 ng/ml
4) t Benzene	7.888	392460	9.061 ng/ml
6) t Toluene	10.626	1133378	26.290 ng/ml
7) t Ethylbenzene	13.066	350499	8.779 ng/ml
8) t m-Xylene	13.199	666286	17.642 ng/ml
9) t O-Xylene	13.927	634657	17.807 ng/ml
10) t 1,2,4-Trimethylbenzene	16.206	500376	17.645 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110419\
Data File : FB022881.D
Signal(s) : FID2B.CH
Acq On : 4 Nov 2019 20:41
Operator : DD/AJ
Sample : K5676-02MS
Misc : 5.06g/5.00ml DI WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
SU-02-110119MS

Integration File: Calibration.e
Quant Time: Nov 05 00:57:36 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
Quant Title :
QLast Update : Thu Oct 31 14:57:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

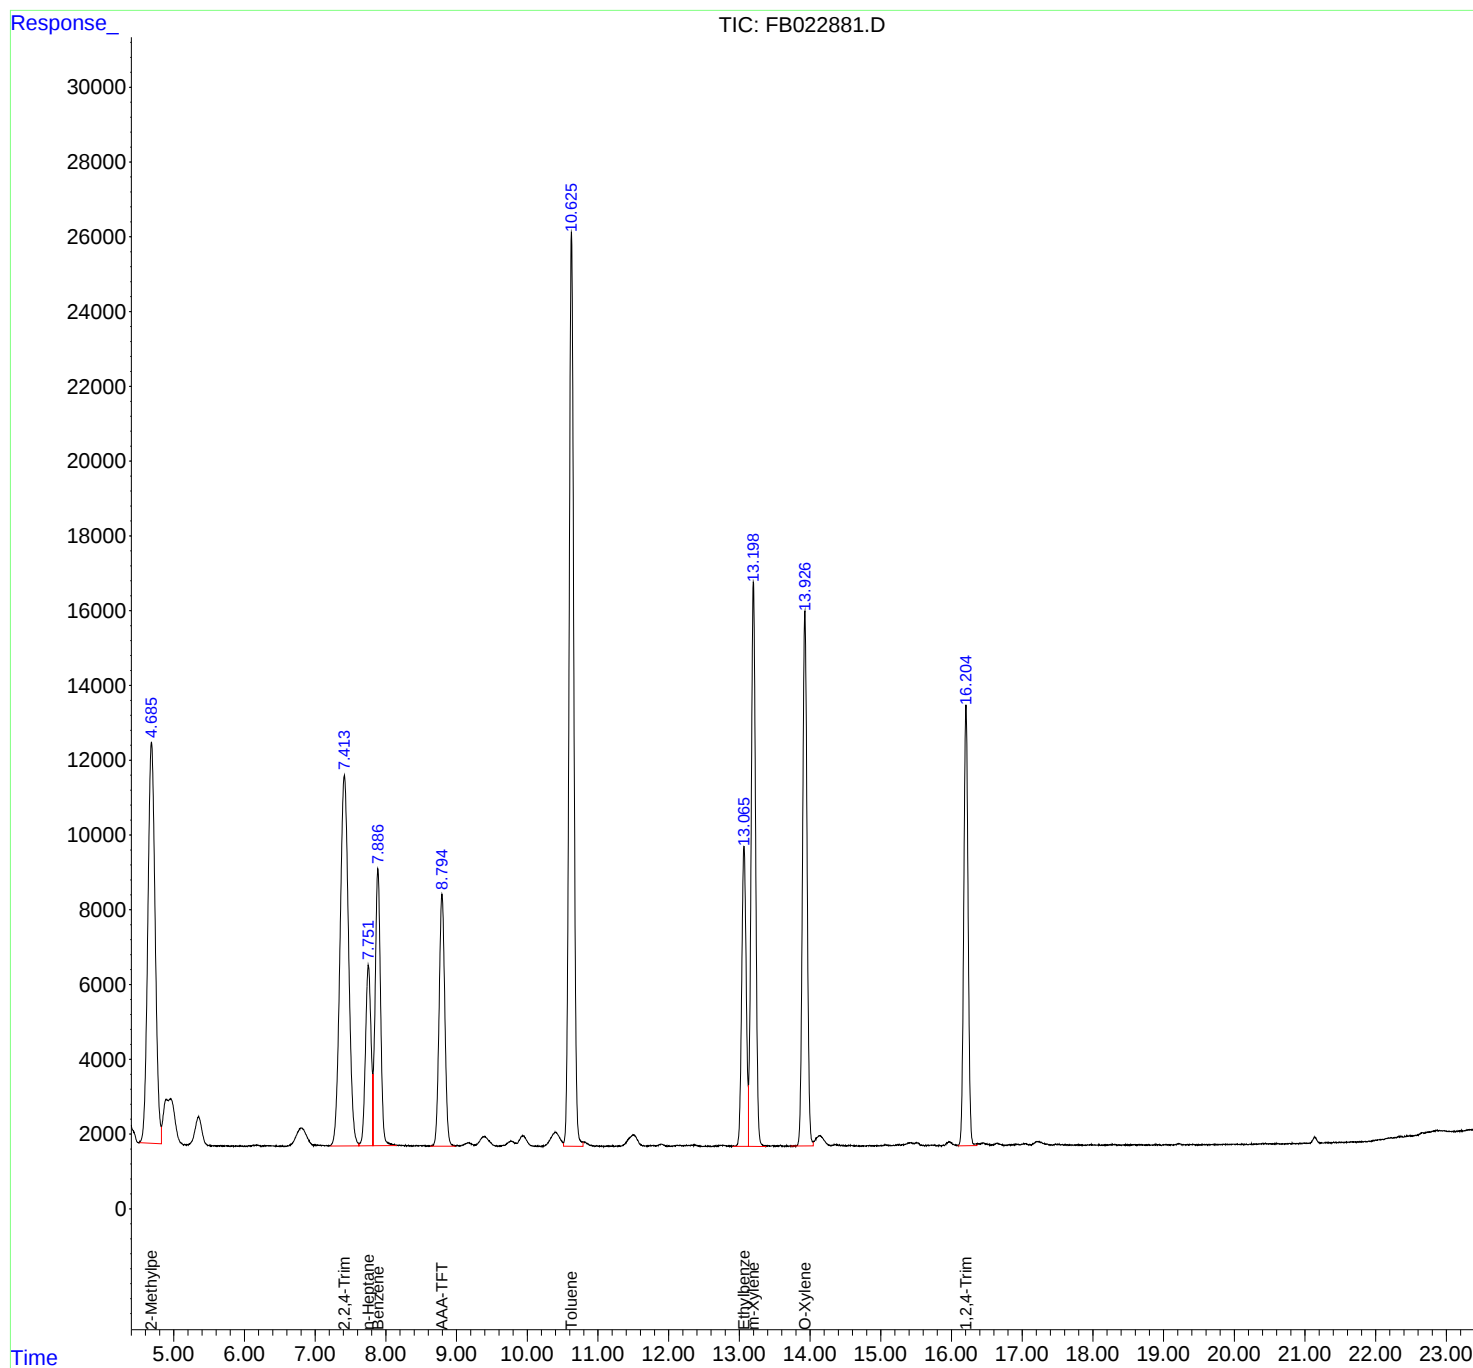


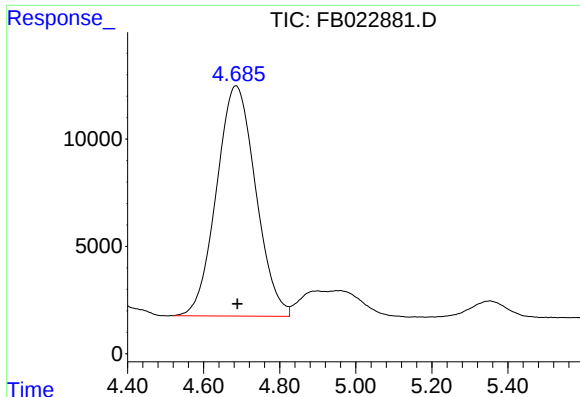

#1 2-Methylpentane


R.T.: 4.686 min
Delta R.T.: -0.003 min
Response: 768154
Conc: 23.88 ng/ml

Instrument :
FID_B
ClientSampleId :
SU-02-110119MS

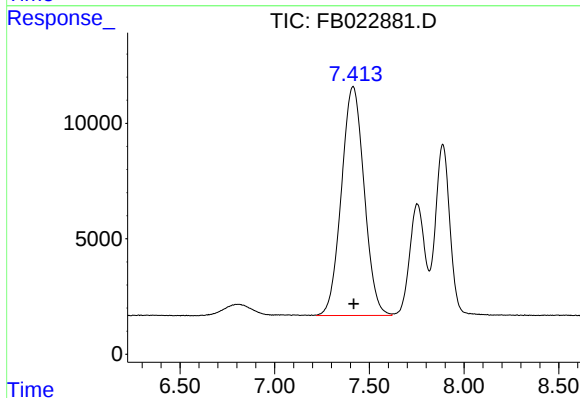


#2 2,2,4-Trimethylpentane

R.T.: 7.414 min
Delta R.T.: -0.004 min
Response: 826937
Conc: 23.43 ng/ml

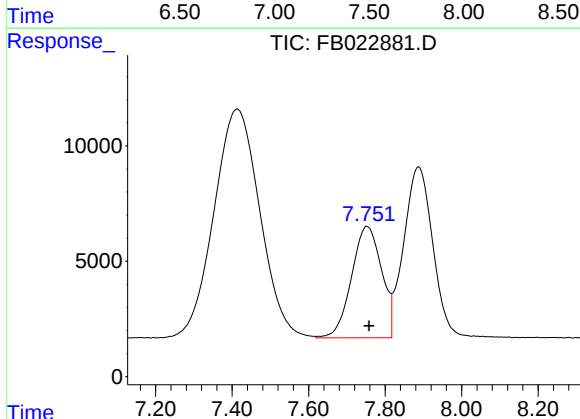


#3 n-Heptane

R.T.: 7.752 min
Delta R.T.: -0.006 min
Response: 263345
Conc: 7.57 ng/ml

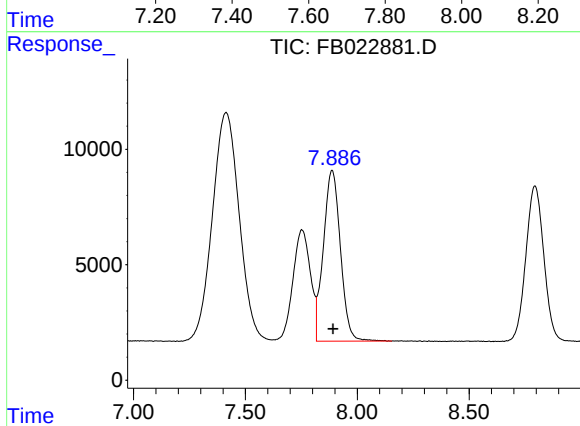

#4 Benzene


R.T.: 7.888 min
Delta R.T.: -0.005 min
Response: 392460
Conc: 9.06 ng/ml

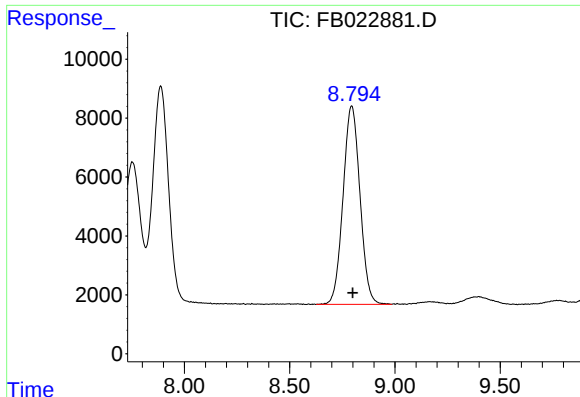

#5 AAA-TFT


R.T.: 8.795 min
Delta R.T.: -0.005 min
Response: 377002
Conc: 16.75 ng/ml

Instrument :
FID_B
ClientSampleId :
SU-02-110119MS

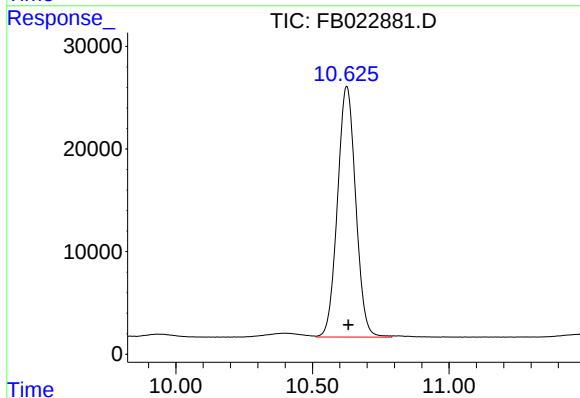


#6 Toluene

R.T.: 10.626 min
Delta R.T.: -0.006 min
Response: 1133378
Conc: 26.29 ng/ml

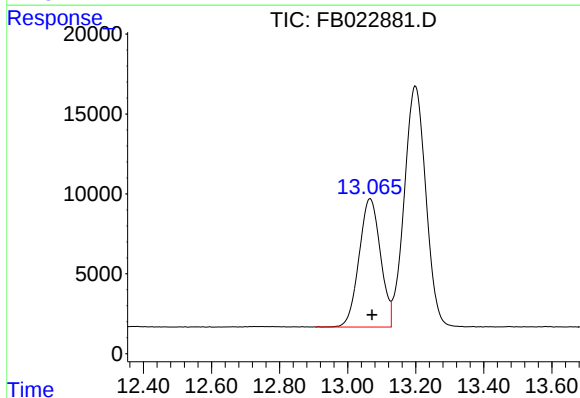


#7 Ethylbenzene

R.T.: 13.066 min
Delta R.T.: -0.005 min
Response: 350499
Conc: 8.78 ng/ml

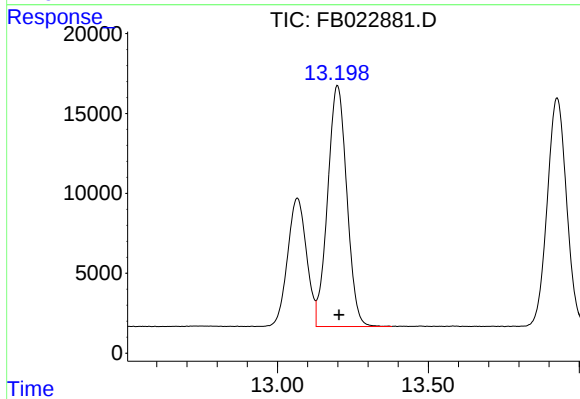

#8 m-Xylene


R.T.: 13.199 min
Delta R.T.: -0.005 min
Response: 666286
Conc: 17.64 ng/ml

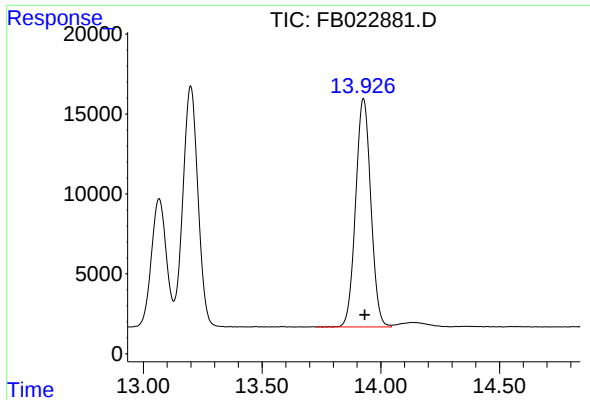

#9 O-Xylene

R.T.: 13.927 min
Delta R.T.: -0.005 min
Response: 634657
Conc: 17.81 ng/ml

Instrument :
FID_B
ClientSampleId :
SU-02-110119MS

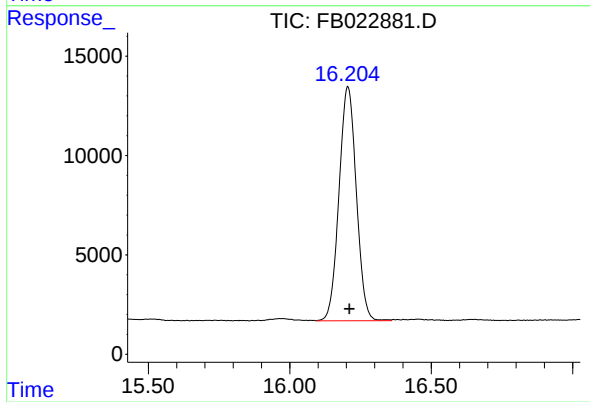

#10 1,2,4-Trimethylbenzene

R.T.: 16.206 min
Delta R.T.: -0.005 min
Response: 500376
Conc: 17.64 ng/ml