

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110420\
 Data File : FB025183.D
 Signal(s) : FID2B.CH
 Acq On : 4 Nov 2020 12:03
 Operator : DD/AJ
 Sample : VBF1104S3
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Nov 05 12:01:28 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110320.M
 Quant Title :
 QLast Update : Wed Nov 04 08:05:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.797	451539	19.998 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.678	26440	0.819 ng/ml
2) t 2,2,4-Trimethylpentane	7.371	48000	1.447 ng/ml
3) t n-Heptane	7.751	68802	2.095 ng/ml
4) t Benzene	7.888	31512	0.793 ng/ml
6) t Toluene	10.628	496126	13.269 ng/ml
7) t Ethylbenzene	13.069	130989	3.814 ng/ml
8) t m-Xylene	13.199	440916	13.059 ng/ml
9) t O-Xylene	13.929	158590	4.850 ng/ml
10) t 1,2,4-Trimethylbenzene	16.207	173004	6.288 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110420\
Data File : FB025183.D
Signal(s) : FID2B.CH
Acq On : 4 Nov 2020 12:03
Operator : DD/AJ
Sample : VBF1104S3
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Nov 05 12:01:28 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110320.M
Quant Title :
QLast Update : Wed Nov 04 08:05:53 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

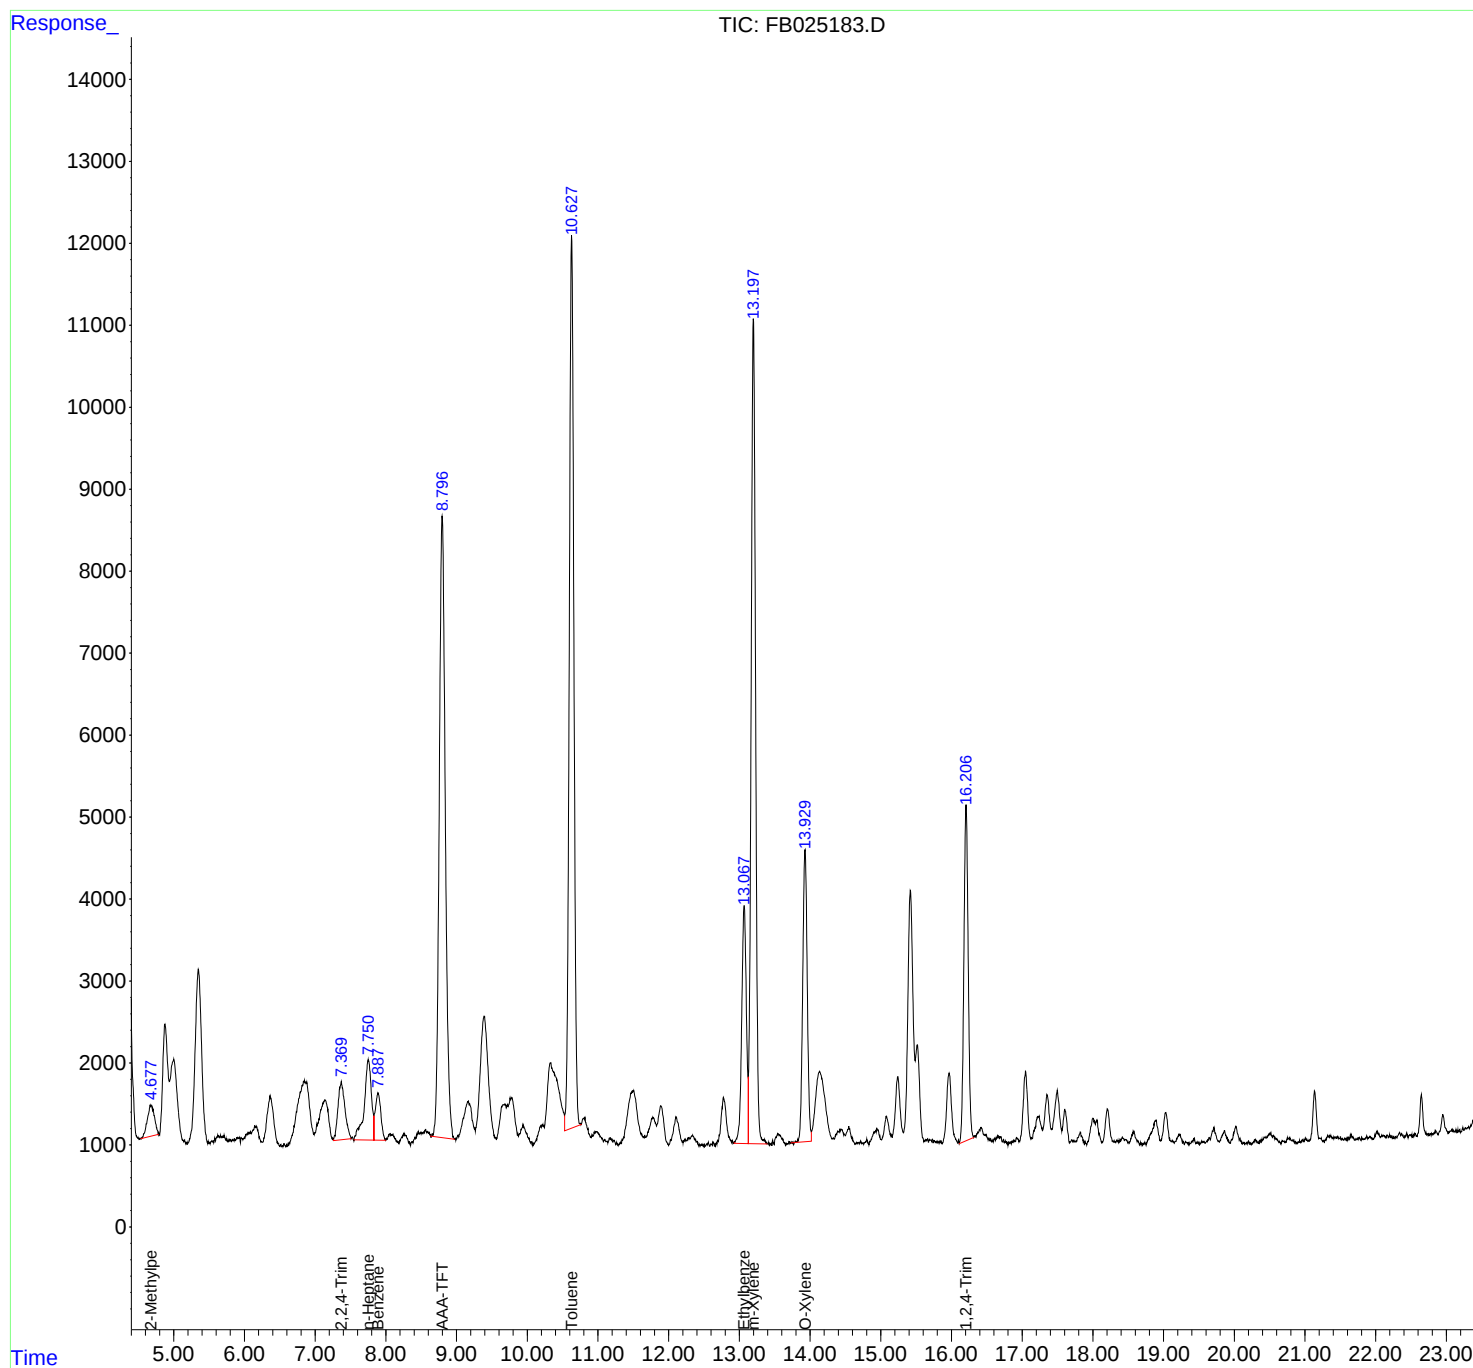


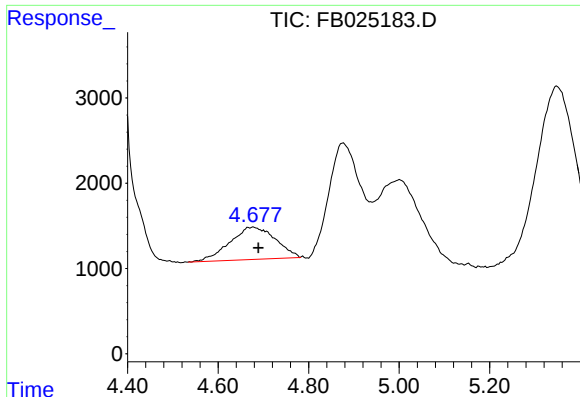

#1 2-Methylpentane


R.T.: 4.678 min
Delta R.T.: -0.011 min
Response: 26440
Conc: 0.82 ng/ml

Instrument :
FID_B
ClientSampleId :

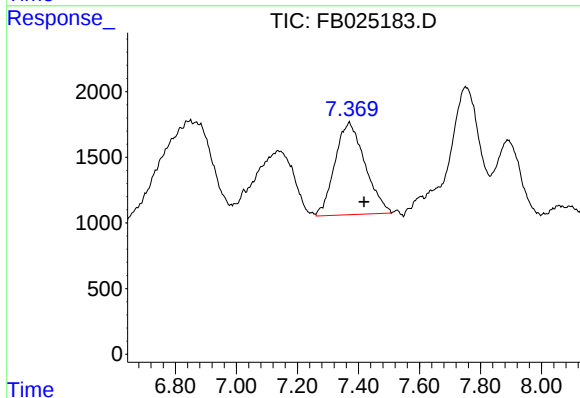


#2 2,2,4-Trimethylpentane

R.T.: 7.371 min
Delta R.T.: -0.047 min
Response: 48000
Conc: 1.45 ng/ml

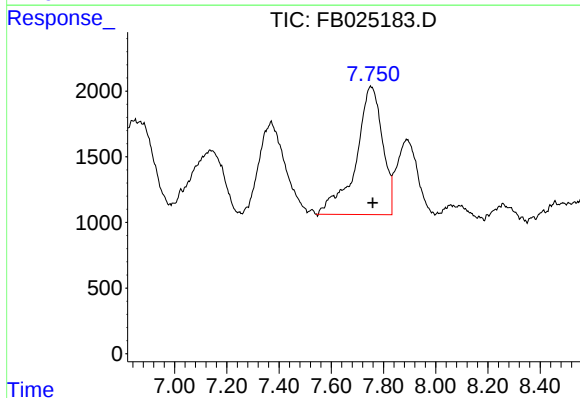


#3 n-Heptane

R.T.: 7.751 min
Delta R.T.: -0.008 min
Response: 68802
Conc: 2.09 ng/ml

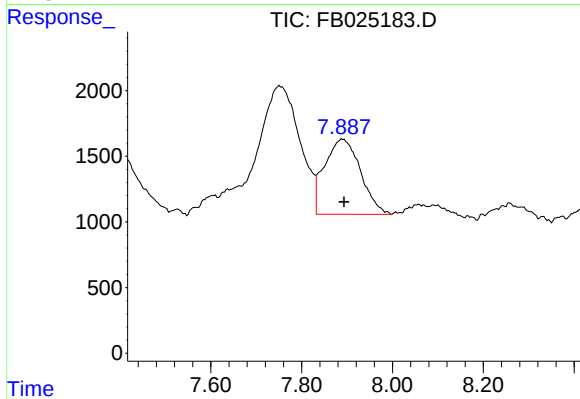

#4 Benzene


R.T.: 7.888 min
Delta R.T.: -0.005 min
Response: 31512
Conc: 0.79 ng/ml

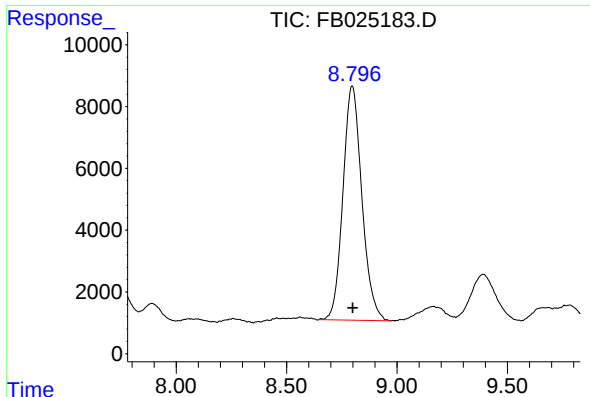

#5 AAA-TFT


R.T.: 8.797 min
Delta R.T.: -0.002 min
Response: 451539
Conc: 20.00 ng/ml

Instrument :
FID_B
ClientSampleId :

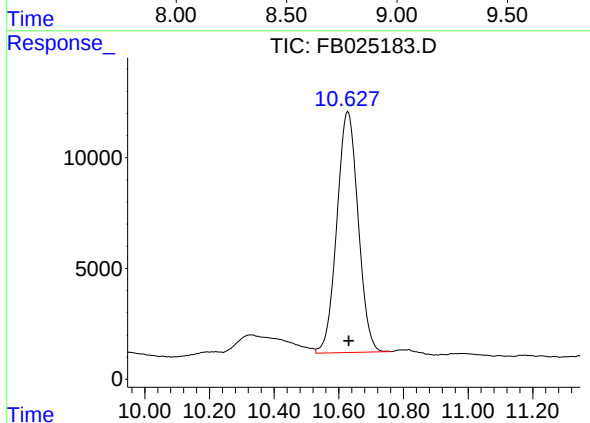


#6 Toluene

R.T.: 10.628 min
Delta R.T.: -0.002 min
Response: 496126
Conc: 13.27 ng/ml

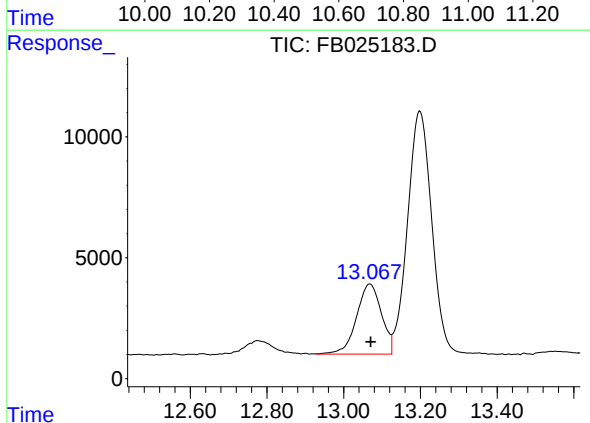


#7 Ethylbenzene

R.T.: 13.069 min
Delta R.T.: -0.002 min
Response: 130989
Conc: 3.81 ng/ml

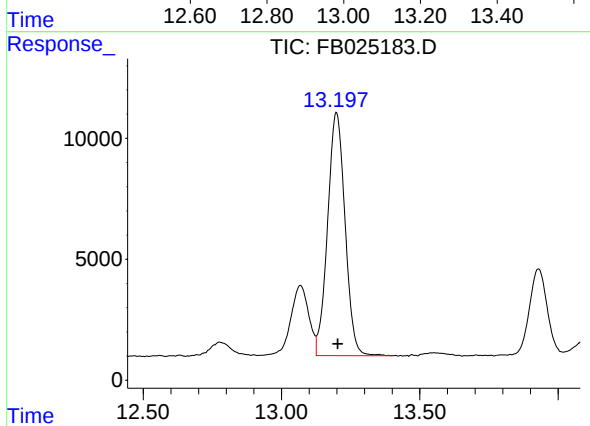

#8 m-Xylene


R.T.: 13.199 min
Delta R.T.: -0.004 min
Response: 440916
Conc: 13.06 ng/ml

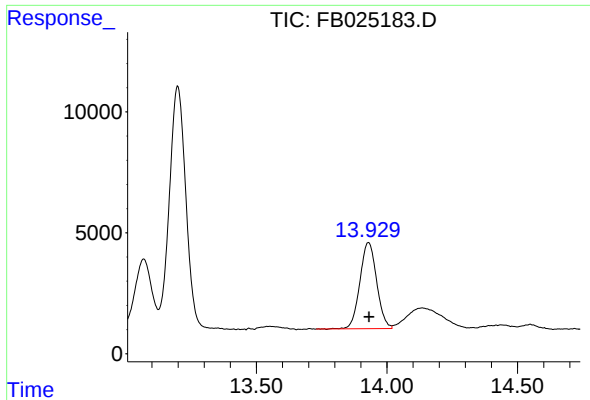

#9 O-Xylene

R.T.: 13.929 min
Delta R.T.: -0.002 min
Response: 158590
Conc: 4.85 ng/ml

Instrument :
FID_B
ClientSampleId :

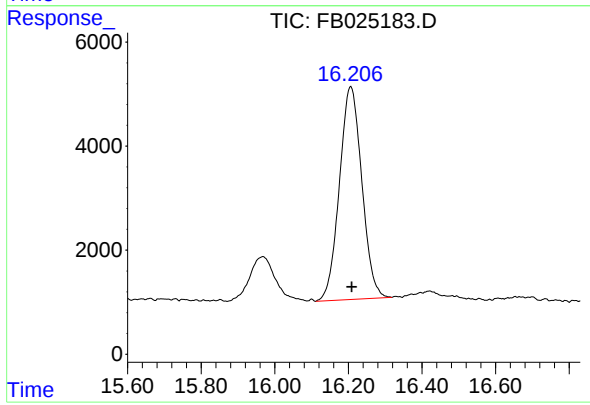

#10 1,2,4-Trimethylbenzene

R.T.: 16.207 min
Delta R.T.: -0.002 min
Response: 173004
Conc: 6.29 ng/ml