

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110420\
 Data File : FB025184.D
 Signal(s) : FID2B.CH
 Acq On : 4 Nov 2020 12:34
 Operator : DD/AJ
 Sample : L4548-15 100X
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Nov 05 12:01:32 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110320.M
 Quant Title :
 QLast Update : Wed Nov 04 08:05:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.854	6121138	271.093 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.679	2751662	85.250 ng/ml
2) t 2,2,4-Trimethylpentane	7.380	6012064	181.206 ng/ml
3) t n-Heptane	7.754	8872520	270.132 ng/ml
4) t Benzene	7.881	1456546	36.633 ng/ml
6) t Toluene	10.630	20349623	544.239 ng/ml
7) t Ethylbenzene	13.069	6533831	190.266 ng/ml
8) t m-Xylene	13.202	18466625	546.925 ng/ml
9) t O-Xylene	13.931	7381423	225.755 ng/ml
10) t 1,2,4-Trimethylbenzene	16.209	7083455	257.439 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110420\
Data File : FB025184.D
Signal(s) : FID2B.CH
Acq On : 4 Nov 2020 12:34
Operator : DD/AJ
Sample : L4548-15 100X
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Nov 05 12:01:32 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110320.M
Quant Title :
QLast Update : Wed Nov 04 08:05:53 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

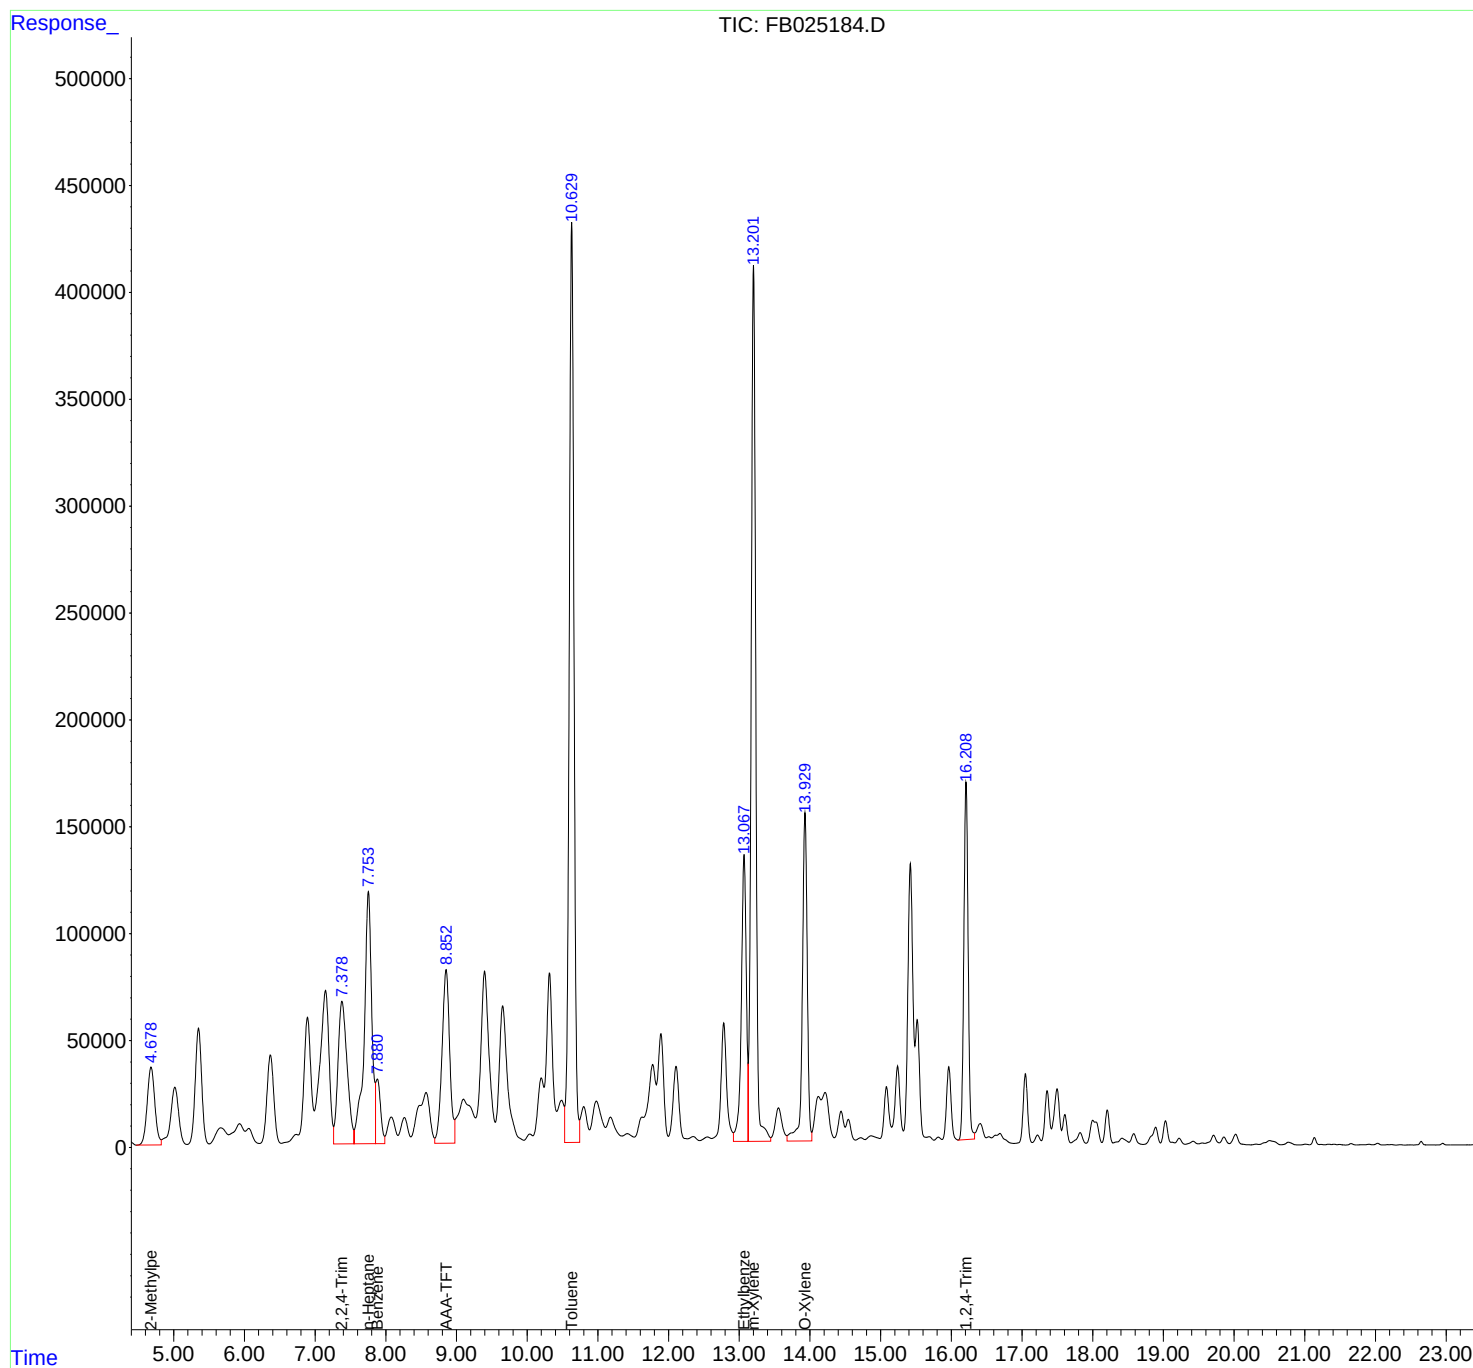


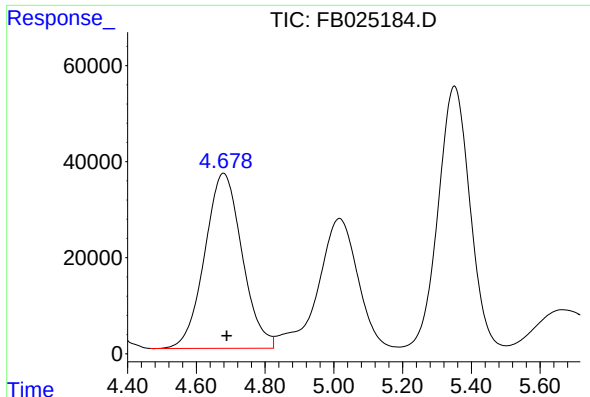

#1 2-Methylpentane


R.T.: 4.679 min
Delta R.T.: -0.010 min
Response: 2751662
Conc: 85.25 ng/ml

Instrument :
FID_B
ClientSampleId :

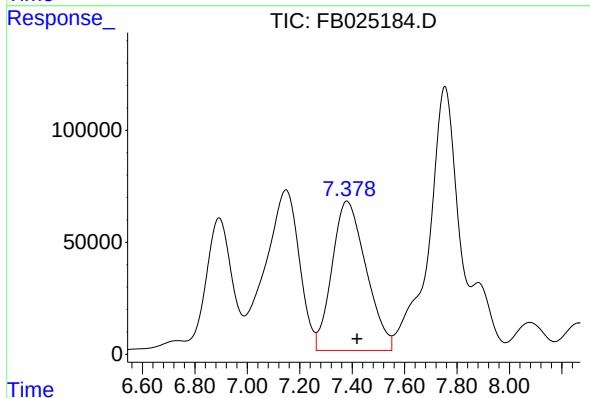


#2 2,2,4-Trimethylpentane

R.T.: 7.380 min
Delta R.T.: -0.038 min
Response: 6012064
Conc: 181.21 ng/ml

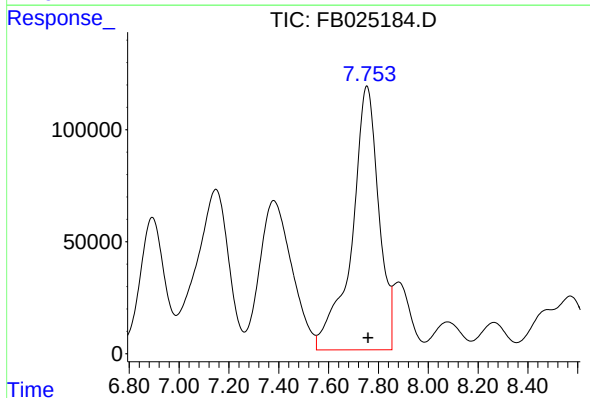


#3 n-Heptane

R.T.: 7.754 min
Delta R.T.: -0.005 min
Response: 8872520
Conc: 270.13 ng/ml

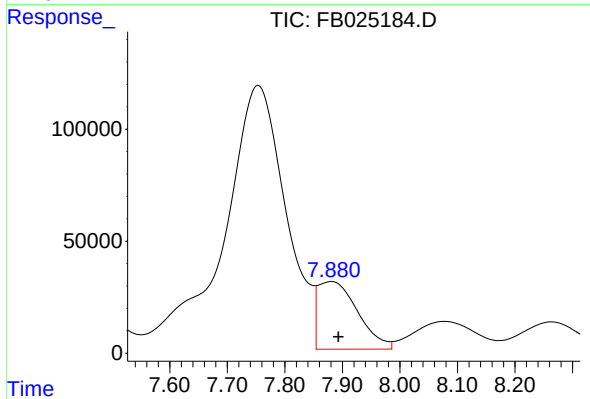

#4 Benzene


R.T.: 7.881 min
Delta R.T.: -0.012 min
Response: 1456546
Conc: 36.63 ng/ml

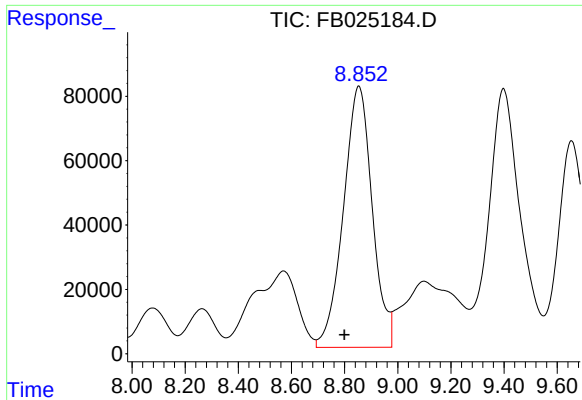

#5 AAA-TFT


R.T.: 8.854 min
Delta R.T.: 0.055 min
Response: 6121138
Conc: 271.09 ng/ml

Instrument :
FID_B
ClientSampleId :

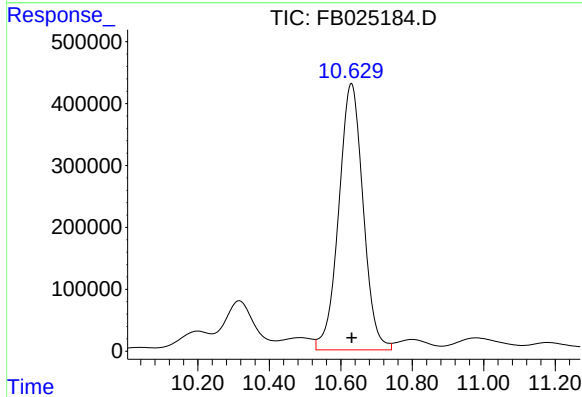


#6 Toluene

R.T.: 10.630 min
Delta R.T.: 0.000 min
Response: 20349623
Conc: 544.24 ng/ml

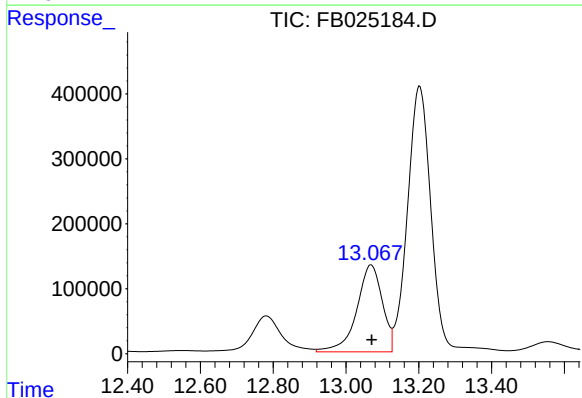


#7 Ethylbenzene

R.T.: 13.069 min
Delta R.T.: -0.002 min
Response: 6533831
Conc: 190.27 ng/ml

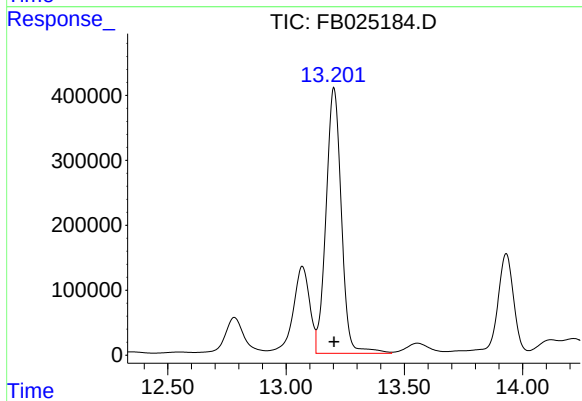

#8 m-Xylene


R.T.: 13.202 min
Delta R.T.: 0.000 min
Response: 18466625
Conc: 546.92 ng/ml

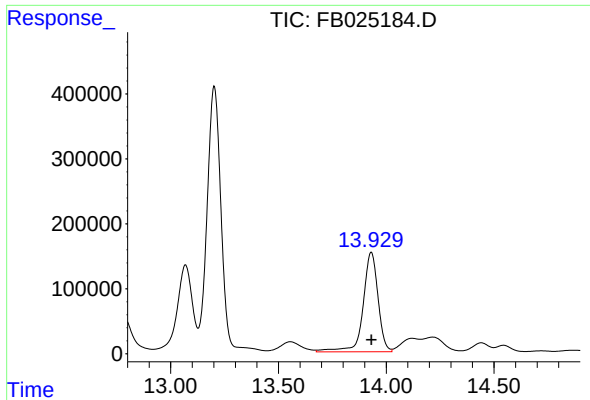

#9 O-Xylene

R.T.: 13.931 min
Delta R.T.: 0.000 min
Response: 7381423
Conc: 225.76 ng/ml

Instrument :
FID_B
ClientSampleId :

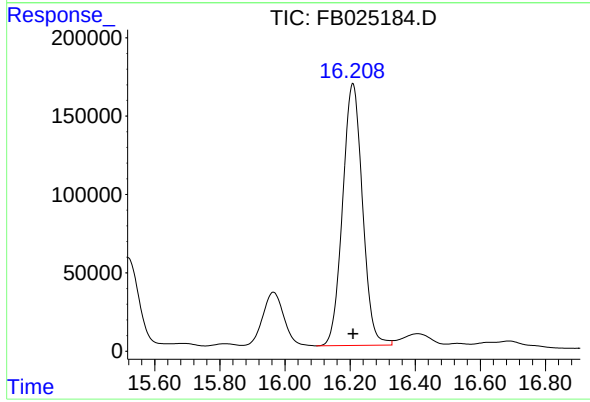

#10 1,2,4-Trimethylbenzene

R.T.: 16.209 min
Delta R.T.: 0.000 min
Response: 7083455
Conc: 257.44 ng/ml