

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110420\
 Data File : FB025185.D
 Signal(s) : FID2B.CH
 Acq On : 4 Nov 2020 13:36
 Operator : DD/AJ
 Sample : L4548-15 500X
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Nov 05 12:01:36 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110320.M
 Quant Title :
 QLast Update : Wed Nov 04 08:05:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.843	1438897	63.726 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.685	543377	16.834 ng/ml
2) t 2,2,4-Trimethylpentane	7.383	1155780	34.836 ng/ml
3) t n-Heptane	7.757	1674181	50.972 ng/ml
4) t Benzene	7.883	275220	6.922 ng/ml
6) t Toluene	10.630	3778677	101.059 ng/ml
7) t Ethylbenzene	13.068	1193919	34.767 ng/ml
8) t m-Xylene	13.200	3346069	99.100 ng/ml
9) t O-Xylene	13.930	1335505	40.845 ng/ml
10) t 1,2,4-Trimethylbenzene	16.207	1339757	48.692 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110420\
Data File : FB025185.D
Signal(s) : FID2B.CH
Acq On : 4 Nov 2020 13:36
Operator : DD/AJ
Sample : L4548-15 500X
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Nov 05 12:01:36 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110320.M
Quant Title :
QLast Update : Wed Nov 04 08:05:53 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

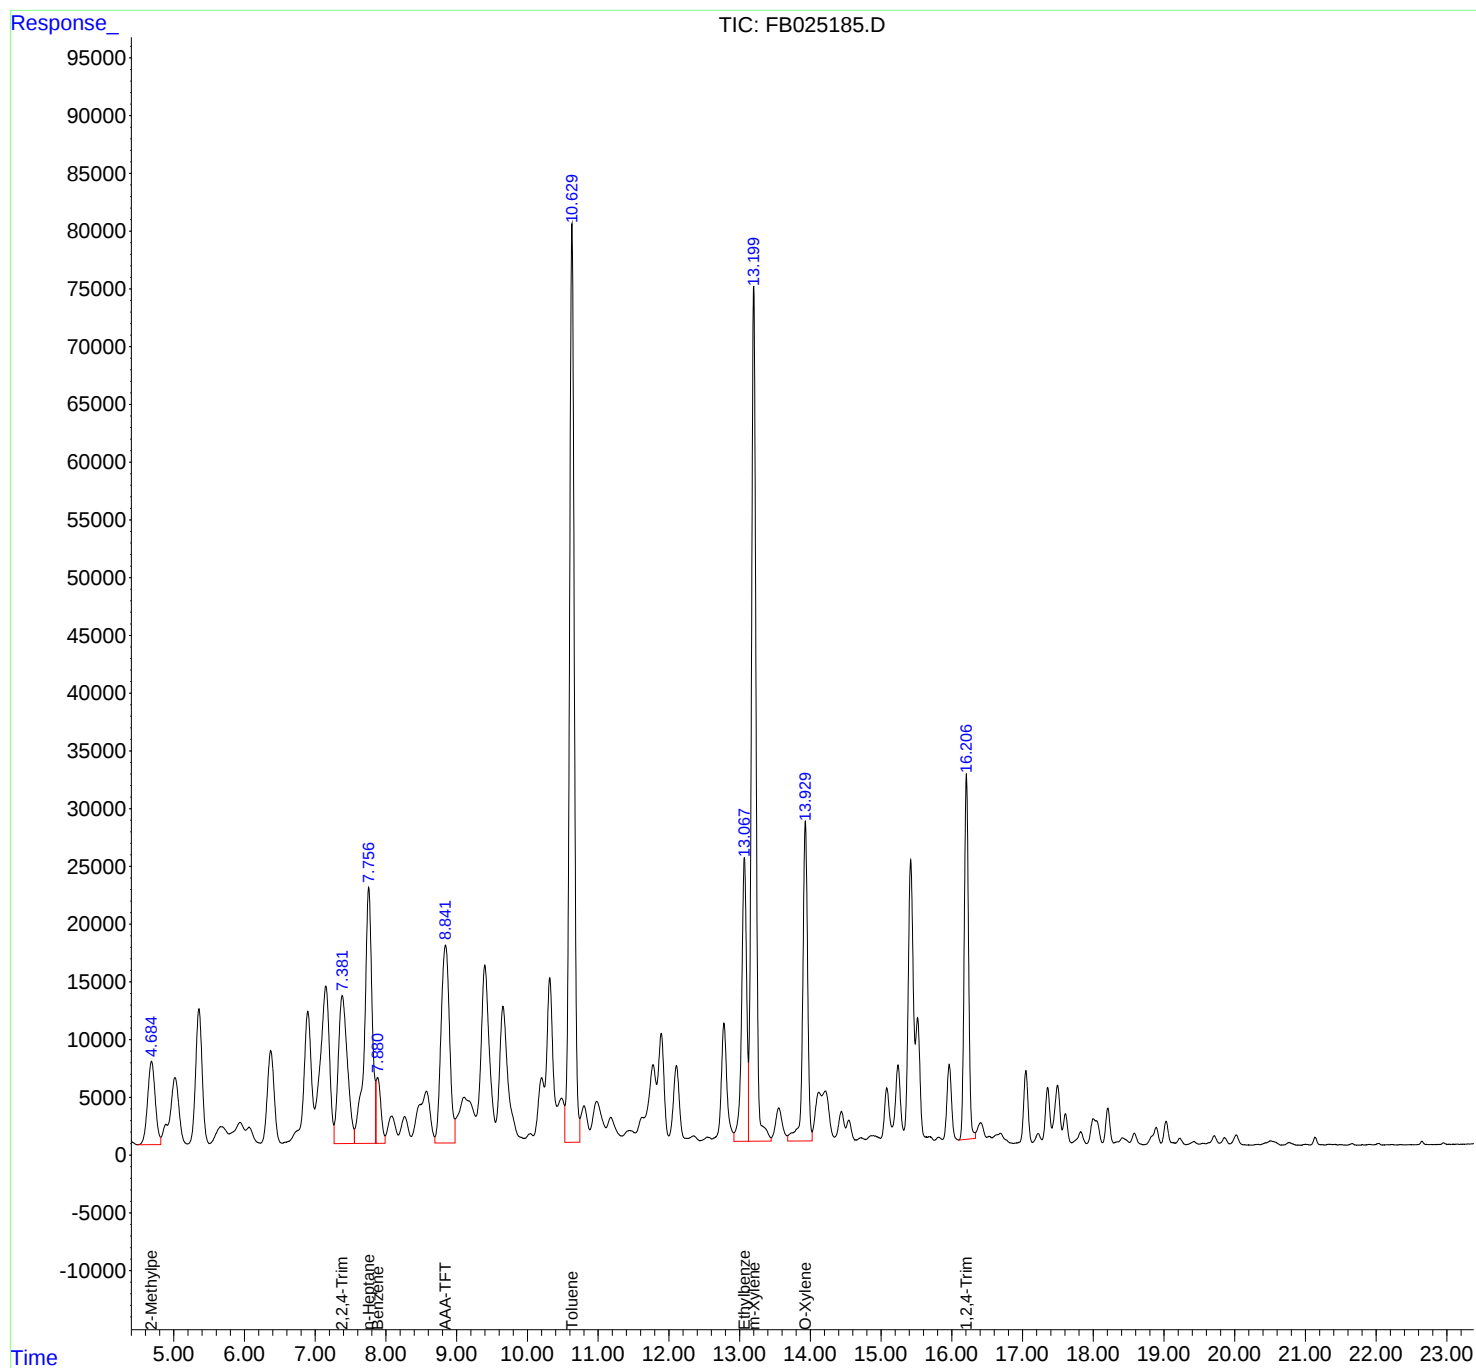


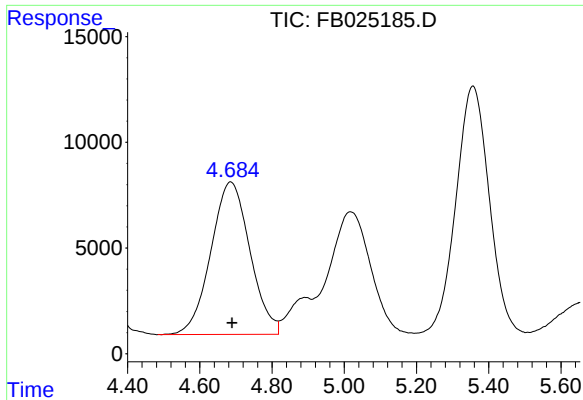

#1 2-Methylpentane


R.T.: 4.685 min
Delta R.T.: -0.004 min
Response: 543377
Conc: 16.83 ng/ml

Instrument :
FID_B
ClientSampleId :

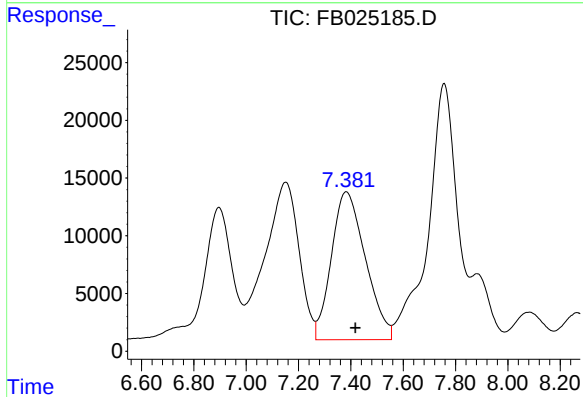


#2 2,2,4-Trimethylpentane

R.T.: 7.383 min
Delta R.T.: -0.035 min
Response: 1155780
Conc: 34.84 ng/ml

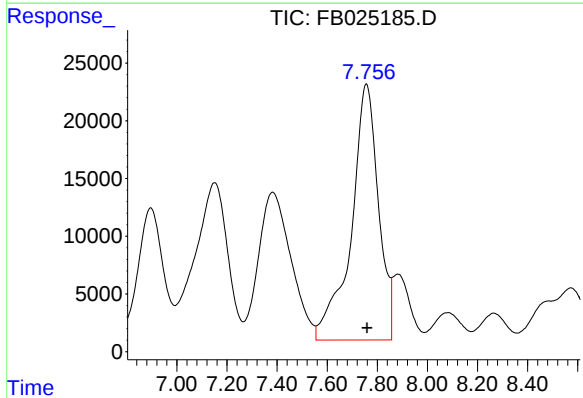


#3 n-Heptane

R.T.: 7.757 min
Delta R.T.: -0.002 min
Response: 1674181
Conc: 50.97 ng/ml

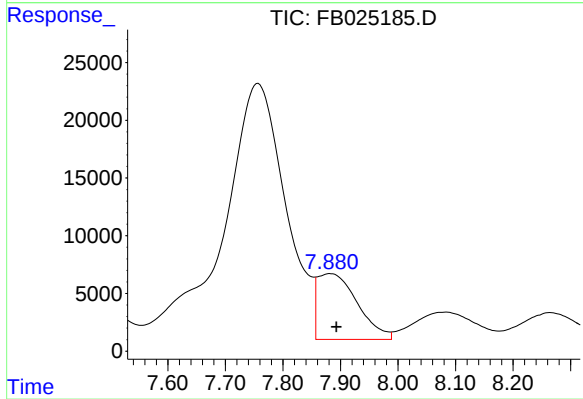

#4 Benzene


R.T.: 7.883 min
Delta R.T.: -0.011 min
Response: 275220
Conc: 6.92 ng/ml

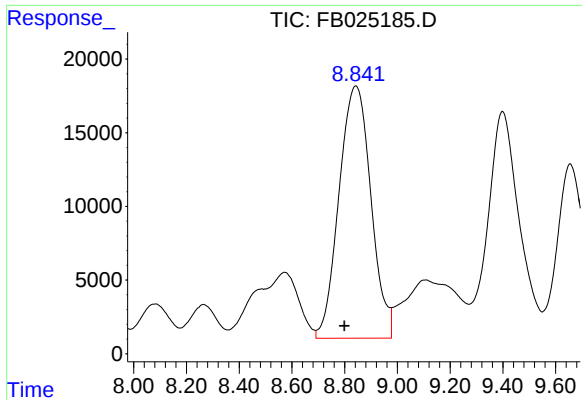

#5 AAA-TFT


R.T.: 8.843 min
Delta R.T.: 0.044 min
Response: 1438897
Conc: 63.73 ng/ml

Instrument :
FID_B
ClientSampleId :

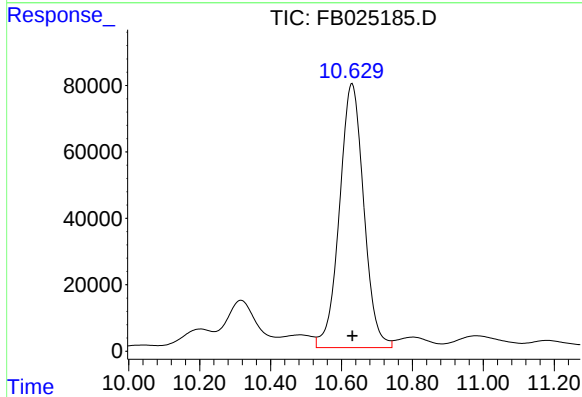


#6 Toluene

R.T.: 10.630 min
Delta R.T.: 0.000 min
Response: 3778677
Conc: 101.06 ng/ml

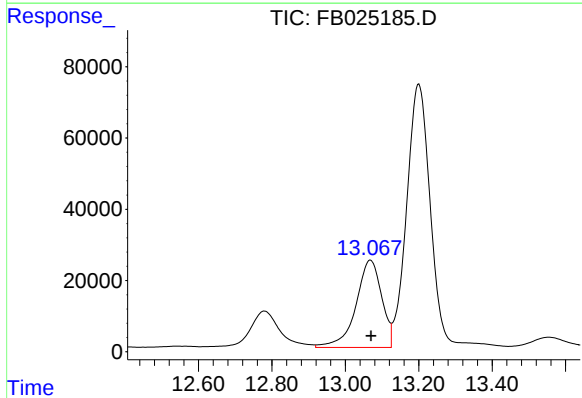


#7 Ethylbenzene

R.T.: 13.068 min
Delta R.T.: -0.002 min
Response: 1193919
Conc: 34.77 ng/ml

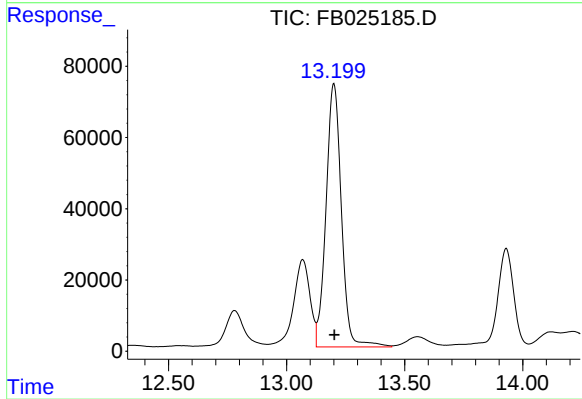

#8 m-Xylene


R.T.: 13.200 min
Delta R.T.: -0.003 min
Response: 3346069
Conc: 99.10 ng/ml

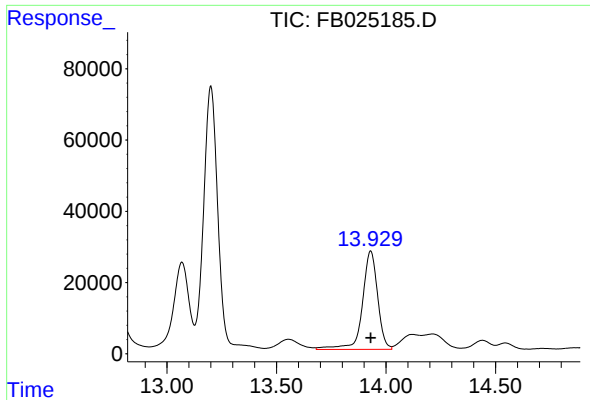

#9 O-Xylene

R.T.: 13.930 min
Delta R.T.: -0.001 min
Response: 1335505
Conc: 40.85 ng/ml

Instrument :
FID_B
ClientSampleId :

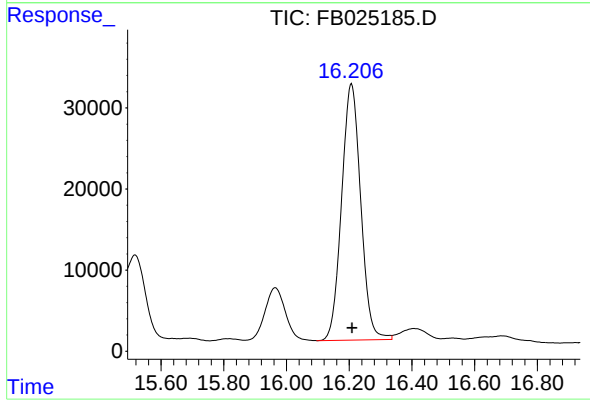

#10 1,2,4-Trimethylbenzene

R.T.: 16.207 min
Delta R.T.: -0.001 min
Response: 1339757
Conc: 48.69 ng/ml