

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110420\
 Data File : FB025181.D
 Signal(s) : FID2B.CH
 Acq On : 4 Nov 2020 10:42
 Operator : DD/AJ
 Sample : BSF1104S1
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1104S1

Integration File: Calibration.e
 Quant Time: Nov 05 12:01:20 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110320.M
 Quant Title :
 QLast Update : Wed Nov 04 08:05:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.795	424644	18.807 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.684	985648	30.537 ng/ml
2) t 2,2,4-Trimethylpentane	7.412	1025761	30.917 ng/ml
3) t n-Heptane	7.754	337260	10.268 ng/ml
4) t Benzene	7.888	402686	10.128 ng/ml
6) t Toluene	10.626	1136726	30.401 ng/ml
7) t Ethylbenzene	13.066	342736	9.981 ng/ml
8) t m-Xylene	13.199	689887	20.432 ng/ml
9) t O-Xylene	13.927	664824	20.333 ng/ml
10) t 1,2,4-Trimethylbenzene	16.204	564935	20.532 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110420\
Data File : FB025181.D
Signal(s) : FID2B.CH
Acq On : 4 Nov 2020 10:42
Operator : DD/AJ
Sample : BSF1104S1
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1104S1

Integration File: Calibration.e
Quant Time: Nov 05 12:01:20 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110320.M
Quant Title :
QLast Update : Wed Nov 04 08:05:53 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

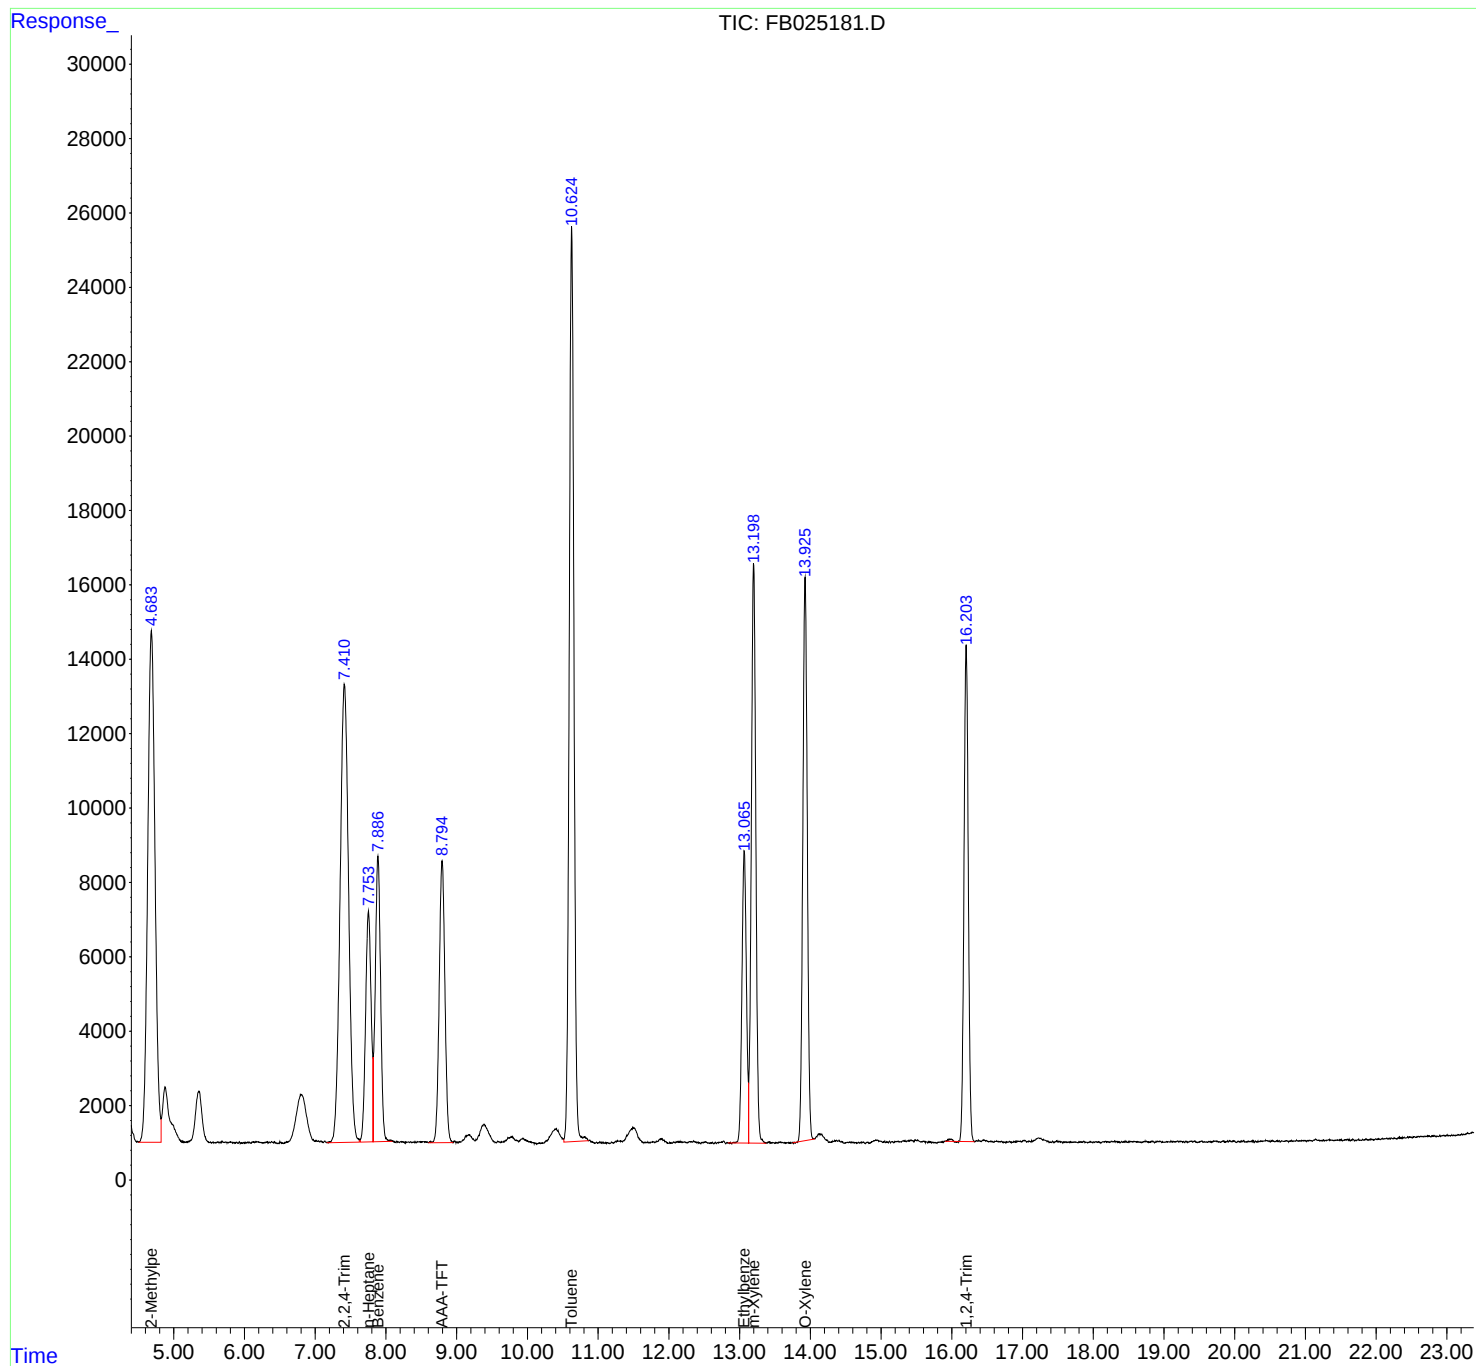


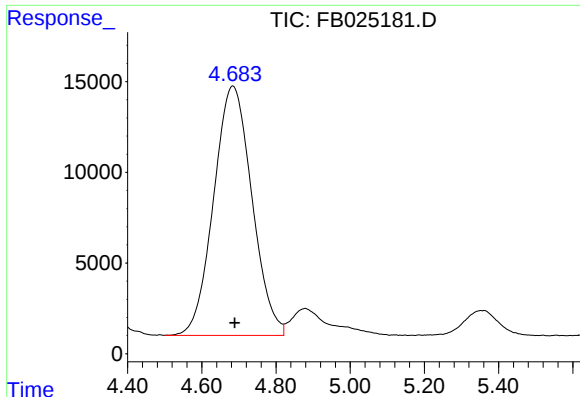

#1 2-Methylpentane


R.T.: 4.684 min
Delta R.T.: -0.005 min
Response: 985648
Conc: 30.54 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1104S1

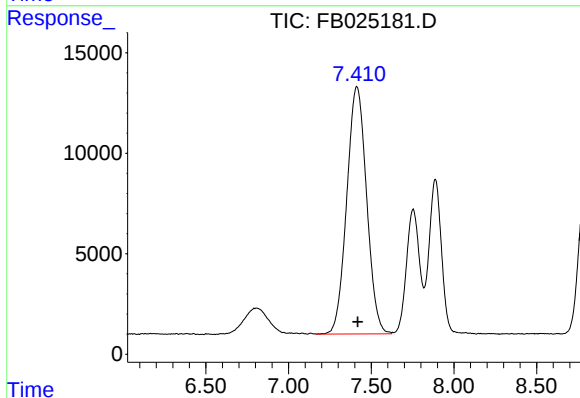


#2 2,2,4-Trimethylpentane

R.T.: 7.412 min
Delta R.T.: -0.006 min
Response: 1025761
Conc: 30.92 ng/ml

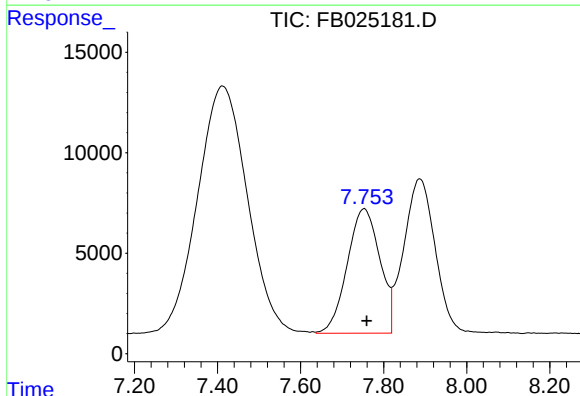


#3 n-Heptane

R.T.: 7.754 min
Delta R.T.: -0.005 min
Response: 337260
Conc: 10.27 ng/ml

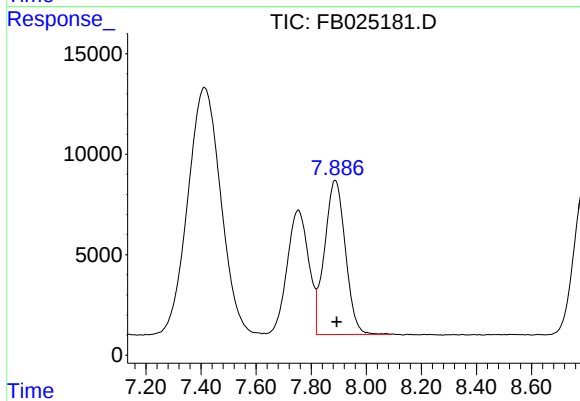

#4 Benzene


R.T.: 7.888 min
Delta R.T.: -0.006 min
Response: 402686
Conc: 10.13 ng/ml

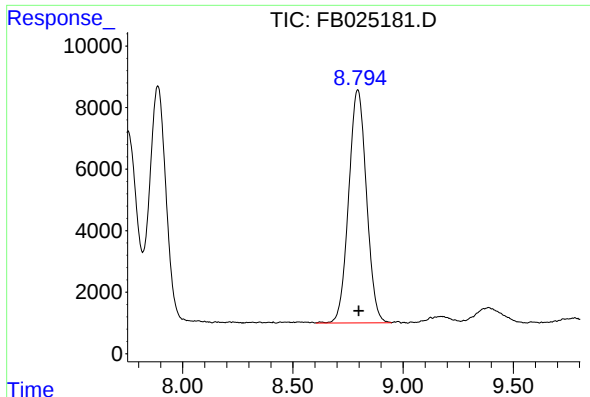

#5 AAA-TFT


R.T.: 8.795 min
Delta R.T.: -0.004 min
Response: 424644
Conc: 18.81 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1104S1

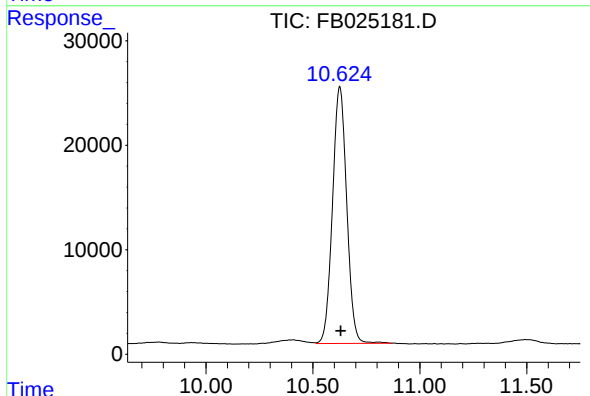


#6 Toluene

R.T.: 10.626 min
Delta R.T.: -0.004 min
Response: 1136726
Conc: 30.40 ng/ml

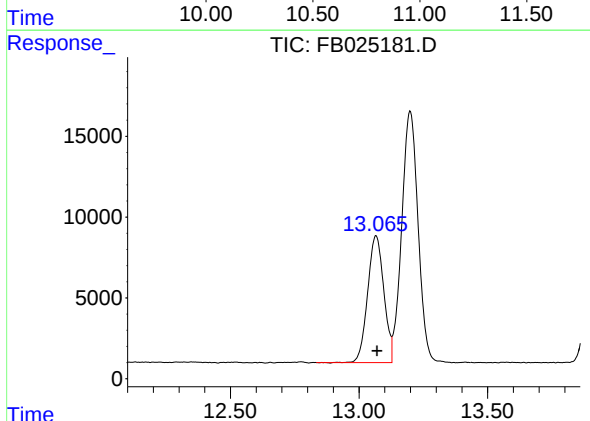


#7 Ethylbenzene

R.T.: 13.066 min
Delta R.T.: -0.004 min
Response: 342736
Conc: 9.98 ng/ml

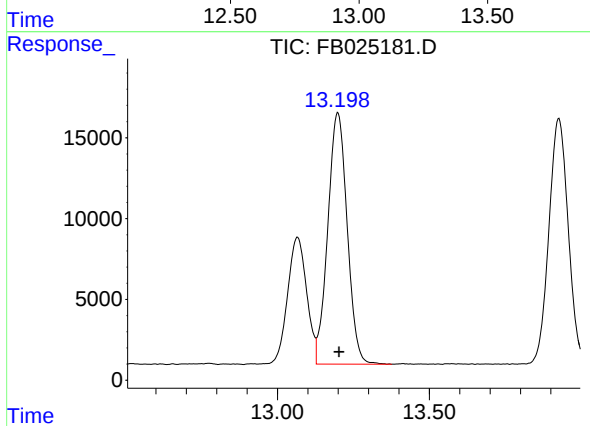

#8 m-Xylene


R.T.: 13.199 min
Delta R.T.: -0.004 min
Response: 689887
Conc: 20.43 ng/ml

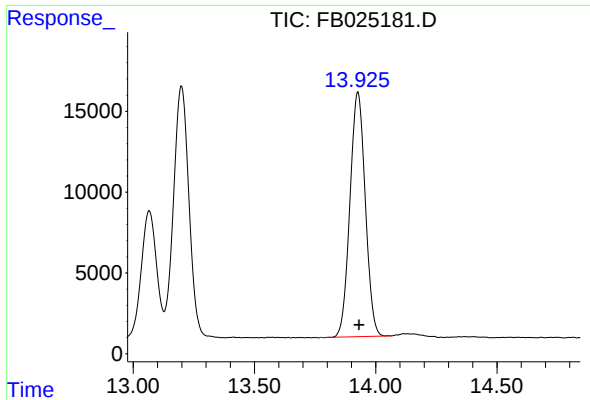

#9 O-Xylene

R.T.: 13.927 min
Delta R.T.: -0.005 min
Response: 664824
Conc: 20.33 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1104S1

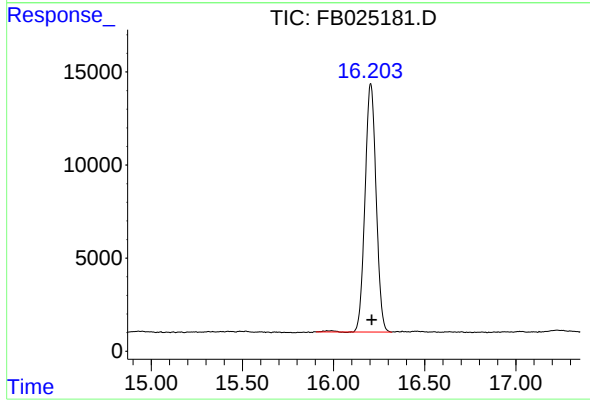

#10 1,2,4-Trimethylbenzene

R.T.: 16.204 min
Delta R.T.: -0.005 min
Response: 564935
Conc: 20.53 ng/ml