

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110518\
 Data File : FB018508.D
 Signal(s) : FID2B.CH
 Acq On : 5 Nov 2018 15:30
 Operator : MJ/SJ
 Sample : 20 PPB GRO STD
 Misc : 5.03g/5.00mL DI Water
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Nov 05 16:56:42 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101218.M
 Quant Title :
 QLast Update : Fri Oct 12 08:04:31 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.105	162708	18.891 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.958	381681	24.956 ng/ml
2) t 2,2,4-Trimethylpentane	7.721	411347	27.838 ng/ml
3) t n-Heptane	8.063	133586	9.427 ng/ml
4) t Benzene	8.201	171116	9.186 ng/ml
6) t Toluene	10.956	422300	27.709 ng/ml
7) t Ethylbenzene	13.405	148113	9.335 ng/ml
8) t m-Xylene	13.538	317463	19.079 ng/ml
9) t O-Xylene	14.270	333326	18.695 ng/ml
10) t 1,2,4-Trimethylbenzene	16.552	385467	18.948 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110518\
Data File : FB018508.D
Signal(s) : FID2B.CH
Acq On : 5 Nov 2018 15:30
Operator : MJ/SJ
Sample : 20 PPB GRO STD
Misc : 5.03g/5.00mL DI Water
ALS Vial : 14 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Nov 05 16:56:42 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101218.M
Quant Title :
QLast Update : Fri Oct 12 08:04:31 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

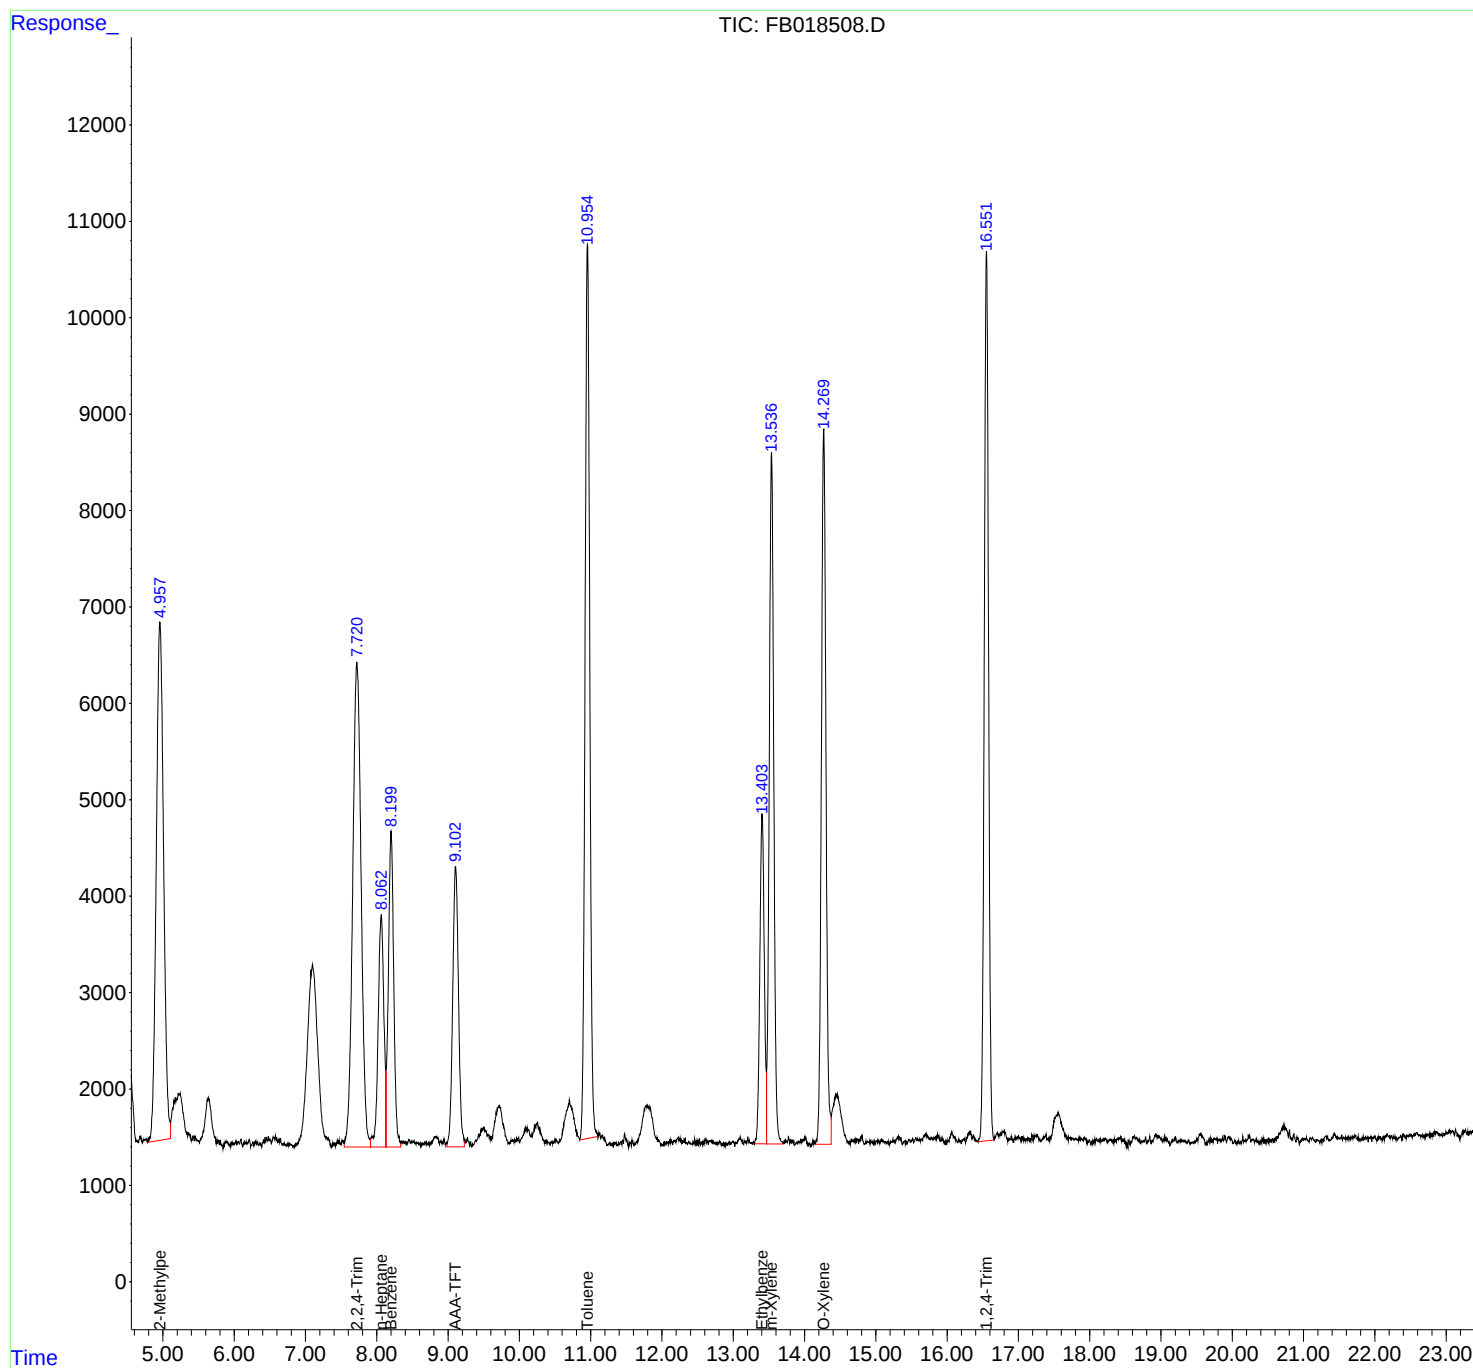


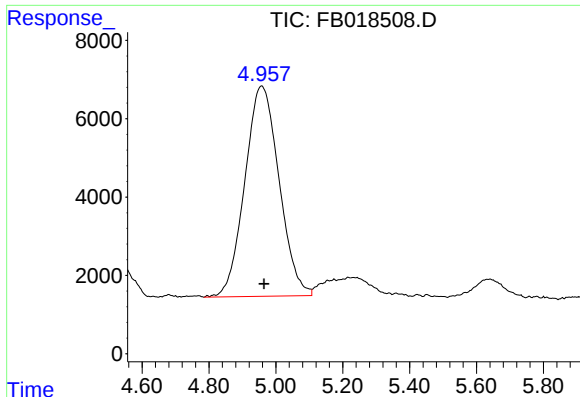

#1 2-Methylpentane


R.T.: 4.958 min
Delta R.T.: -0.007 min
Response: 381681
Conc: 24.96 ng/ml

Instrument :
FID_B
ClientSampleId :

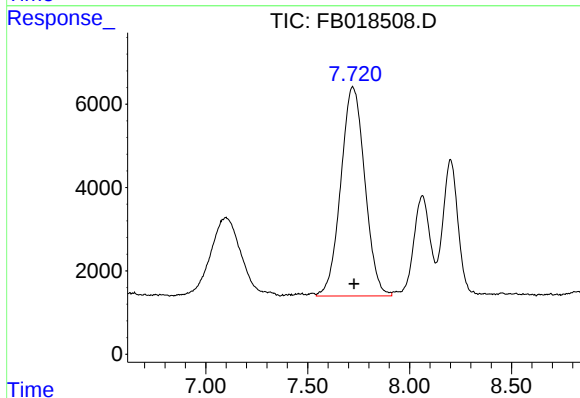


#2 2,2,4-Trimethylpentane

R.T.: 7.721 min
Delta R.T.: -0.008 min
Response: 411347
Conc: 27.84 ng/ml

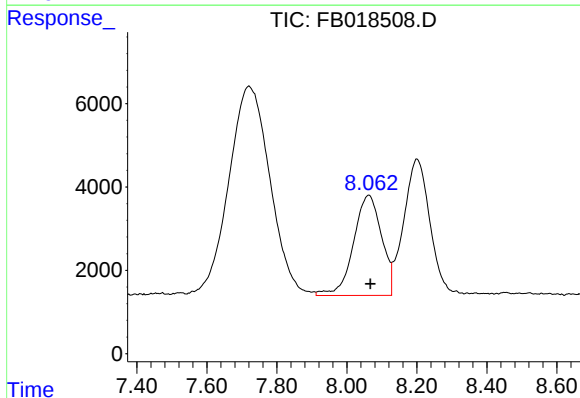


#3 n-Heptane

R.T.: 8.063 min
Delta R.T.: -0.004 min
Response: 133586
Conc: 9.43 ng/ml

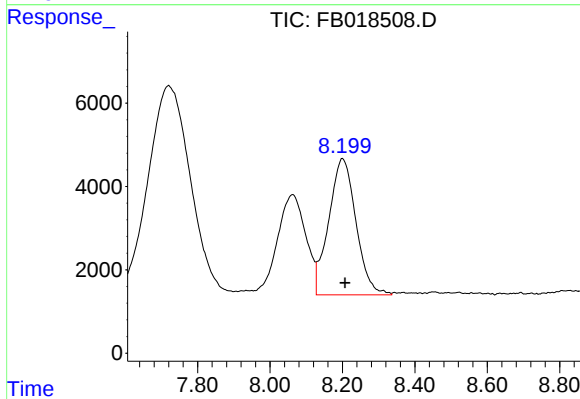

#4 Benzene


R.T.: 8.201 min
Delta R.T.: -0.006 min
Response: 171116
Conc: 9.19 ng/ml

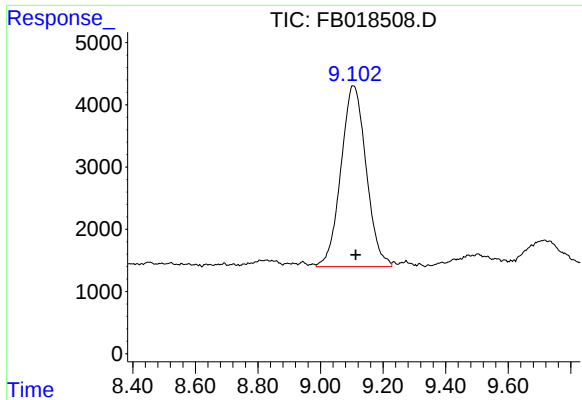

#5 AAA-TFT


R.T.: 9.105 min
Delta R.T.: -0.007 min
Response: 162708
Conc: 18.89 ng/ml

Instrument :
FID_B
ClientSampleId :

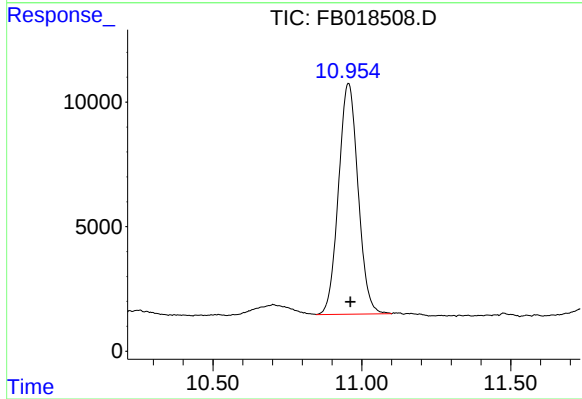


#6 Toluene

R.T.: 10.956 min
Delta R.T.: -0.006 min
Response: 422300
Conc: 27.71 ng/ml

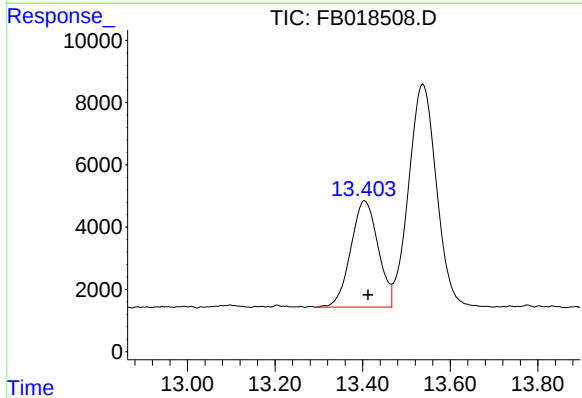


#7 Ethylbenzene

R.T.: 13.405 min
Delta R.T.: -0.007 min
Response: 148113
Conc: 9.34 ng/ml

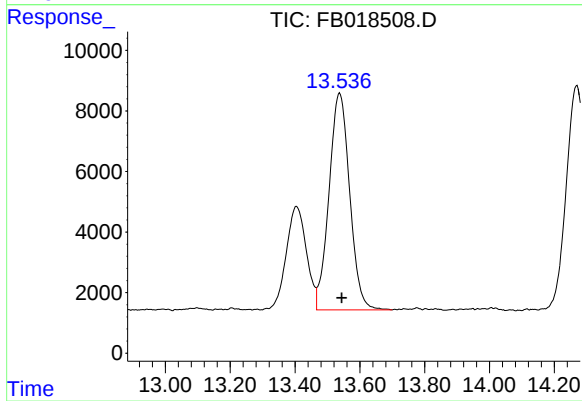

#8 m-Xylene


R.T.: 13.538 min
Delta R.T.: -0.007 min
Response: 317463
Conc: 19.08 ng/ml

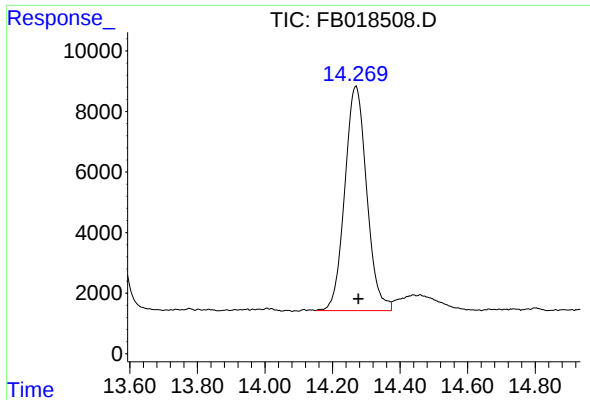

#9 O-Xylene

R.T.: 14.270 min
Delta R.T.: -0.007 min
Response: 333326
Conc: 18.70 ng/ml

Instrument :
FID_B
ClientSampleId :

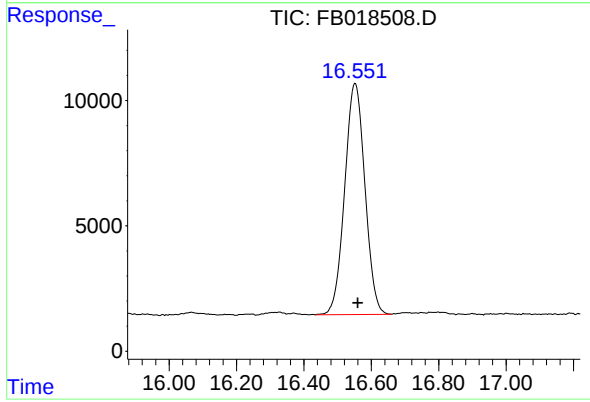

#10 1,2,4-Trimethylbenzene

R.T.: 16.552 min
Delta R.T.: -0.007 min
Response: 385467
Conc: 18.95 ng/ml