

Data Path : \\74.0.250.170\Terastorage\pestpcbsrv\HPCHEM1\FID_B\Data\FB110518\
 Data File : FB018535.D
 Signal(s) : FID2B.CH
 Acq On : 6 Nov 2018 5:53
 Operator : MJ/SJ
 Sample : J5764-03MS
 Misc : 5.00g/5.00mL DI Water
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Nov 06 07:36:54 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101218.M
 Quant Title :
 QLast Update : Fri Oct 12 08:04:31 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.107	182105	21.143 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.959	493108	32.241 ng/ml
2) t 2,2,4-Trimethylpentane	7.725	518316	35.077 ng/ml
3) t n-Heptane	8.064	160039	11.293 ng/ml
4) t Benzene	8.203	208054	11.169 ng/ml
6) t Toluene	10.956	542440	35.592 ng/ml
7) t Ethylbenzene	13.407	174568	11.003 ng/ml
8) t m-Xylene	13.539	367579	22.091 ng/ml
9) t O-Xylene	14.271	381084	21.374 ng/ml
10) t 1,2,4-Trimethylbenzene	16.554	446302	21.938 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : \\74.0.250.170\Terastorage\pestpcbsrv\HPCHEM1\FID_B\Data\FB110518\
Data File : FB018535.D
Signal(s) : FID2B.CH
Acq On : 6 Nov 2018 5:53
Operator : MJ/SJ
Sample : J5764-03MS
Misc : 5.00g/5.00mL DI Water
ALS Vial : 28 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Nov 06 07:36:54 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101218.M
Quant Title :
QLast Update : Fri Oct 12 08:04:31 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

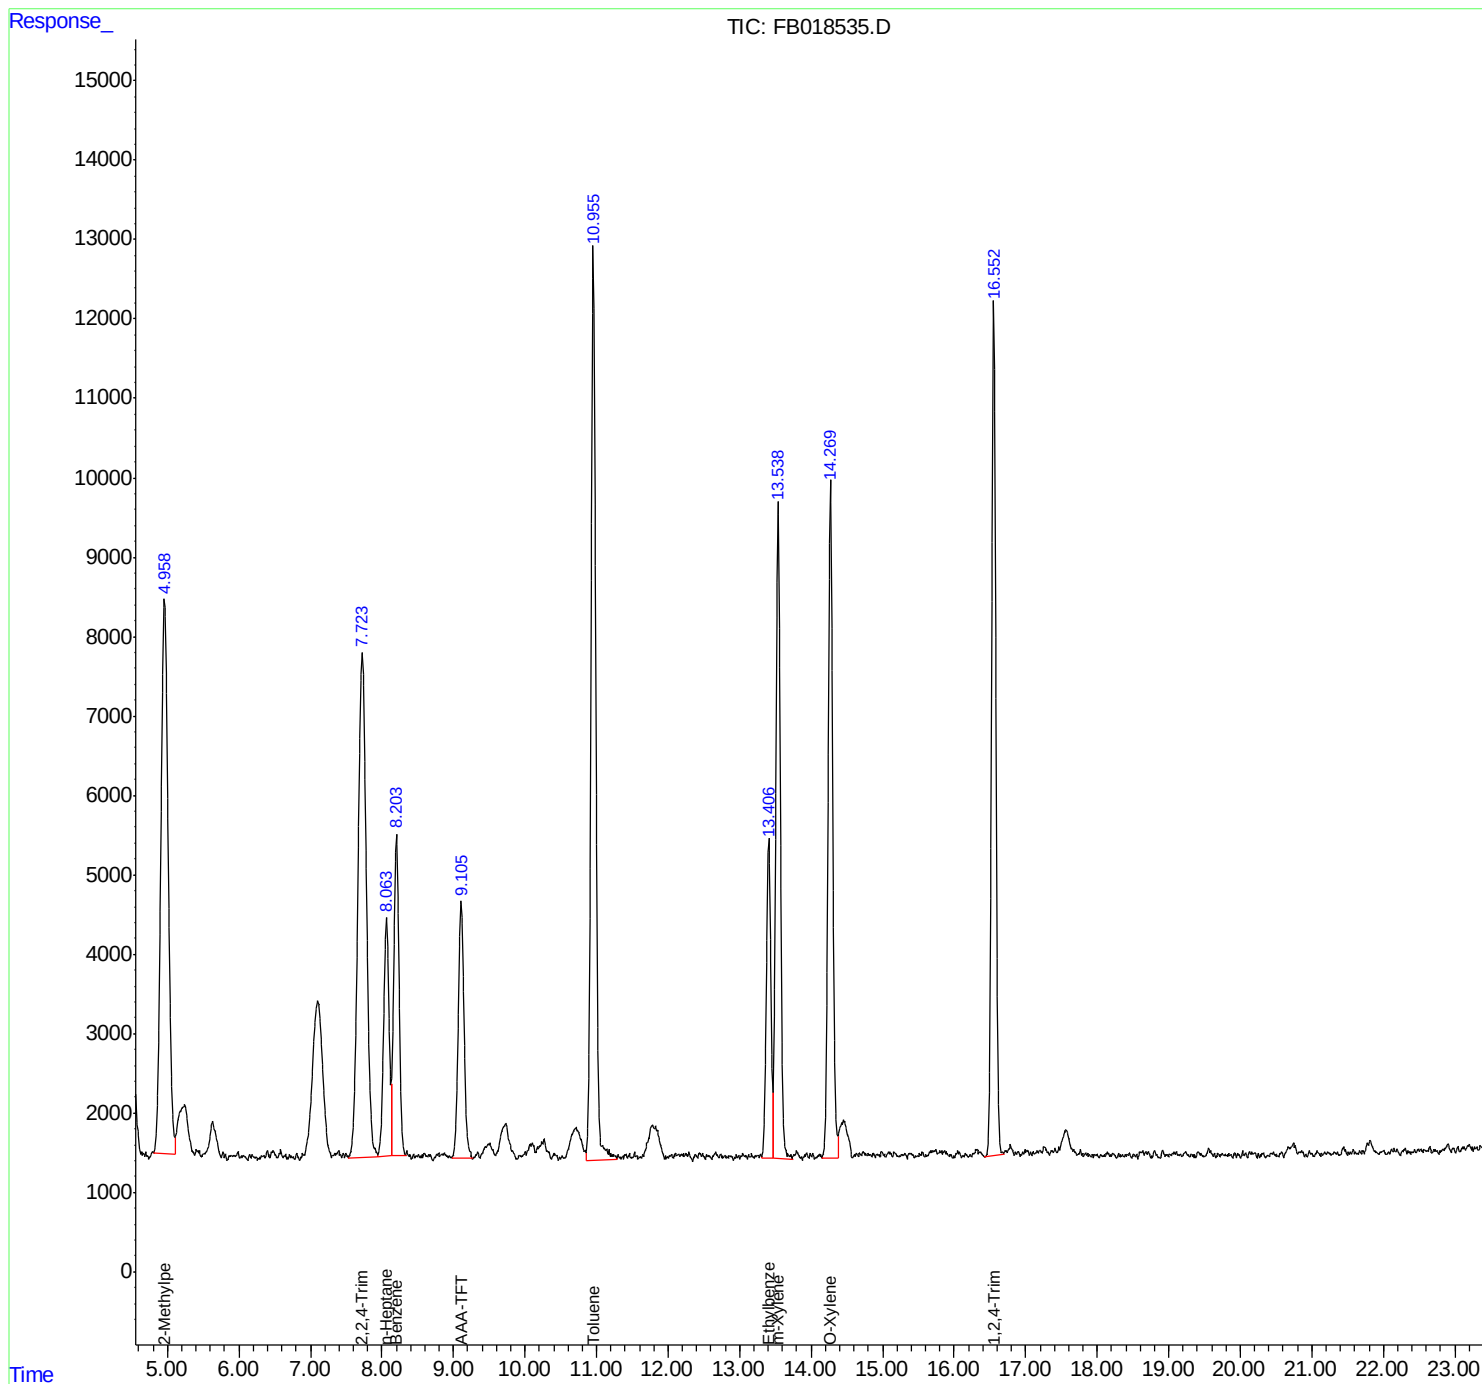


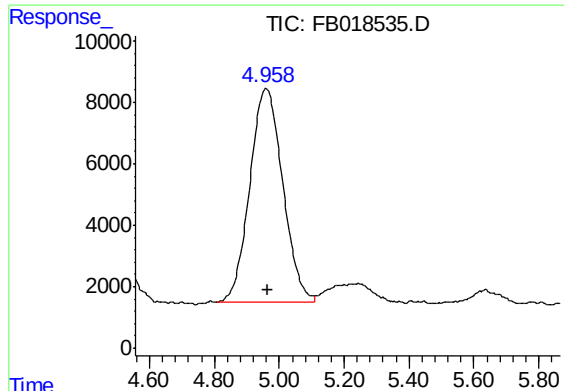

#1 2-Methylpentane


R.T.: 4.959 min
Delta R.T.: -0.006 min
Response: 493108
Conc: 32.24 ng/ml

Instrument :
FID_B
ClientSampleId :

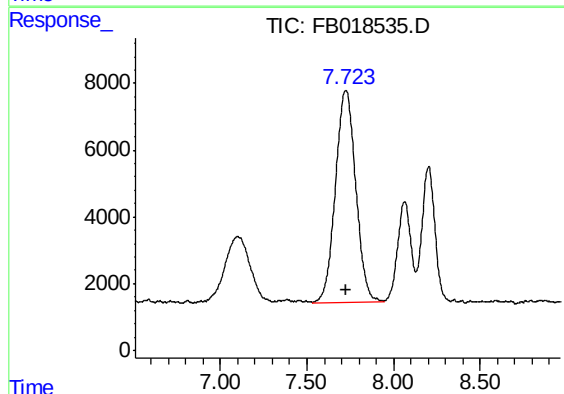


#2 2,2,4-Trimethylpentane

R.T.: 7.725 min
Delta R.T.: -0.004 min
Response: 518316
Conc: 35.08 ng/ml

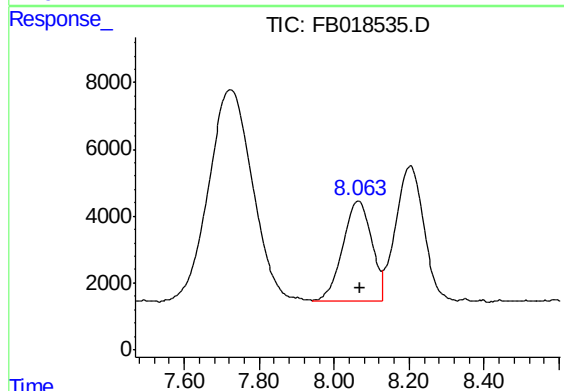


#3 n-Heptane

R.T.: 8.064 min
Delta R.T.: -0.004 min
Response: 160039
Conc: 11.29 ng/ml

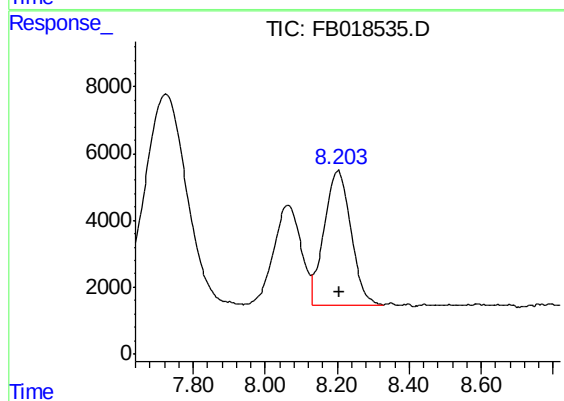

#4 Benzene


R.T.: 8.203 min
Delta R.T.: -0.004 min
Response: 208054
Conc: 11.17 ng/ml

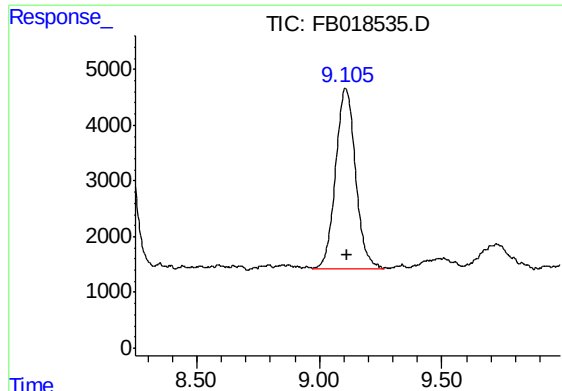

#5 AAA-TFT


R.T.: 9.107 min
Delta R.T.: -0.005 min
Response: 182105
Conc: 21.14 ng/ml

Instrument :
FID_B
ClientSampleId :

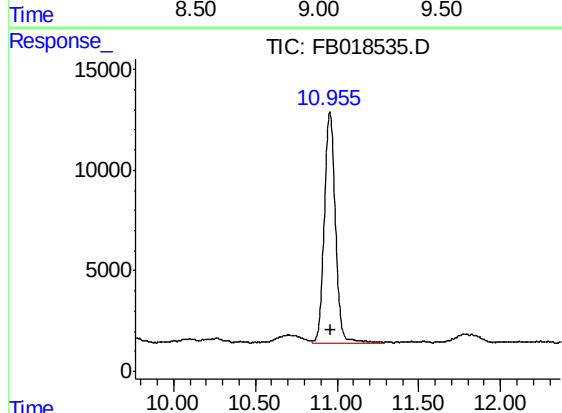


#6 Toluene

R.T.: 10.956 min
Delta R.T.: -0.006 min
Response: 542440
Conc: 35.59 ng/ml

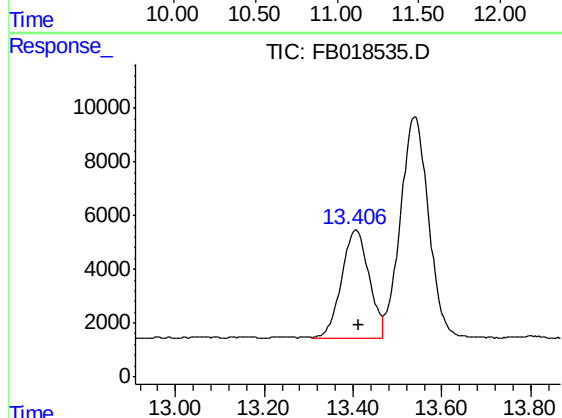


#7 Ethylbenzene

R.T.: 13.407 min
Delta R.T.: -0.006 min
Response: 174568
Conc: 11.00 ng/ml

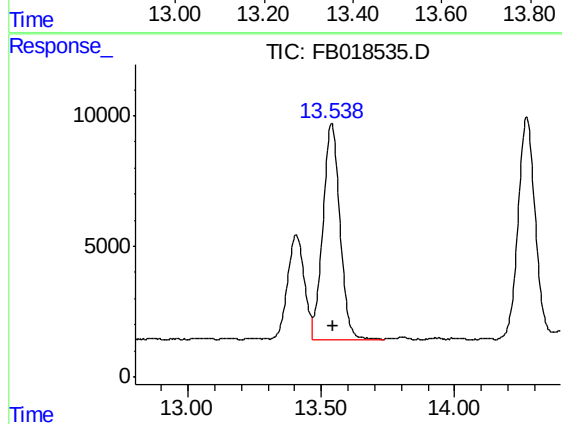

#8 m-Xylene


R.T.: 13.539 min
Delta R.T.: -0.005 min
Response: 367579
Conc: 22.09 ng/ml

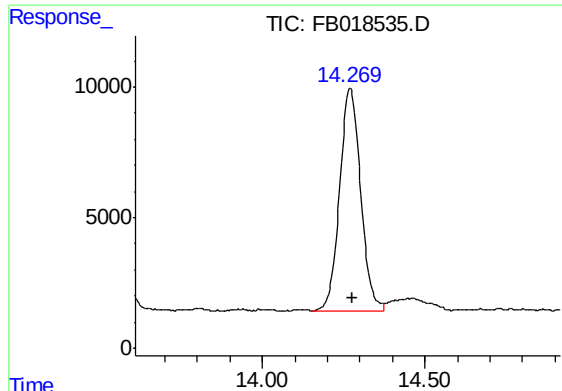

#9 O-Xylene

R.T.: 14.271 min
Delta R.T.: -0.006 min
Response: 381084
Conc: 21.37 ng/ml

Instrument :
FID_B
ClientSampleId :

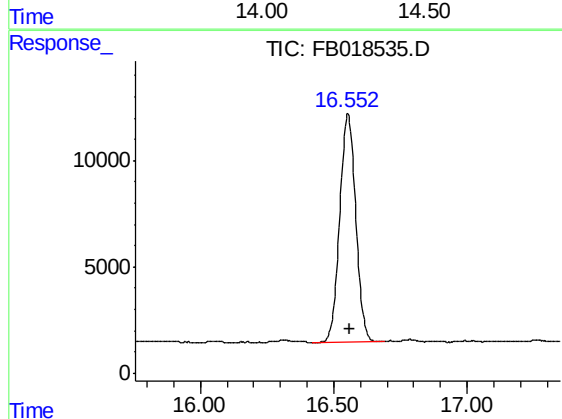

#10 1,2,4-Trimethylbenzene

R.T.: 16.554 min
Delta R.T.: -0.006 min
Response: 446302
Conc: 21.94 ng/ml