

Data Path : \\74.0.250.170\Terastorage\pestpcbsrv\HPCHEM1\FID_B\Data\FB110518\
 Data File : FB018536.D
 Signal(s) : FID2B.CH
 Acq On : 6 Nov 2018 6:23
 Operator : MJ/SJ
 Sample : J5764-03MSD
 Misc : 5.01g/5.00mL DI Water
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Nov 06 07:36:58 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101218.M
 Quant Title :
 QLast Update : Fri Oct 12 08:04:31 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.108	177087	20.561 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.962	422184	27.604 ng/ml
2) t 2,2,4-Trimethylpentane	7.725	443950	30.044 ng/ml
3) t n-Heptane	8.063	140788	9.935 ng/ml
4) t Benzene	8.203	183227	9.836 ng/ml
6) t Toluene	10.957	457988	30.050 ng/ml
7) t Ethylbenzene	13.406	155872	9.824 ng/ml
8) t m-Xylene	13.539	329061	19.777 ng/ml
9) t O-Xylene	14.271	340452	19.095 ng/ml
10) t 1,2,4-Trimethylbenzene	16.554	398157	19.572 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : \\74.0.250.170\Terastorage\pestpcbsrv\HPCHEM1\FID_B\Data\FB110518\
Data File : FB018536.D
Signal(s) : FID2B.CH
Acq On : 6 Nov 2018 6:23
Operator : MJ/SJ
Sample : J5764-03MSD
Misc : 5.01g/5.00mL DI Water
ALS Vial : 29 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Nov 06 07:36:58 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101218.M
Quant Title :
QLast Update : Fri Oct 12 08:04:31 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

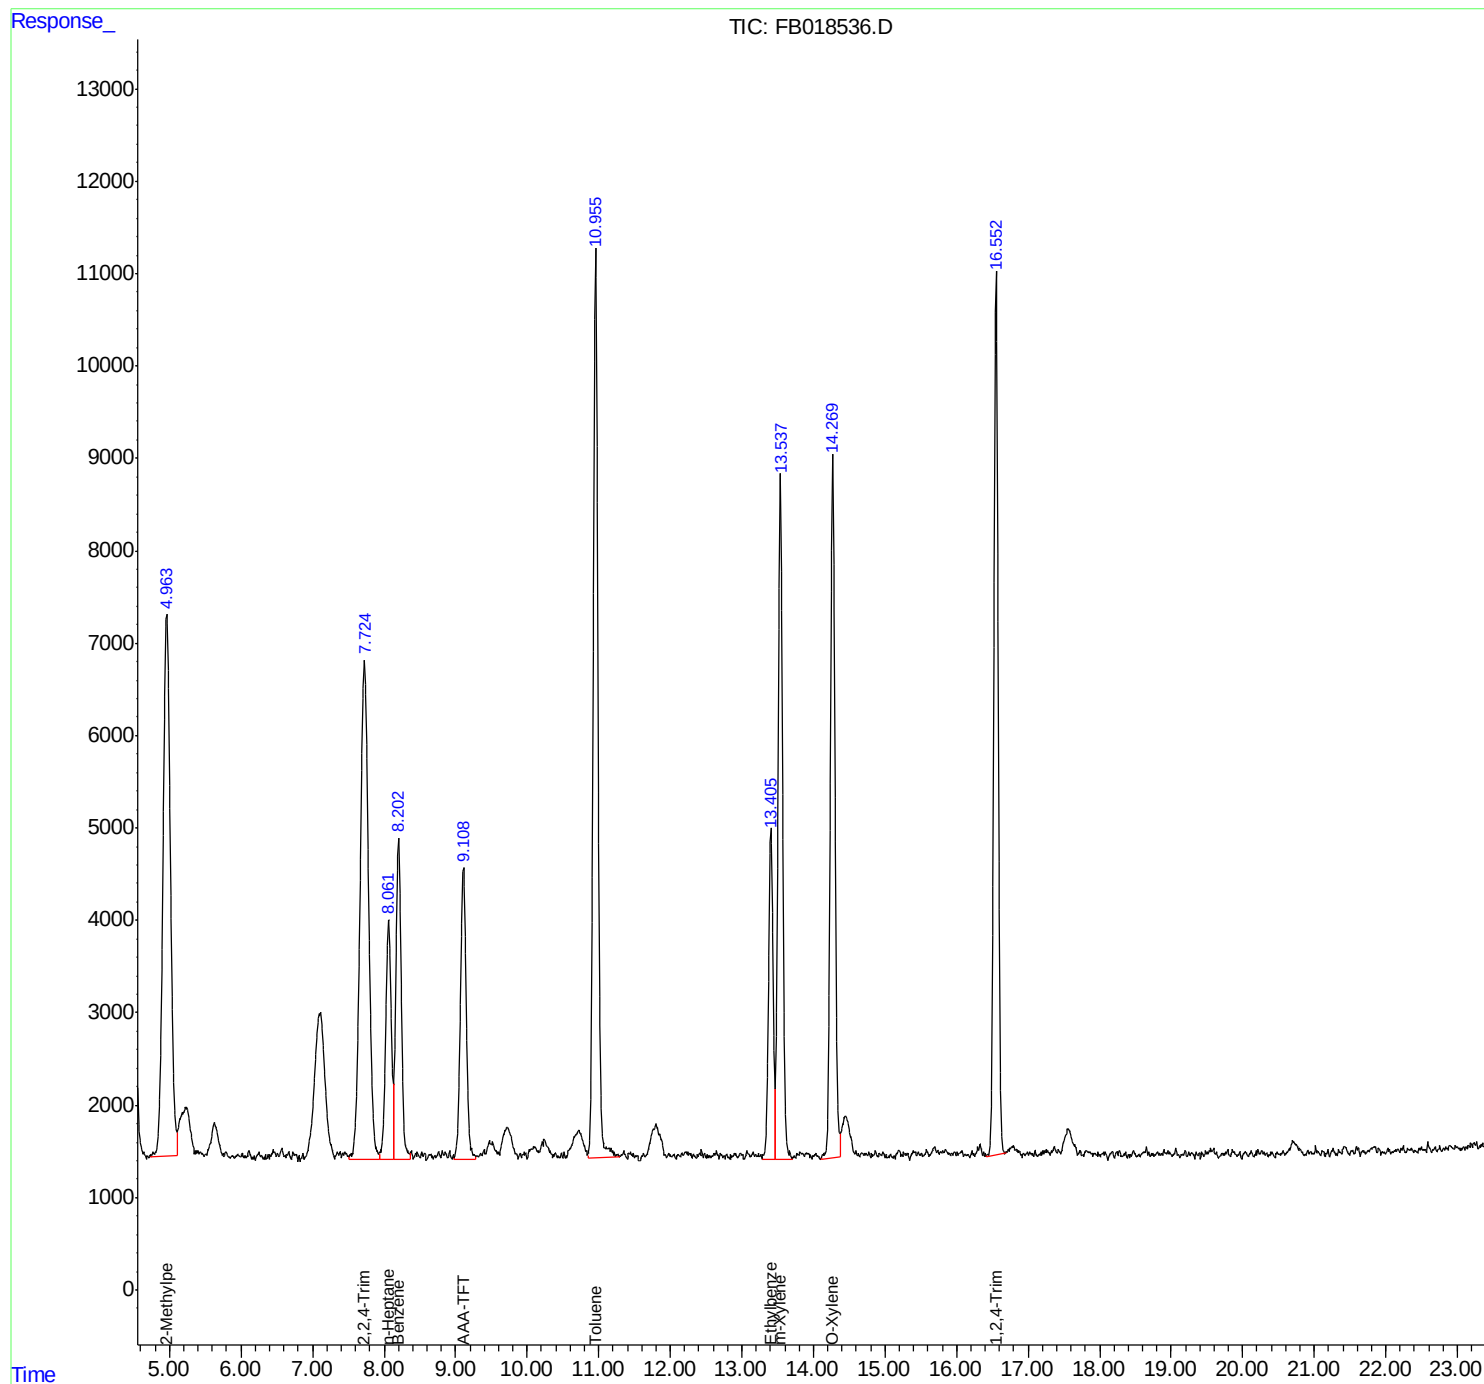


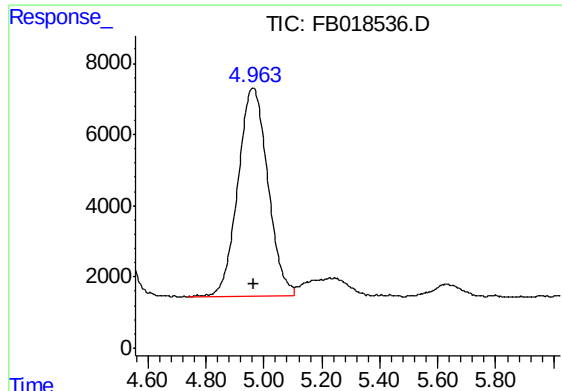

#1 2-Methylpentane


R.T.: 4.962 min
Delta R.T.: -0.003 min
Response: 422184
Conc: 27.60 ng/ml

Instrument :
FID_B
ClientSampleId :

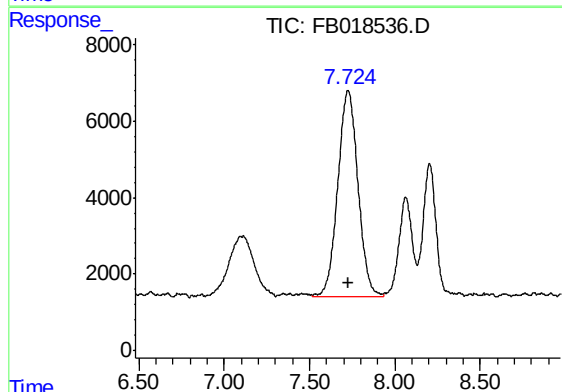


#2 2,2,4-Trimethylpentane

R.T.: 7.725 min
Delta R.T.: -0.003 min
Response: 443950
Conc: 30.04 ng/ml

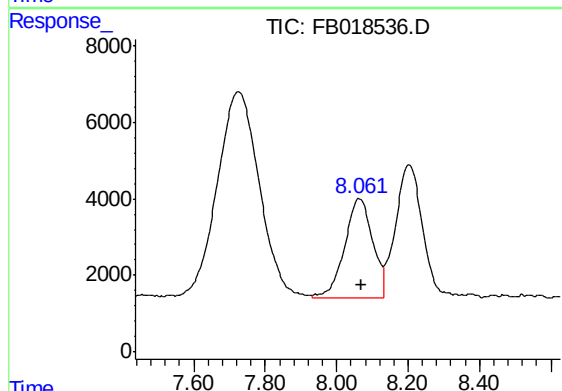


#3 n-Heptane

R.T.: 8.063 min
Delta R.T.: -0.004 min
Response: 140788
Conc: 9.93 ng/ml

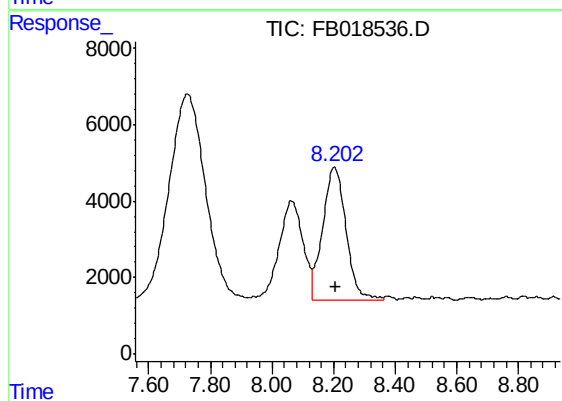

#4 Benzene


R.T.: 8.203 min
Delta R.T.: -0.003 min
Response: 183227
Conc: 9.84 ng/ml

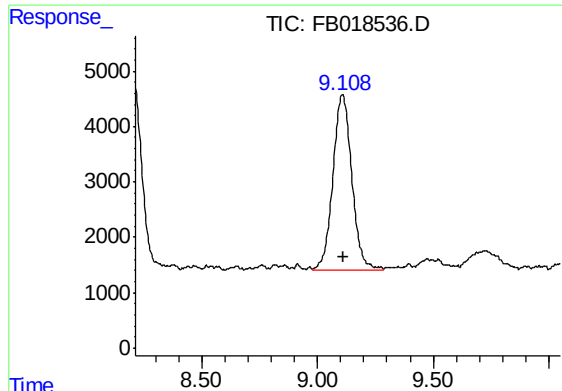

#5 AAA-TFT


R.T.: 9.108 min
Delta R.T.: -0.004 min
Response: 177087
Conc: 20.56 ng/ml

Instrument :
FID_B
ClientSampleId :

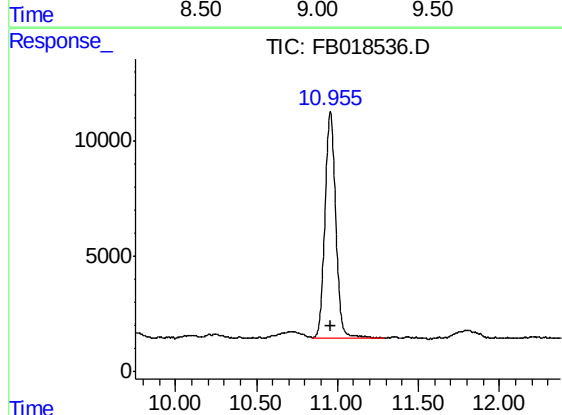


#6 Toluene

R.T.: 10.957 min
Delta R.T.: -0.005 min
Response: 457988
Conc: 30.05 ng/ml

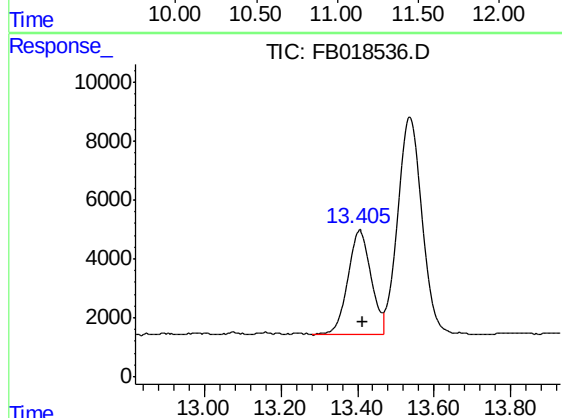


#7 Ethylbenzene

R.T.: 13.406 min
Delta R.T.: -0.006 min
Response: 155872
Conc: 9.82 ng/ml

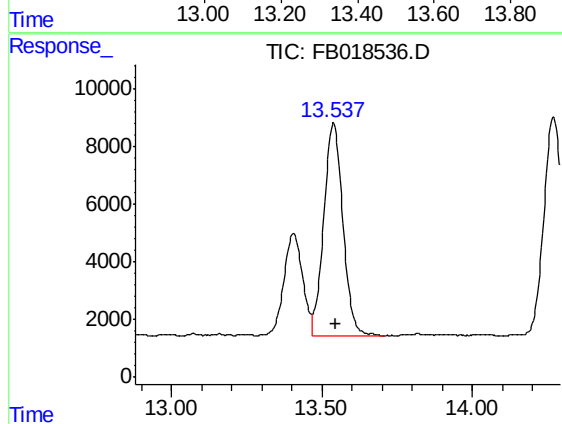

#8 m-Xylene


R.T.: 13.539 min
Delta R.T.: -0.006 min
Response: 329061
Conc: 19.78 ng/ml

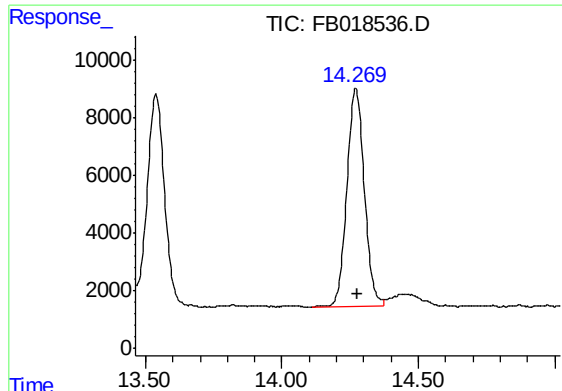

#9 O-Xylene

R.T.: 14.271 min
Delta R.T.: -0.006 min
Response: 340452
Conc: 19.09 ng/ml

Instrument :
FID_B
ClientSampleId :

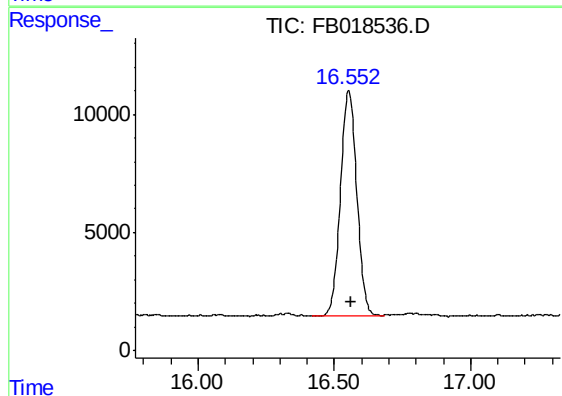

#10 1,2,4-Trimethylbenzene

R.T.: 16.554 min
Delta R.T.: -0.006 min
Response: 398157
Conc: 19.57 ng/ml